

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091919\
 Data File : P0061153.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 18:48
 Operator : SM/AJ
 Sample : K4957-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-42-COMP

Manual Integrations
 APPROVED

Ankita
 9/21/2019 1:11:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:25:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.528	850934	705301	23.129	25.260
2) SA Decachlor...	10.026	8.404	887739	688017	19.321	19.629
Target Compounds						
26) L6 AR-1254-1	6.372	5.361	44037	26608	22.857	12.911 #
27) L6 AR-1254-2	6.597	5.505	77122	18713	24.507	9.917 #
28) L6 AR-1254-3	6.966	5.900	67351	52977	19.123	16.662
29) L6 AR-1254-4	7.246	6.124	29106	23136	10.752	11.112
30) L6 AR-1254-5	7.663	6.535	58625	65886	19.881m	20.818

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091919\
Data File : PO061153.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 18:48
Operator : SM/AJ
Sample : K4957-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-42-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:25:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

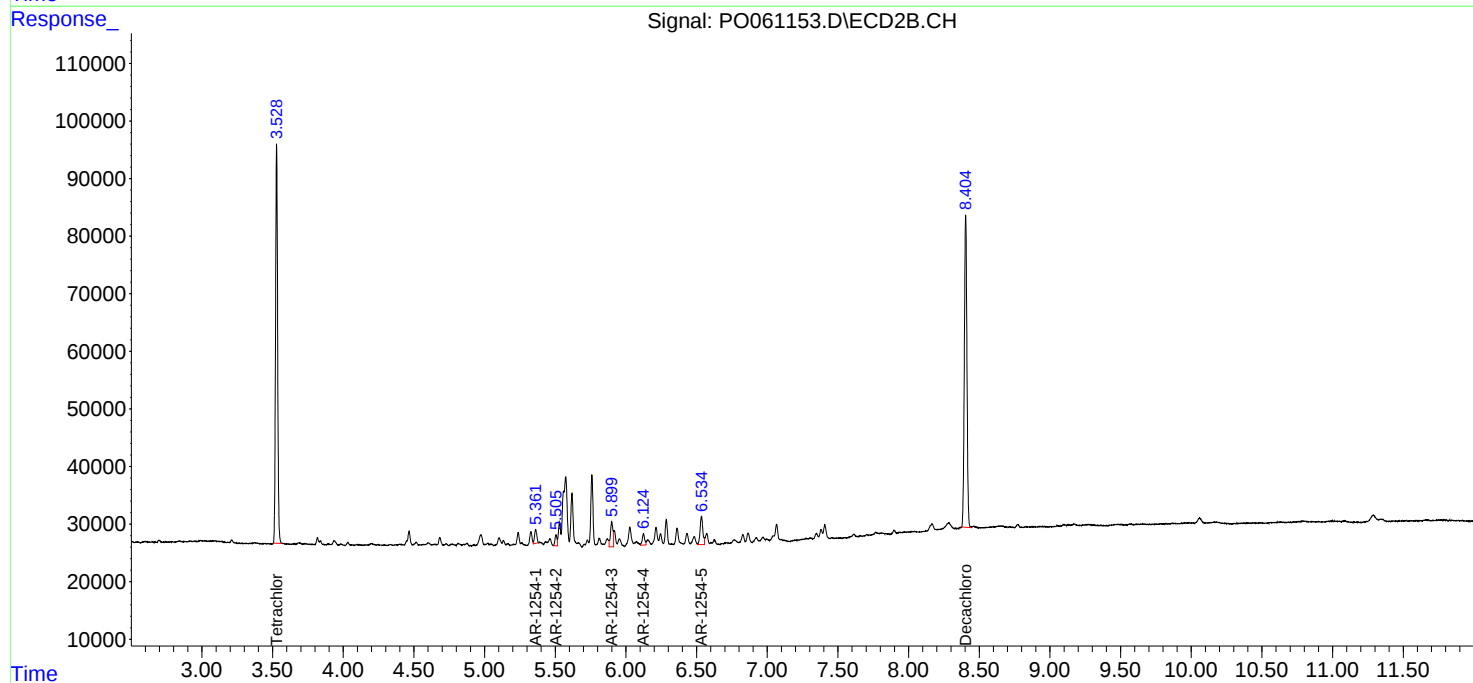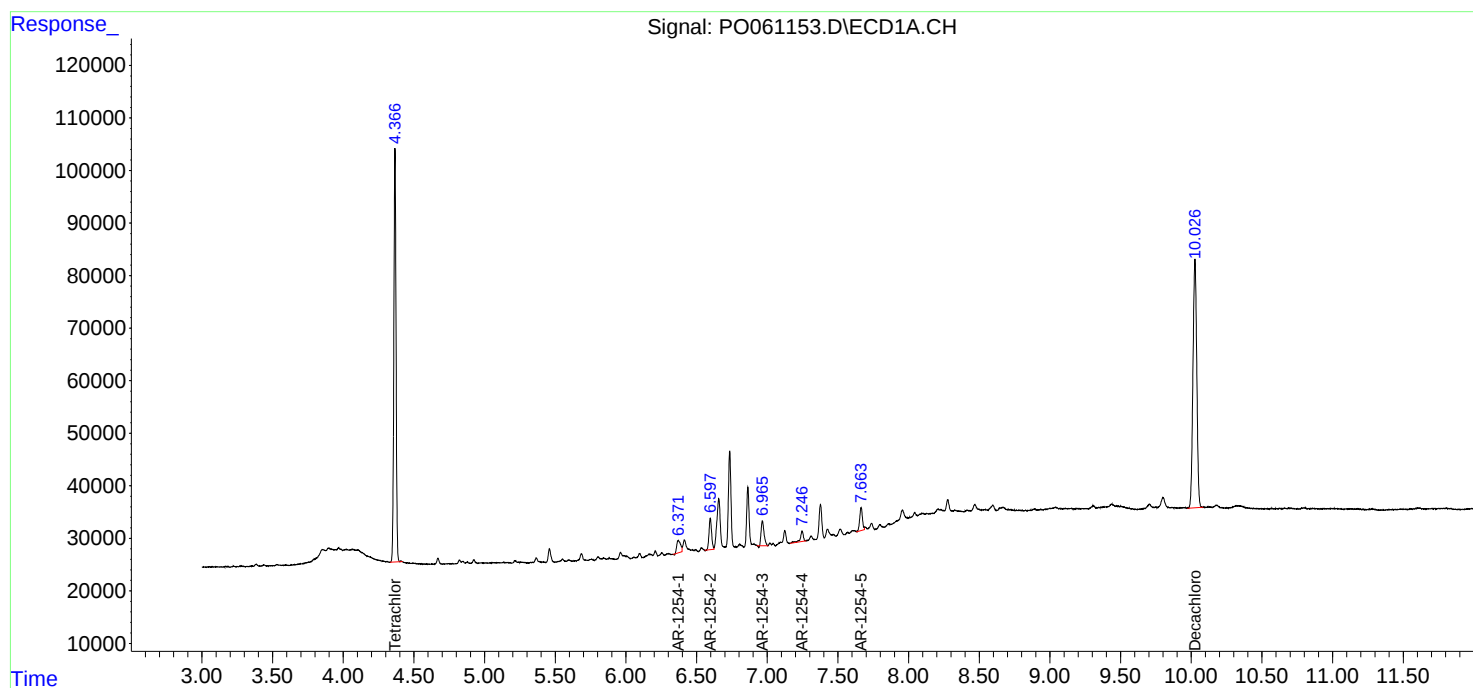

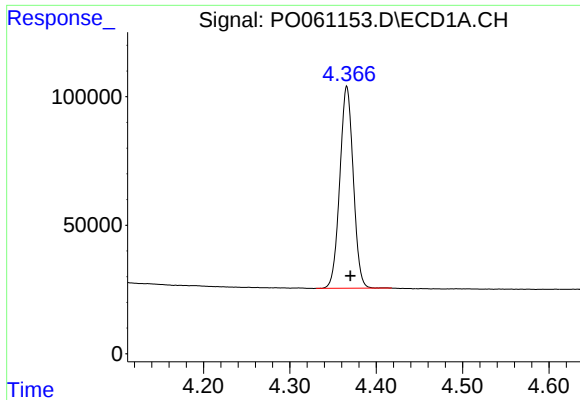


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 850934
Conc: 23.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-42-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:27 PM

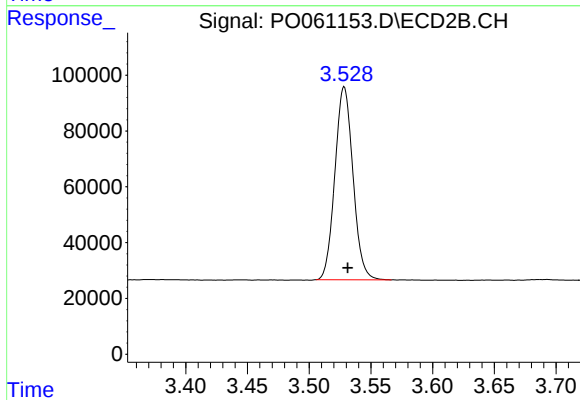


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.003 min
Response: 705301
Conc: 25.26 ng/ml

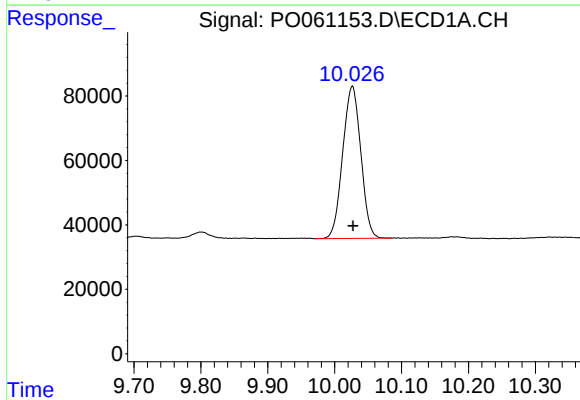


#2 Decachlorobiphenyl

R.T.: 10.026 min
Delta R.T.: -0.001 min
Response: 887739
Conc: 19.32 ng/ml

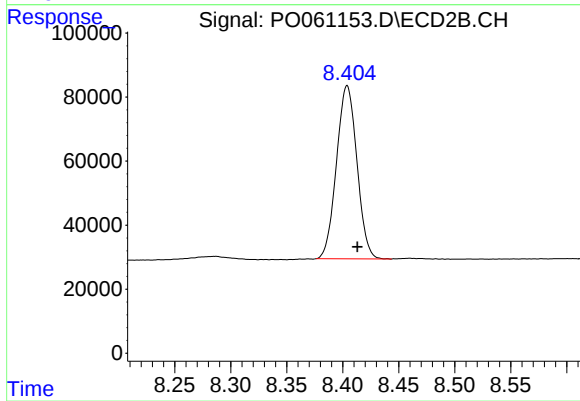

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.009 min
Response: 688017
Conc: 19.63 ng/ml

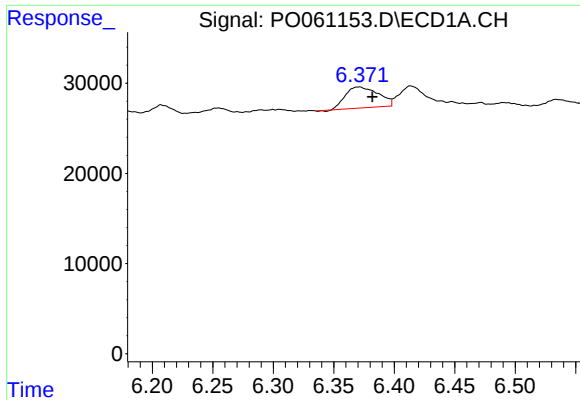


#26 AR-1254-1

R.T.: 6.372 min
Delta R.T.: -0.010 min
Response: 44037
Conc: 22.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-42-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:27 PM

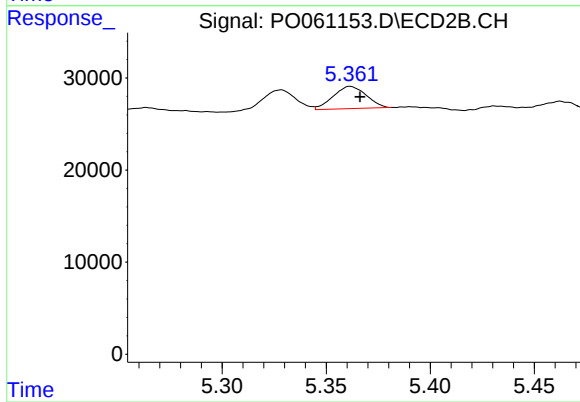


#26 AR-1254-1

R.T.: 5.361 min
Delta R.T.: -0.005 min
Response: 26608
Conc: 12.91 ng/ml

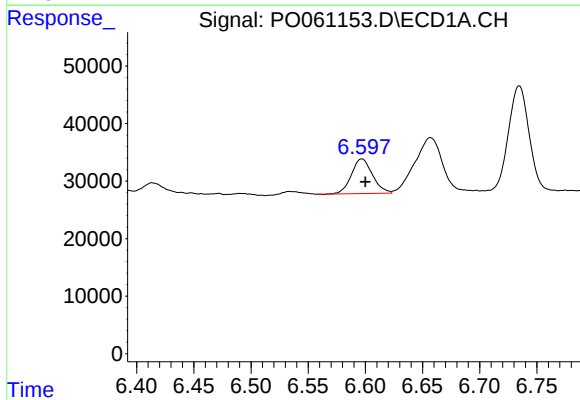


#27 AR-1254-2

R.T.: 6.597 min
Delta R.T.: -0.003 min
Response: 77122
Conc: 24.51 ng/ml

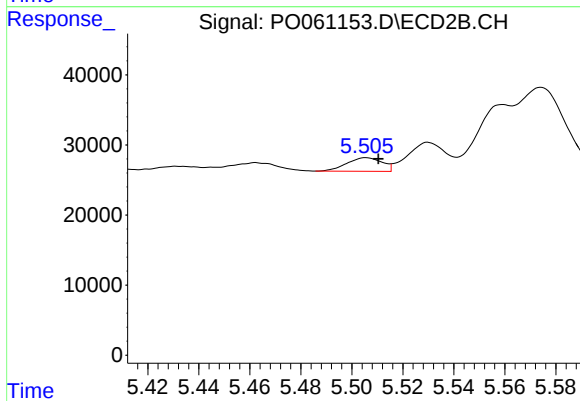

#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: -0.005 min
Response: 18713
Conc: 9.92 ng/ml

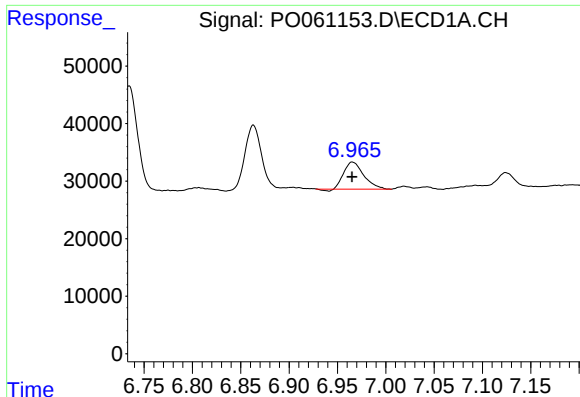


#28 AR-1254-3

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 67351
Conc: 19.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-42-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:27 PM

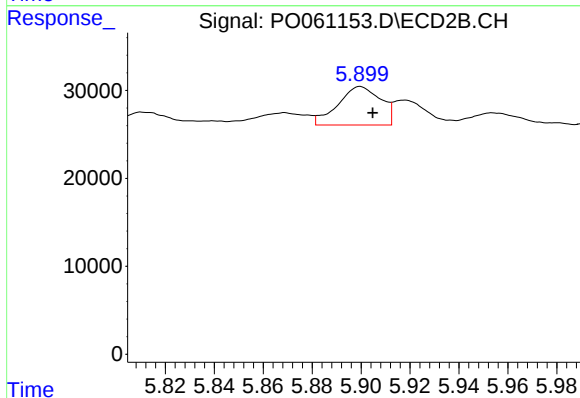


#28 AR-1254-3

R.T.: 5.900 min
Delta R.T.: -0.005 min
Response: 52977
Conc: 16.66 ng/ml

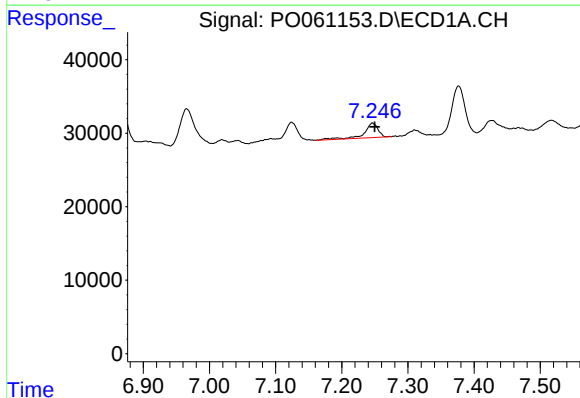


#29 AR-1254-4

R.T.: 7.246 min
Delta R.T.: -0.004 min
Response: 29106
Conc: 10.75 ng/ml

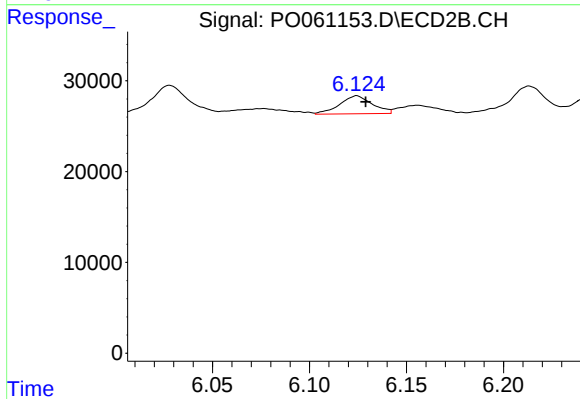

#29 AR-1254-4

R.T.: 6.124 min
Delta R.T.: -0.005 min
Response: 23136
Conc: 11.11 ng/ml

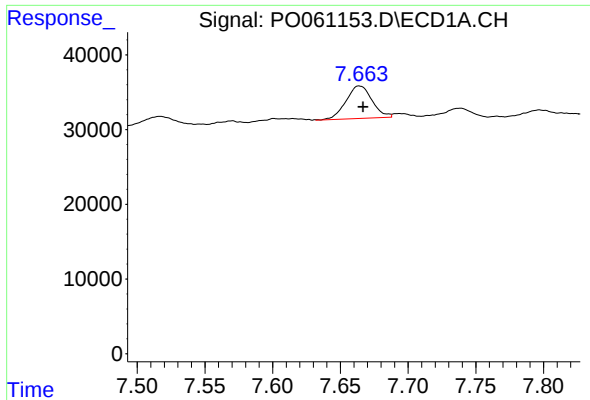


#30 AR-1254-5

R.T.: 7.663 min
Delta R.T.: -0.003 min
Response: 58625
Conc: 19.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-42-COMP

Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:27 PM

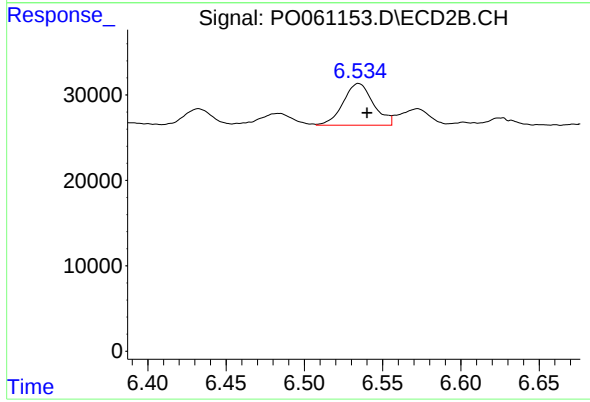

#30 AR-1254-5

R.T.: 6.535 min
Delta R.T.: -0.005 min
Response: 65886
Conc: 20.82 ng/ml