

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091919\
 Data File : P0061157.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 19:53
 Operator : SM/AJ
 Sample : K4957-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-26-COMP

Manual Integrations
 APPROVED

Ankita
 9/21/2019 1:11:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:26:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.529	921431	738736	25.045	26.457
2) SA Decachlor...	10.027	8.403	770217	597284	16.763	17.040m
Target Compounds						
31) L7 AR-1260-1	7.124	6.028	258500	199776	106.177	94.978
32) L7 AR-1260-2	7.379	6.214	275455	232247	91.109	90.036
33) L7 AR-1260-3	7.737	6.362	118092	132843	49.485	55.166
34) L7 AR-1260-4	7.956	6.827	208618	87452	74.568	40.861 #
35) L7 AR-1260-5	8.277	7.066	173124	200629	31.793	41.517 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091919\
Data File : PO061157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 19:53
Operator : SM/AJ
Sample : K4957-12
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-26-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:26:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

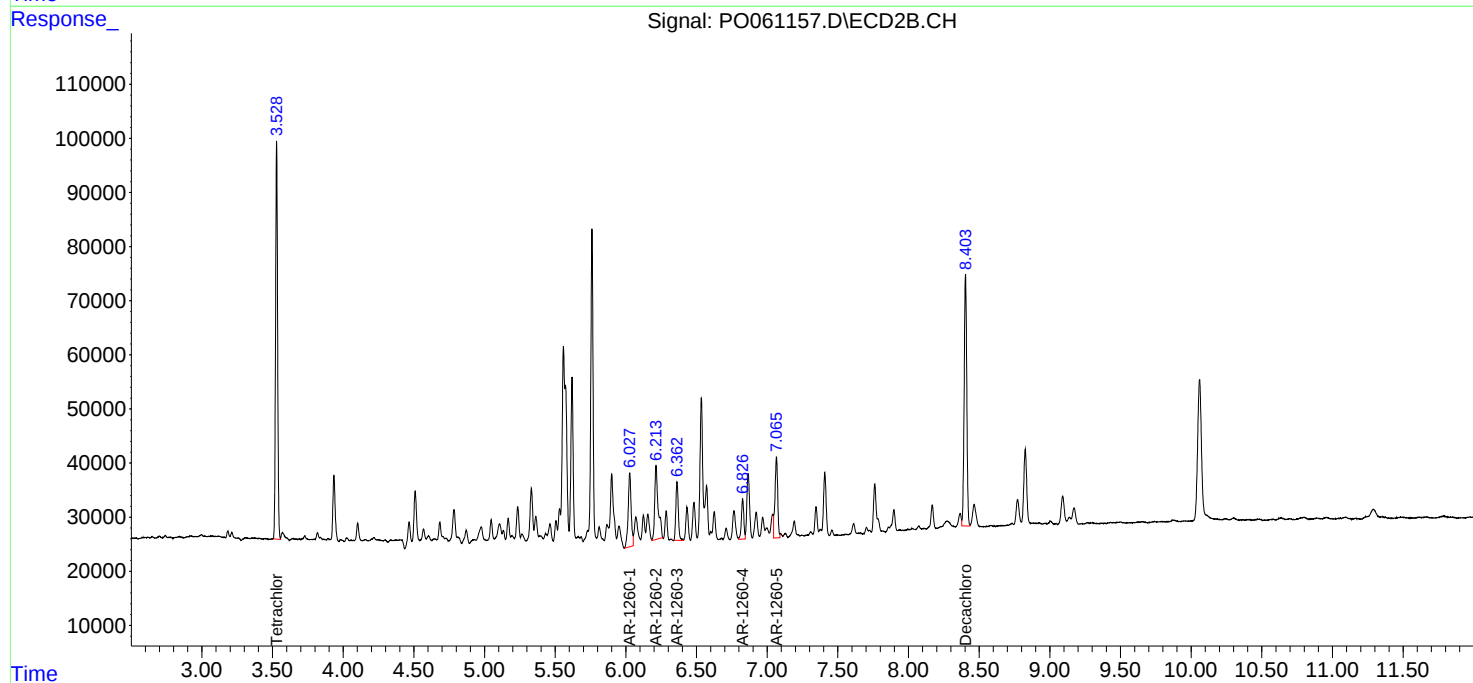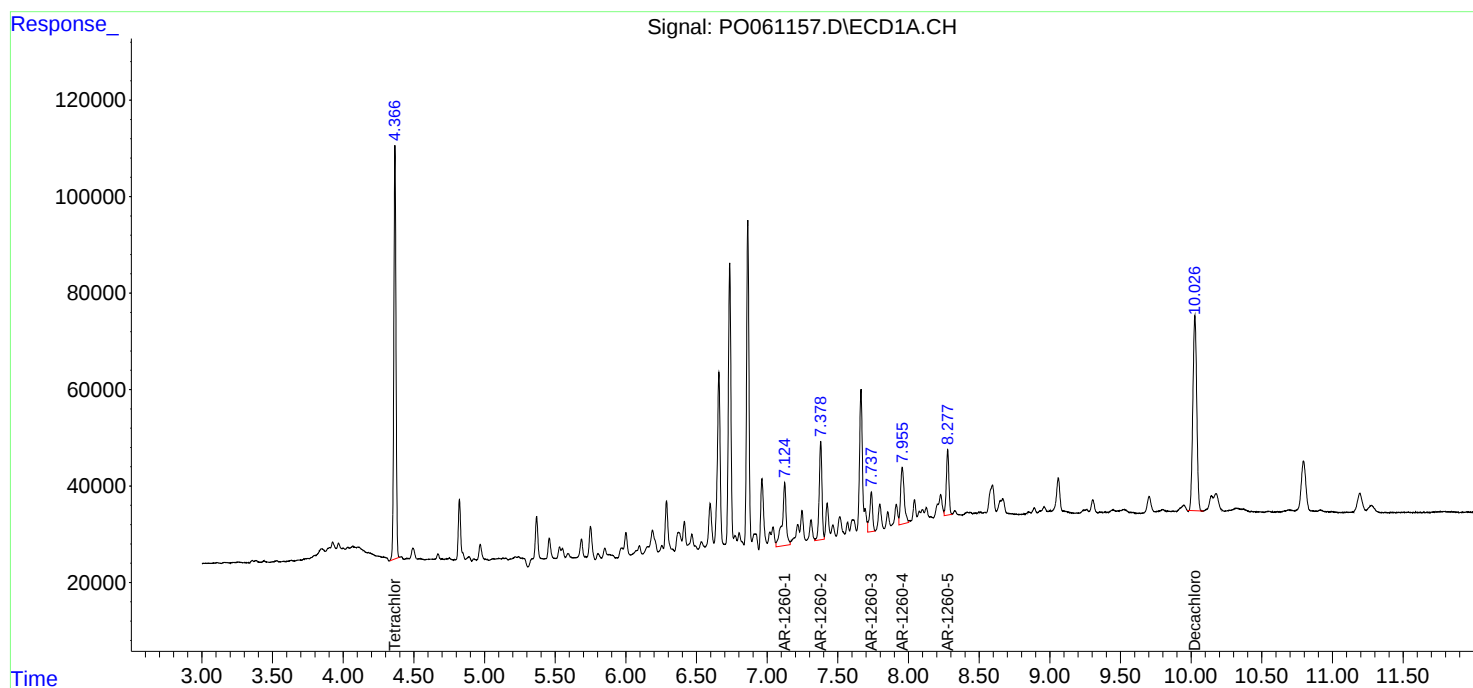

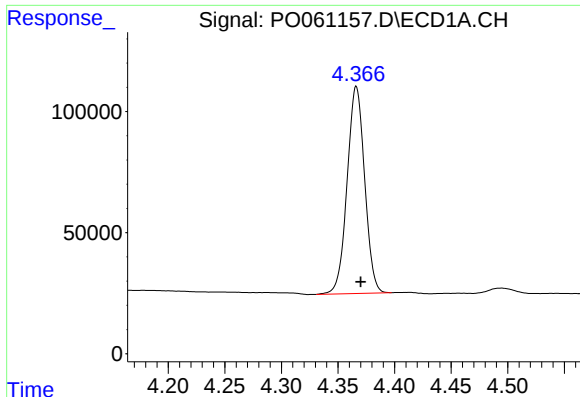


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 921431
Conc: 25.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-26-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:29 PM

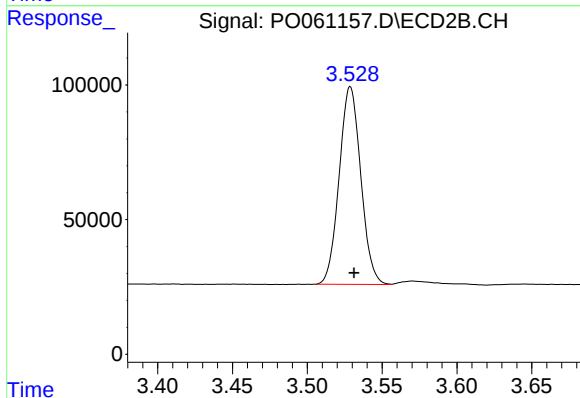


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.002 min
Response: 738736
Conc: 26.46 ng/ml

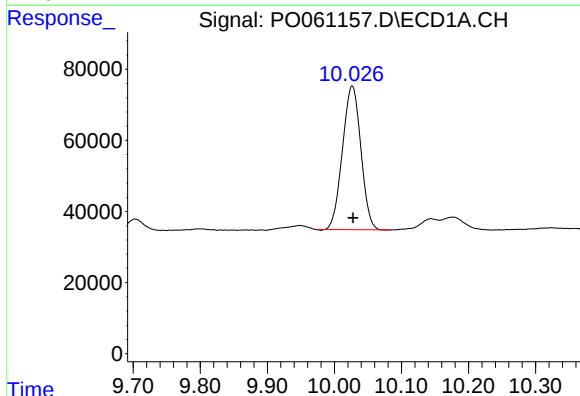


#2 Decachlorobiphenyl

R.T.: 10.027 min
Delta R.T.: -0.001 min
Response: 770217
Conc: 16.76 ng/ml

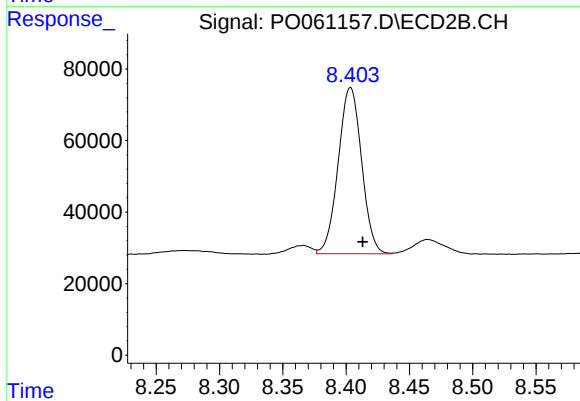

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.010 min
Response: 597284
Conc: 17.04 ng/ml m

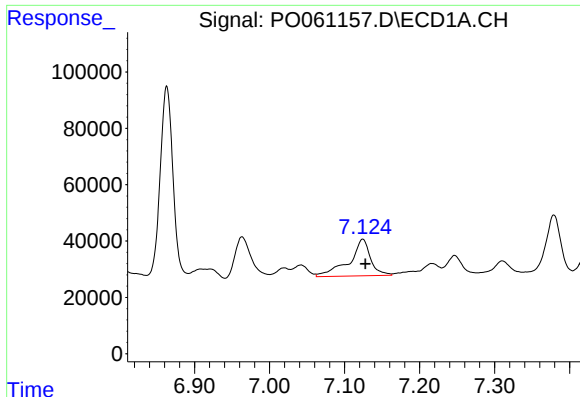


#31 AR-1260-1

R.T.: 7.124 min
Delta R.T.: -0.004 min
Response: 258500
Conc: 106.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-26-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:29 PM

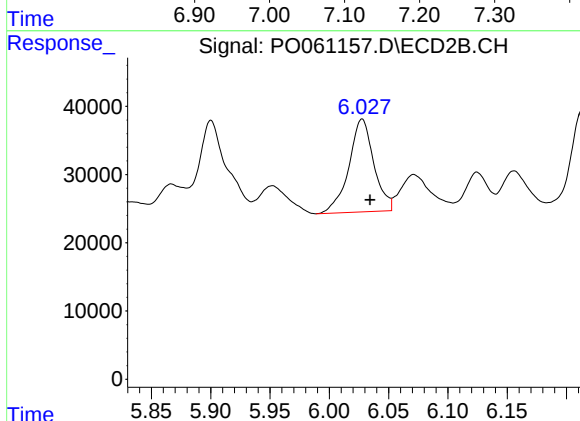


#31 AR-1260-1

R.T.: 6.028 min
Delta R.T.: -0.007 min
Response: 199776
Conc: 94.98 ng/ml

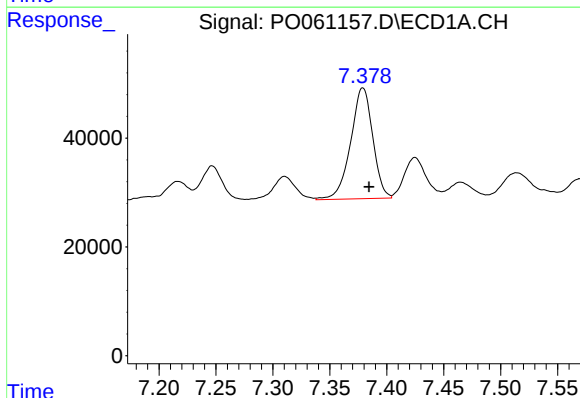


#32 AR-1260-2

R.T.: 7.379 min
Delta R.T.: -0.005 min
Response: 275455
Conc: 91.11 ng/ml

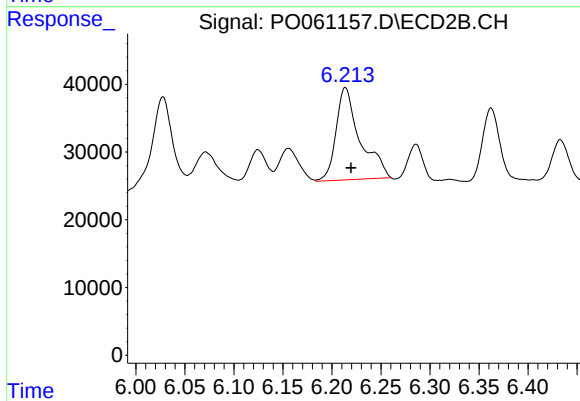

#32 AR-1260-2

R.T.: 6.214 min
Delta R.T.: -0.006 min
Response: 232247
Conc: 90.04 ng/ml

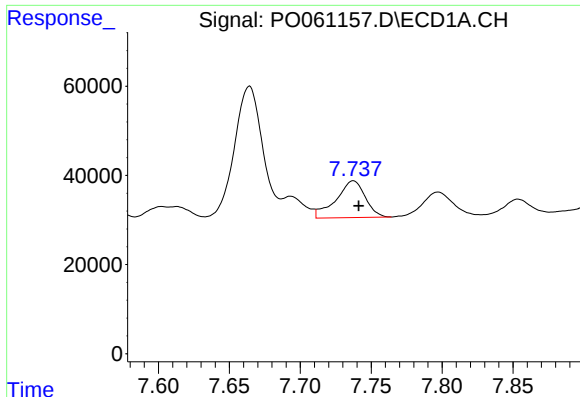


#33 AR-1260-3

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 118092
Conc: 49.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-26-COMP


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:29 PM

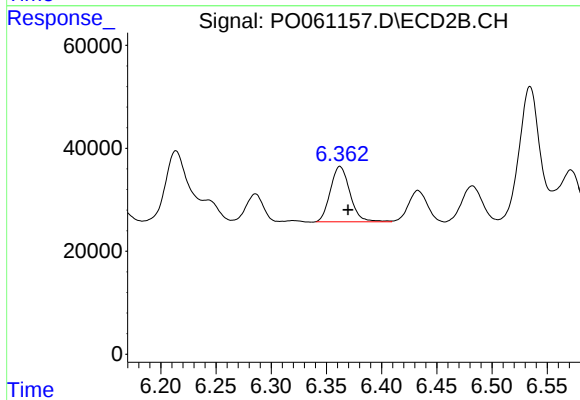


#33 AR-1260-3

R.T.: 6.362 min
Delta R.T.: -0.007 min
Response: 132843
Conc: 55.17 ng/ml

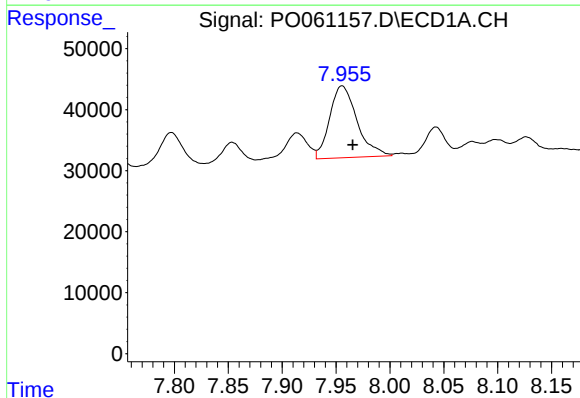


#34 AR-1260-4

R.T.: 7.956 min
Delta R.T.: -0.010 min
Response: 208618
Conc: 74.57 ng/ml

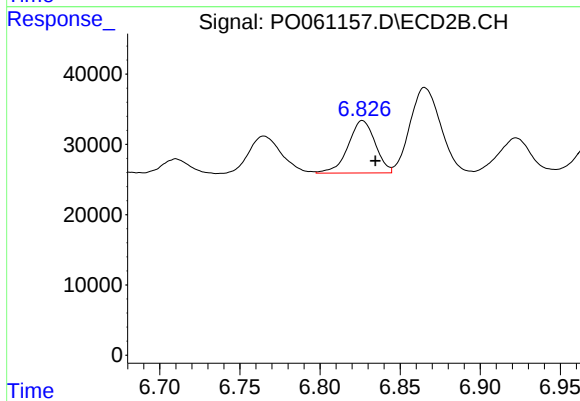

#34 AR-1260-4

R.T.: 6.827 min
Delta R.T.: -0.008 min
Response: 87452
Conc: 40.86 ng/ml

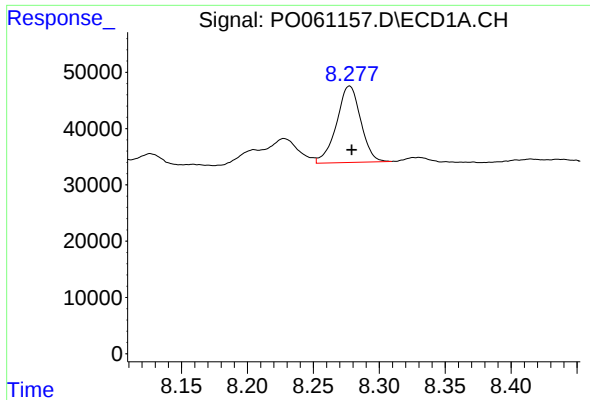


#35 AR-1260-5

R.T.: 8.277 min
Delta R.T.: -0.002 min
Response: 173124
Conc: 31.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-26-COMP

Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:29 PM

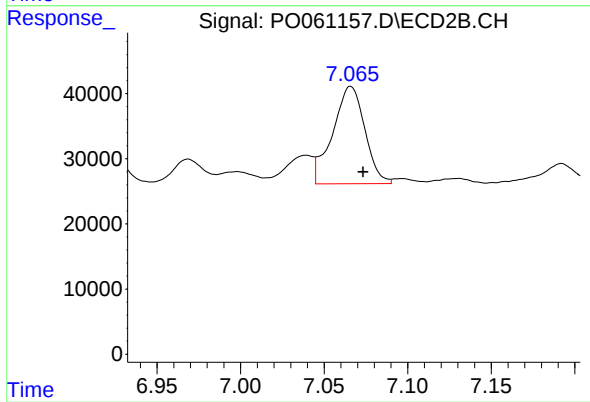

#35 AR-1260-5

R.T.: 7.066 min
Delta R.T.: -0.007 min
Response: 200629
Conc: 41.52 ng/ml