

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091919\
 Data File : P0061158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 20:09
 Operator : SM/AJ
 Sample : K4959-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WALL-1

Manual Integrations
 APPROVED

Ankita
 9/21/2019 1:11:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:26:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.529	923933	752220	25.113	26.940
2) SA Decachlor...	10.025	8.404	1004583	756601	21.864	21.585m
Target Compounds						
26) L6 AR-1254-1	6.379	5.362	27421	45980	14.232	22.310 #
27) L6 AR-1254-2	6.598	5.505	85104	36658	27.044	19.426 #
28) L6 AR-1254-3	6.963	5.900	82837	83730	23.520	26.334
29) L6 AR-1254-4	7.248	6.124	61643	49847	22.771	23.942
30) L6 AR-1254-5	7.664	6.534	55303	80874	18.754	25.553 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091919\
Data File : PO061158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 20:09
Operator : SM/AJ
Sample : K4959-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
WALL-1


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:26:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

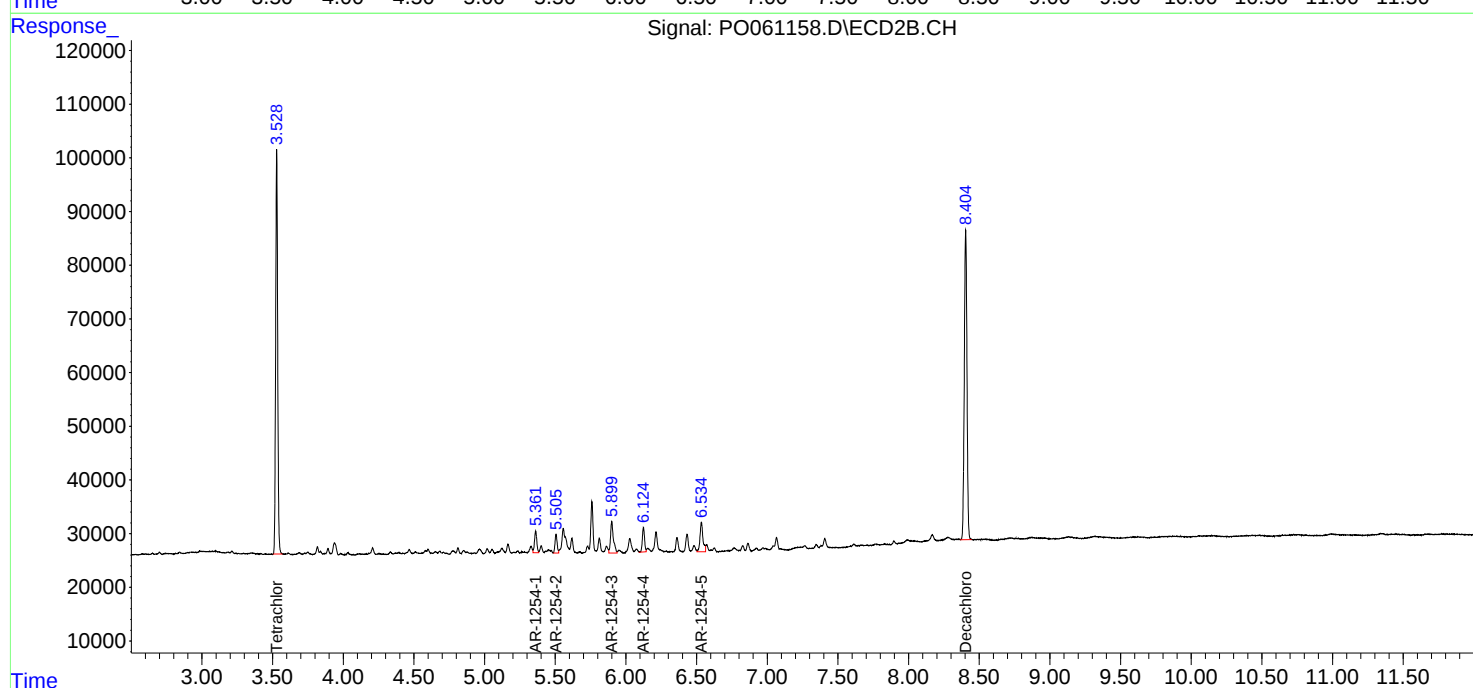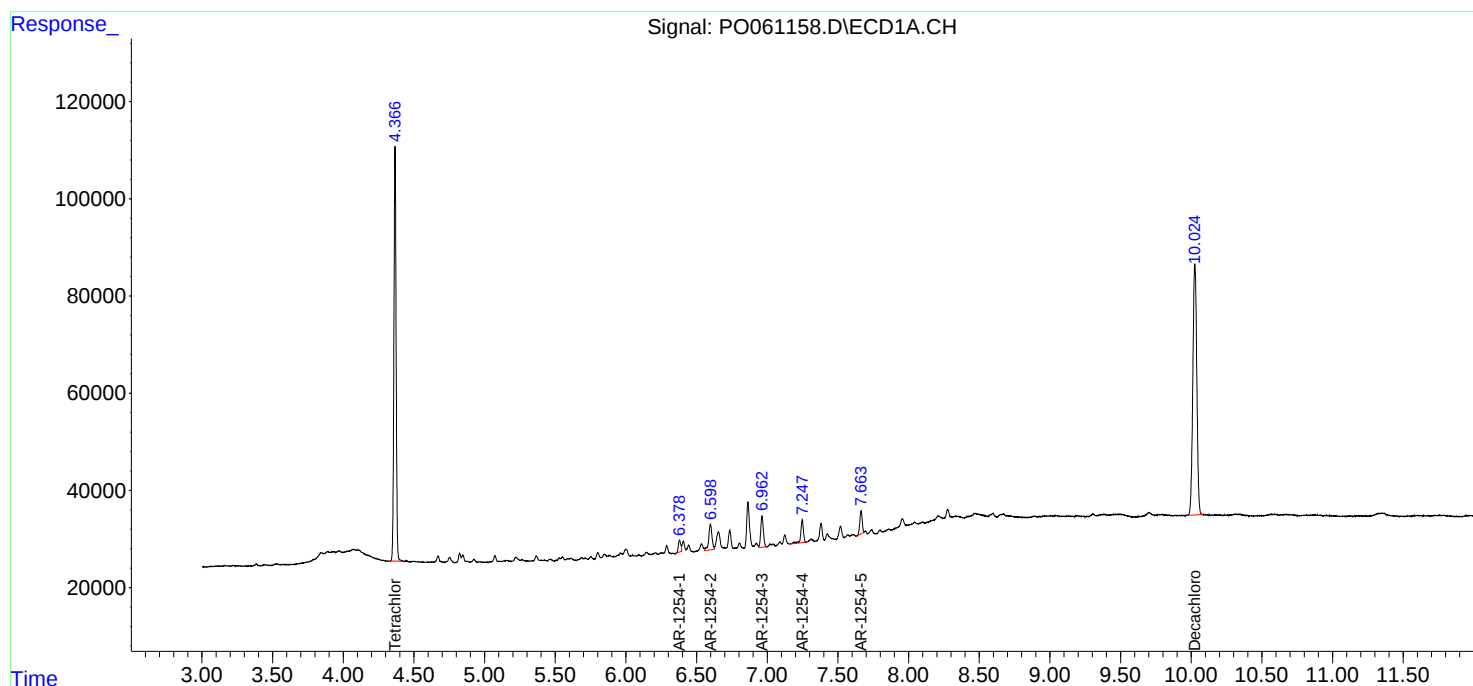

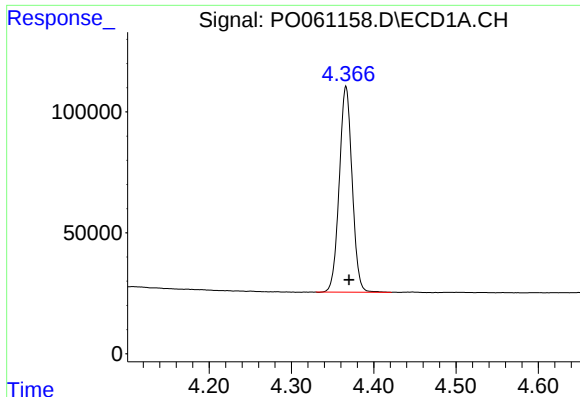


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 923933
Conc: 25.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
WALL-1


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:30 PM

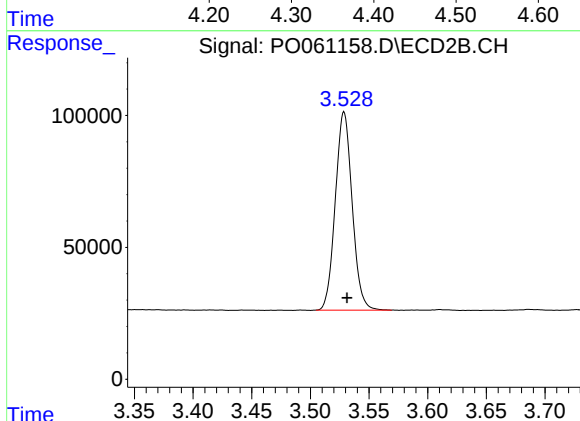


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.003 min
Response: 752220
Conc: 26.94 ng/ml

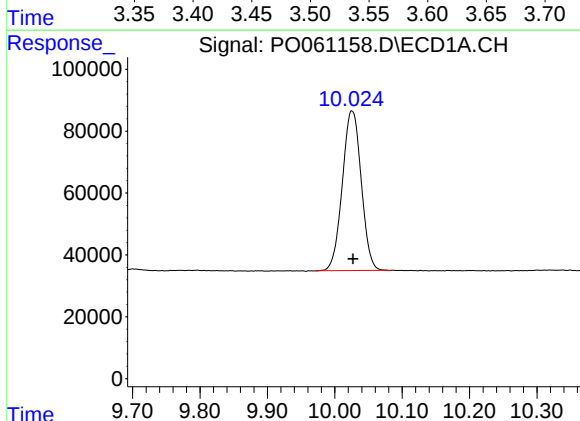


#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.002 min
Response: 1004583
Conc: 21.86 ng/ml

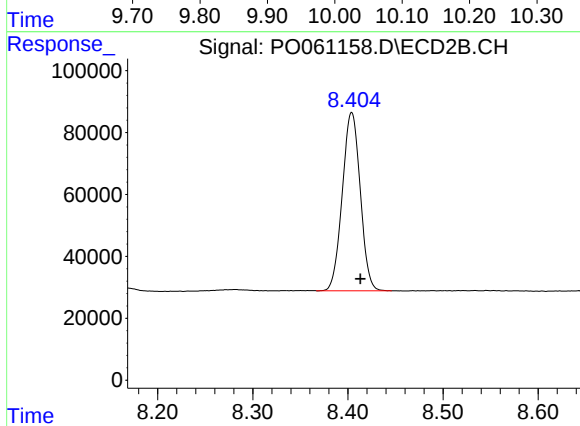

#2 Decachlorobiphenyl

R.T.: 8.404 min
Delta R.T.: -0.009 min
Response: 756601
Conc: 21.59 ng/ml m

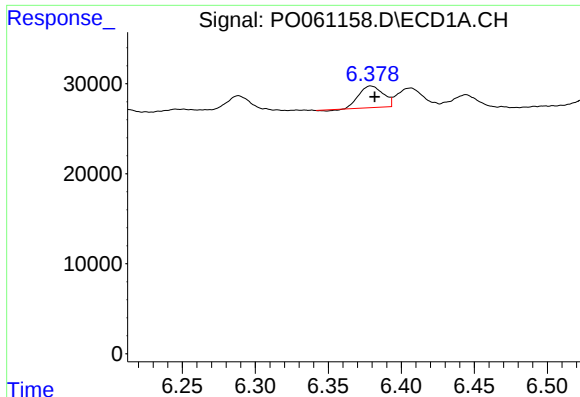


#26 AR-1254-1

R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 27421
Conc: 14.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
WALL-1


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:30 PM

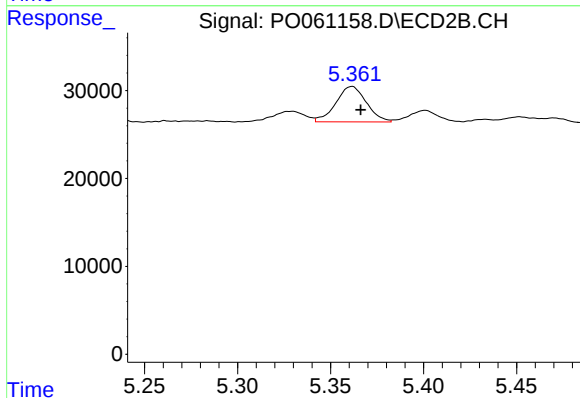


#26 AR-1254-1

R.T.: 5.362 min
Delta R.T.: -0.005 min
Response: 45980
Conc: 22.31 ng/ml

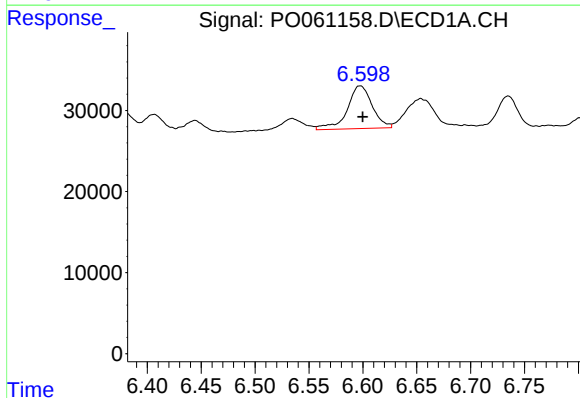


#27 AR-1254-2

R.T.: 6.598 min
Delta R.T.: -0.002 min
Response: 85104
Conc: 27.04 ng/ml

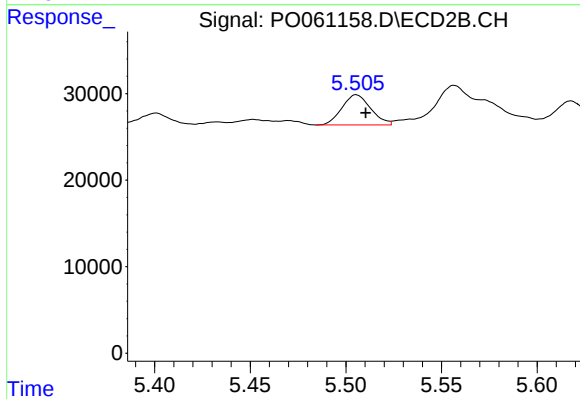

#27 AR-1254-2

R.T.: 5.505 min
Delta R.T.: -0.005 min
Response: 36658
Conc: 19.43 ng/ml

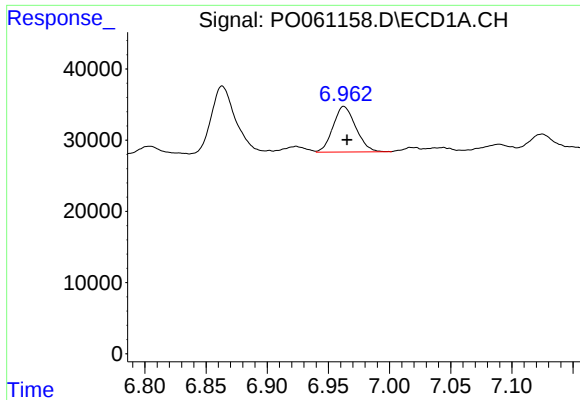


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.002 min
Response: 82837
Conc: 23.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
WALL-1


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:30 PM

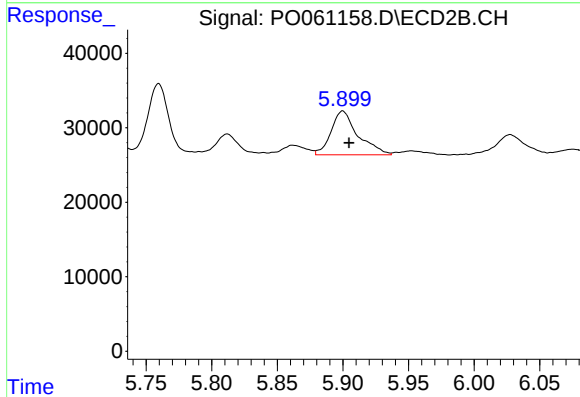


#28 AR-1254-3

R.T.: 5.900 min
Delta R.T.: -0.005 min
Response: 83730
Conc: 26.33 ng/ml

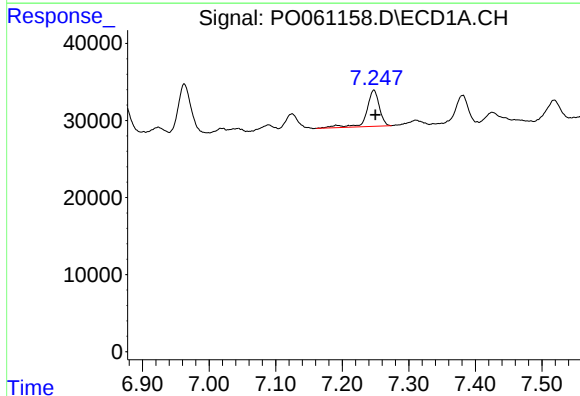


#29 AR-1254-4

R.T.: 7.248 min
Delta R.T.: -0.002 min
Response: 61643
Conc: 22.77 ng/ml

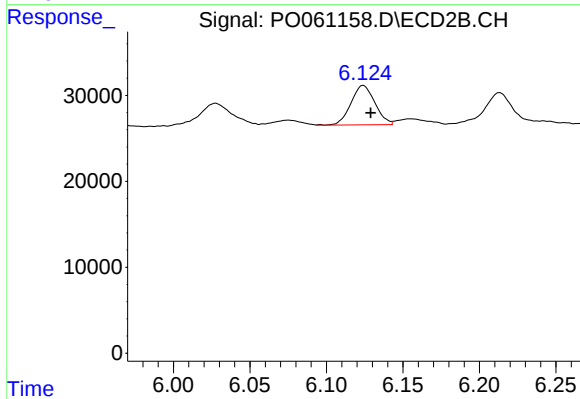

#29 AR-1254-4

R.T.: 6.124 min
Delta R.T.: -0.005 min
Response: 49847
Conc: 23.94 ng/ml

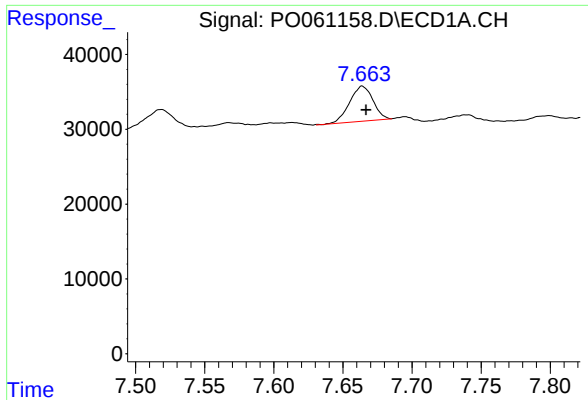


#30 AR-1254-5

R.T.: 7.664 min
Delta R.T.: -0.003 min
Response: 55303
Conc: 18.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
WALL-1

Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:30 PM

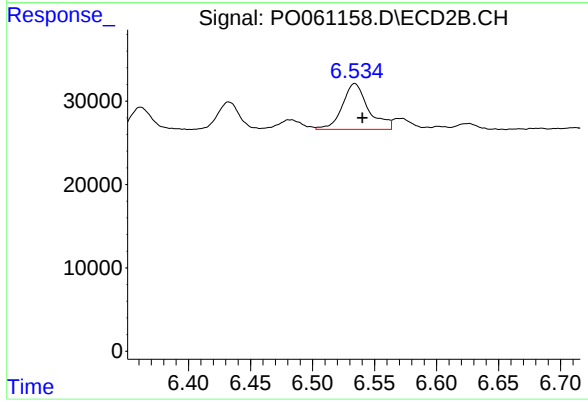

#30 AR-1254-5

R.T.: 6.534 min
Delta R.T.: -0.006 min
Response: 80874
Conc: 25.55 ng/ml