

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091919\
 Data File : P0061171.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Sep 2019 00:28
 Operator : SM/AJ
 Sample : K4962-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-5

Manual Integrations
 APPROVED

Ankita
 9/21/2019 1:11:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:31:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.528	900409	726280	24.474	26.011
2) SA Decachlor...	10.024	8.403	992722	761347	21.606	21.721
Target Compounds						
31) L7 AR-1260-1	7.123	6.027	66162	98006	27.175	46.594 #
32) L7 AR-1260-2	7.380	6.212	113397	112974	37.507	43.797
33) L7 AR-1260-3	7.738	6.361	89404	55481	37.463	23.040 #
34) L7 AR-1260-4	7.961	6.826	103735	66679	37.079m	31.155
35) L7 AR-1260-5	8.275	7.065	146653	159406	26.932	32.986

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091919\
Data File : PO061171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Sep 2019 00:28
Operator : SM/AJ
Sample : K4962-09
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-1-5


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:31:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

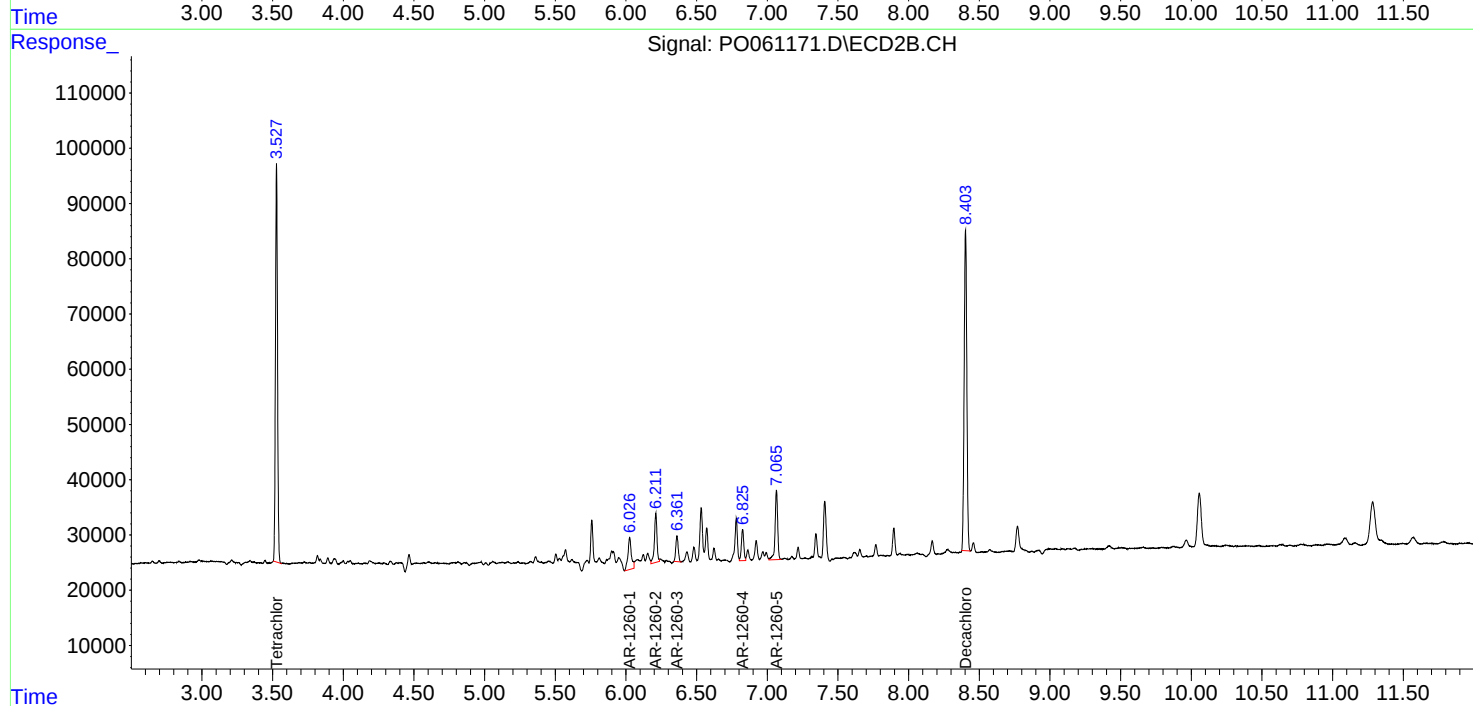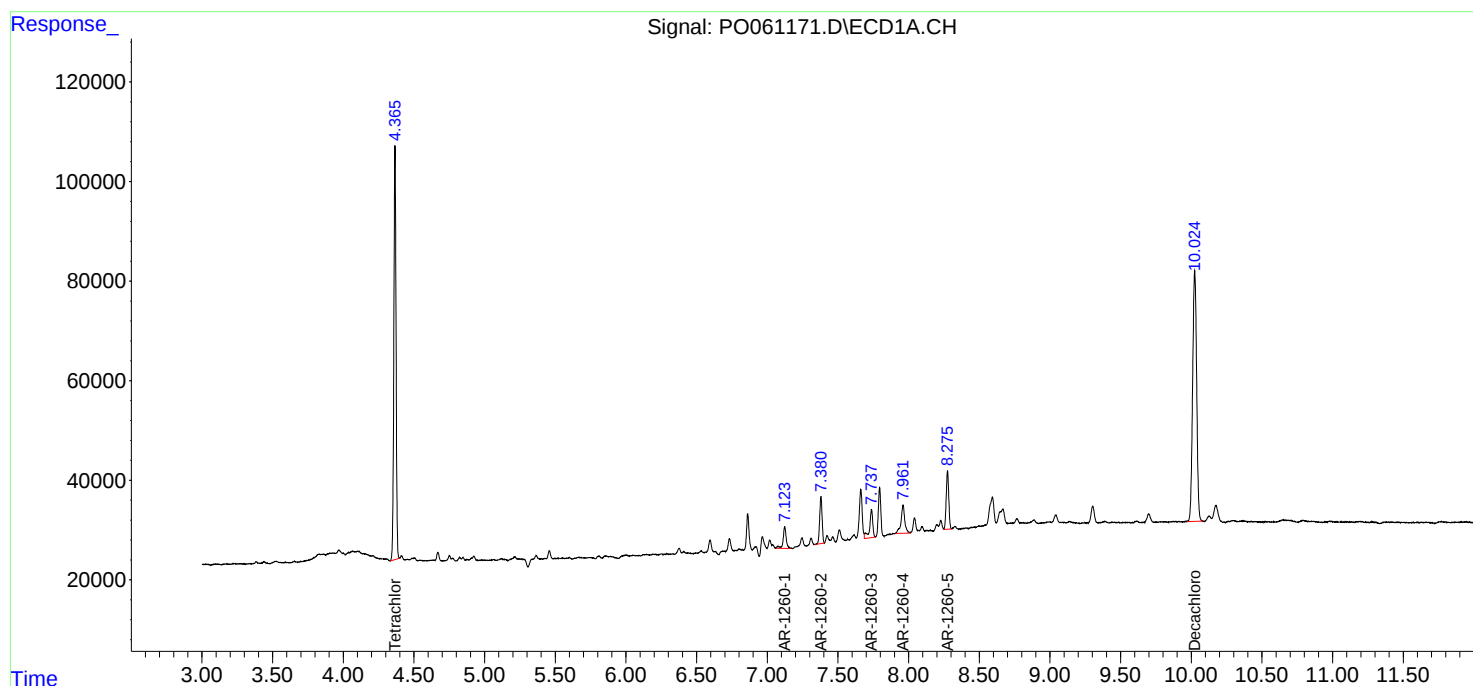

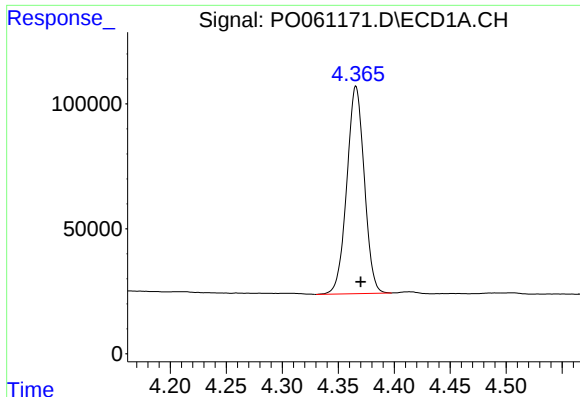


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 900409
Conc: 24.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-5


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:58 PM

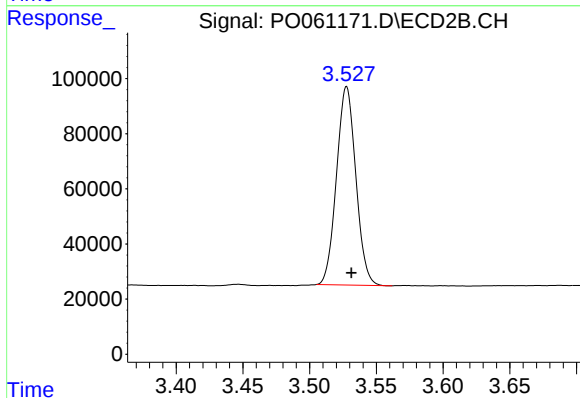


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.003 min
Response: 726280
Conc: 26.01 ng/ml

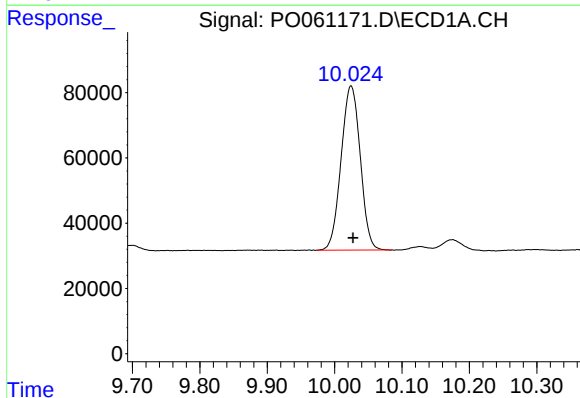


#2 Decachlorobiphenyl

R.T.: 10.024 min
Delta R.T.: -0.003 min
Response: 992722
Conc: 21.61 ng/ml

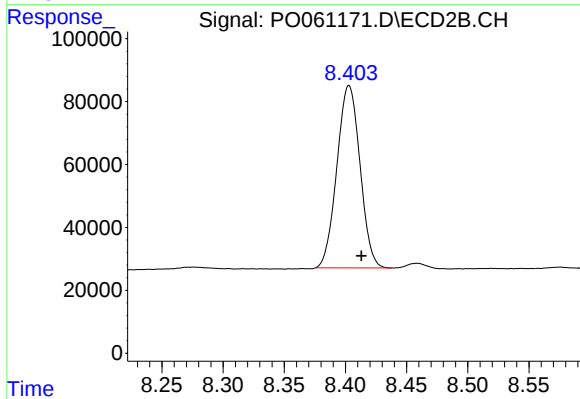

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.010 min
Response: 761347
Conc: 21.72 ng/ml

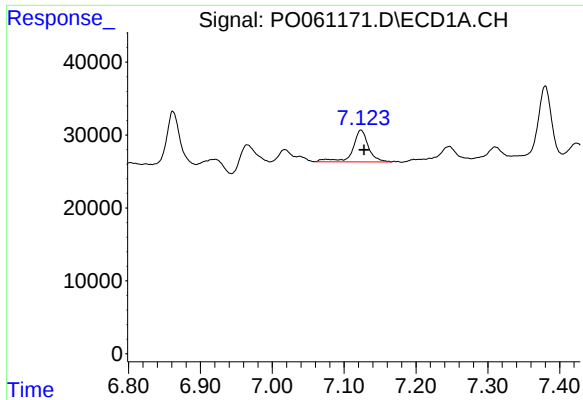


#31 AR-1260-1

R.T.: 7.123 min
Delta R.T.: -0.004 min
Response: 66162
Conc: 27.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-5


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:58 PM

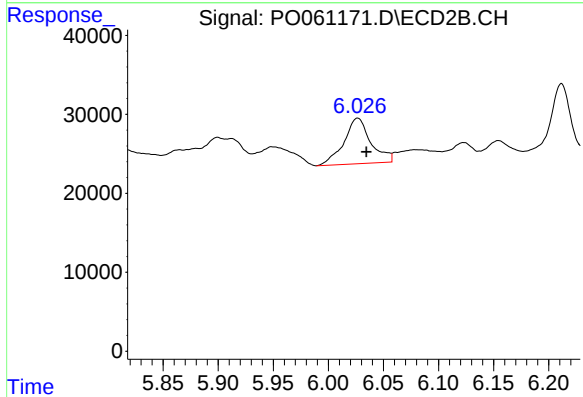


#31 AR-1260-1

R.T.: 6.027 min
Delta R.T.: -0.008 min
Response: 98006
Conc: 46.59 ng/ml

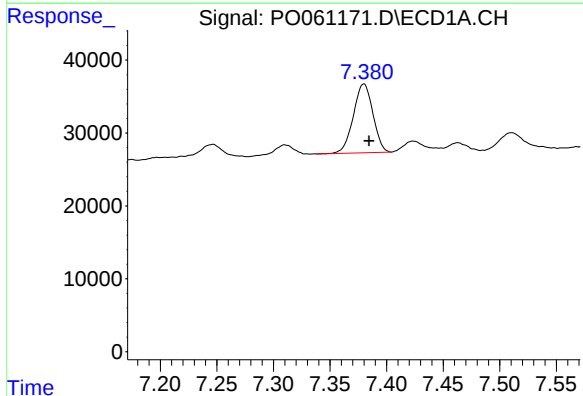


#32 AR-1260-2

R.T.: 7.380 min
Delta R.T.: -0.005 min
Response: 113397
Conc: 37.51 ng/ml

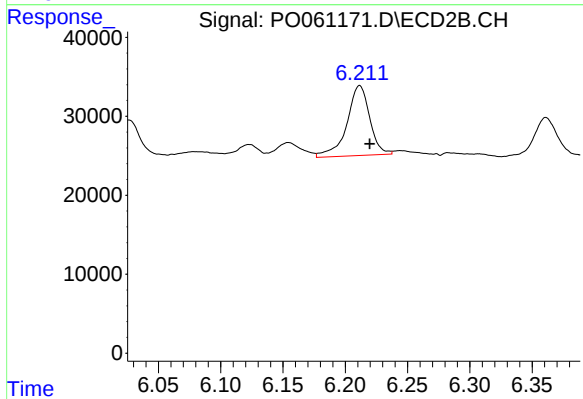

#32 AR-1260-2

R.T.: 6.212 min
Delta R.T.: -0.008 min
Response: 112974
Conc: 43.80 ng/ml

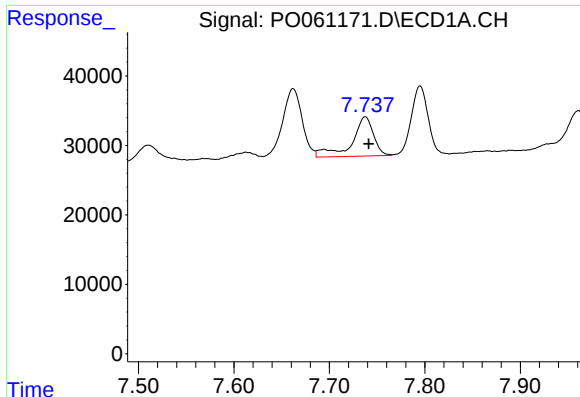


#33 AR-1260-3

R.T.: 7.738 min
Delta R.T.: -0.004 min
Response: 89404
Conc: 37.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-5


Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:58 PM

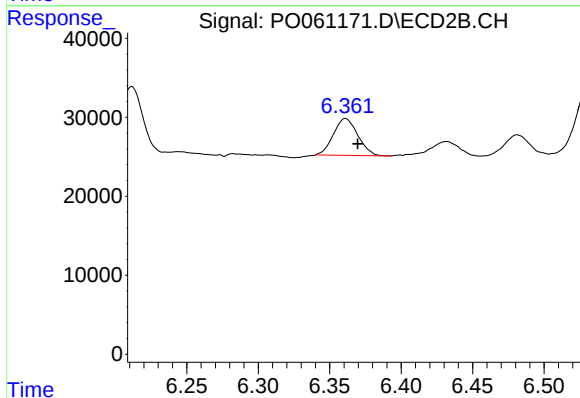


#33 AR-1260-3

R.T.: 6.361 min
Delta R.T.: -0.009 min
Response: 55481
Conc: 23.04 ng/ml

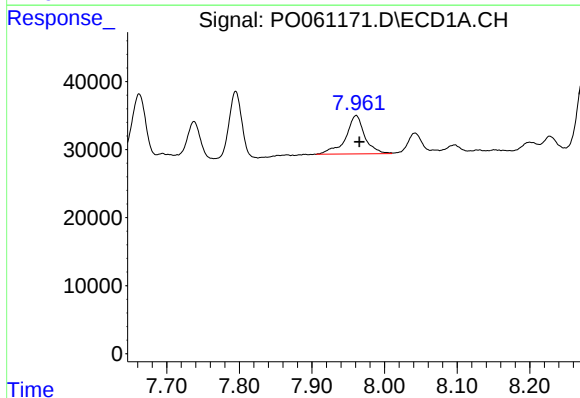


#34 AR-1260-4

R.T.: 7.961 min
Delta R.T.: -0.005 min
Response: 103735
Conc: 37.08 ng/ml m

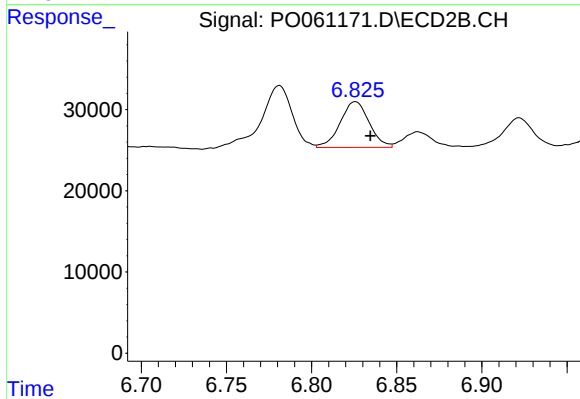

#34 AR-1260-4

R.T.: 6.826 min
Delta R.T.: -0.009 min
Response: 66679
Conc: 31.15 ng/ml

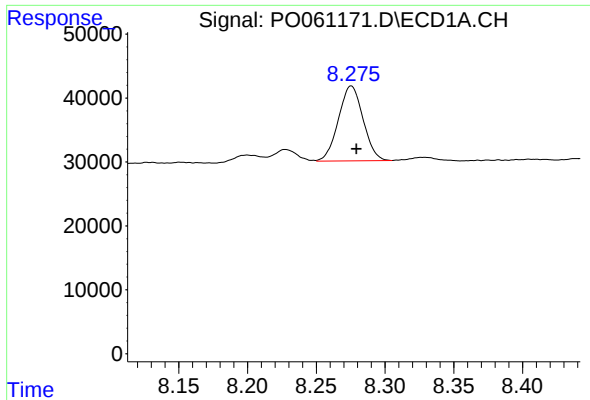


#35 AR-1260-5

R.T.: 8.275 min
Delta R.T.: -0.004 min
Response: 146653
Conc: 26.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-5

Manual Integrations
APPROVED

Ankita
9/21/2019 1:11:58 PM

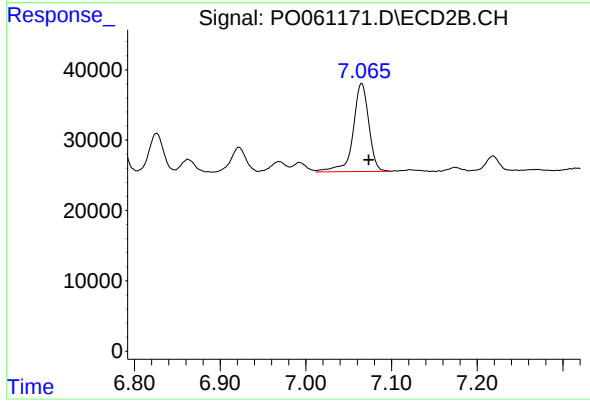

#35 AR-1260-5

R.T.: 7.065 min
Delta R.T.: -0.008 min
Response: 159406
Conc: 32.99 ng/ml