

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0091925\
 Data File : P0113867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2025 17:40
 Operator : YP/AJ
 Sample : Q3138-04 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-25-0239-0241

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2025
 Supervised By :mohammad ahmed 09/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 04:15:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.649	7381709	5611903	0.837m	1.051m#
2) SA Decachlor...	8.671	8.615	9636924	3416256	1.440	1.636

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO091925\
Data File : PO113867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2025 17:40
Operator : YP/AJ
Sample : Q3138-04 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-25-0239-0241


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2025
Supervised By :mohammad ahmed 09/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 04:15:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

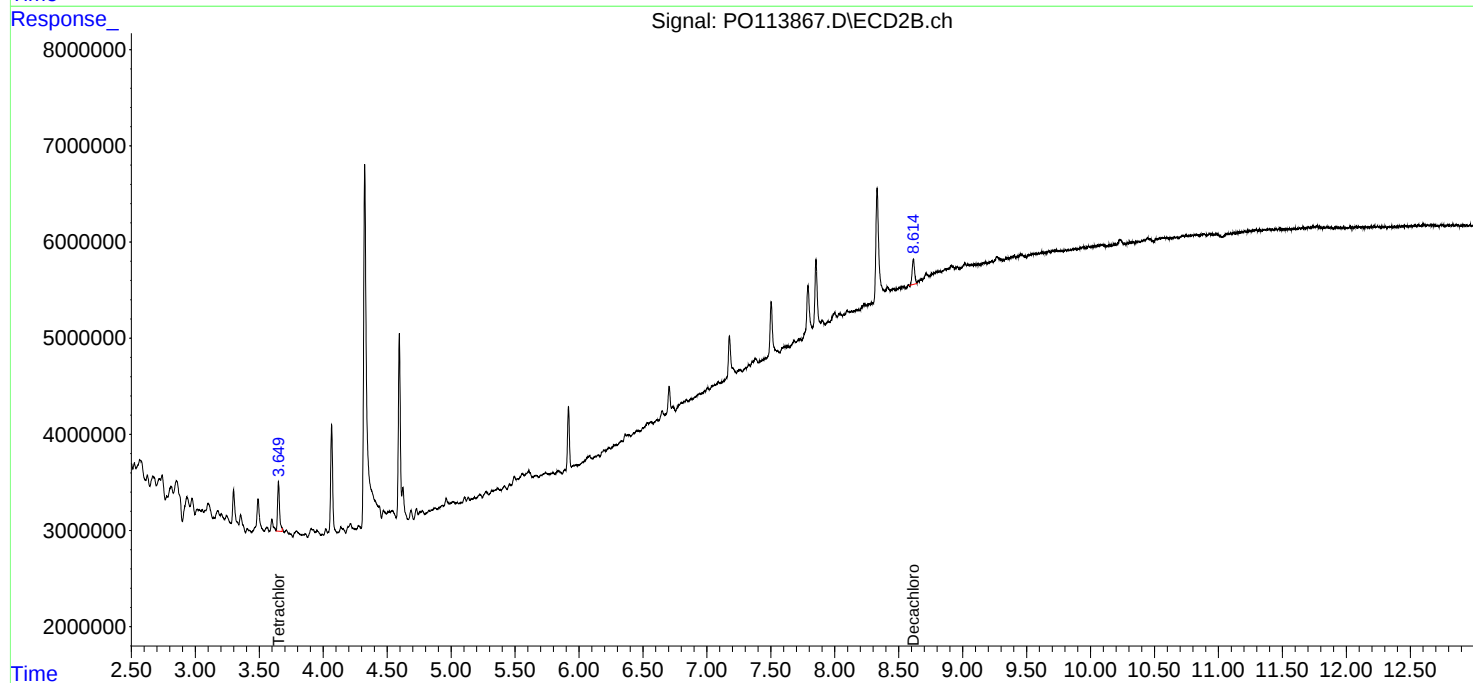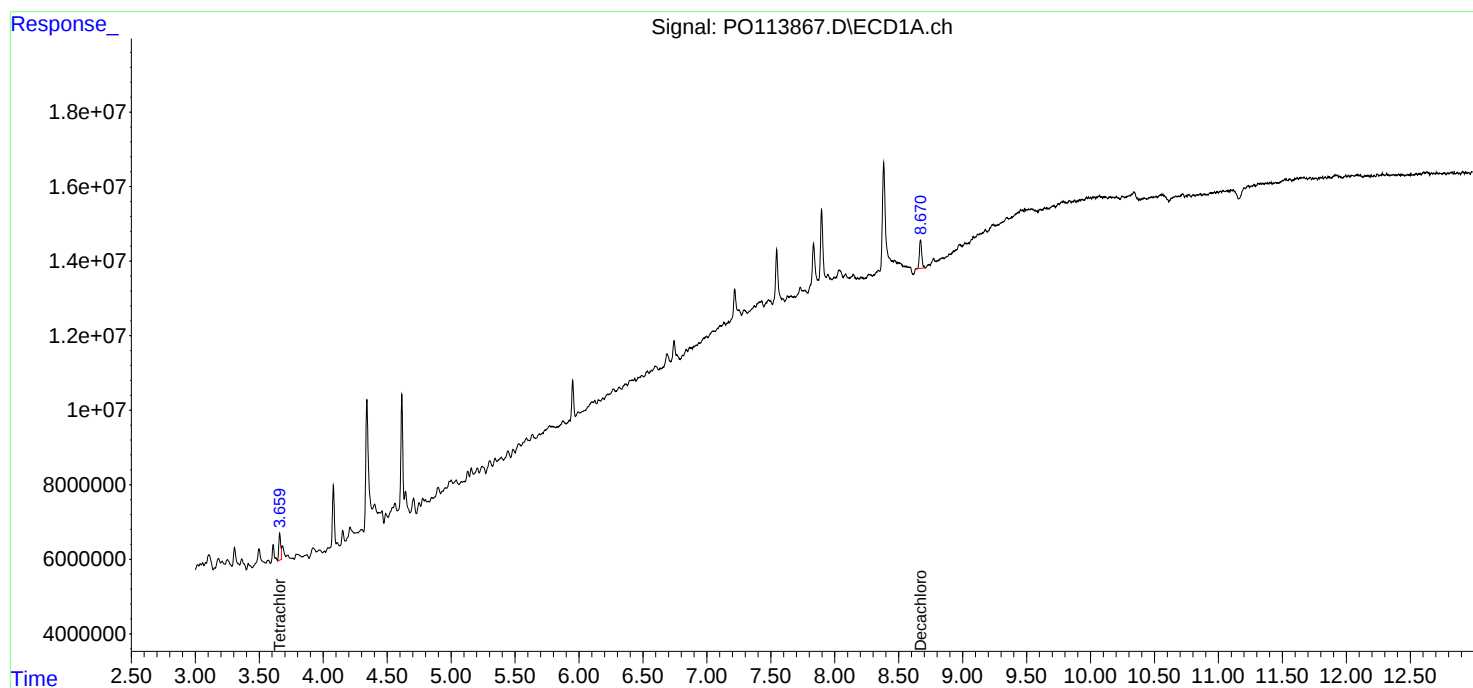

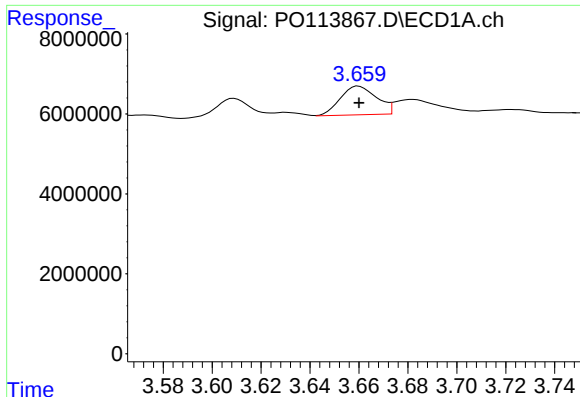


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: 0.000 min
Response: 7381709
Conc: 0.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-25-0239-0241


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2025
Supervised By :mohammad ahmed 09/23/2025

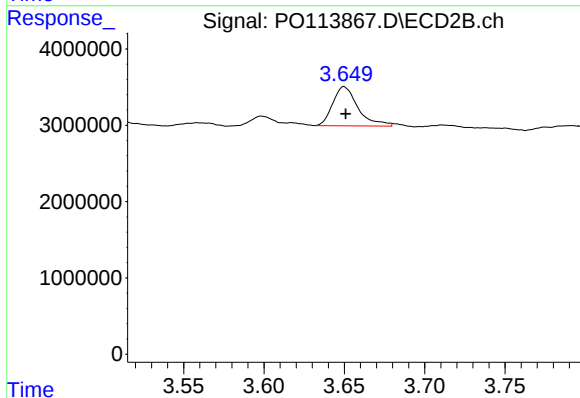


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 5611903
Conc: 1.05 ng/ml m

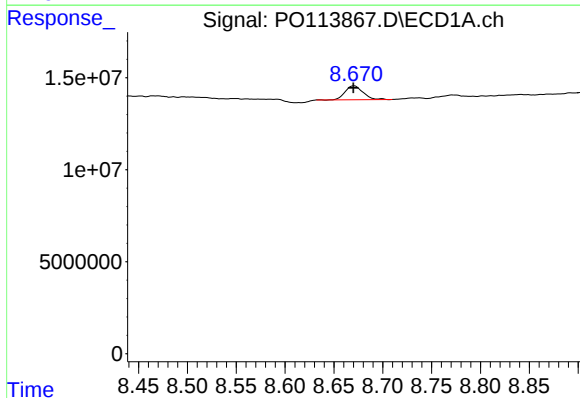

#2 Decachlorobiphenyl

R.T.: 8.671 min
Delta R.T.: 0.000 min
Response: 9636924
Conc: 1.44 ng/ml

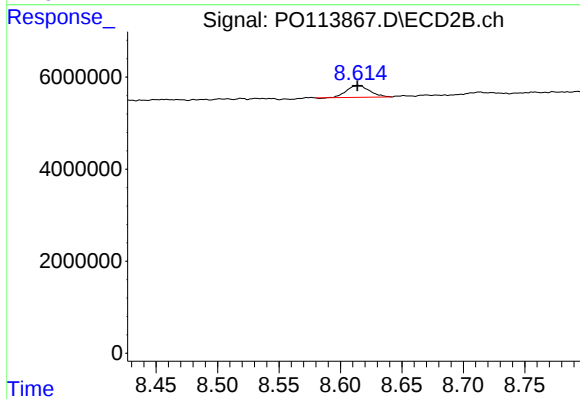

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: 0.001 min
Response: 3416256
Conc: 1.64 ng/ml