

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092023\
 Data File : P0098174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 11:54
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 15:40:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 20 07:12:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.640	61194486	26872529	20.460	24.205m
2) SA Decachlor...	10.340	8.667	38657832	25155833	22.144m	22.835m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092023\
Data File : PO098174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 11:54
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 15:40:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 20 07:12:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

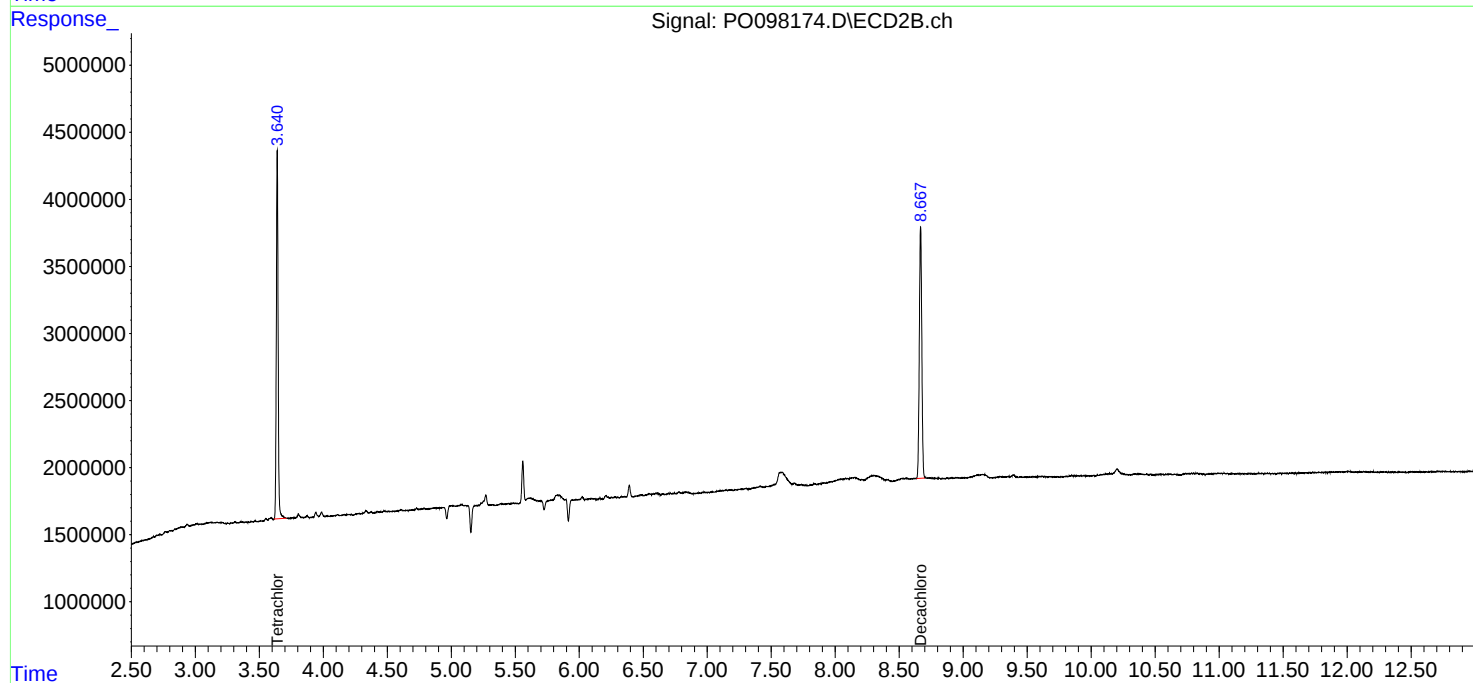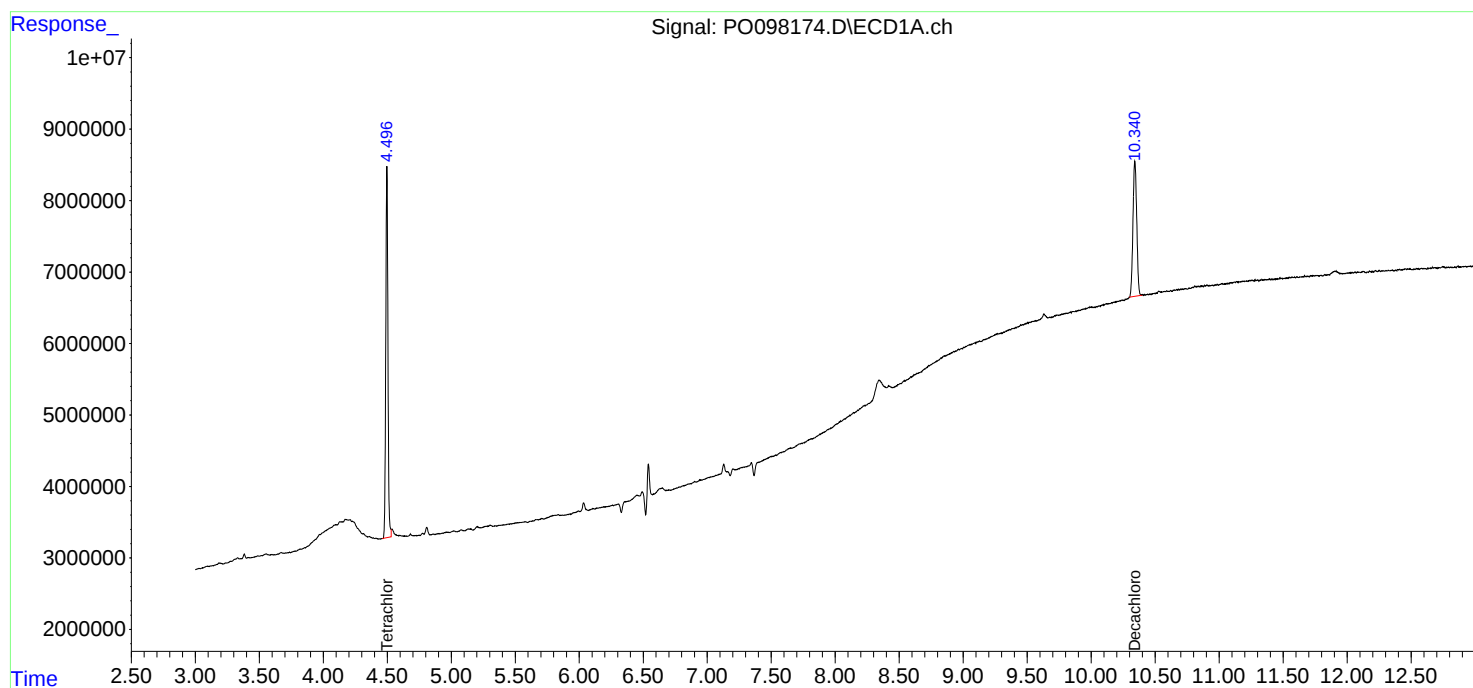

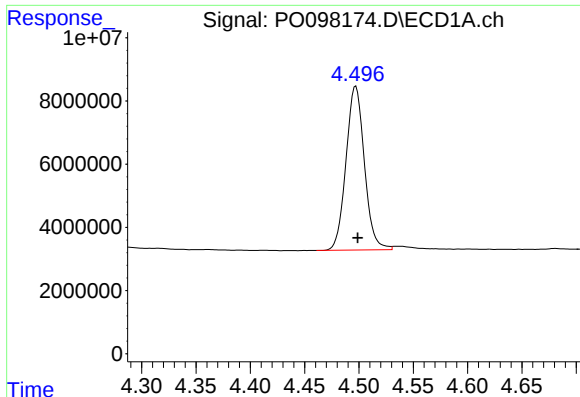


#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: -0.002 min
Response: 61194486
Conc: 20.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

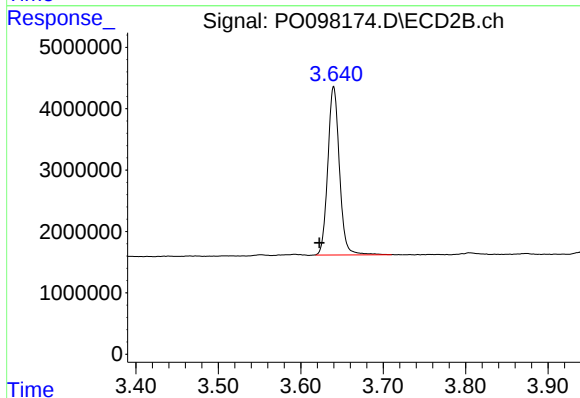


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.017 min
Response: 26872529
Conc: 24.20 ng/ml m

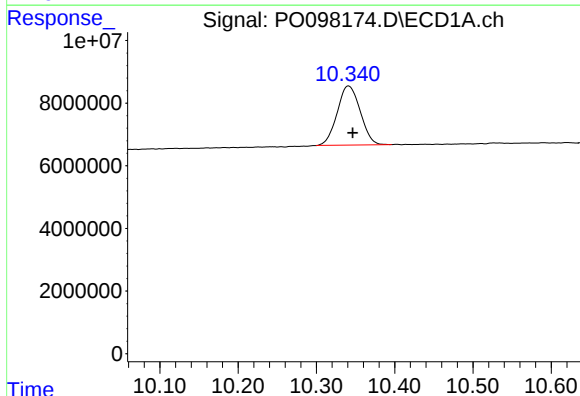

#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: -0.006 min
Response: 38657832
Conc: 22.14 ng/ml m

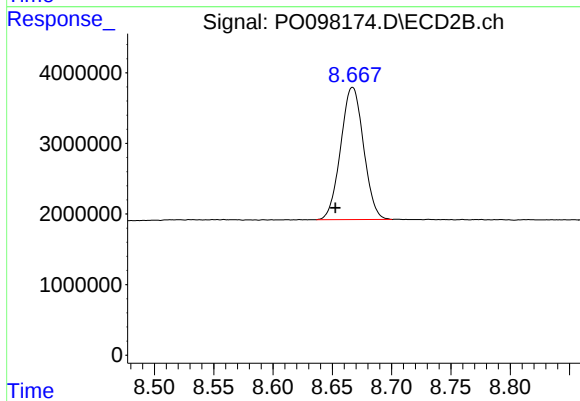

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: 0.014 min
Response: 25155833
Conc: 22.83 ng/ml m