

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092023\
 Data File : P0098175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 14:19
 Operator : YP/AJ
 Sample : PB155704BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB155704BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 15:40:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 20 07:12:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.498	3.638	61006631	25895274	20.397	23.325m
2) SA Decachlor...	10.345	8.665	46673136	23943870	26.735m	21.735m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092023\
Data File : PO098175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 14:19
Operator : YP/AJ
Sample : PB155704BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB155704BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 15:40:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 20 07:12:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

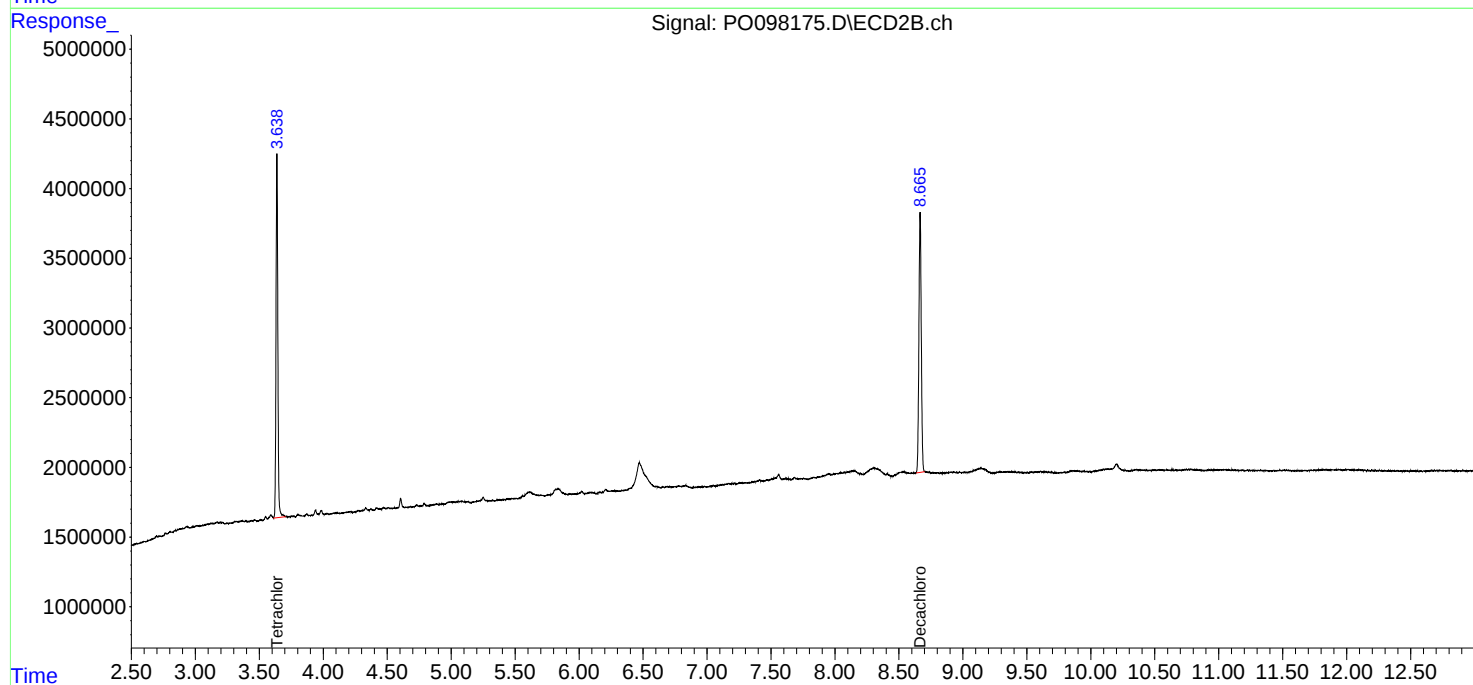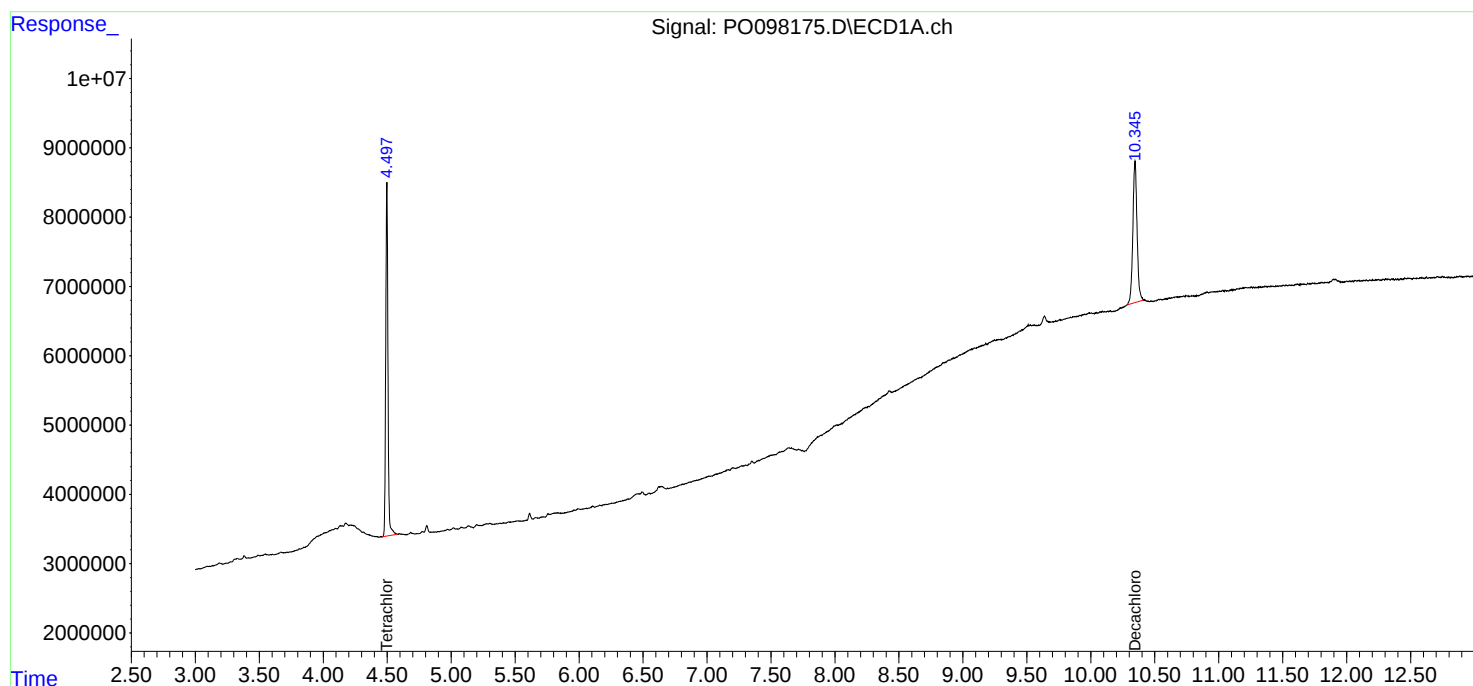

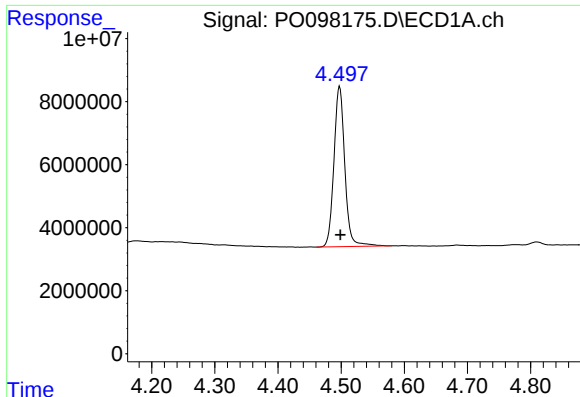


#1 Tetrachloro-m-xylene

R.T.: 4.498 min
Delta R.T.: -0.001 min
Response: 61006631
Conc: 20.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB155704BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

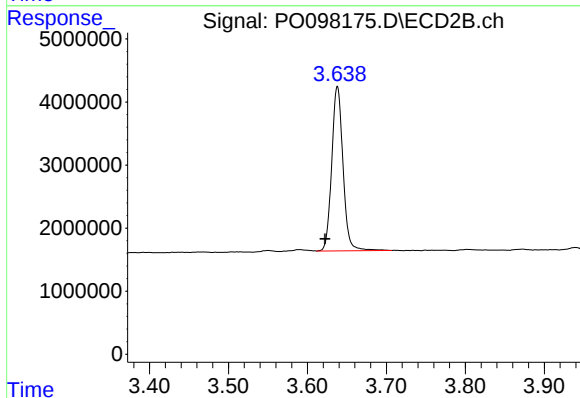


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.015 min
Response: 25895274
Conc: 23.32 ng/ml m

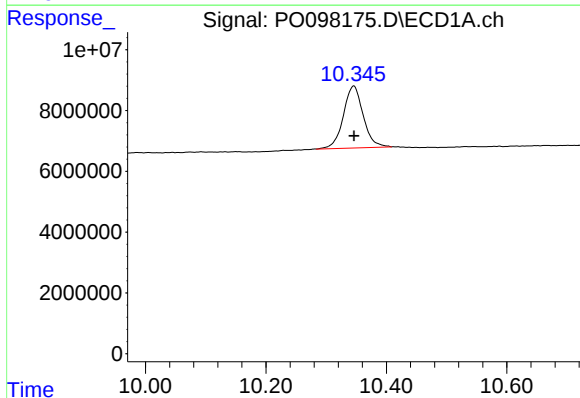

#2 Decachlorobiphenyl

R.T.: 10.345 min
Delta R.T.: 0.000 min
Response: 46673136
Conc: 26.74 ng/ml m

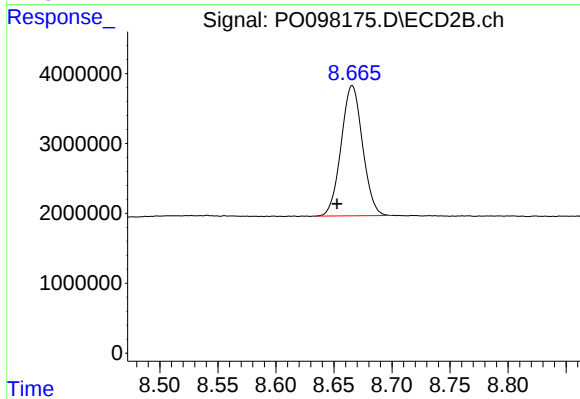

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: 0.013 min
Response: 23943870
Conc: 21.73 ng/ml m