

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092024\
 Data File : P0106722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 12:16
 Operator : YP/AJ
 Sample : P4099-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GAS-TRANSMISSION-DEBRISRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 03:43:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.443	3.714	58099575	112.3E6	7.745m	42.056m#
2) SA Decachlor...	10.205	8.733	174.6E6	51373196	35.323	25.683 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092024\
Data File : PO106722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 12:16
Operator : YP/AJ
Sample : P4099-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GAS-TRANSMISSION-DEBRISRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 03:43:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

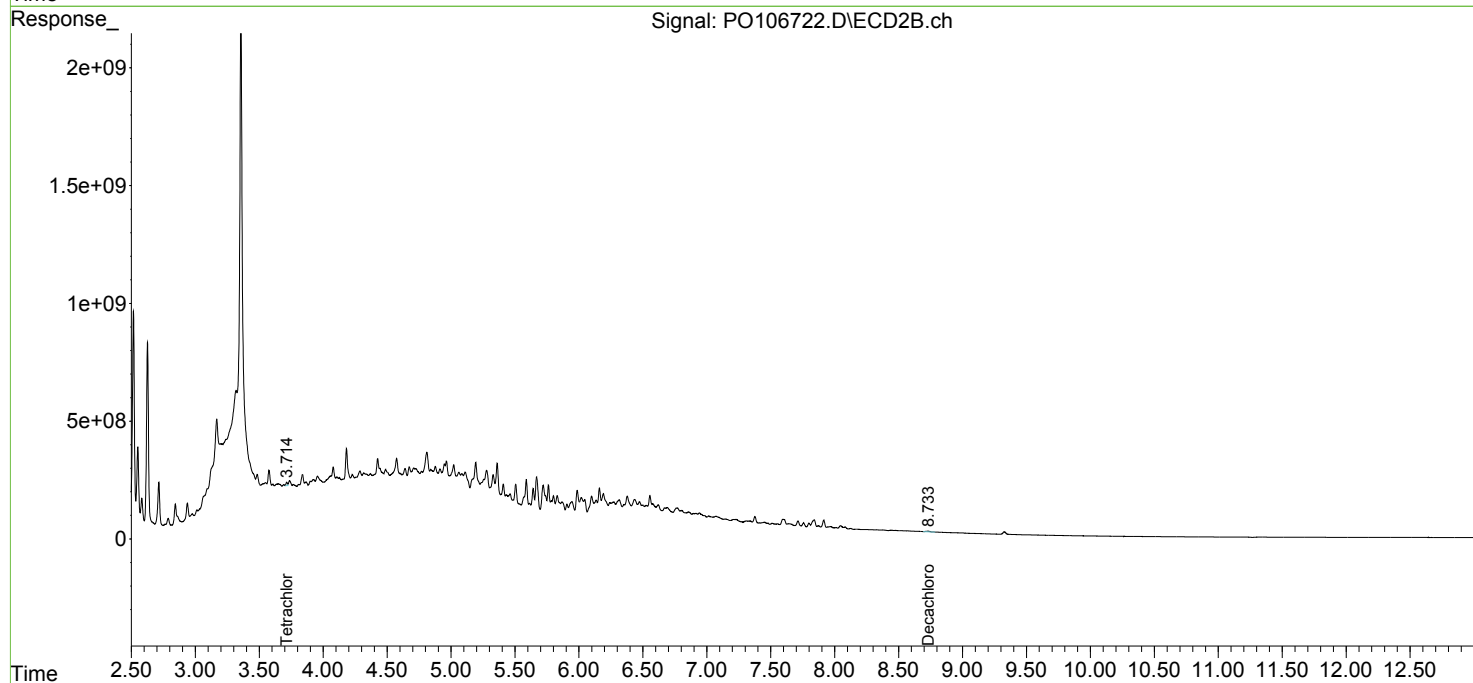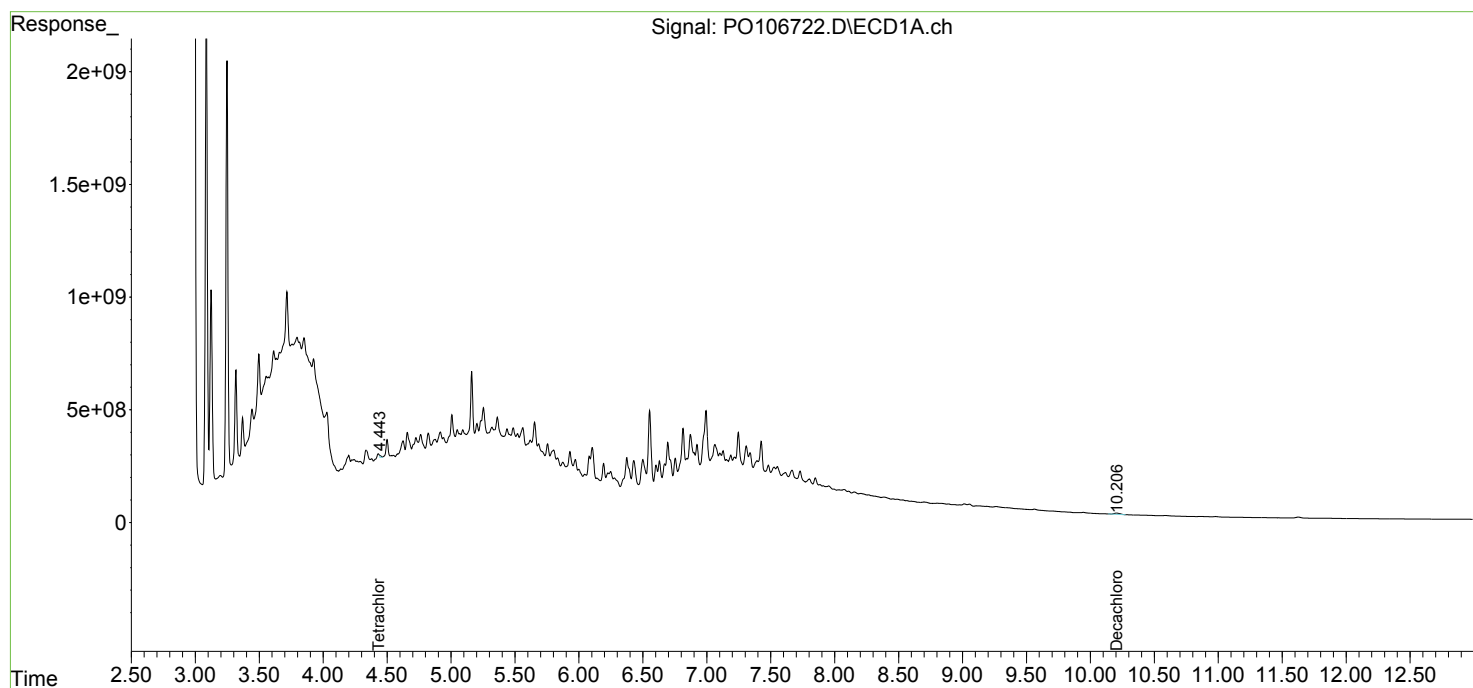

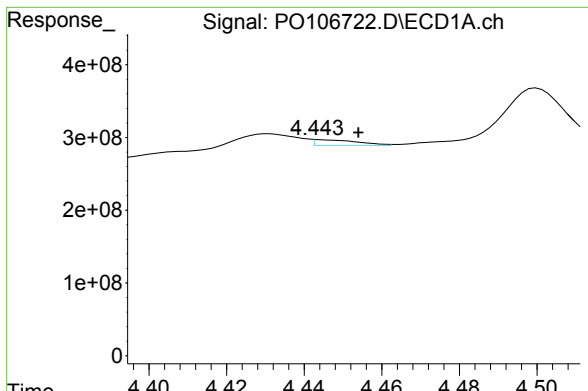


#1 Tetrachloro-m-xylene

R.T.: 4.443 min
Delta R.T.: -0.011 min
Response: 58099575
Conc: 7.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
GAS-TRANSMISSION-DEBRISRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

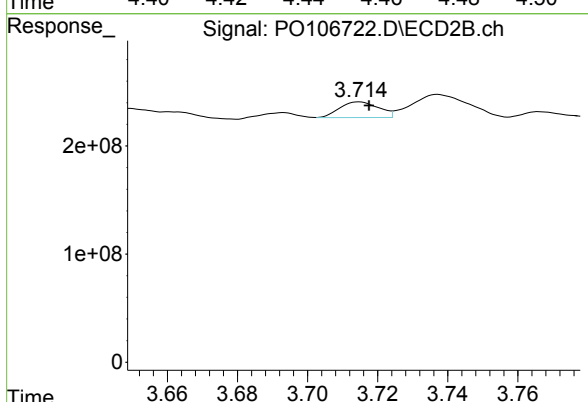


#1 Tetrachloro-m-xylene

R.T.: 3.714 min
Delta R.T.: -0.003 min
Response: 112341919
Conc: 42.06 ng/ml m

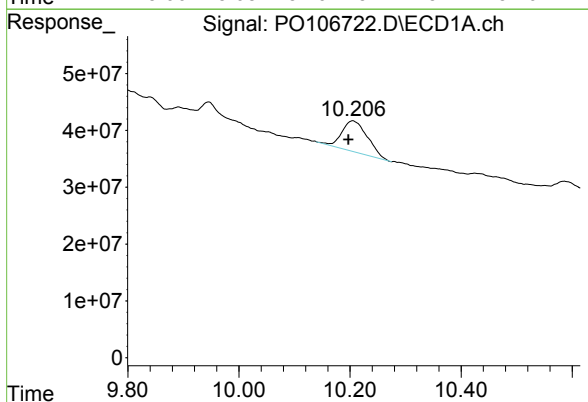

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.008 min
Response: 174597667
Conc: 35.32 ng/ml

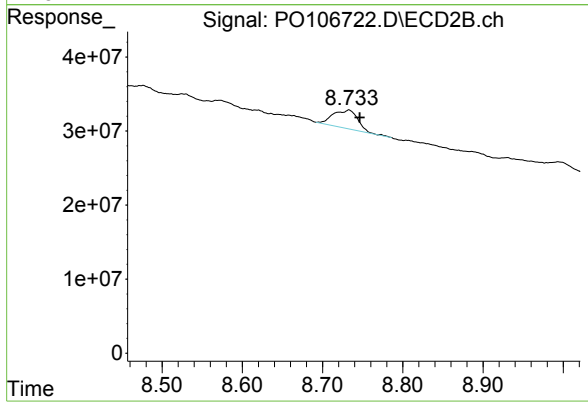

#2 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.013 min
Response: 51373196
Conc: 25.68 ng/ml