

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092024\
 Data File : P0106723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 12:34
 Operator : YP/AJ
 Sample : PB163553BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB163553BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 03:45:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.712	149.7E6	52073028	19.951	19.494
2) SA Decachlor...	10.195	8.736	102.2E6	35033324	20.682	17.515m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092024\
Data File : PO106723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 12:34
Operator : YP/AJ
Sample : PB163553BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB163553BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 03:45:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

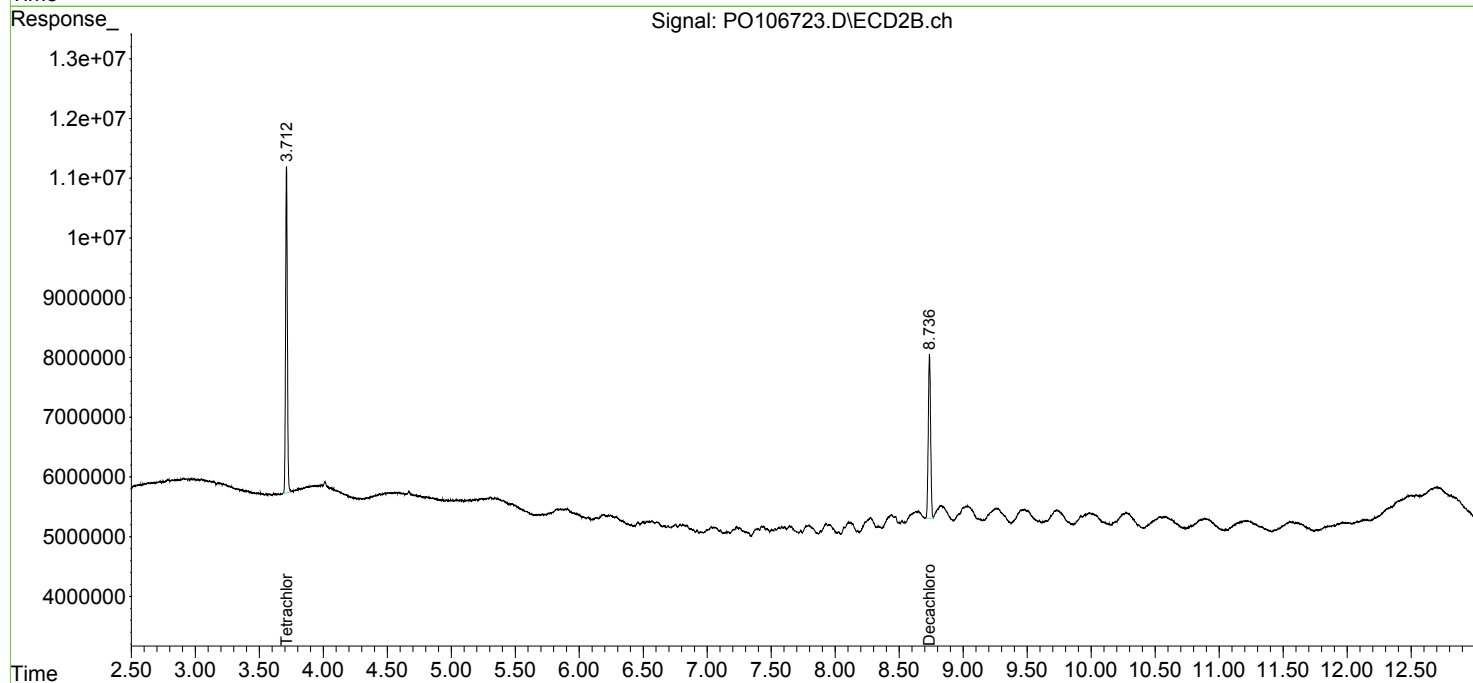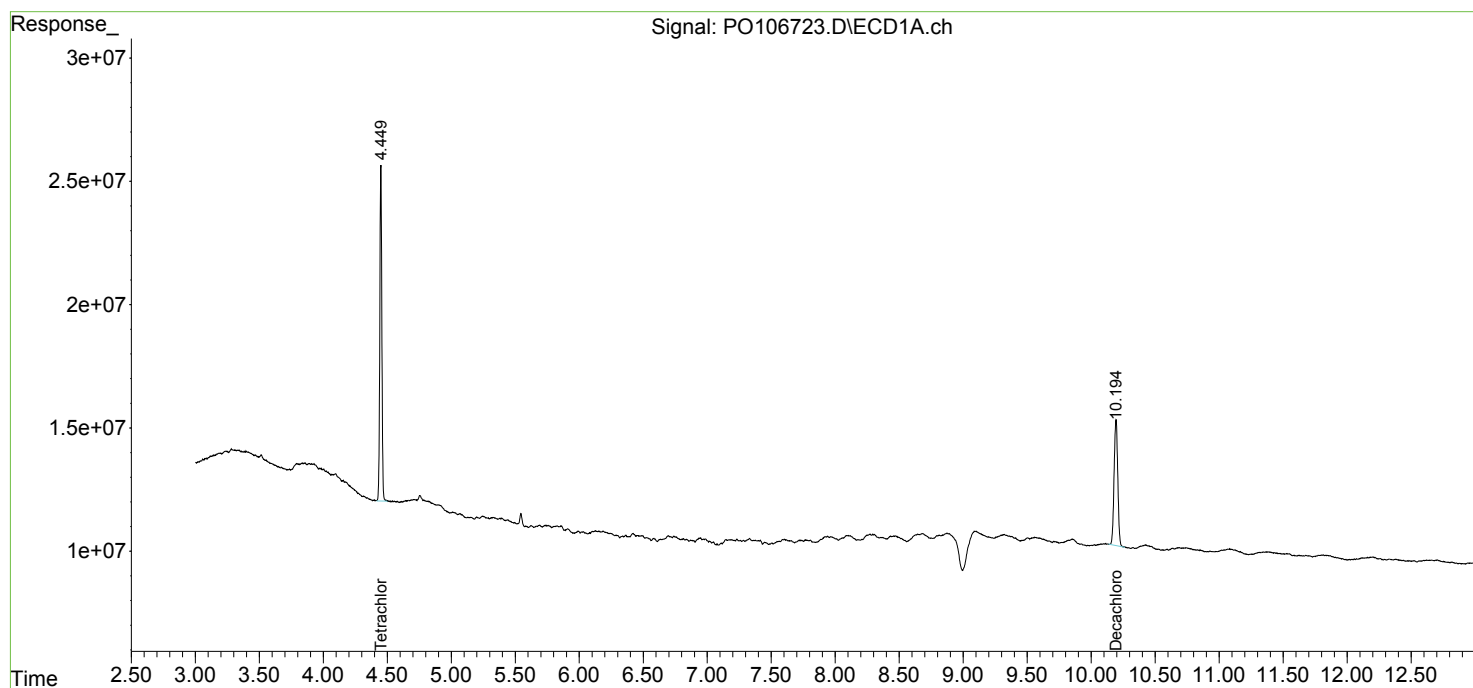

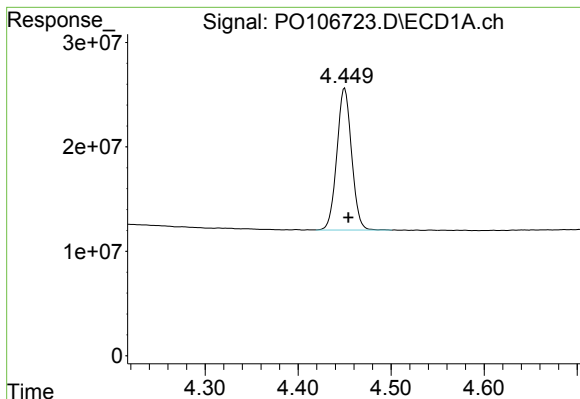

#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.004 min
Response: 149662442
Conc: 19.95 ng/ml

Instrument :

ECD_O


ClientSampleId :

PB163553BL

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

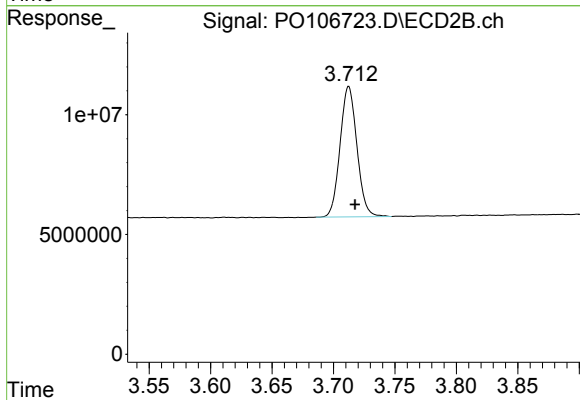


#1 Tetrachloro-m-xylene

R.T.: 3.712 min
Delta R.T.: -0.005 min
Response: 52073028
Conc: 19.49 ng/ml

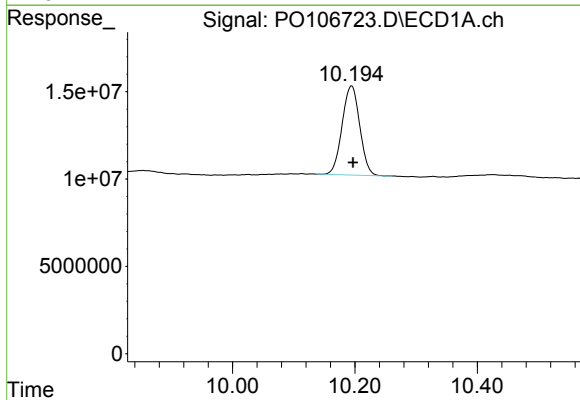

#2 Decachlorobiphenyl

R.T.: 10.195 min
Delta R.T.: -0.002 min
Response: 102225174
Conc: 20.68 ng/ml

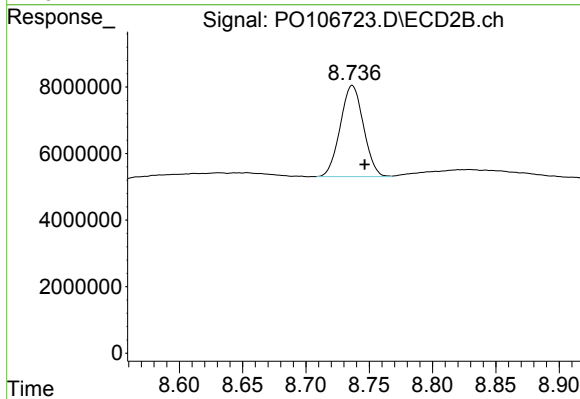

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.010 min
Response: 35033324
Conc: 17.51 ng/ml m