

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092024\
 Data File : P0106756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2024 03:58
 Operator : YP/AJ
 Sample : P4110-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-066-IDWGW-20240918

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/23/2024
 Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 07:06:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.713	175.5E6	61569793	23.391m	23.049
2) SA Decachlor...	10.193	8.736	45508384	17328647	9.207	8.663

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092024\
Data File : PO106756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2024 03:58
Operator : YP/AJ
Sample : P4110-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-066-IDWGW-20240918


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 07:06:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

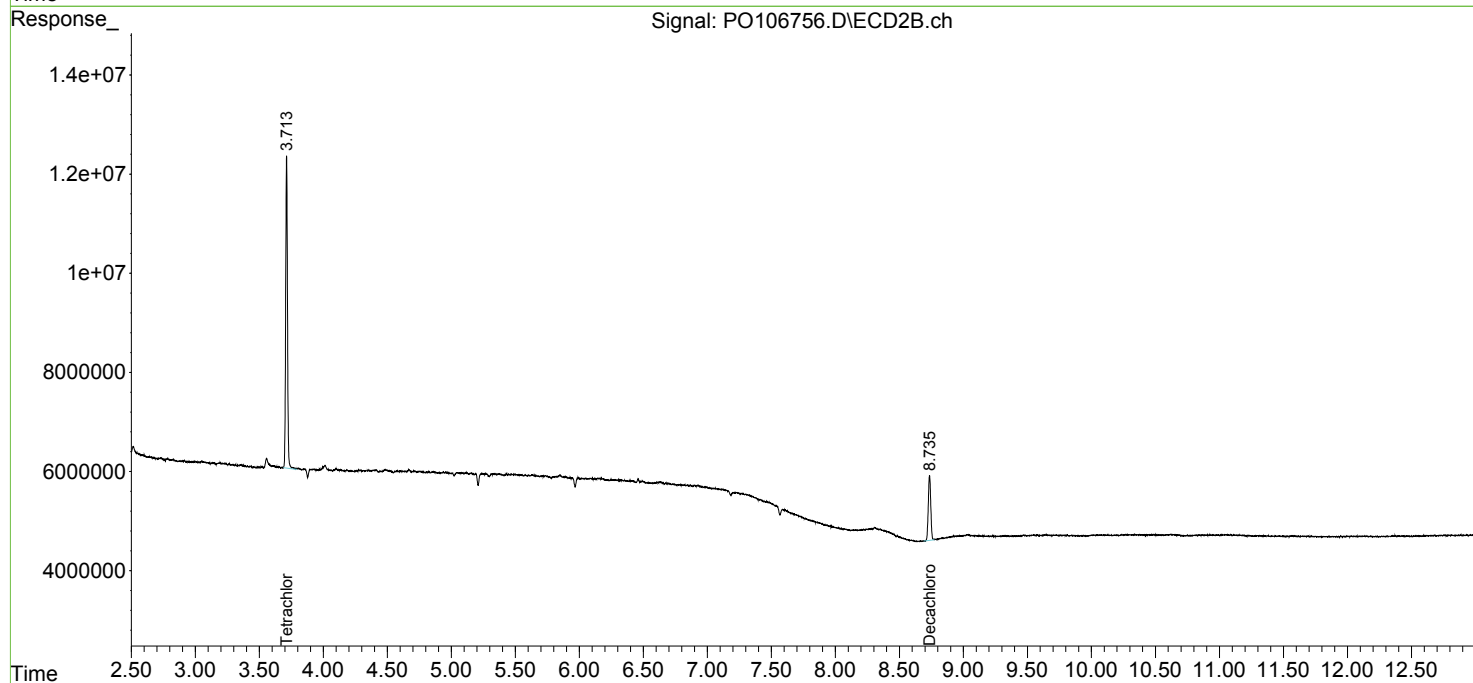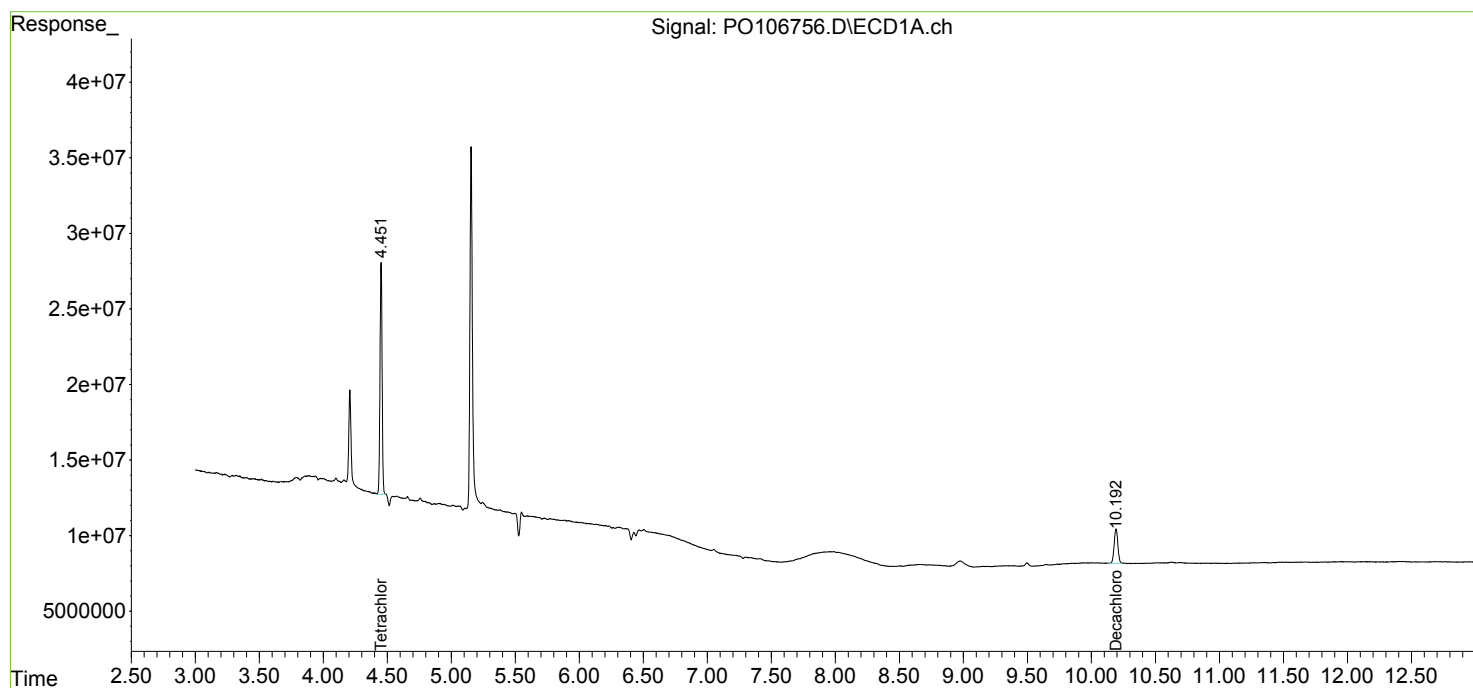

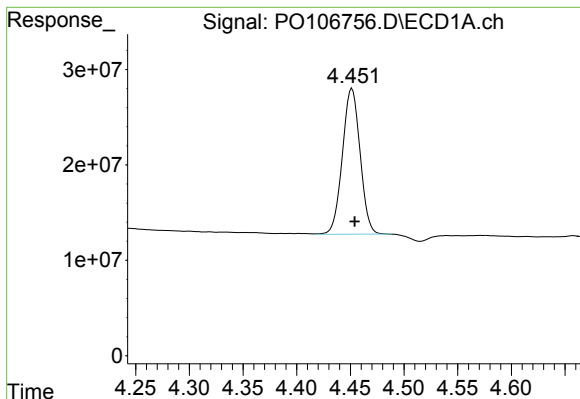


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: -0.003 min
Response: 175462426
Conc: 23.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-066-IDWGW-20240918


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2024
Supervised By :Ankita Jodhani 09/23/2024

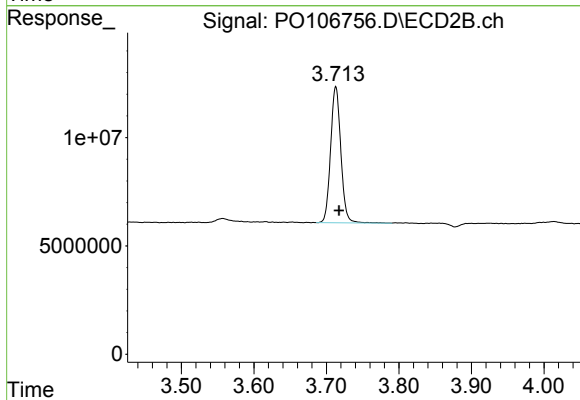


#1 Tetrachloro-m-xylene

R.T.: 3.713 min
Delta R.T.: -0.005 min
Response: 61569793
Conc: 23.05 ng/ml

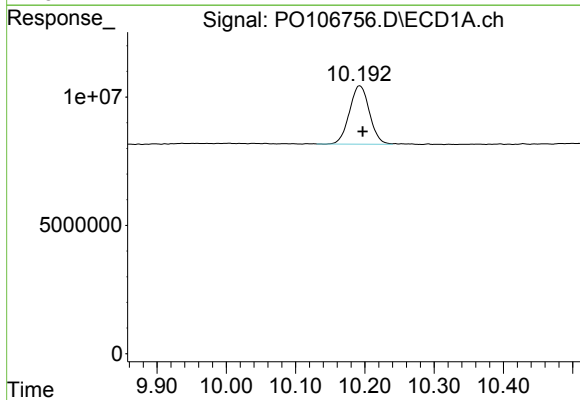

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.005 min
Response: 45508384
Conc: 9.21 ng/ml

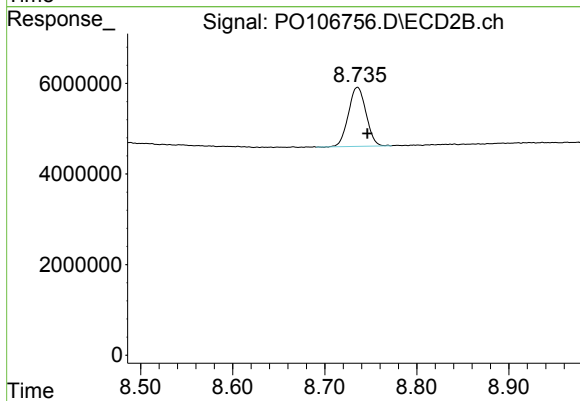

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.011 min
Response: 17328647
Conc: 8.66 ng/ml