

Data Path : P:\HPCHEM1\ECD_0\Data\P0092115\
Data File : P0024759.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 17:16
Operator : IZ/UA
Sample : G3745-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091815-D534-E-D-B

Manual Integrations
APPROVED

ugo
9/22/2015 11:54:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:20:17 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.115	3.225	4203964	5549781	18.952m	19.726
2) SA Decachlor...	9.643	8.021	2223381	4494753	18.248	16.626

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0092115\
Data File : P0024759.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 17:16
Operator : IZ/UA
Sample : G3745-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
091815-D534-E-D-B


Manual Integrations
APPROVED

ugo
9/22/2015 11:54:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:20:17 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

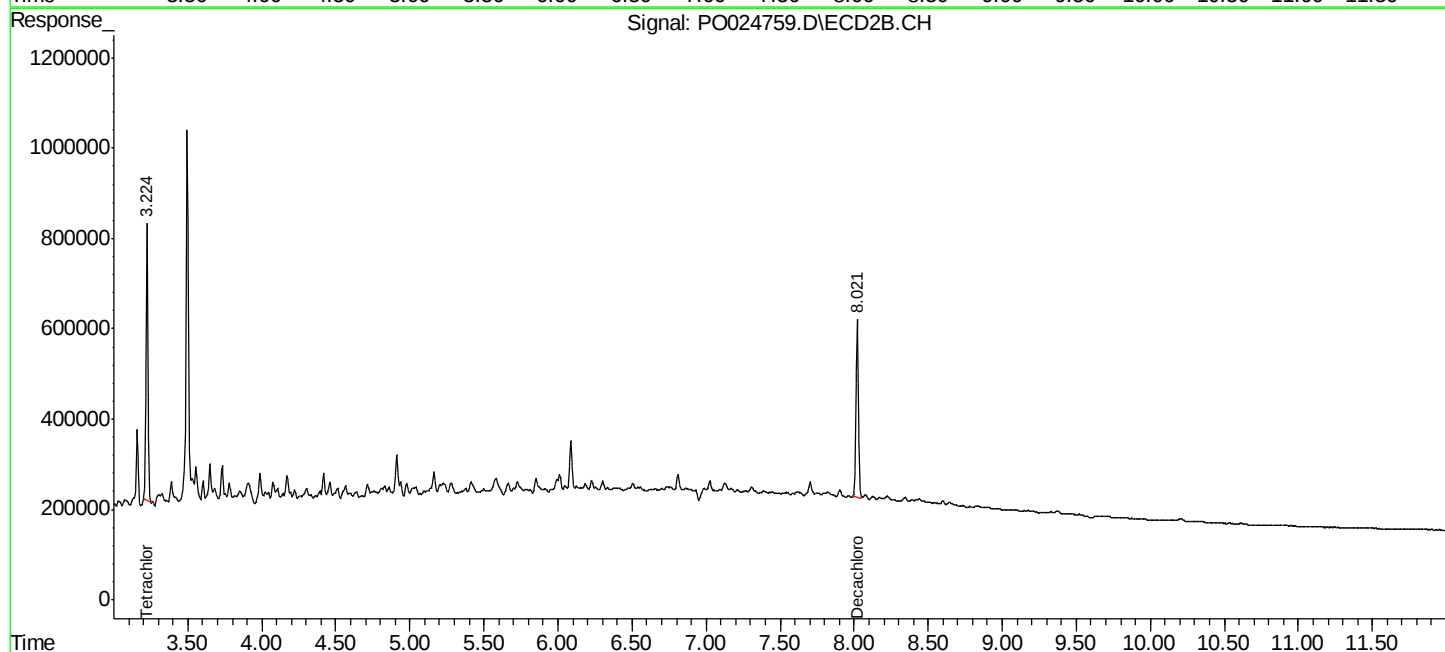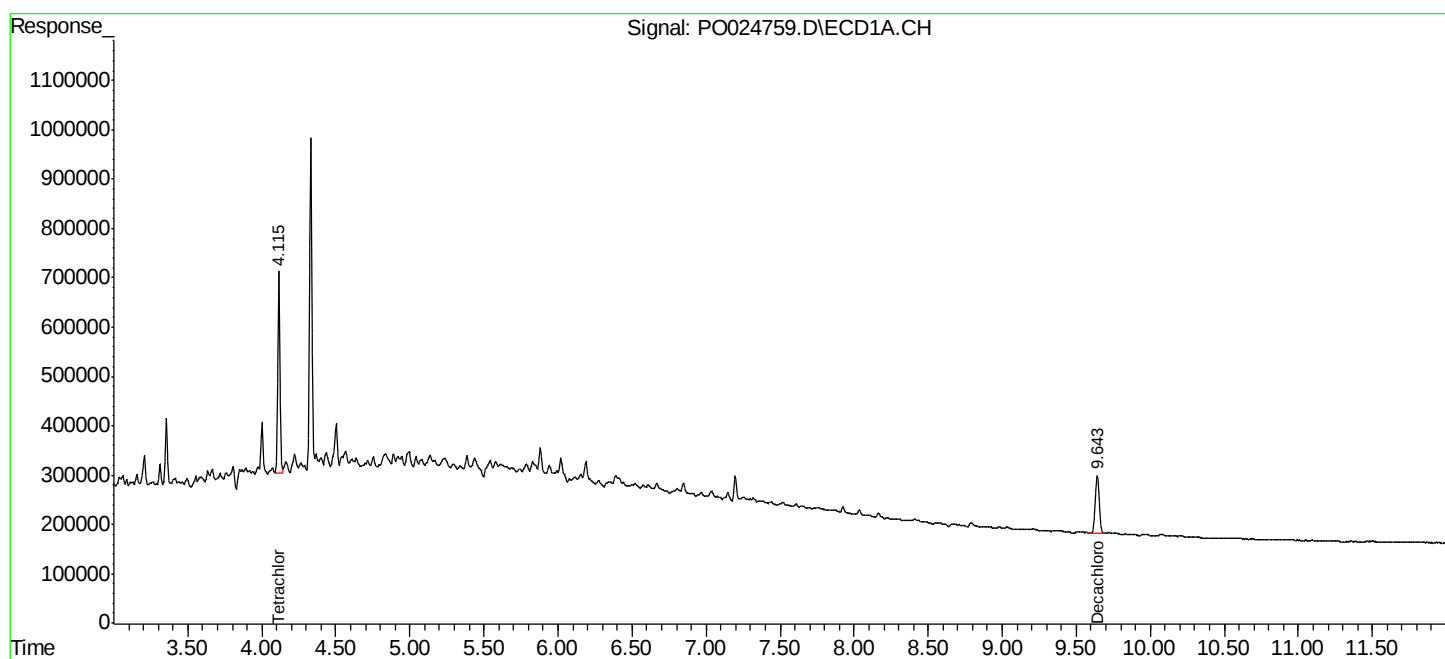

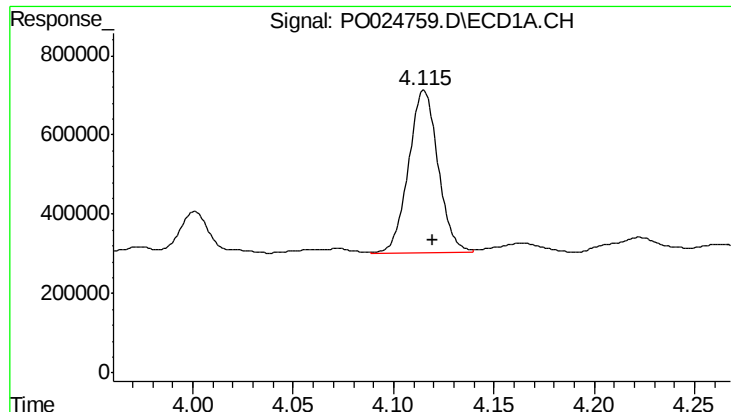


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.005 min
Response: 4203964
Conc: 18.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
091815-D534-E-D-B


Manual Integrations
APPROVED

ugo
9/22/2015 11:54:24 AM

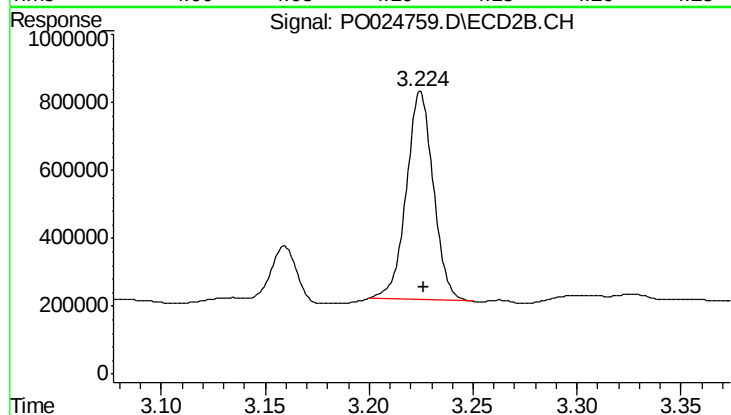


#1 Tetrachloro-m-xylene

R.T.: 3.225 min
Delta R.T.: -0.001 min
Response: 5549781
Conc: 19.73 ng/ml

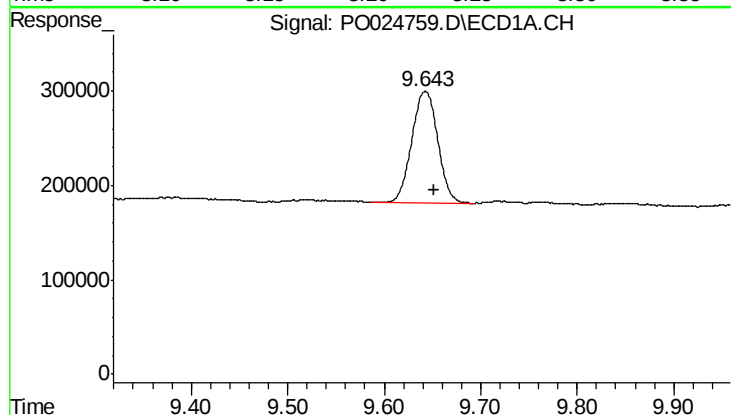

#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.009 min
Response: 2223381
Conc: 18.25 ng/ml

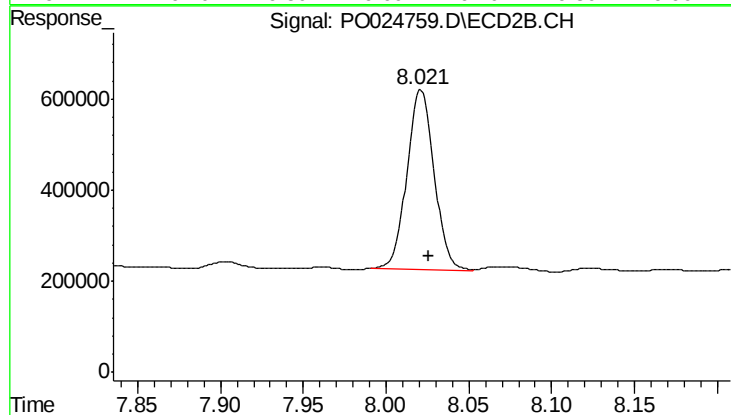

#2 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: -0.005 min
Response: 4494753
Conc: 16.63 ng/ml