

Data Path : P:\HPCHEM1\ECD_0\Data\P0092115\
Data File : P0024774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 21:15
Operator : IZ/UA
Sample : G3746-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
091715-D549-F-D-S

Manual Integrations
APPROVED

ugo
9/22/2015 11:55:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:27:51 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.115	3.224	4139898	5588863	18.663m	19.864m
2) SA Decachlor...	9.642	8.020	1916967	4047244	15.734	14.970

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0092115\
Data File : P0024774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 21:15
Operator : IZ/UA
Sample : G3746-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
091715-D549-F-D-S


Manual Integrations
APPROVED

ugo
9/22/2015 11:55:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:27:51 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

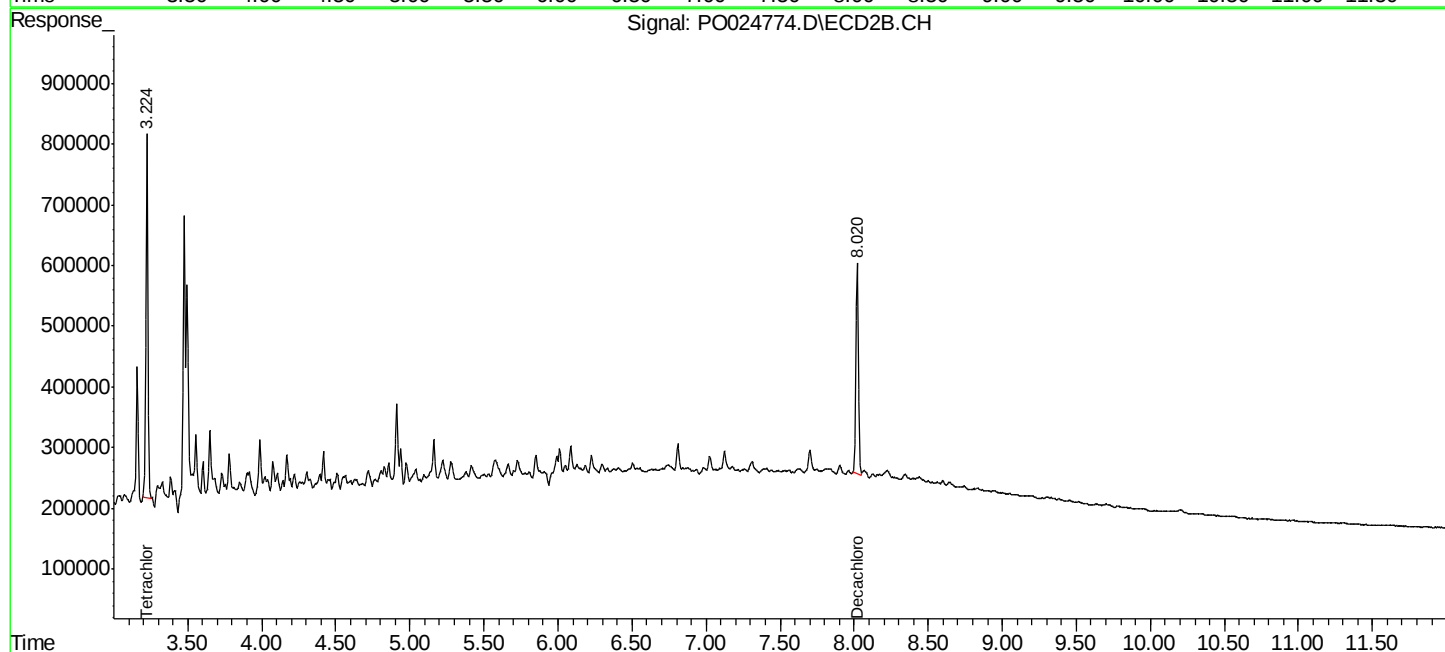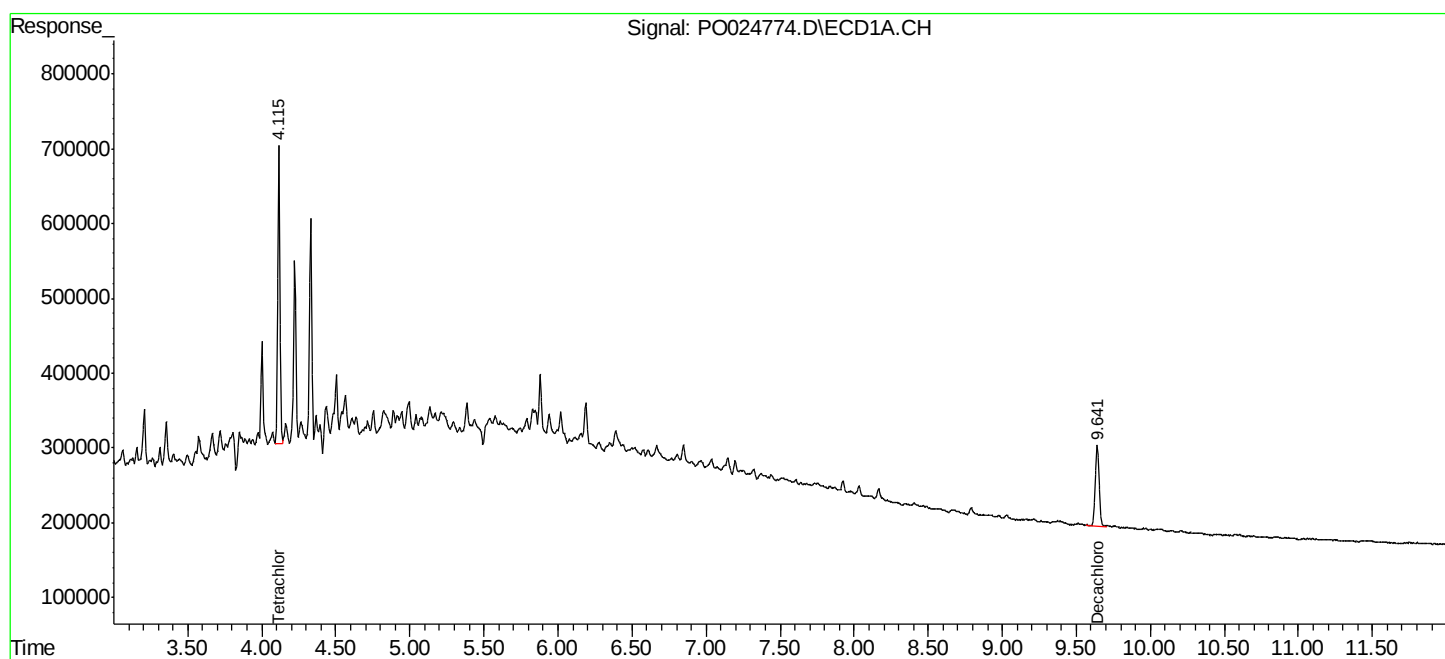

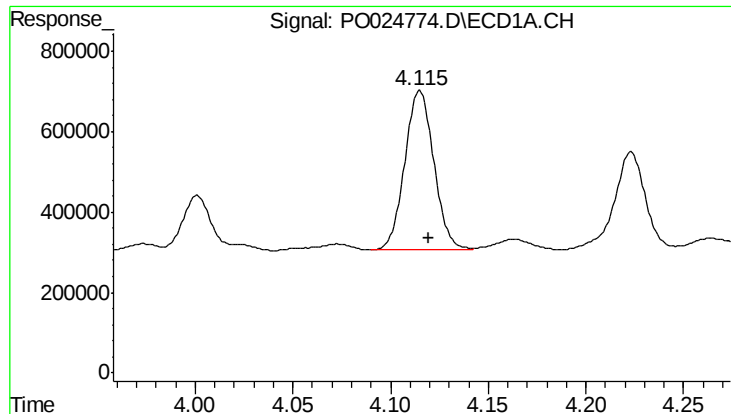


#1 Tetrachloro-m-xylene

R.T.: 4.115 min
Delta R.T.: -0.005 min
Response: 4139898
Conc: 18.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
091715-D549-F-D-S


Manual Integrations
APPROVED

ugo
9/22/2015 11:55:22 AM

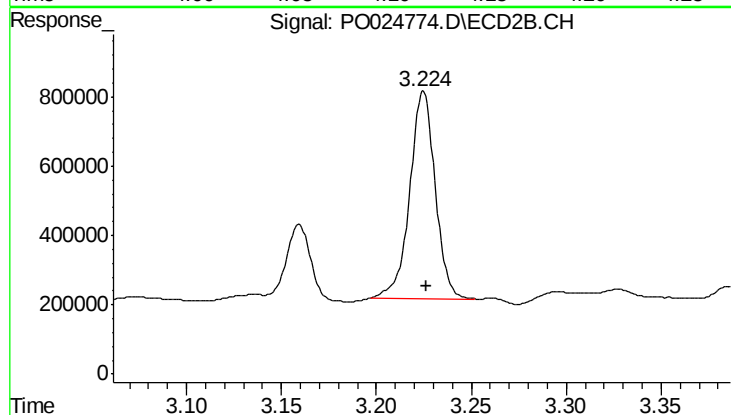


#1 Tetrachloro-m-xylene

R.T.: 3.224 min
Delta R.T.: -0.002 min
Response: 5588863
Conc: 19.86 ng/ml m

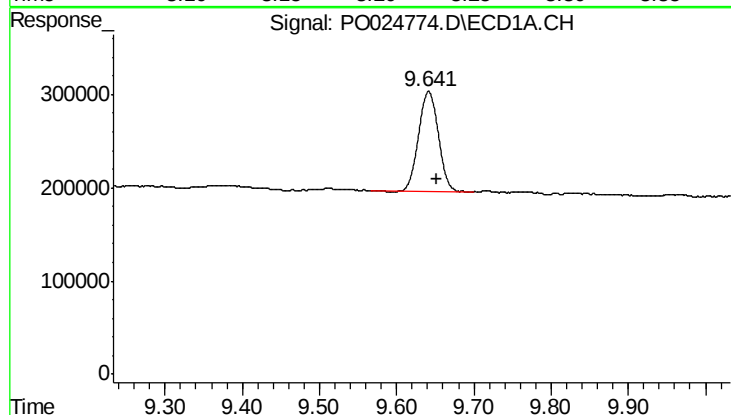

#2 Decachlorobiphenyl

R.T.: 9.642 min
Delta R.T.: -0.010 min
Response: 1916967
Conc: 15.73 ng/ml

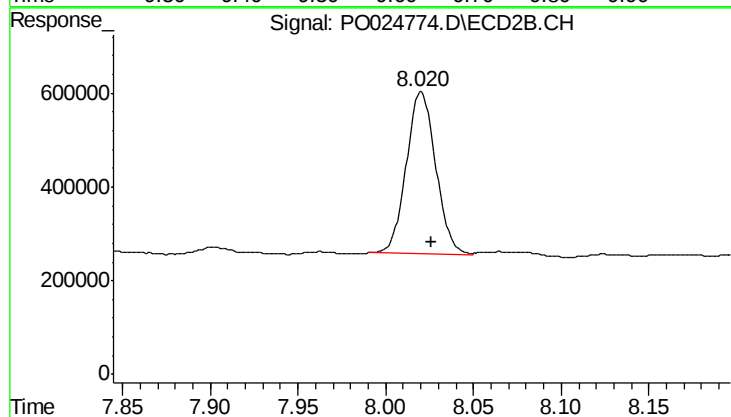

#2 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: -0.006 min
Response: 4047244
Conc: 14.97 ng/ml