

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092120\
 Data File : P0071507.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Sep 2020 16:20
 Operator : DD\AJ
 Sample : L4062-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EROC-NI4-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 17:14:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.340	3.524	1593801	839965	22.490	21.515
2)	SA Decachlor...	9.950	8.701	1780931	1005479	19.098	18.254
Target Compounds							
6)	L1 AR-1016-4	5.828	0.000	74498	0	34.804	N.D. #
14)	L3 AR-1232-4	5.828	0.000	74498	0	89.568	N.D. #
19)	L4 AR-1242-4	5.828	0.000	74498	0	43.969	N.D. #
33)	L7 AR-1260-3	7.937	0.000	242389	0	39.996	N.D. #
35)	L7 AR-1260-5	8.494f	0.000	195827	0	15.443	N.D. #
36)	L8 AR-1262-1	7.937	0.000	242389	0	28.571	N.D. #
37)	L8 AR-1262-2	8.494f	0.000	195827	0	13.565	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092120\
Data File : PO071507.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2020 16:20
Operator : DD\AJ
Sample : L4062-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
ERO-C-NI4-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 17:14:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

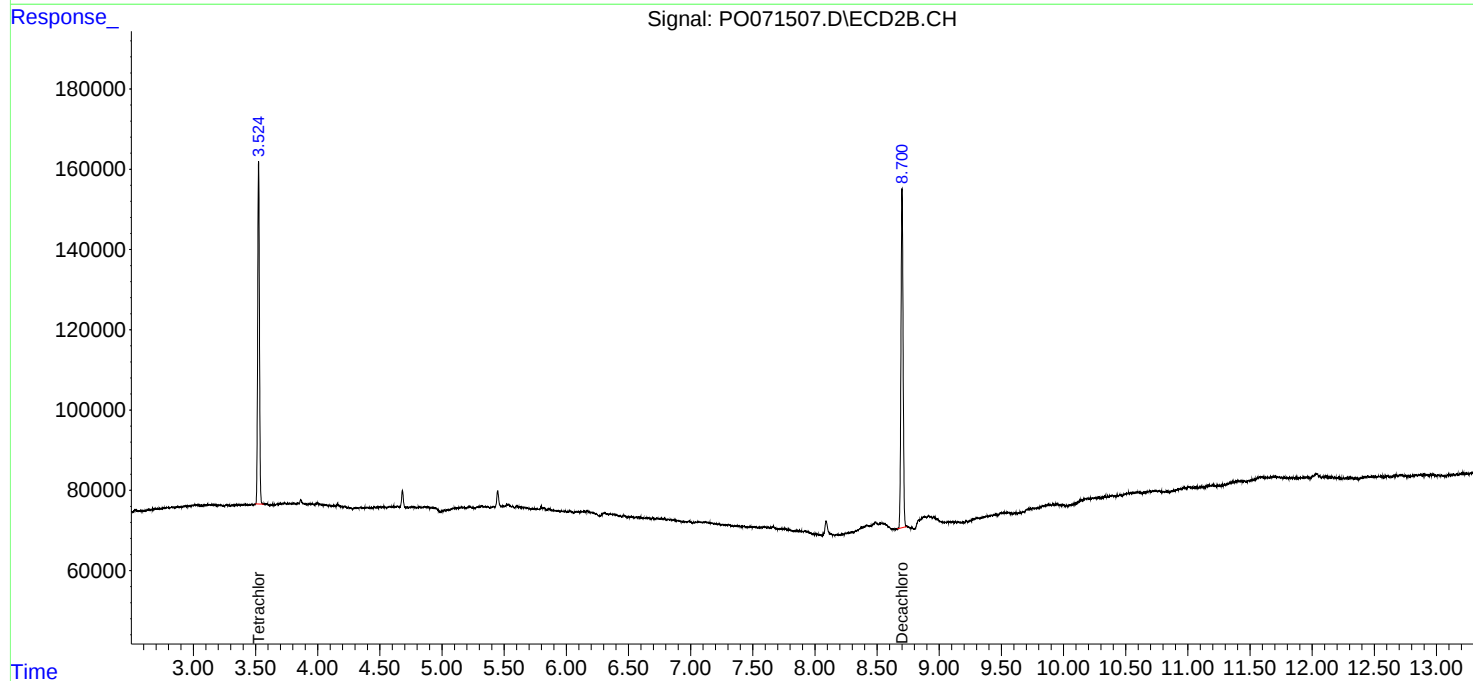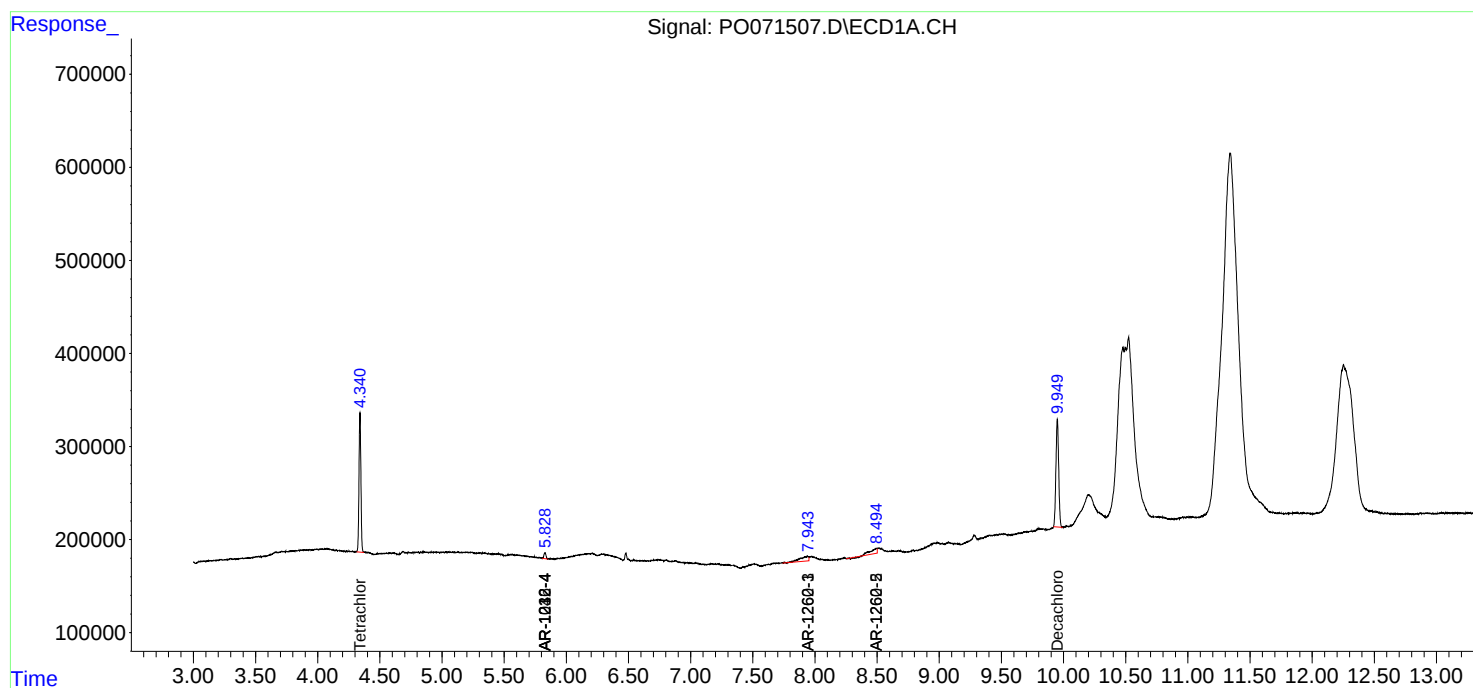


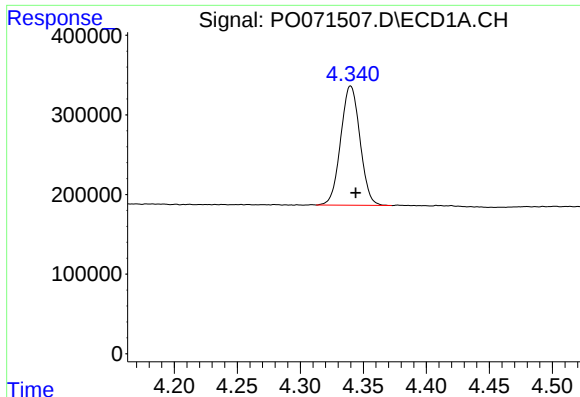

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 1593801
Conc: 22.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
EROC-NI4-1

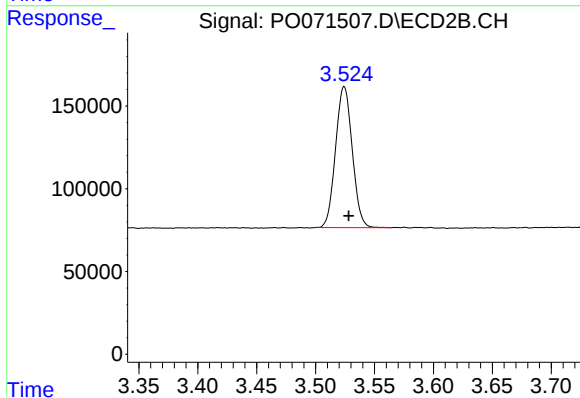


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.004 min
Response: 839965
Conc: 21.51 ng/ml

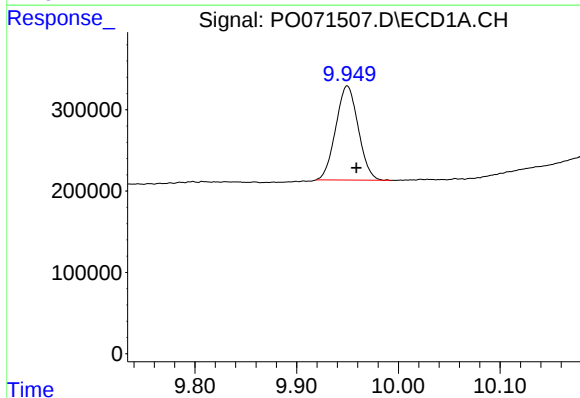


#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.009 min
Response: 1780931
Conc: 19.10 ng/ml

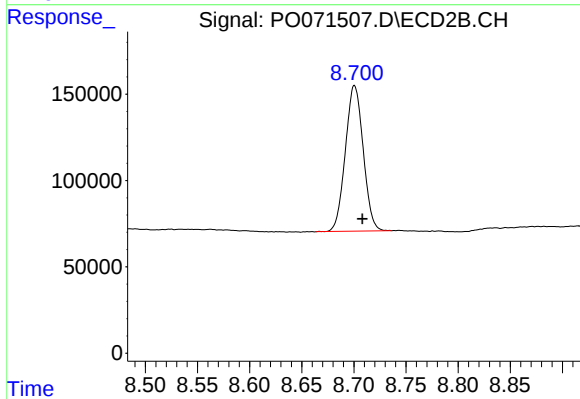

#2 Decachlorobiphenyl


R.T.: 8.701 min
Delta R.T.: -0.008 min
Response: 1005479
Conc: 18.25 ng/ml

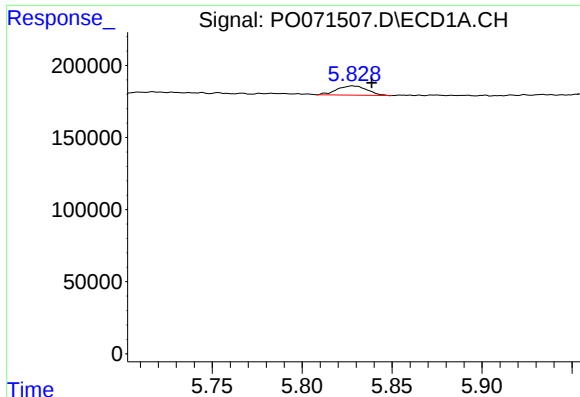

#6 AR-1016-4


R.T.: 5.828 min
Delta R.T.: -0.010 min
Response: 74498
Conc: 34.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
EROC-NI4-1

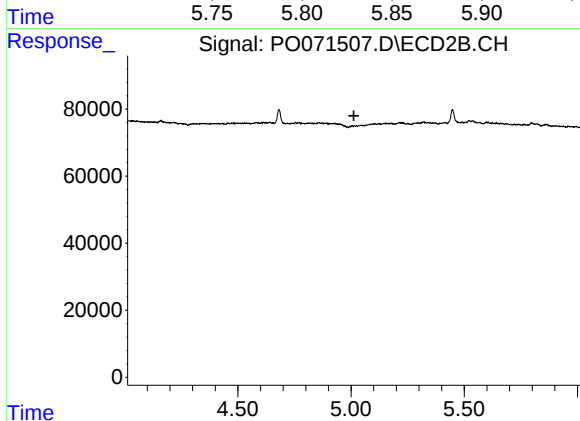


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.013 min
Response: 0
Conc: N.D.

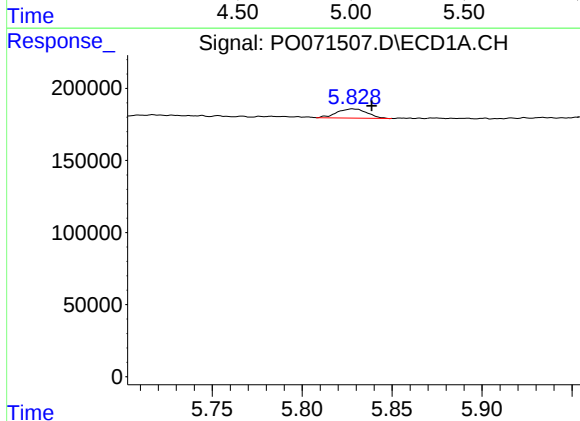


#14 AR-1232-4

R.T.: 5.828 min
Delta R.T.: -0.010 min
Response: 74498
Conc: 89.57 ng/ml

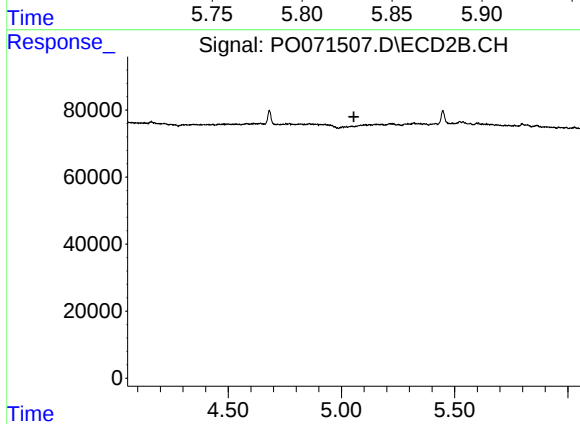

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

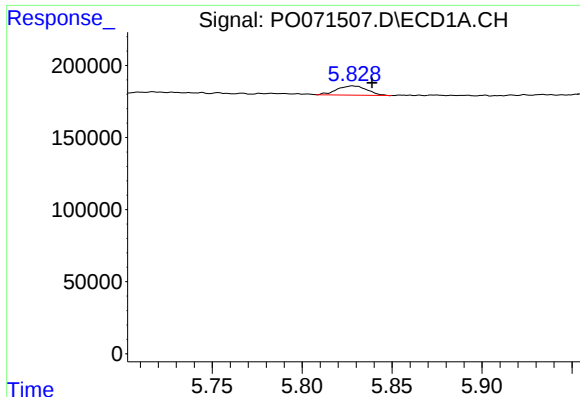

#19 AR-1242-4


R.T.: 5.828 min
Delta R.T.: -0.010 min
Response: 74498
Conc: 43.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
EROC-NI4-1

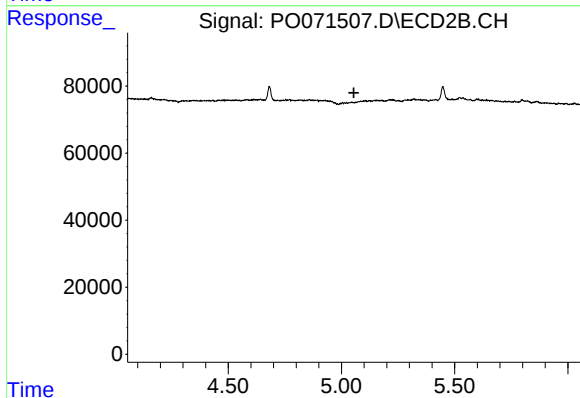


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

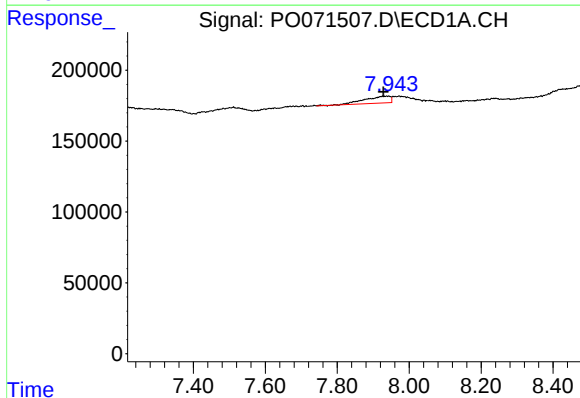


#33 AR-1260-3

R.T.: 7.937 min
Delta R.T.: 0.009 min
Response: 242389
Conc: 40.00 ng/ml

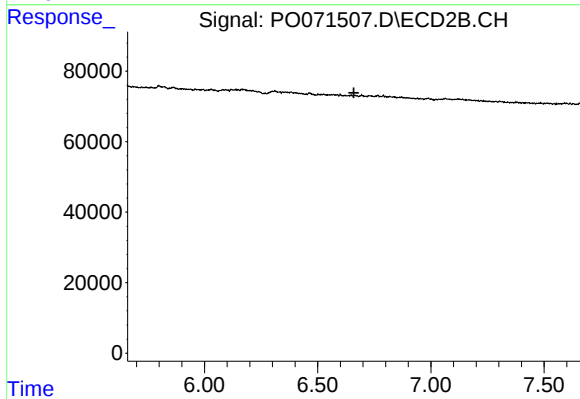

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.660 min
Response: 0
Conc: N.D.

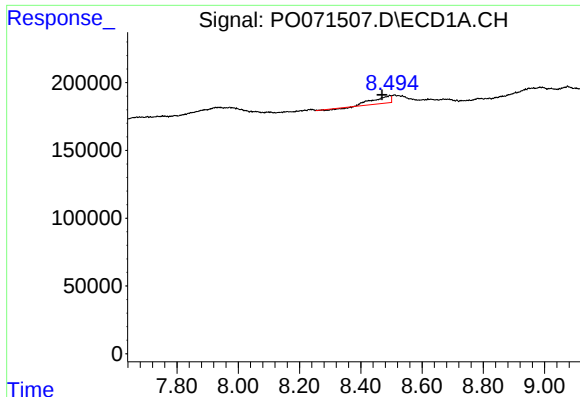

#35 AR-1260-5


R.T.: 8.494 min
Delta R.T.: 0.024 min
Response: 195827
Conc: 15.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
ERO-C-NI4-1

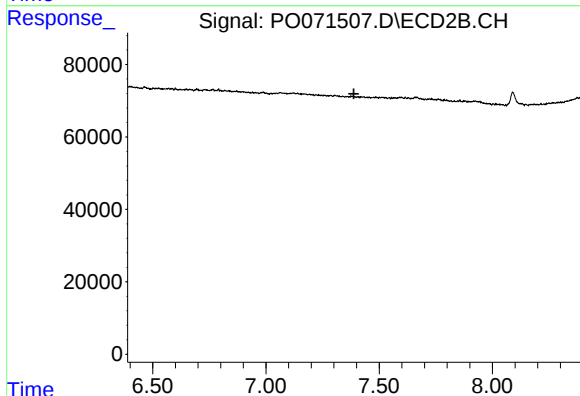


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

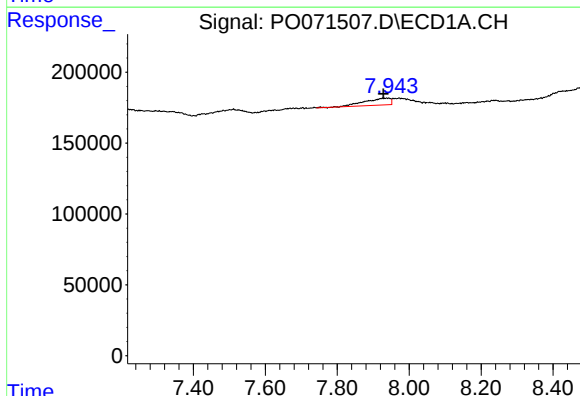


#36 AR-1262-1

R.T.: 7.937 min
Delta R.T.: 0.009 min
Response: 242389
Conc: 28.57 ng/ml

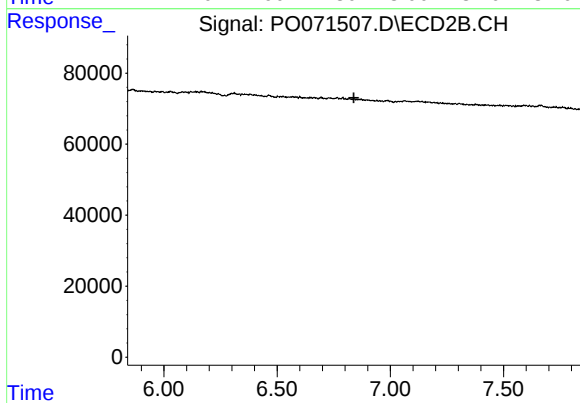

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

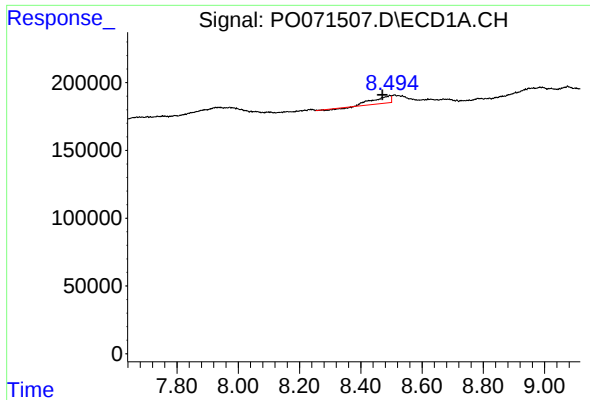

#37 AR-1262-2

R.T.: 8.494 min
Delta R.T.: 0.023 min
Response: 195827
Conc: 13.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
EROC-NI4-1

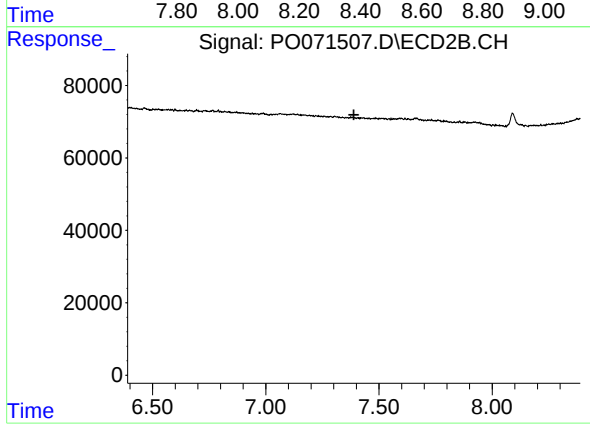

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.