

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092120\
 Data File : P0071529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Sep 2020 22:36
 Operator : DD\AJ
 Sample : L4054-02 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ075N-BOTTOM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 05:18:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.343	3.527	131984	111614	1.862	2.859 #
2)	SA Decachlor...	9.958	8.708	232129	120631	2.489	2.190
Target Compounds							
33)	L7 AR-1260-3	7.925	0.000	25264	0	4.169	N.D. #
35)	L7 AR-1260-5	8.469	0.000	32275	0	2.545	N.D. #
36)	L8 AR-1262-1	7.925	0.000	25264	0	2.978	N.D. #
37)	L8 AR-1262-2	8.469	0.000	32275	0	2.236	N.D. #
39)	L8 AR-1262-4	8.842f	0.000	73561	0	11.569	N.D. #
42)	L9 AR-1268-2	8.842f	0.000	73561	0	5.262	N.D. #
45)	L9 AR-1268-5	9.697	0.000	95513	0	2.739	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092120\
Data File : PO071529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2020 22:36
Operator : DD\AJ
Sample : L4054-02 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 05:18:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

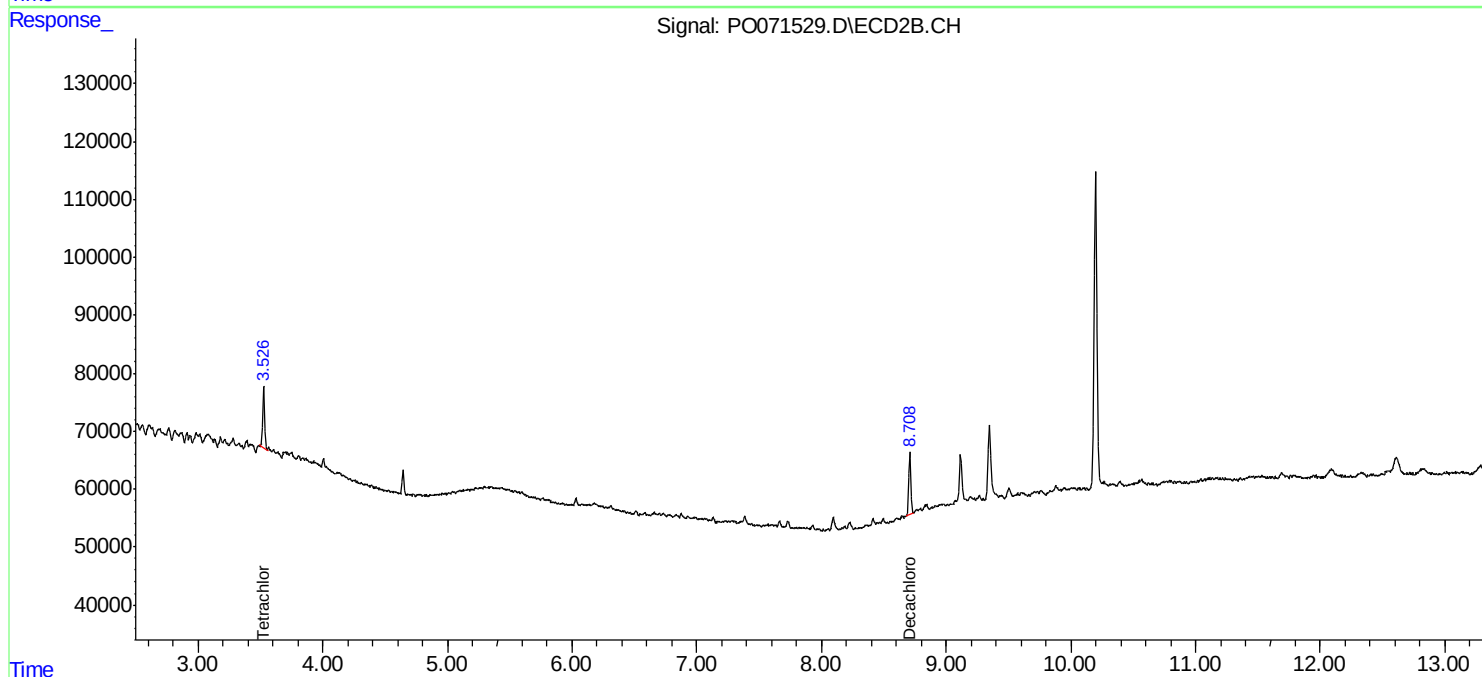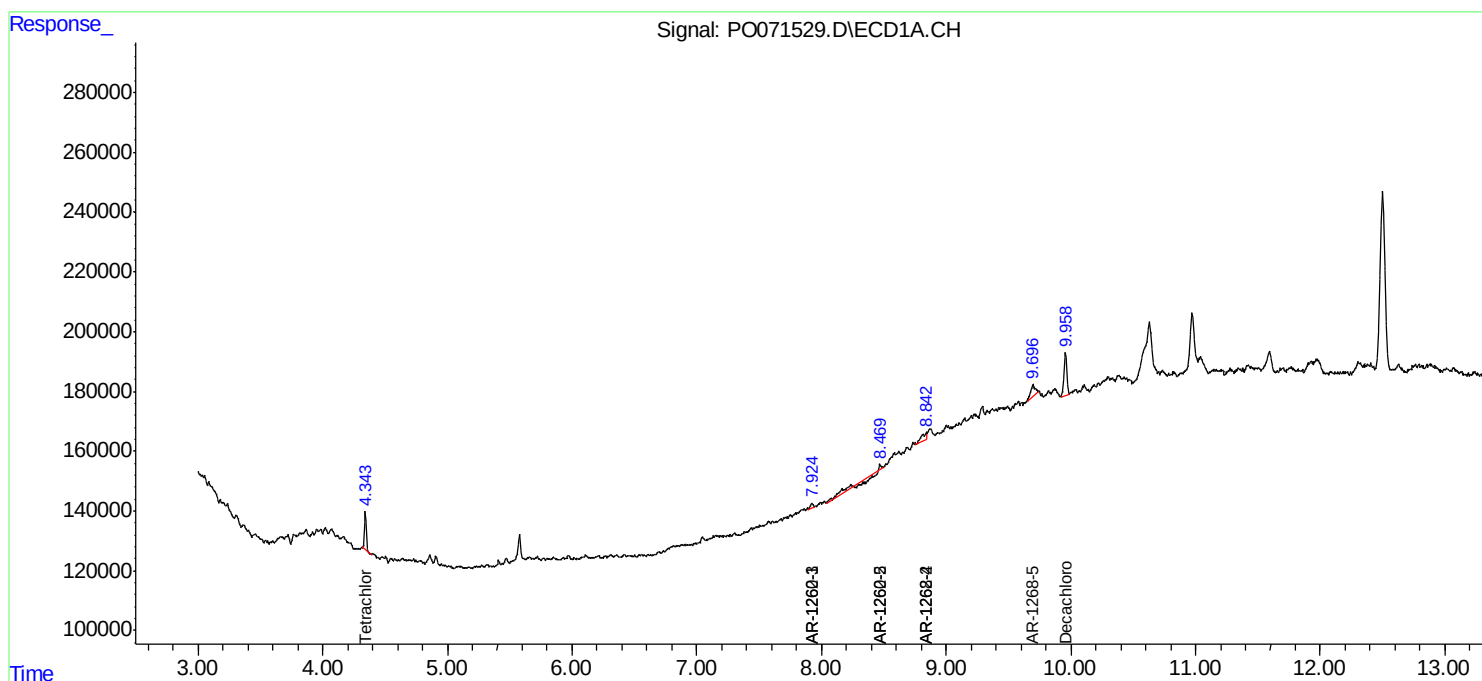


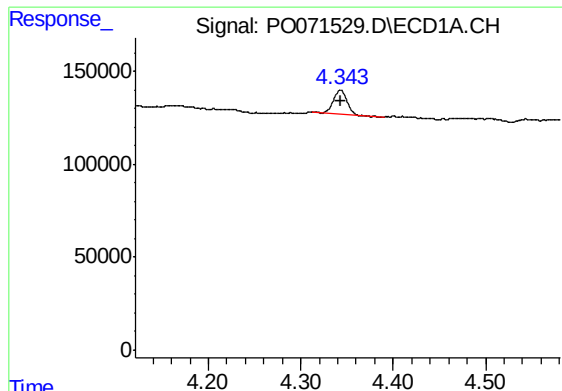

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 131984
Conc: 1.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

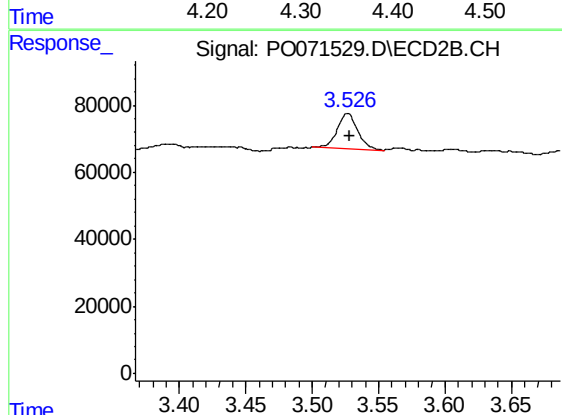


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.001 min
Response: 111614
Conc: 2.86 ng/ml

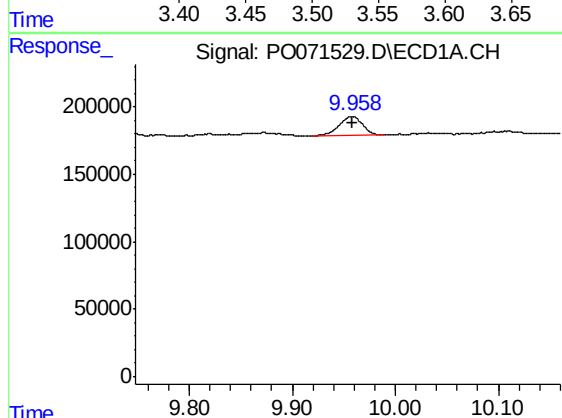


#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.000 min
Response: 232129
Conc: 2.49 ng/ml

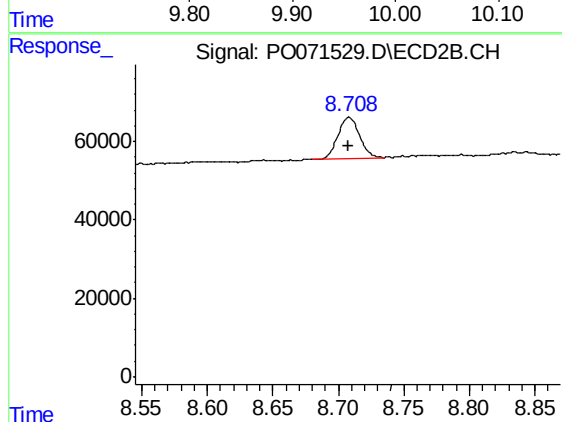

#2 Decachlorobiphenyl


R.T.: 8.708 min
Delta R.T.: 0.000 min
Response: 120631
Conc: 2.19 ng/ml

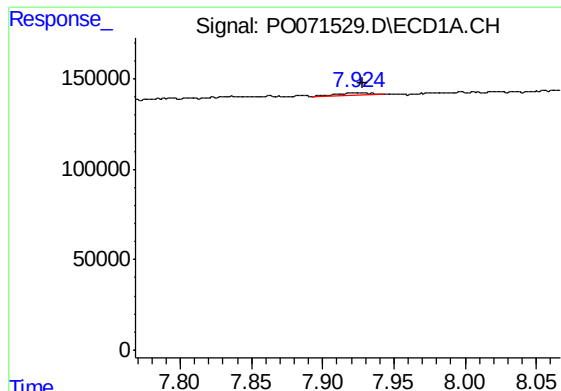

#33 AR-1260-3


R.T.: 7.925 min
Delta R.T.: -0.004 min
Response: 25264
Conc: 4.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

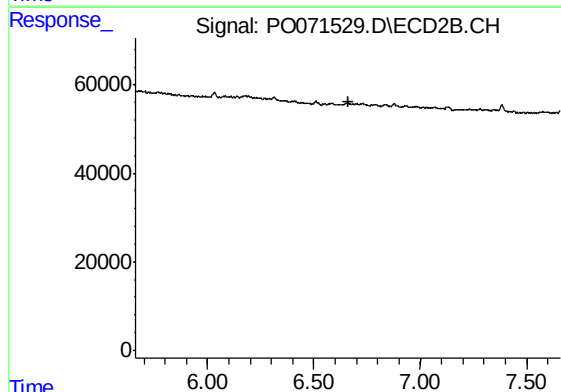


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.660 min
Response: 0
Conc: N.D.

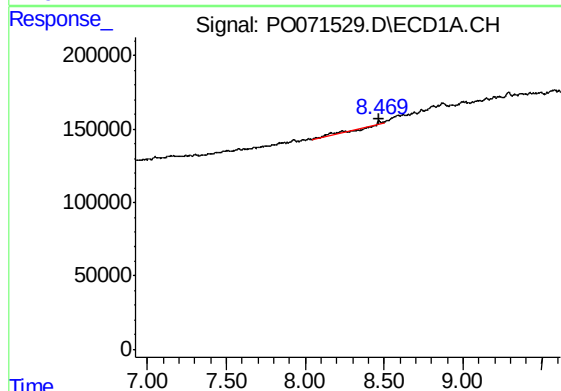


#35 AR-1260-5

R.T.: 8.469 min
Delta R.T.: -0.001 min
Response: 32275
Conc: 2.55 ng/ml

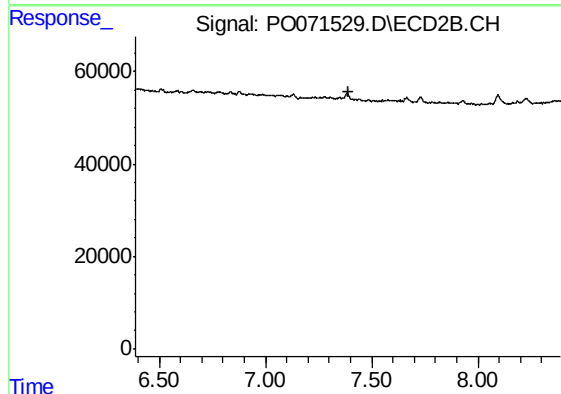

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

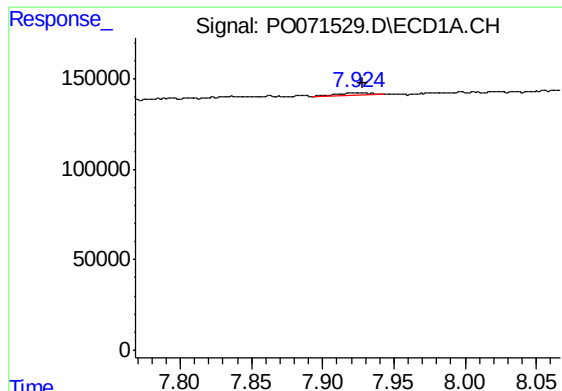

#36 AR-1262-1


R.T.: 7.925 min
Delta R.T.: -0.004 min
Response: 25264
Conc: 2.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

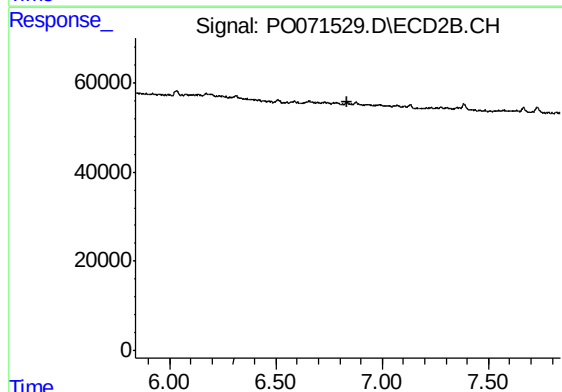


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.839 min
Response: 0
Conc: N.D.

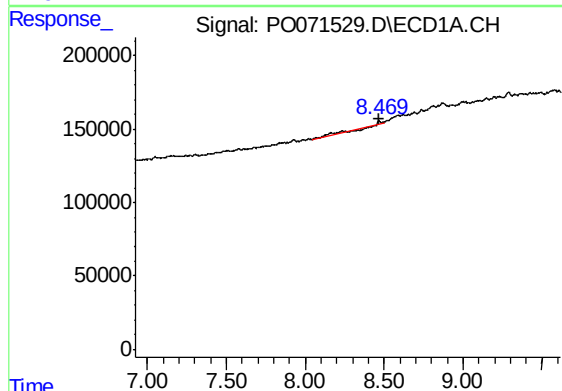


#37 AR-1262-2

R.T.: 8.469 min
Delta R.T.: -0.003 min
Response: 32275
Conc: 2.24 ng/ml

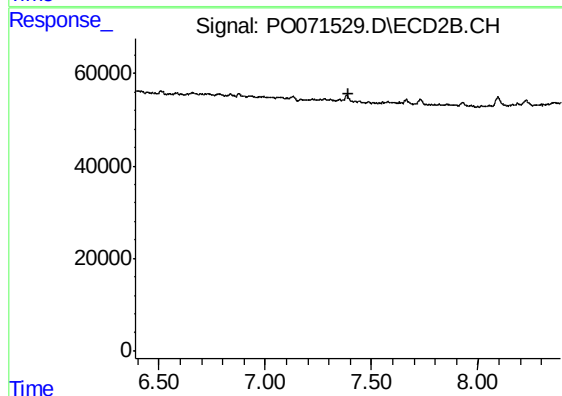

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

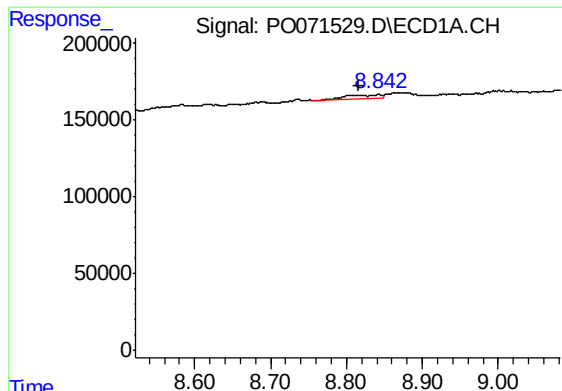

#39 AR-1262-4


R.T.: 8.842 min
Delta R.T.: 0.026 min
Response: 73561
Conc: 11.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

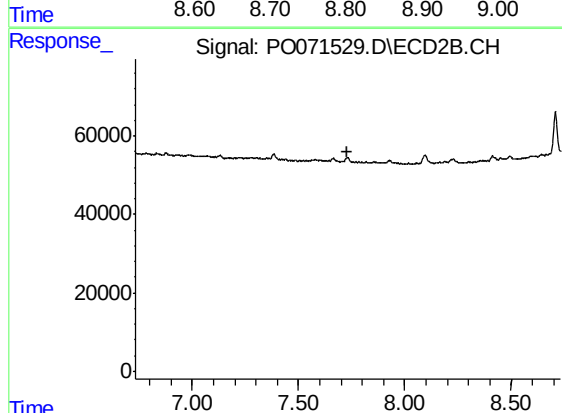


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.732 min
Response: 0
Conc: N.D.

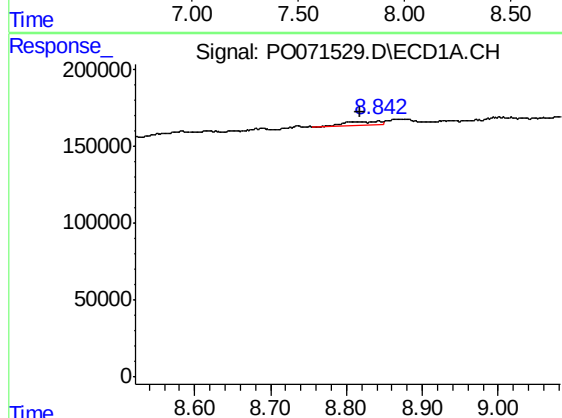


#42 AR-1268-2

R.T.: 8.842 min
Delta R.T.: 0.024 min
Response: 73561
Conc: 5.26 ng/ml

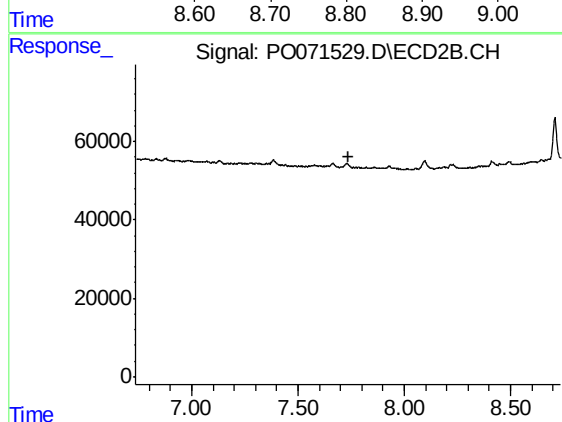

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 7.735 min
Response: 0
Conc: N.D.

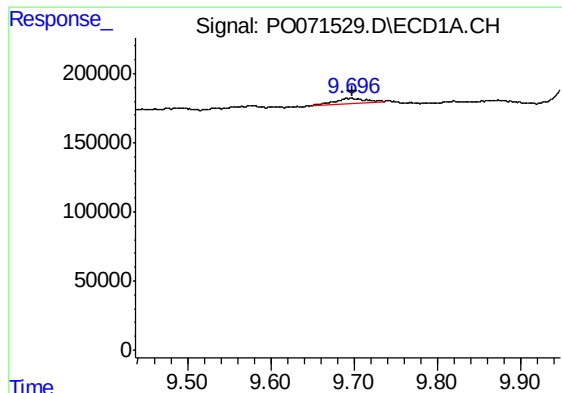

#45 AR-1268-5

R.T.: 9.697 min
Delta R.T.: -0.001 min
Response: 95513
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ075N-BOTTOM

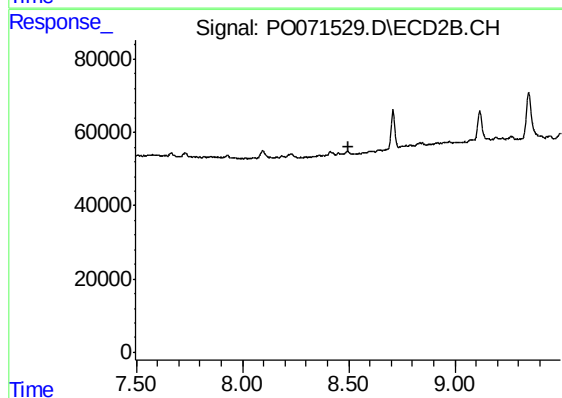

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.496 min
Response: 0
Conc: N.D.