

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092120\
 Data File : P0071489.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Sep 2020 11:13
 Operator : DD\AJ
 Sample : L4068-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PE-3B-(4.5-5)

Manual Integrations
 APPROVED

Ankita
 9/22/2020 1:10:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 15:18:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.525	1950427	995333	27.522	25.494
2) SA Decachlor...	9.950	8.701	2565506	1378200	27.511m	25.020

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092120\
Data File : P0071489.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2020 11:13
Operator : DD\AJ
Sample : L4068-08
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PE-3B-(4.5-5)


Manual Integrations
APPROVED

Ankita
9/22/2020 1:10:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 15:18:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

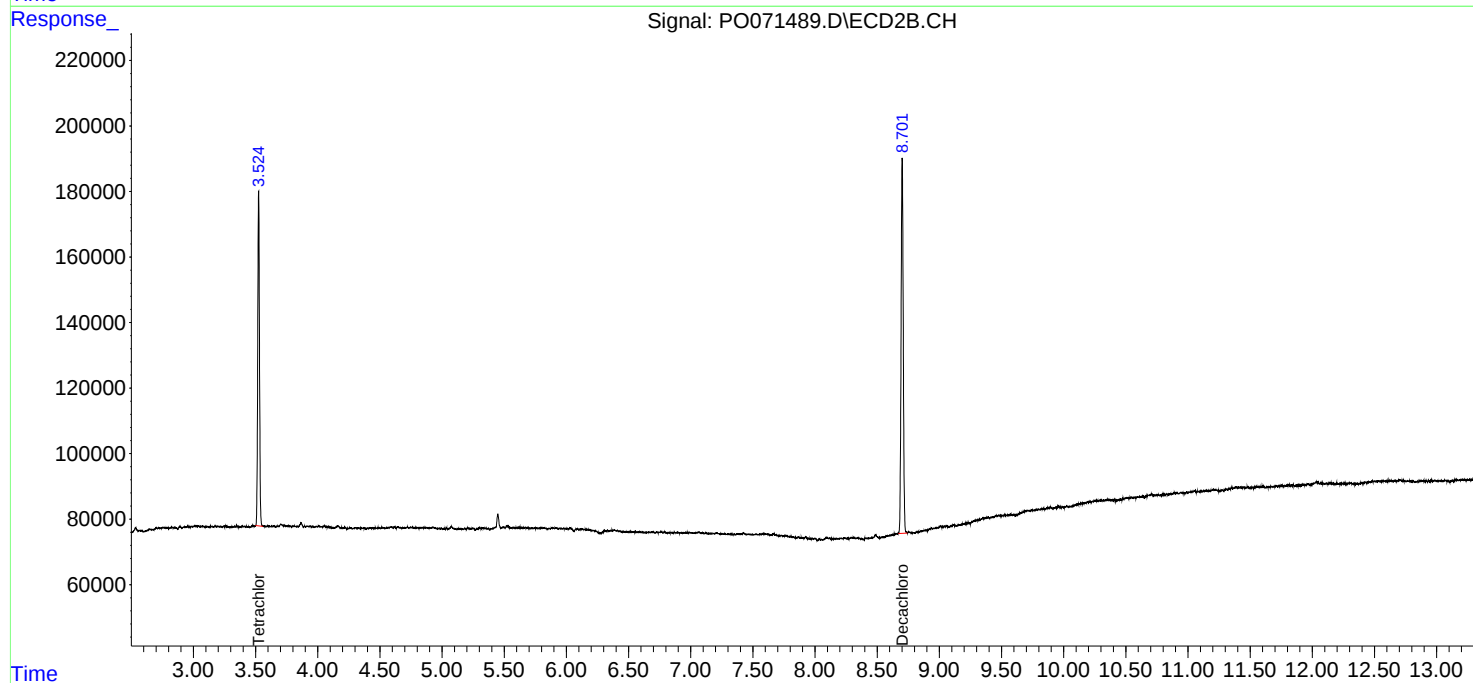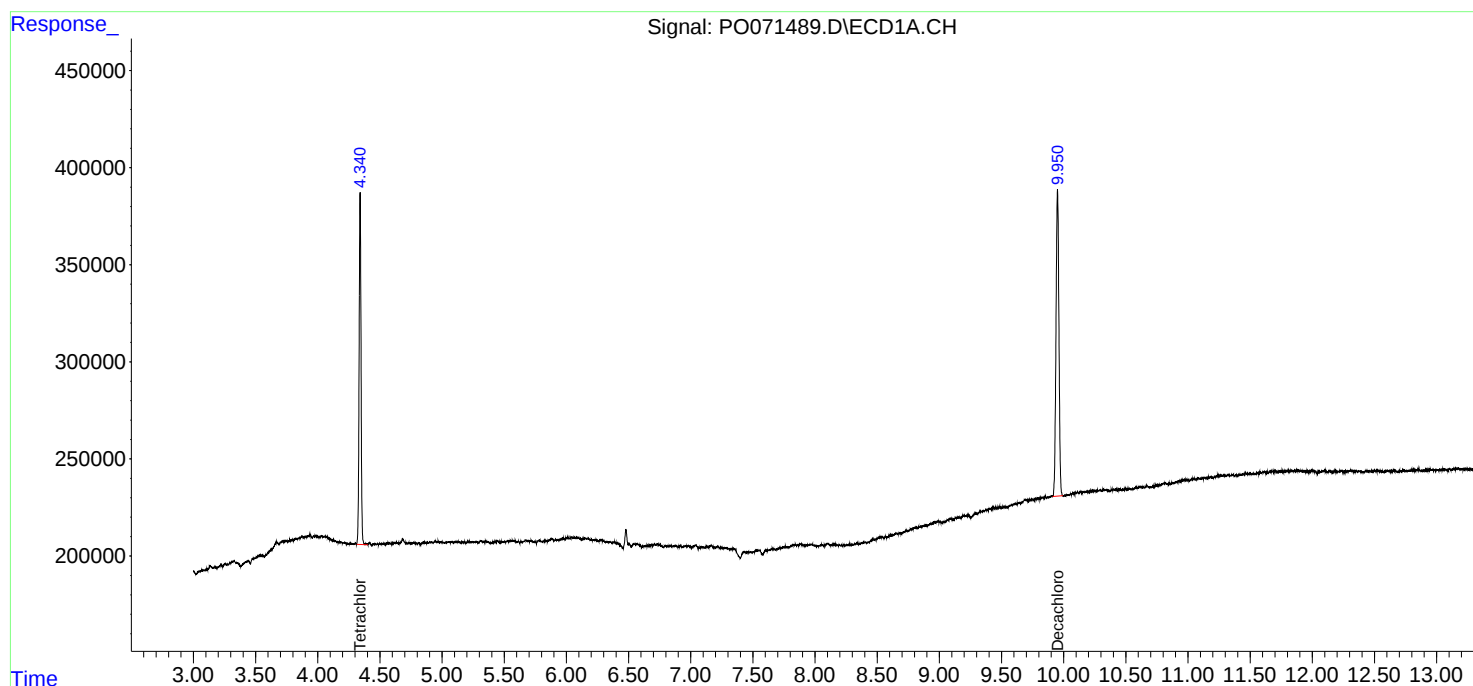

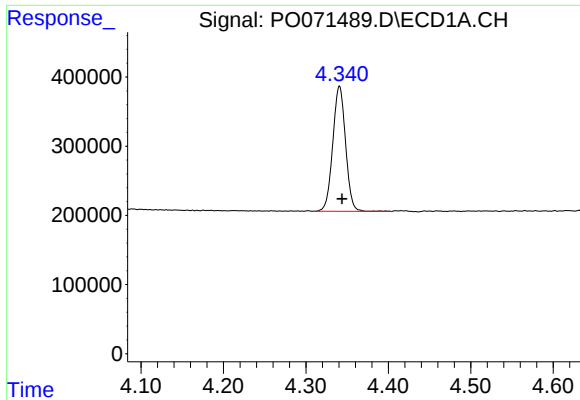


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: -0.003 min
Response: 1950427
Conc: 27.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
PE-3B-(4.5-5)


Manual Integrations
APPROVED

Ankita
9/22/2020 1:10:57 PM

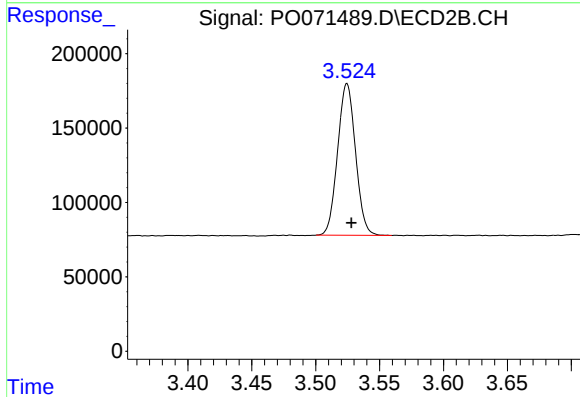


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.003 min
Response: 995333
Conc: 25.49 ng/ml

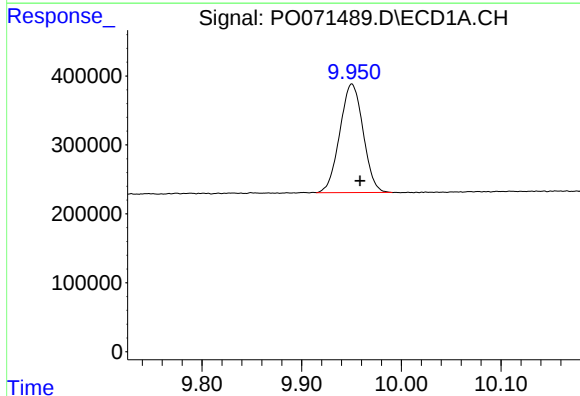

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.009 min
Response: 2565506
Conc: 27.51 ng/ml m

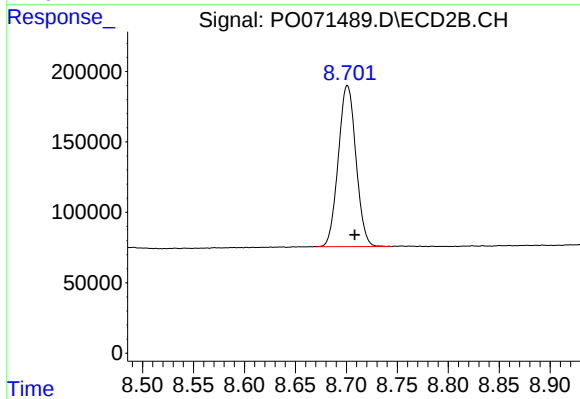

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.007 min
Response: 1378200
Conc: 25.02 ng/ml