

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092120\
 Data File : P0071494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Sep 2020 12:38
 Operator : DD\AJ
 Sample : L4074-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KTS-ST-0102-0-6

Manual Integrations
 APPROVED

Ankita
 9/22/2020 4:22:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 15:20:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 09 16:04:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.526	1083334	574332	15.287m	14.711
2) SA Decachlor...	9.951	8.702	1197585	674515	12.842	12.245
Target Compounds						
31) L7 AR-1260-1	7.302	6.309	679972	382826	149.959	137.407
32) L7 AR-1260-2	7.568	6.509	1120530	431897	160.733	119.481 #
33) L7 AR-1260-3	7.924	6.655	915977	401160	151.144	124.315
34) L7 AR-1260-4	8.152	7.131	813894	350462	142.181	120.979
35) L7 AR-1260-5	8.466	7.383	1934765	883133	152.579	116.468

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092120\
Data File : PO071494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2020 12:38
Operator : DD\AJ
Sample : L4074-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
KTS-ST-0102-0-6


Manual Integrations
APPROVED

Ankita
9/22/2020 4:22:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 15:20:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 09 16:04:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

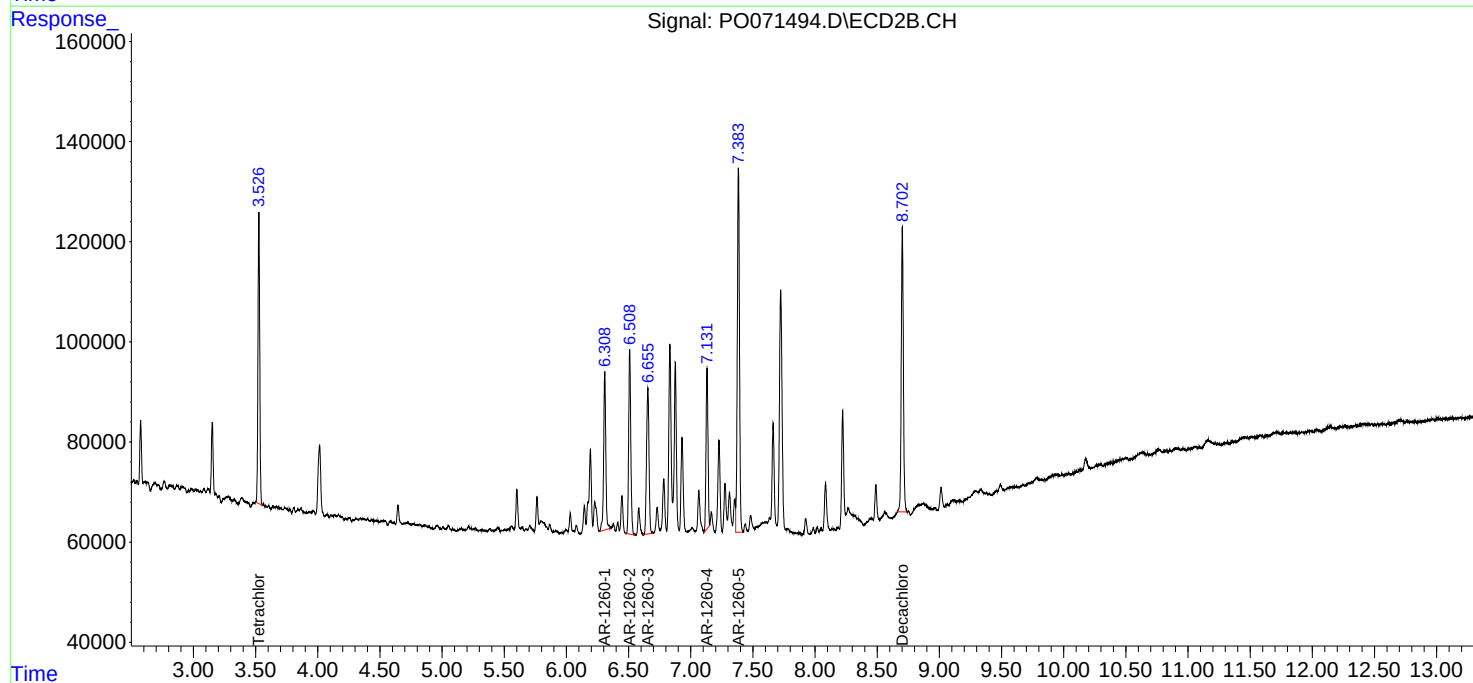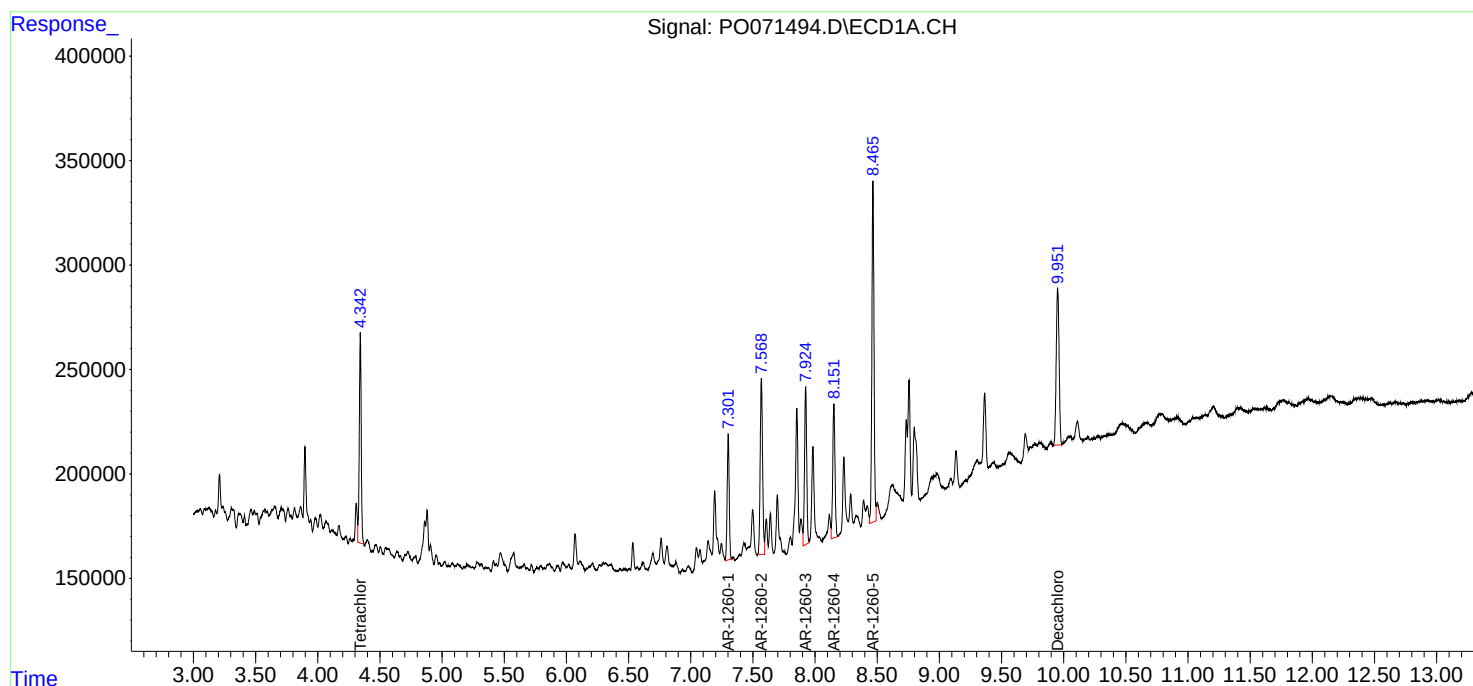

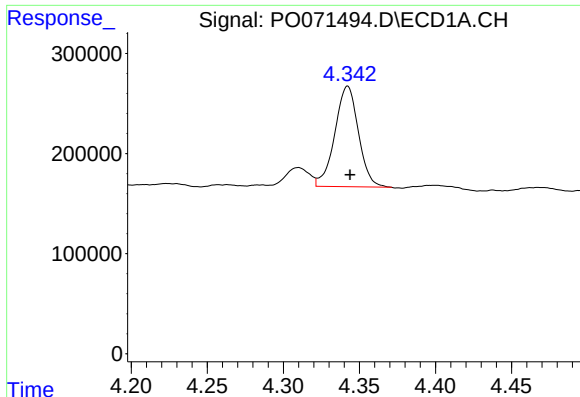


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1083334
Conc: 15.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KTS-ST-0102-0-6


Manual Integrations
APPROVED

Ankita
9/22/2020 4:22:23 PM

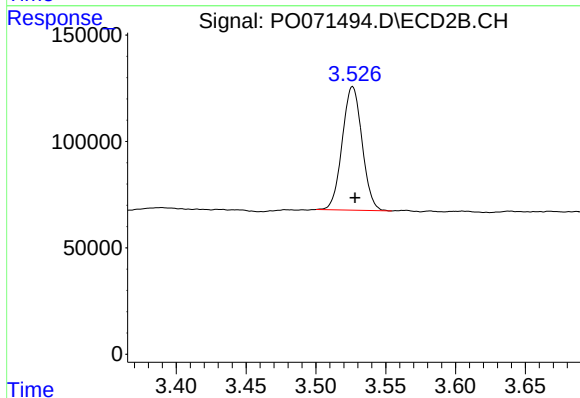


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.002 min
Response: 574332
Conc: 14.71 ng/ml

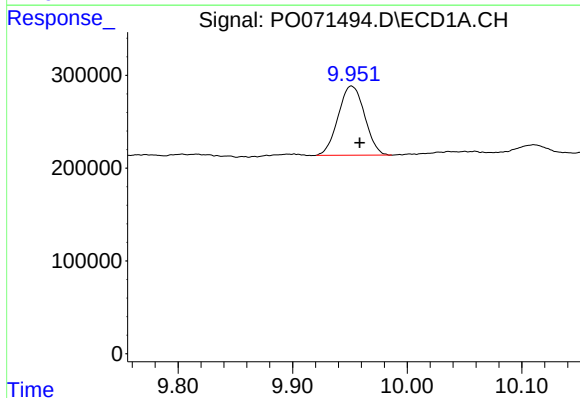


#2 Decachlorobiphenyl

R.T.: 9.951 min
Delta R.T.: -0.007 min
Response: 1197585
Conc: 12.84 ng/ml

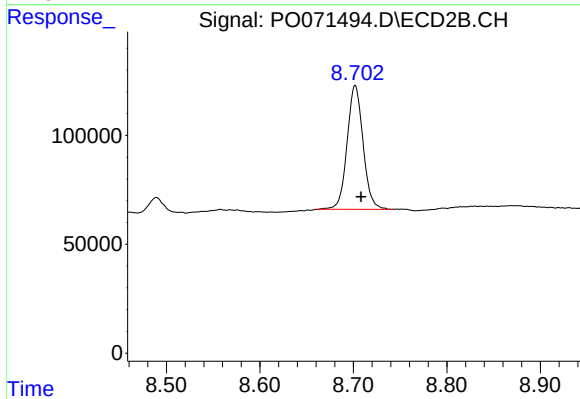

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.006 min
Response: 674515
Conc: 12.25 ng/ml

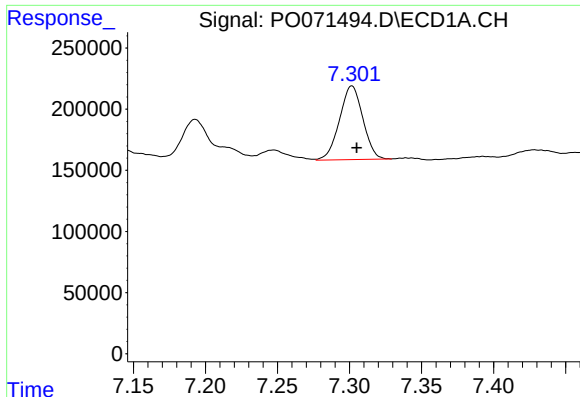


#31 AR-1260-1

R.T.: 7.302 min
Delta R.T.: -0.003 min
Response: 679972
Conc: 149.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-ST-0102-0-6


Manual Integrations
APPROVED

Ankita
9/22/2020 4:22:23 PM

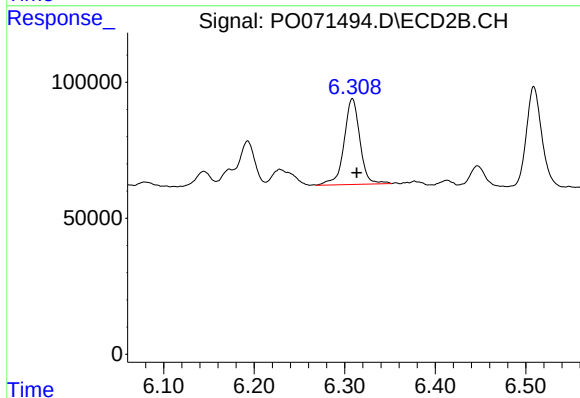


#31 AR-1260-1

R.T.: 6.309 min
Delta R.T.: -0.005 min
Response: 382826
Conc: 137.41 ng/ml

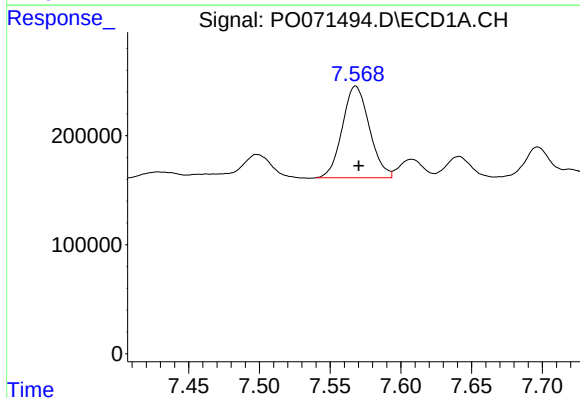


#32 AR-1260-2

R.T.: 7.568 min
Delta R.T.: -0.002 min
Response: 1120530
Conc: 160.73 ng/ml

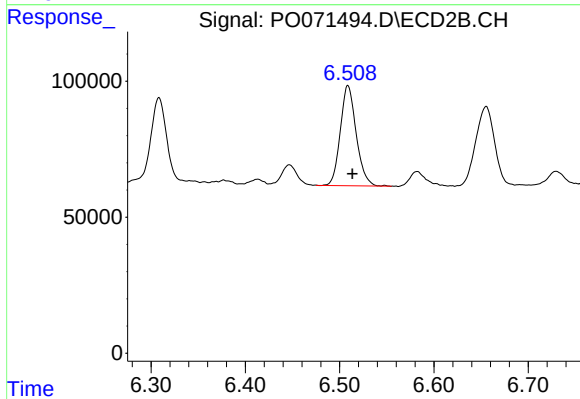

#32 AR-1260-2

R.T.: 6.509 min
Delta R.T.: -0.005 min
Response: 431897
Conc: 119.48 ng/ml

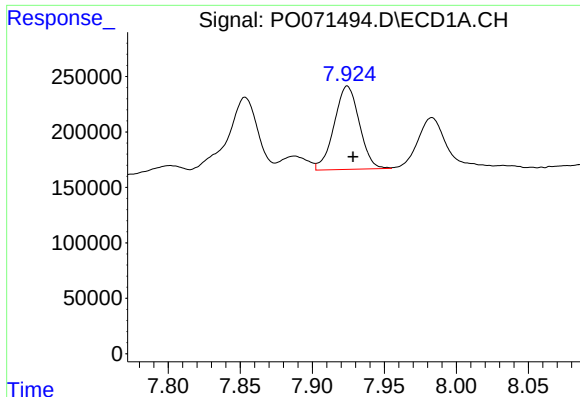


#33 AR-1260-3

R.T.: 7.924 min
Delta R.T.: -0.004 min
Response: 915977
Conc: 151.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-ST-0102-0-6


Manual Integrations
APPROVED

Ankita
9/22/2020 4:22:23 PM

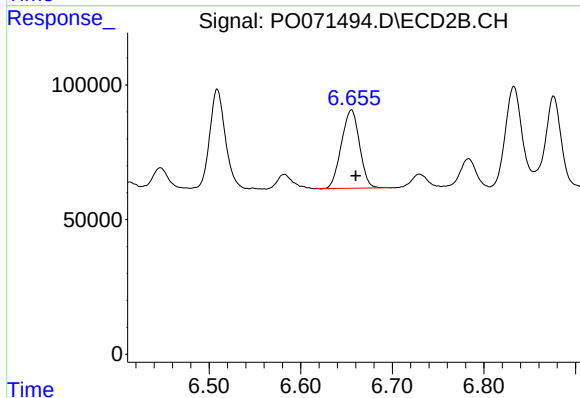


#33 AR-1260-3

R.T.: 6.655 min
Delta R.T.: -0.005 min
Response: 401160
Conc: 124.31 ng/ml

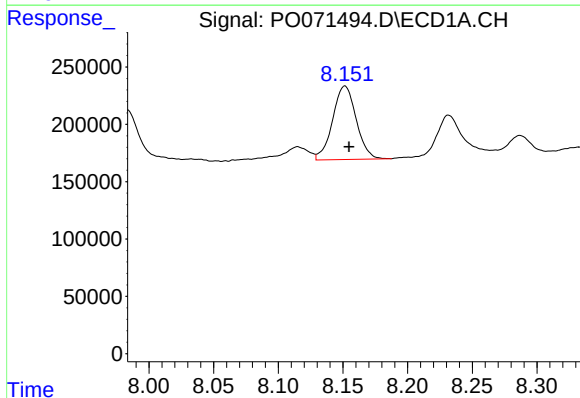


#34 AR-1260-4

R.T.: 8.152 min
Delta R.T.: -0.003 min
Response: 813894
Conc: 142.18 ng/ml

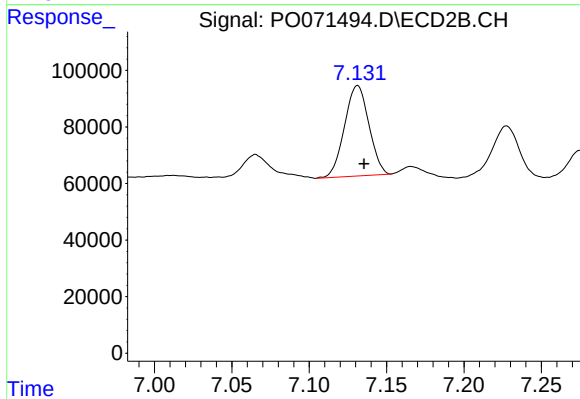

#34 AR-1260-4

R.T.: 7.131 min
Delta R.T.: -0.004 min
Response: 350462
Conc: 120.98 ng/ml

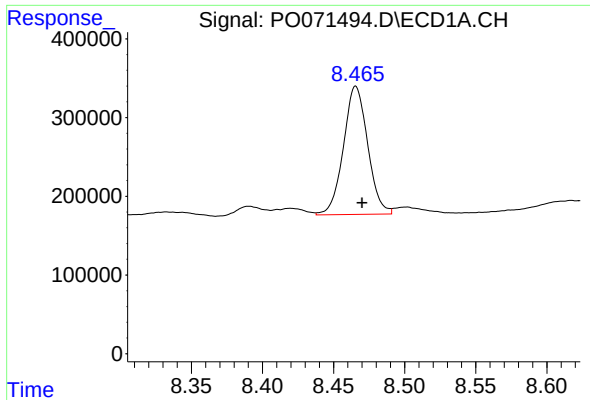


#35 AR-1260-5

R.T.: 8.466 min
Delta R.T.: -0.004 min
Response: 1934765
Conc: 152.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
KTS-ST-0102-0-6

Manual Integrations
APPROVED

Ankita
9/22/2020 4:22:23 PM

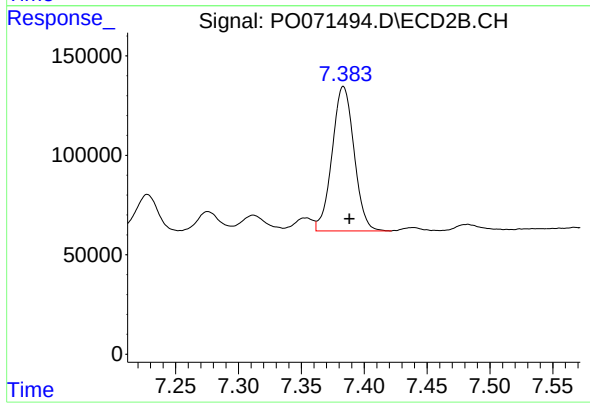

#35 AR-1260-5

R.T.: 7.383 min
Delta R.T.: -0.005 min
Response: 883133
Conc: 116.47 ng/ml