

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092123\
 Data File : P0098222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2023 15:45
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2023
 Supervised By :Ankita Jodhani 09/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 15:57:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 20 07:12:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.494	3.640	52997658	25300524	17.719	22.789 #
2) SA Decachlor...	10.337	8.660	33499784	22174270	19.189	20.128m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092123\
Data File : PO098222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2023 15:45
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2023
Supervised By :Ankita Jodhani 09/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 15:57:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091923.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 20 07:12:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

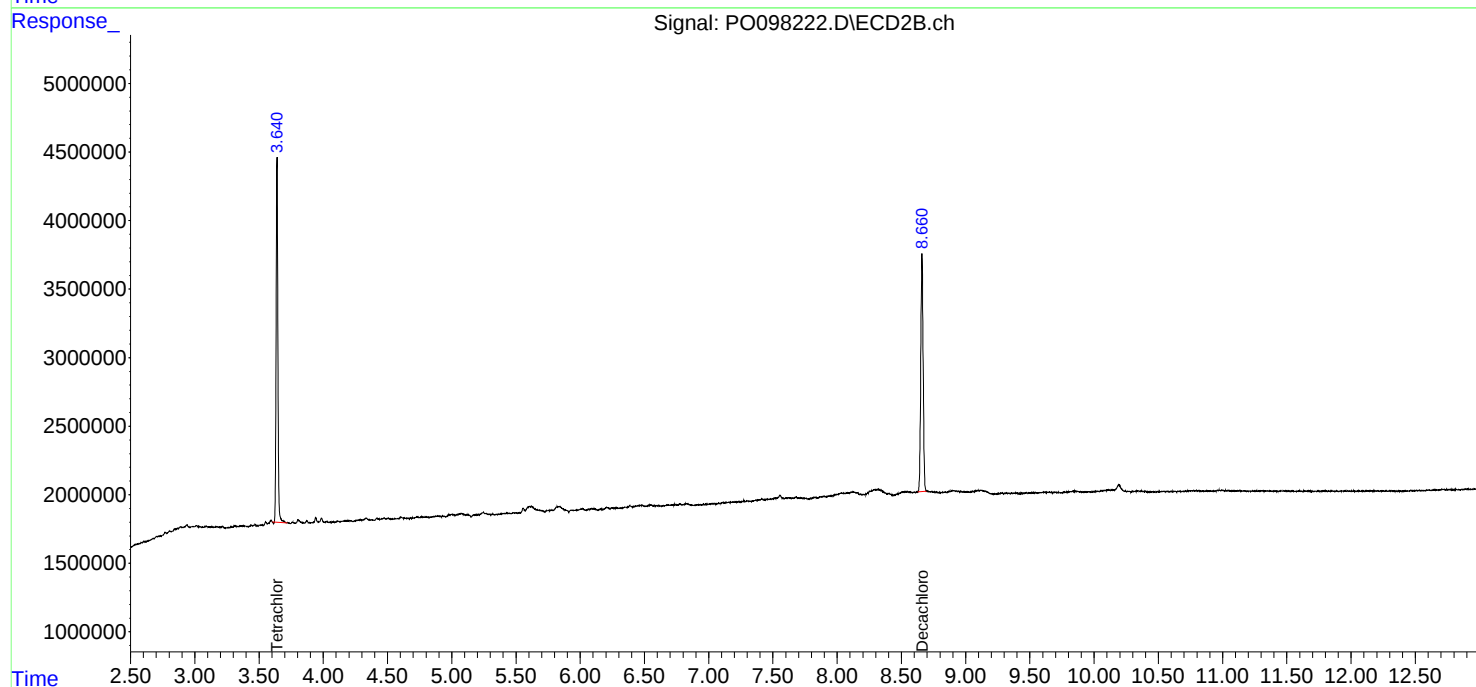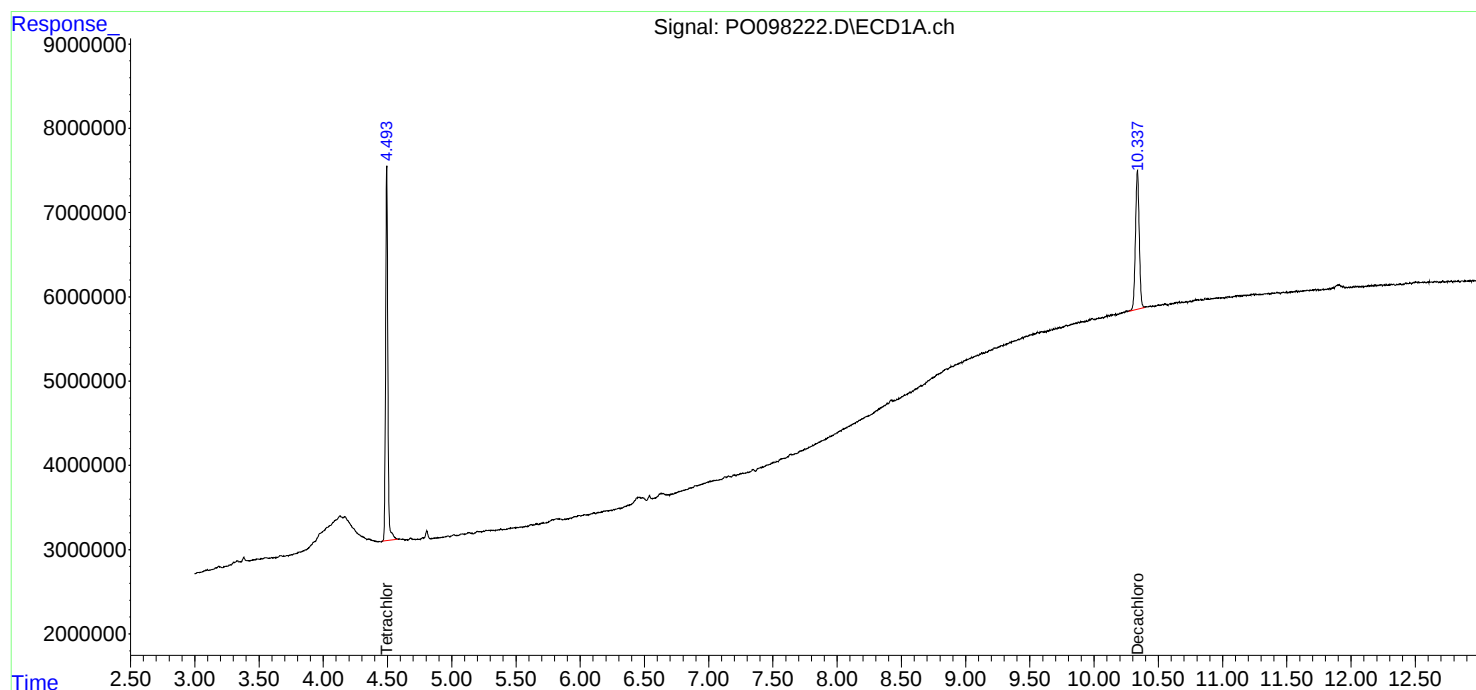

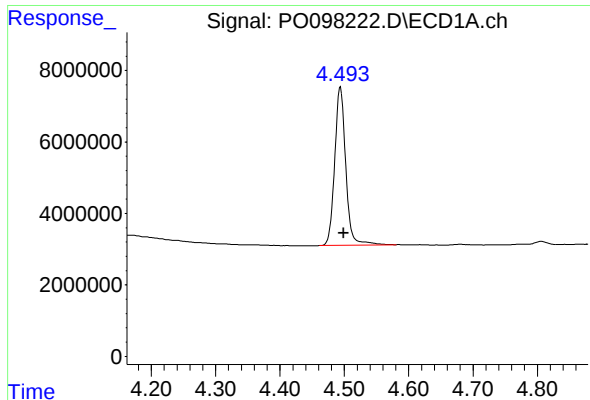


#1 Tetrachloro-m-xylene

R.T.: 4.494 min
Delta R.T.: -0.005 min
Response: 52997658
Conc: 17.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2023
Supervised By :Ankita Jodhani 09/22/2023

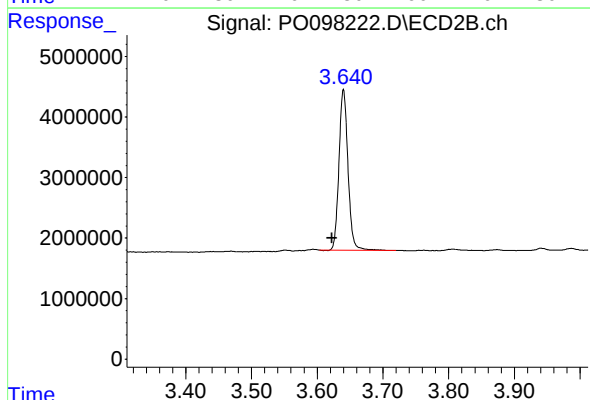


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.017 min
Response: 25300524
Conc: 22.79 ng/ml

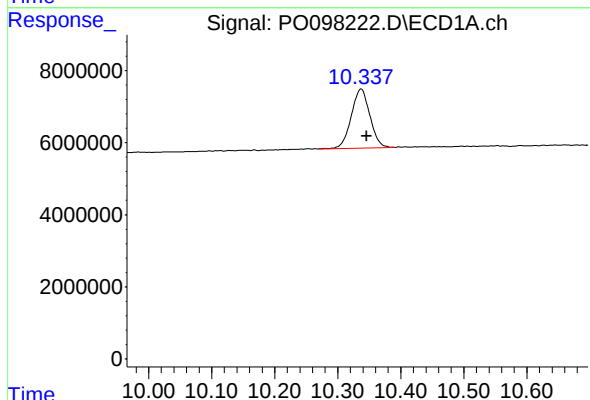

#2 Decachlorobiphenyl

R.T.: 10.337 min
Delta R.T.: -0.009 min
Response: 33499784
Conc: 19.19 ng/ml

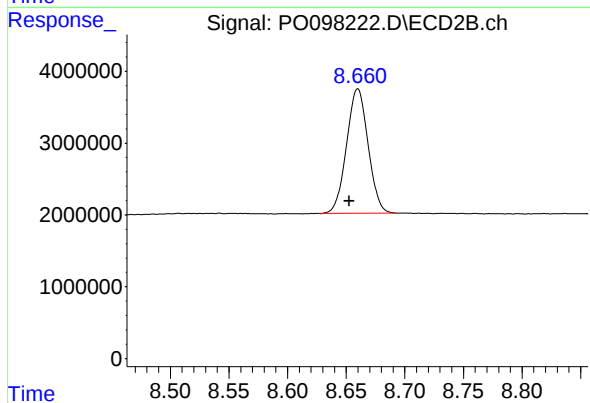

#2 Decachlorobiphenyl

R.T.: 8.660 min
Delta R.T.: 0.007 min
Response: 22174270
Conc: 20.13 ng/ml m