

Data Path : P:\HPCHEM1\ECD_0\Data\P0092215\
 Data File : P0024780.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Sep 2015 12:28
 Operator : IZ/UA
 Sample : TEST
 Misc : 200PPB SUR 10X
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 03:24:57 2015
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0091115.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 12 04:39:58 2015
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.132	3.226	4130064	5202038	18.619	18.490
2) SA Decachlor...	9.666	8.027	2323554	5111444	19.071	18.907

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO092215\
Data File : PO024780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2015 12:28
Operator : IZ/UA
Sample : TEST
Misc : 200PPB SUR 10X
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 03:24:57 2015
Quant Method : P:\HPCHEM1\ECD_0\methods\PO091115.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 12 04:39:58 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

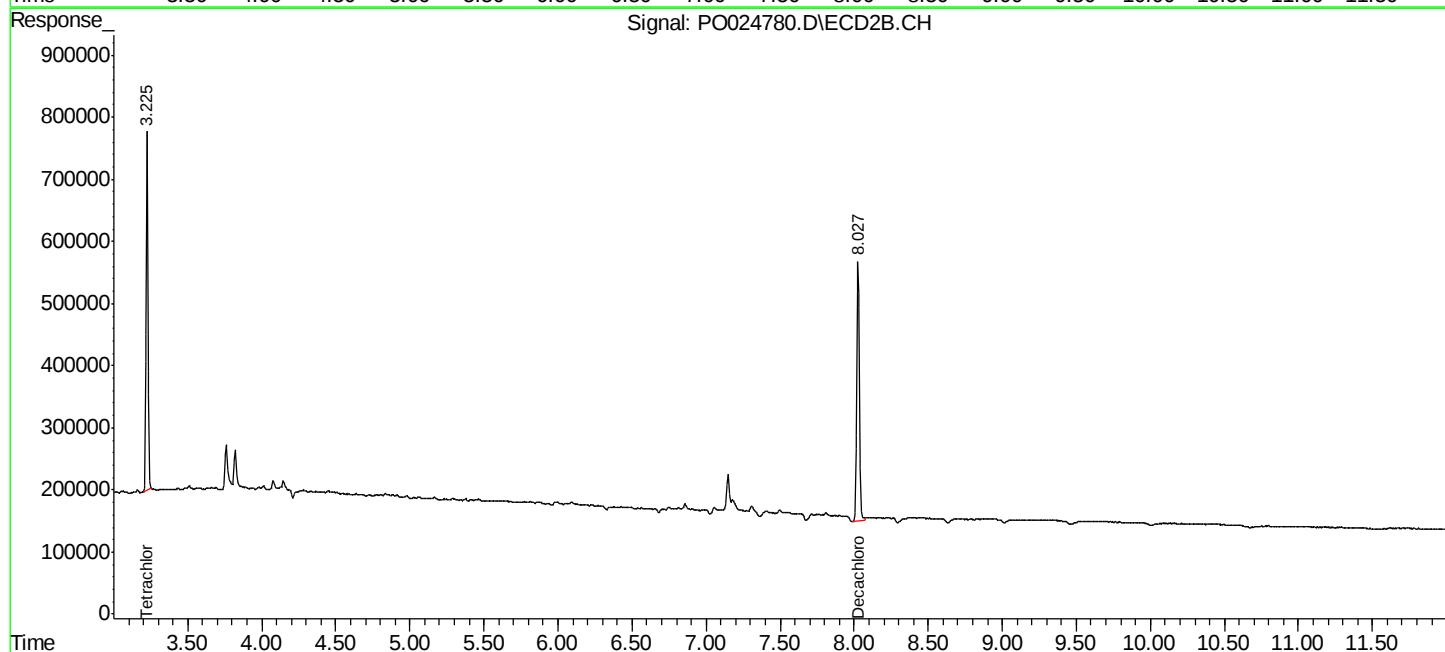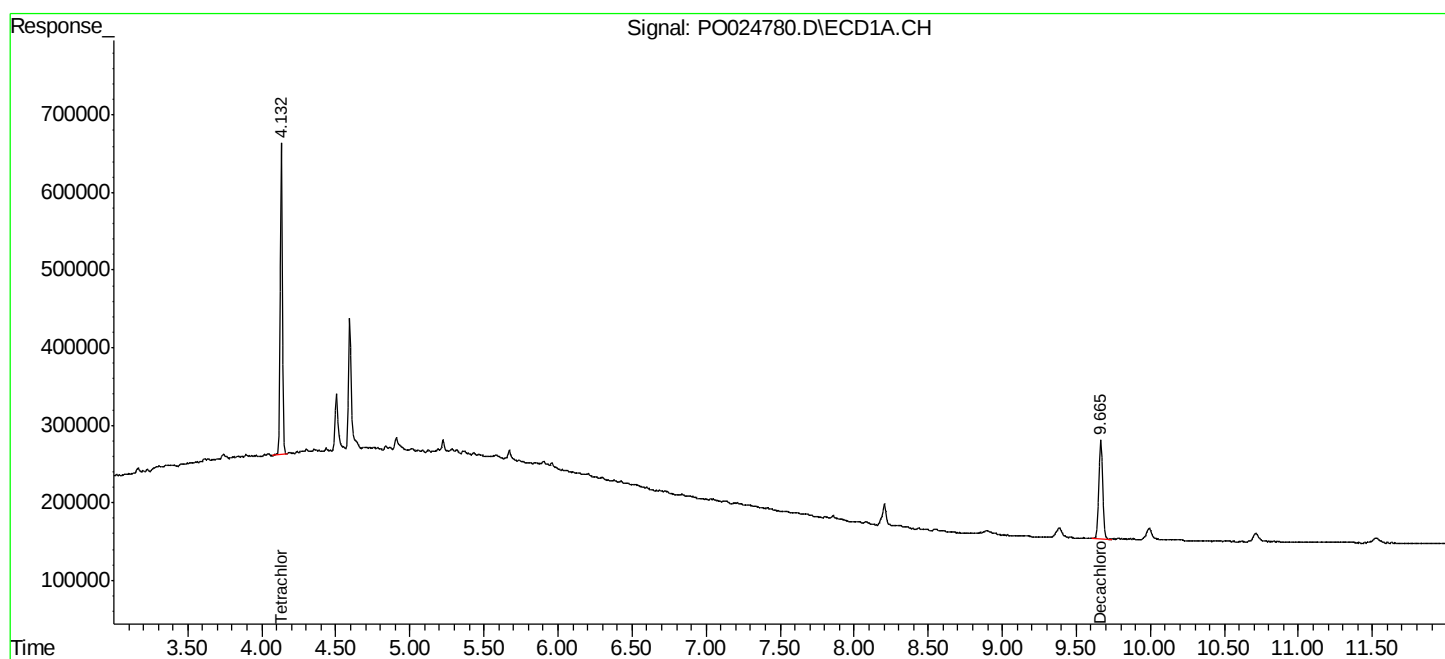


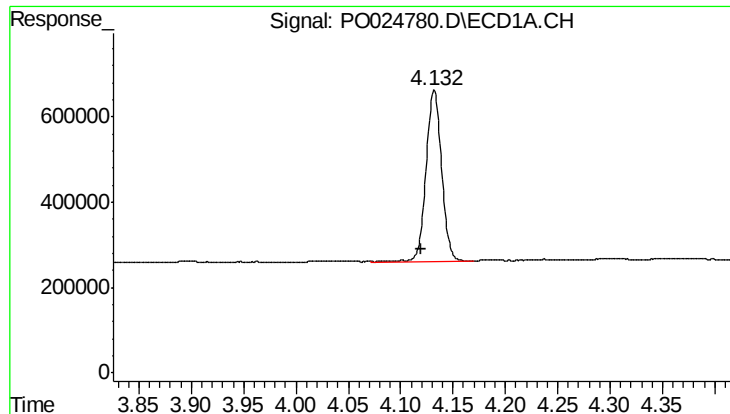

#1 Tetrachloro-m-xylene


R.T.: 4.132 min
Delta R.T.: 0.012 min
Response: 4130064
Conc: 18.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST

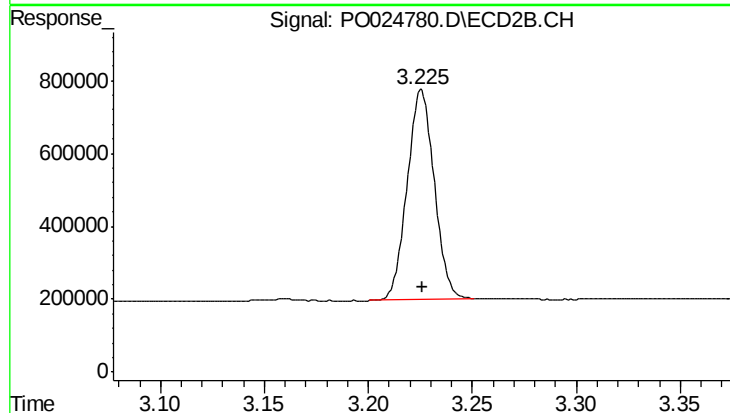


#1 Tetrachloro-m-xylene

R.T.: 3.226 min
Delta R.T.: 0.000 min
Response: 5202038
Conc: 18.49 ng/ml

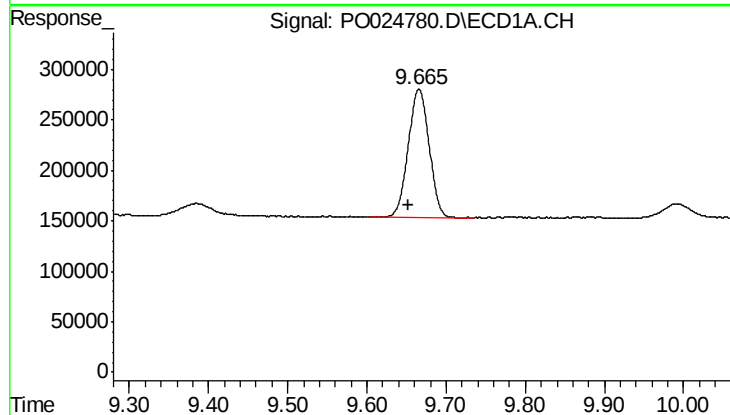

#2 Decachlorobiphenyl

R.T.: 9.666 min
Delta R.T.: 0.014 min
Response: 2323554
Conc: 19.07 ng/ml

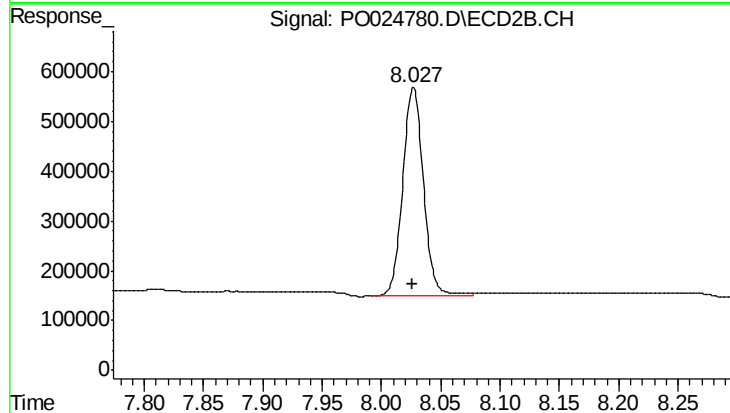

#2 Decachlorobiphenyl

R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 5111444
Conc: 18.91 ng/ml