

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
 Data File : P0061274.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Sep 2019 16:45
 Operator : SM/AJ
 Sample : K4968-01MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-010-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:26:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.370	3.530	570053	497179	15.494	17.806
2)	SA Decachlor...	10.038	8.407	1154534	834679	25.128	23.813
Target Compounds							
3)	L1 AR-1016-1	5.534	4.585	327827	261111	205.129	211.214
4)	L1 AR-1016-2	5.557	4.603	470177	356223	205.376	209.379
5)	L1 AR-1016-3	5.618	4.773	294379	197179	205.059	203.389
6)	L1 AR-1016-4	5.717	4.815	244434	167396	207.223	204.510
7)	L1 AR-1016-5	6.009	5.021	259397	221184	206.929	211.180
8)	L2 AR-1221-1	4.575	3.739	22948	21115	52.284	59.650
9)	L2 AR-1221-2	4.666	3.822	35567	37174	104.133	132.274 #
10)	L2 AR-1221-3	4.742	3.896	131913	117263	124.539	141.270
11)	L3 AR-1232-1	4.742	3.896	131913	117263	113.058	128.671
12)	L3 AR-1232-2	5.268	4.603	214033	356223	330.099	352.813
13)	L3 AR-1232-3	5.557	4.773	470177	197179	351.048	351.353
14)	L3 AR-1232-4	5.717	4.855	244434	206236	355.726	394.921
15)	L3 AR-1232-5	5.806	5.021	227793	221184	415.989	390.831
16)	L4 AR-1242-1	5.534	4.585	327827	261111	274.696	286.815
17)	L4 AR-1242-2	5.557	4.603	470177	356223	275.103	284.556
18)	L4 AR-1242-3	5.618	4.773	294379	197179	271.848	275.947
19)	L4 AR-1242-4	5.717	4.855	244434	206236	276.885	283.198
20)	L4 AR-1242-5	6.451	5.364	42025	189124	37.500	191.053 #
21)	L5 AR-1248-1	5.534	4.585	327827	261111	356.101	368.138
22)	L5 AR-1248-2	5.806	4.815	227793	167396	170.344	173.253
23)	L5 AR-1248-3	6.009	4.855	259397	206236	171.395	204.776
24)	L5 AR-1248-4	6.413	5.021	45535	221184	24.993	184.178 #
25)	L5 AR-1248-5	6.451	5.403	42025	31197	24.020	24.678
26)	L6 AR-1254-1	6.385	5.364	213130	189124	110.622	91.766
27)	L6 AR-1254-2	6.603	5.509	250243	191556	79.520	101.512 #
28)	L6 AR-1254-3	6.970	5.918	160216	355170	45.491	111.706 #
29)	L6 AR-1254-4	7.254	6.127	100140	47748	36.992	22.934 #
30)	L6 AR-1254-5	7.671	6.537	961617	743938	326.103	235.059 #
31)	L7 AR-1260-1	7.132	6.031	631838	496255	259.523	235.930
32)	L7 AR-1260-2	7.389	6.216	770955	613959	255.000	238.015
33)	L7 AR-1260-3	7.746	6.367	515262	579203	215.913	240.526
34)	L7 AR-1260-4	7.971	6.831	647841	453177	231.563	211.741
35)	L7 AR-1260-5	8.287	7.070	1239270	1040865	227.584	215.389
36)	L8 AR-1262-1	7.746	6.576	515262	470341	145.871	157.468
37)	L8 AR-1262-2	8.287	7.070	1239270	1040865	198.778	200.187
38)	L8 AR-1262-3	8.605	7.349	815082	226187	191.294	106.570 #
39)	L8 AR-1262-4	8.658	7.411	453956	771125	139.233	201.893 #
40)	L8 AR-1262-5	9.316	7.900	303454	245778	149.236	146.841
41)	L9 AR-1268-1	8.605	7.349	815082	226187	110.438	38.585 #
42)	L9 AR-1268-2	8.658	7.411	453956	771125	67.202	144.677 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061274.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Sep 2019 16:45
Operator : SM/AJ
Sample : K4968-01MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:26:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	8.900	7.616	30629	26952	5.454	6.080
44)	L9 AR-1268-4	9.316	7.900	303454	245778	131.552	128.622
45)	L9 AR-1268-5	9.715	8.172	100891	89653	6.361	7.450



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092319\
Data File : PO061274.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Sep 2019 16:45
Operator : SM/AJ
Sample : K4968-01MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:26:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

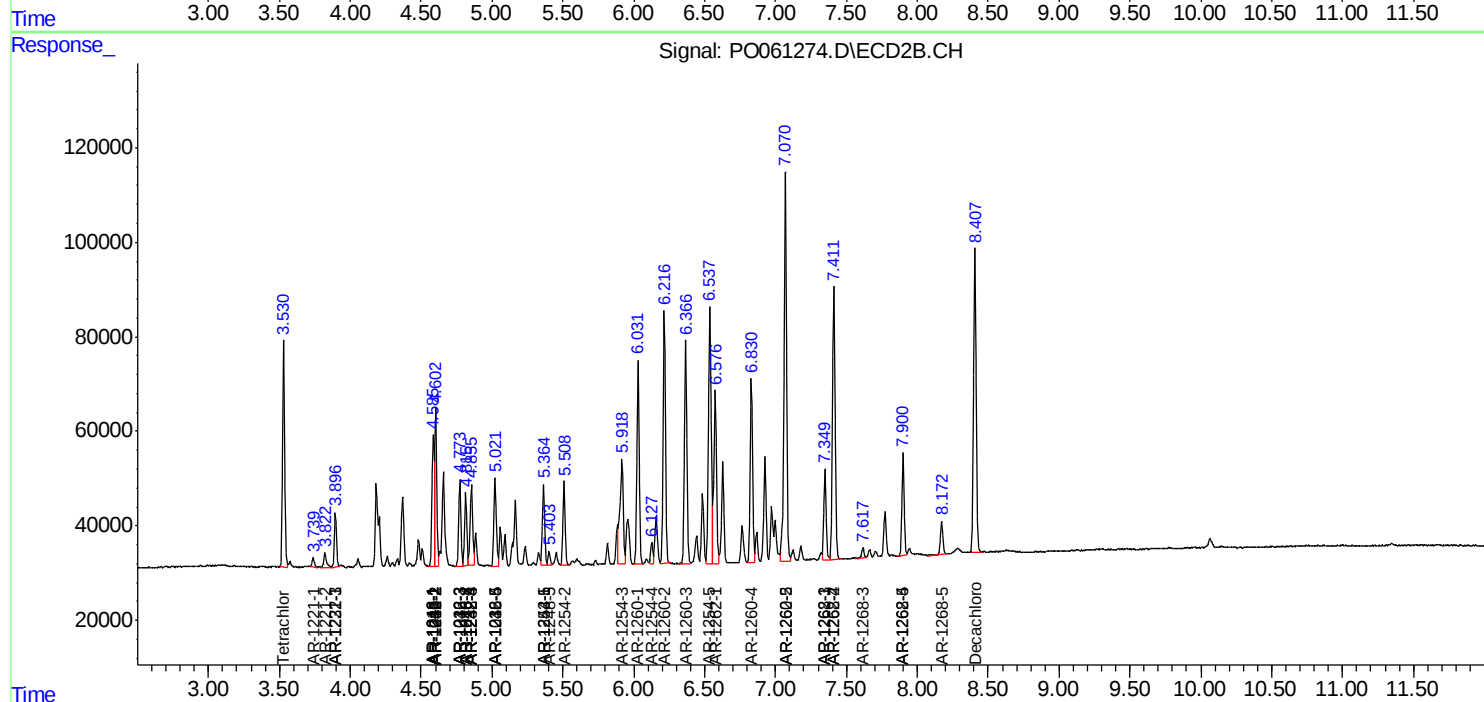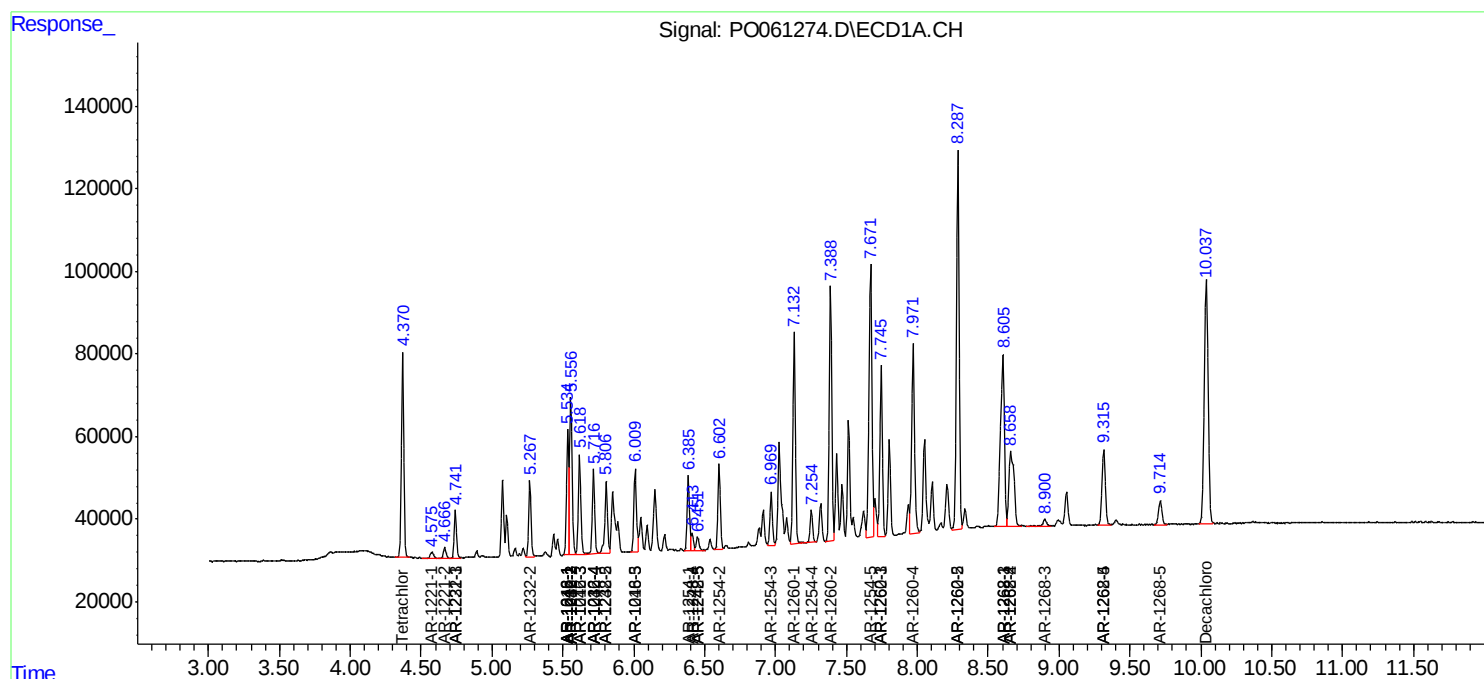




#1 Tetrachloro-m-xylene


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 570053
Conc: 15.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 497179
Conc: 17.81 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.038 min
Delta R.T.: 0.011 min
Response: 1154534
Conc: 25.13 ng/ml

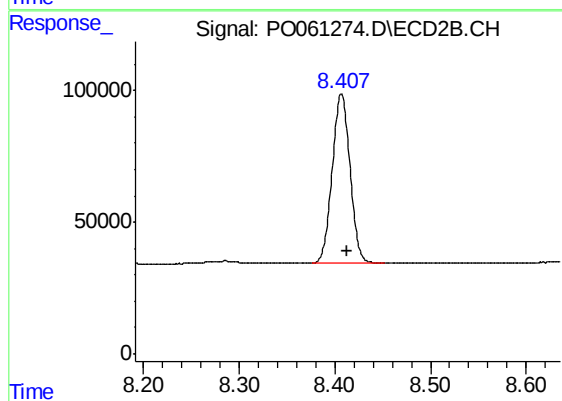

#2 Decachlorobiphenyl


R.T.: 8.407 min
Delta R.T.: -0.006 min
Response: 834679
Conc: 23.81 ng/ml

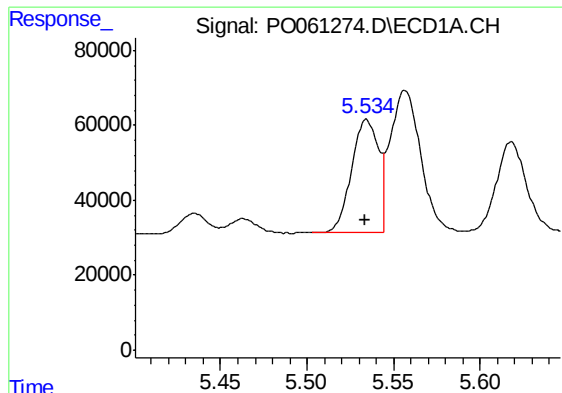

#3 AR-1016-1


R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 327827
Conc: 205.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

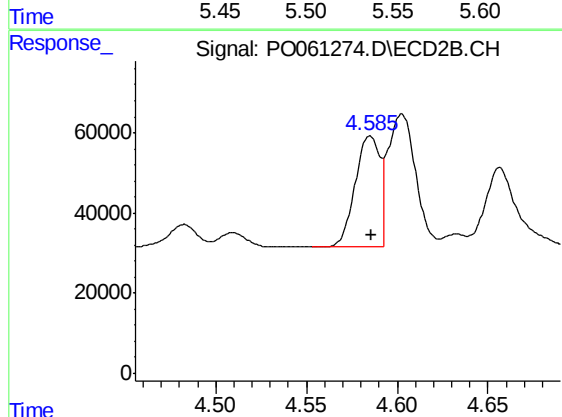


#3 AR-1016-1

R.T.: 4.585 min
Delta R.T.: -0.001 min
Response: 261111
Conc: 211.21 ng/ml

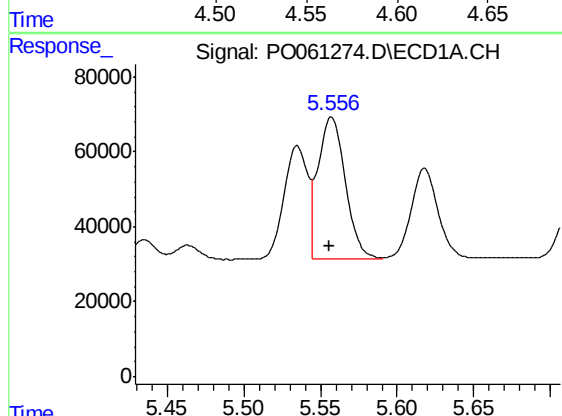


#4 AR-1016-2

R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 470177
Conc: 205.38 ng/ml

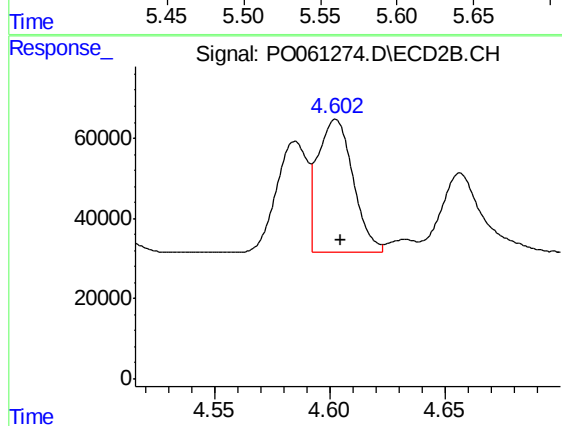

#4 AR-1016-2


R.T.: 4.603 min
Delta R.T.: -0.002 min
Response: 356223
Conc: 209.38 ng/ml

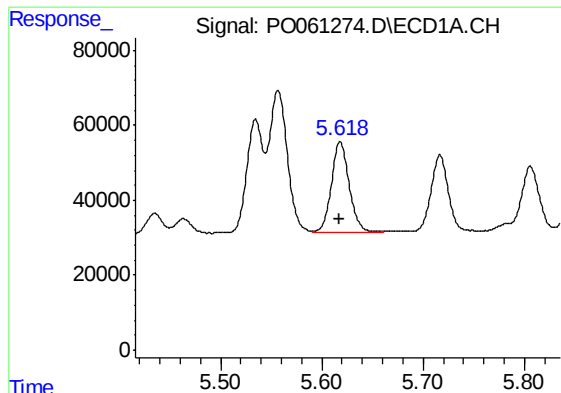

#5 AR-1016-3


R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 294379
Conc: 205.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

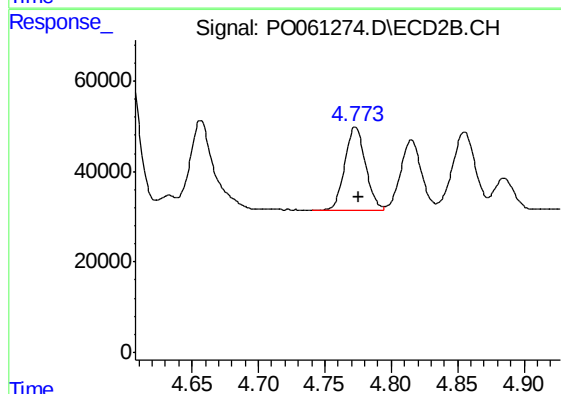


#5 AR-1016-3

R.T.: 4.773 min
Delta R.T.: -0.002 min
Response: 197179
Conc: 203.39 ng/ml

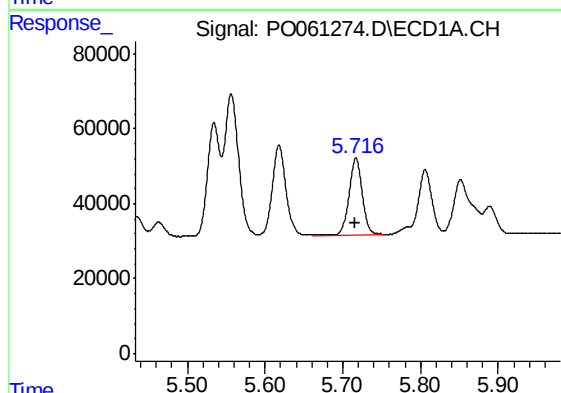


#6 AR-1016-4

R.T.: 5.717 min
Delta R.T.: 0.001 min
Response: 244434
Conc: 207.22 ng/ml

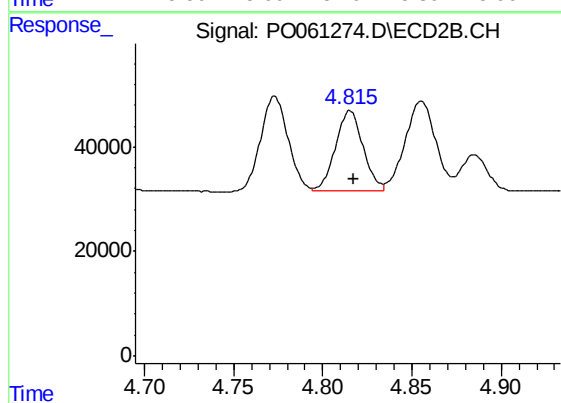

#6 AR-1016-4


R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 167396
Conc: 204.51 ng/ml



#7 AR-1016-5


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 259397
Conc: 206.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#7 AR-1016-5

R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 221184
Conc: 211.18 ng/ml

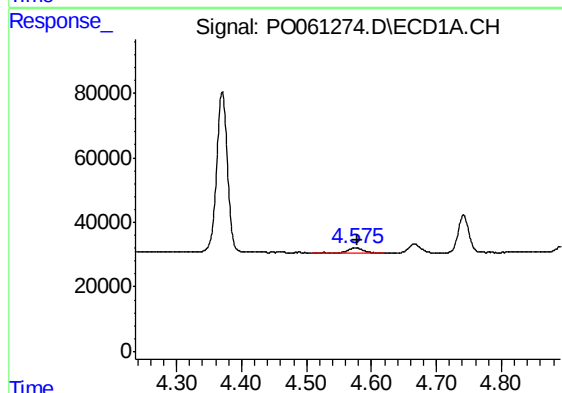


#8 AR-1221-1

R.T.: 4.575 min
Delta R.T.: -0.003 min
Response: 22948
Conc: 52.28 ng/ml

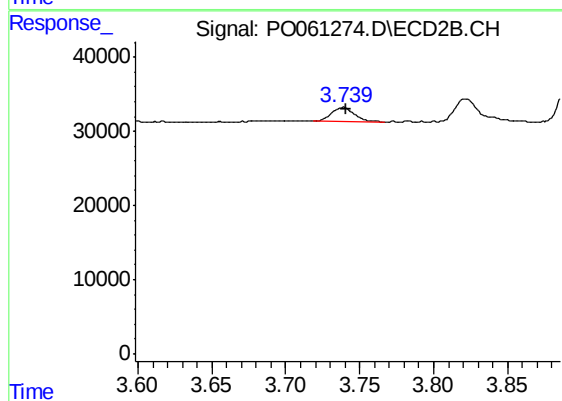

#8 AR-1221-1


R.T.: 3.739 min
Delta R.T.: -0.002 min
Response: 21115
Conc: 59.65 ng/ml



#9 AR-1221-2


R.T.: 4.666 min
Delta R.T.: 0.002 min
Response: 35567
Conc: 104.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

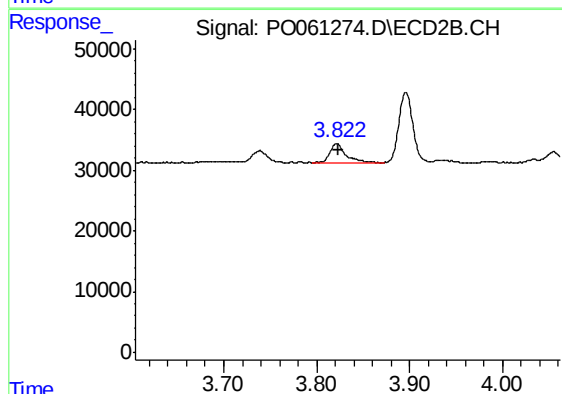


#9 AR-1221-2

R.T.: 3.822 min
Delta R.T.: -0.001 min
Response: 37174
Conc: 132.27 ng/ml

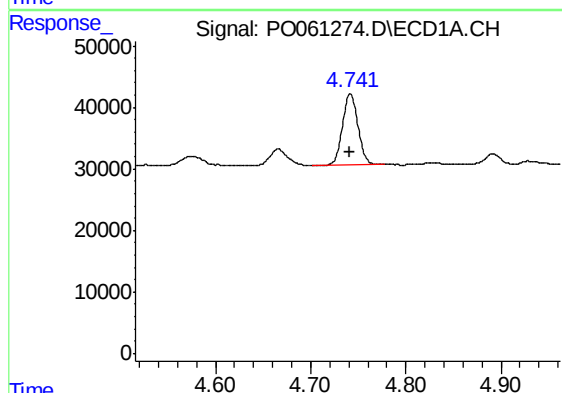


#10 AR-1221-3

R.T.: 4.742 min
Delta R.T.: 0.000 min
Response: 131913
Conc: 124.54 ng/ml

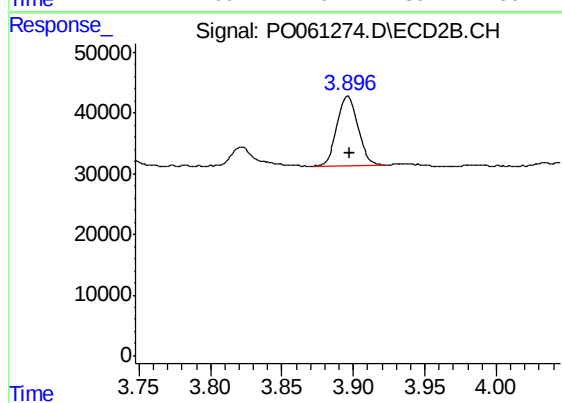

#10 AR-1221-3


R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 117263
Conc: 141.27 ng/ml

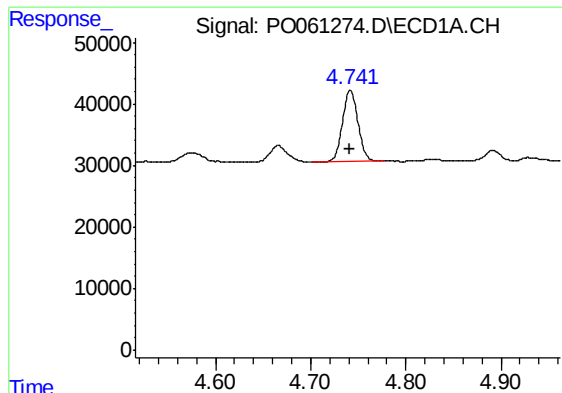

#11 AR-1232-1


R.T.: 4.742 min
Delta R.T.: 0.001 min
Response: 131913
Conc: 113.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

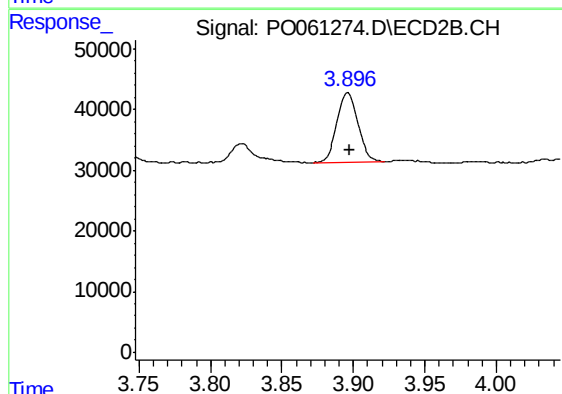


#11 AR-1232-1

R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 117263
Conc: 128.67 ng/ml

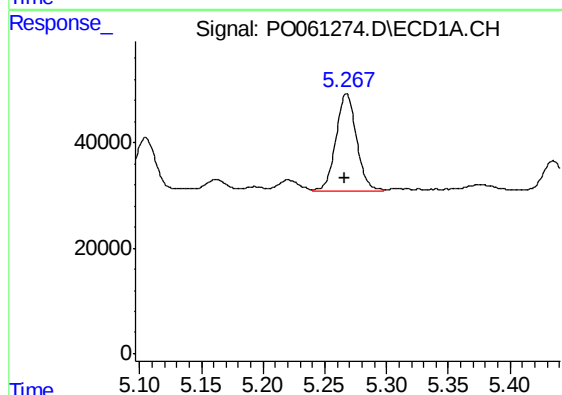


#12 AR-1232-2

R.T.: 5.268 min
Delta R.T.: 0.001 min
Response: 214033
Conc: 330.10 ng/ml

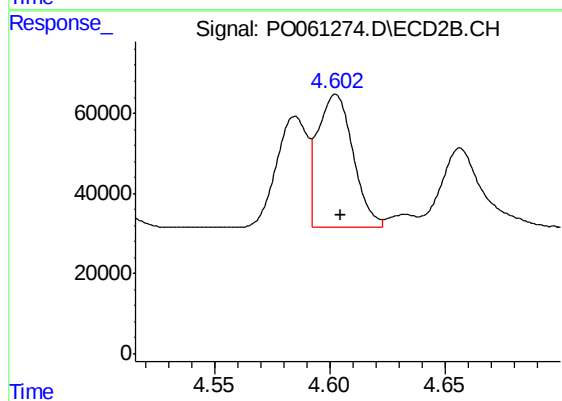

#12 AR-1232-2


R.T.: 4.603 min
Delta R.T.: -0.002 min
Response: 356223
Conc: 352.81 ng/ml



#13 AR-1232-3


R.T.: 5.557 min
Delta R.T.: 0.002 min
Response: 470177
Conc: 351.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#13 AR-1232-3

R.T.: 4.773 min
Delta R.T.: -0.002 min
Response: 197179
Conc: 351.35 ng/ml




#14 AR-1232-4

R.T.: 5.717 min
Delta R.T.: 0.002 min
Response: 244434
Conc: 355.73 ng/ml

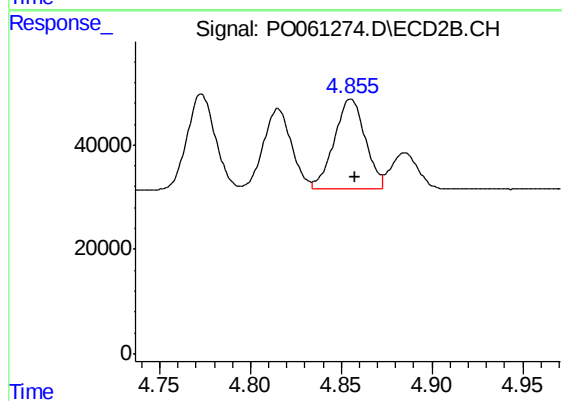

#14 AR-1232-4


R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 206236
Conc: 394.92 ng/ml

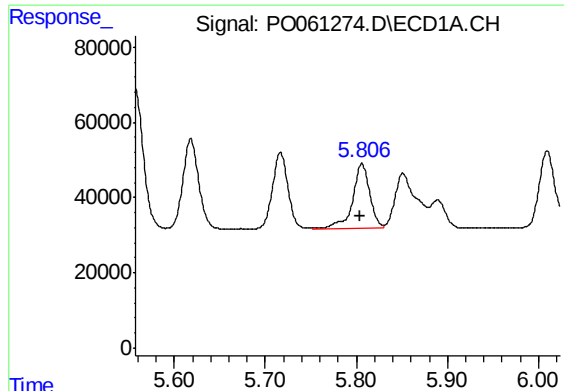

#15 AR-1232-5


R.T.: 5.806 min
Delta R.T.: 0.002 min
Response: 227793
Conc: 415.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

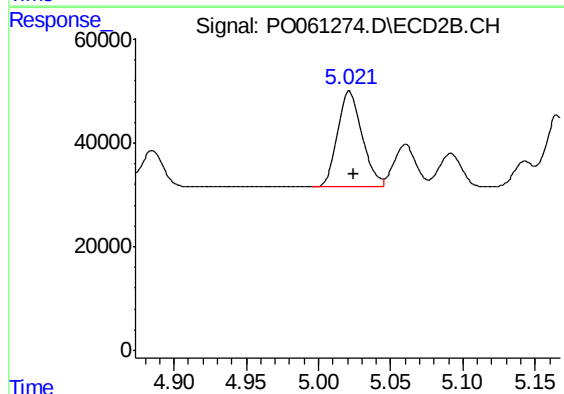


#15 AR-1232-5

R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 221184
Conc: 390.83 ng/ml

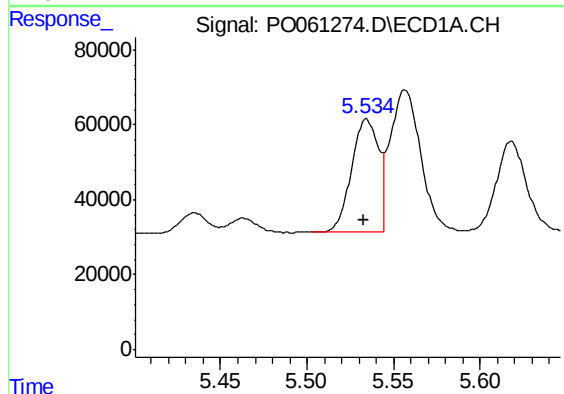


#16 AR-1242-1

R.T.: 5.534 min
Delta R.T.: 0.001 min
Response: 327827
Conc: 274.70 ng/ml

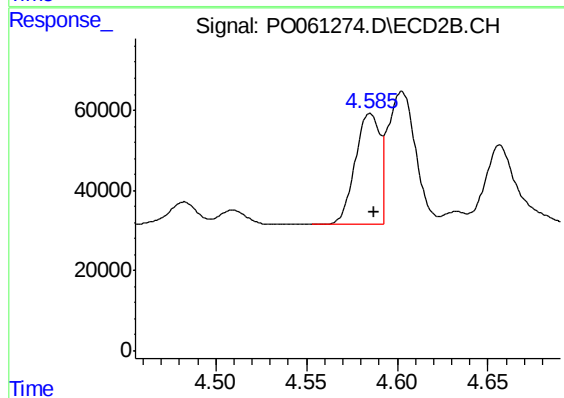

#16 AR-1242-1


R.T.: 4.585 min
Delta R.T.: -0.002 min
Response: 261111
Conc: 286.82 ng/ml



#17 AR-1242-2


R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 470177
Conc: 275.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#17 AR-1242-2

R.T.: 4.603 min
Delta R.T.: -0.002 min
Response: 356223
Conc: 284.56 ng/ml




#18 AR-1242-3

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 294379
Conc: 271.85 ng/ml

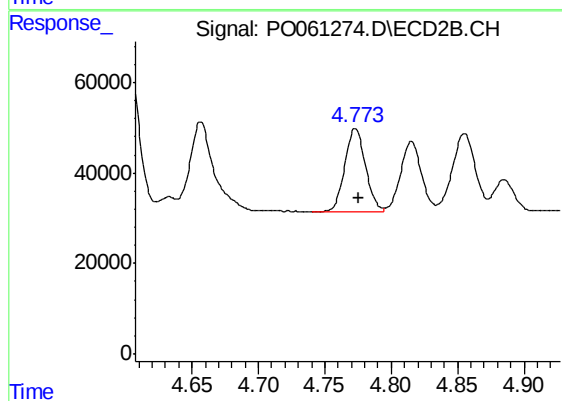

#18 AR-1242-3


R.T.: 4.773 min
Delta R.T.: -0.003 min
Response: 197179
Conc: 275.95 ng/ml



#19 AR-1242-4


R.T.: 5.717 min
Delta R.T.: 0.001 min
Response: 244434
Conc: 276.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

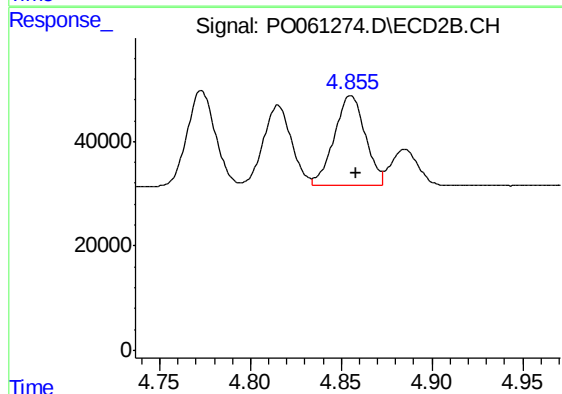


#19 AR-1242-4

R.T.: 4.855 min
Delta R.T.: -0.003 min
Response: 206236
Conc: 283.20 ng/ml




#20 AR-1242-5

R.T.: 6.451 min
Delta R.T.: 0.003 min
Response: 42025
Conc: 37.50 ng/ml

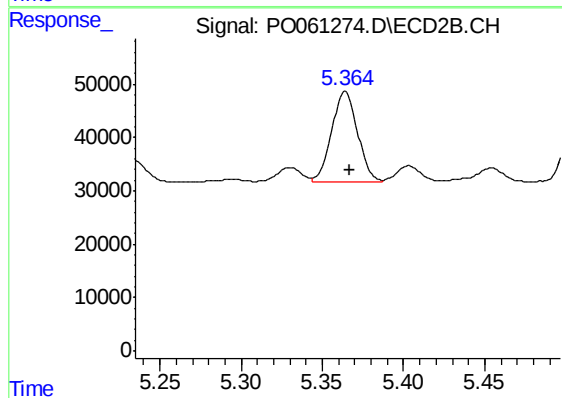

#20 AR-1242-5


R.T.: 5.364 min
Delta R.T.: -0.003 min
Response: 189124
Conc: 191.05 ng/ml

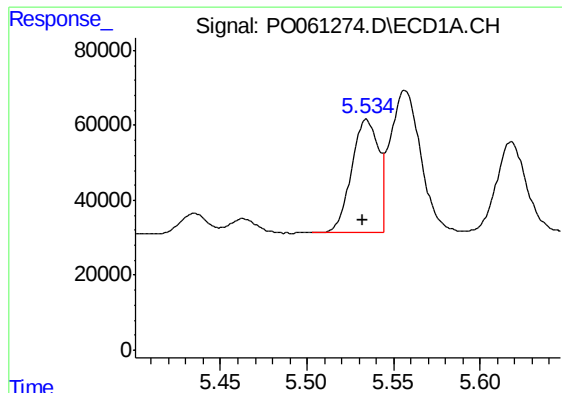

#21 AR-1248-1


R.T.: 5.534 min
Delta R.T.: 0.002 min
Response: 327827
Conc: 356.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

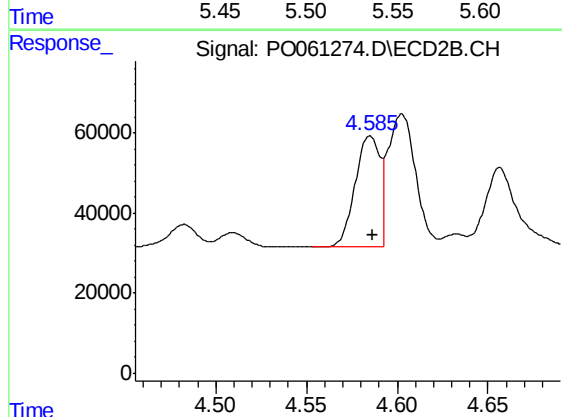


#21 AR-1248-1

R.T.: 4.585 min
Delta R.T.: -0.001 min
Response: 261111
Conc: 368.14 ng/ml

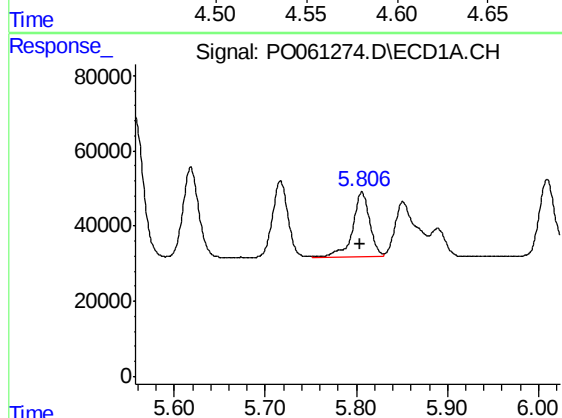


#22 AR-1248-2

R.T.: 5.806 min
Delta R.T.: 0.003 min
Response: 227793
Conc: 170.34 ng/ml

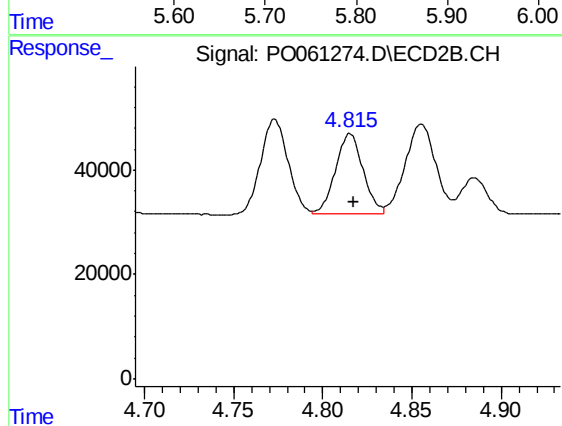

#22 AR-1248-2


R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 167396
Conc: 173.25 ng/ml



#23 AR-1248-3


R.T.: 6.009 min
Delta R.T.: 0.002 min
Response: 259397
Conc: 171.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#23 AR-1248-3

R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 206236
Conc: 204.78 ng/ml




#24 AR-1248-4

R.T.: 6.413 min
Delta R.T.: 0.003 min
Response: 45535
Conc: 24.99 ng/ml

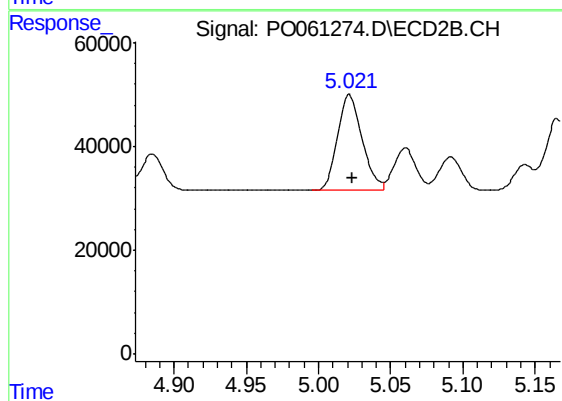

#24 AR-1248-4


R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 221184
Conc: 184.18 ng/ml

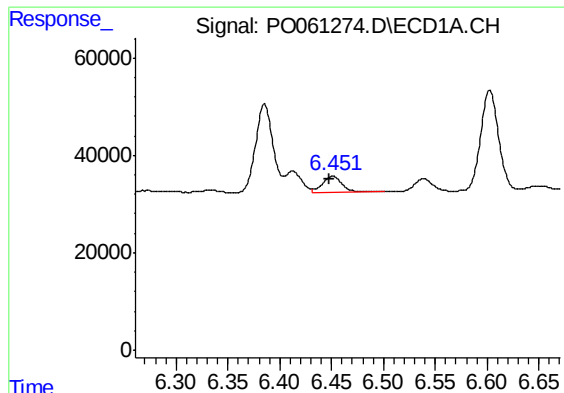

#25 AR-1248-5


R.T.: 6.451 min
Delta R.T.: 0.003 min
Response: 42025
Conc: 24.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

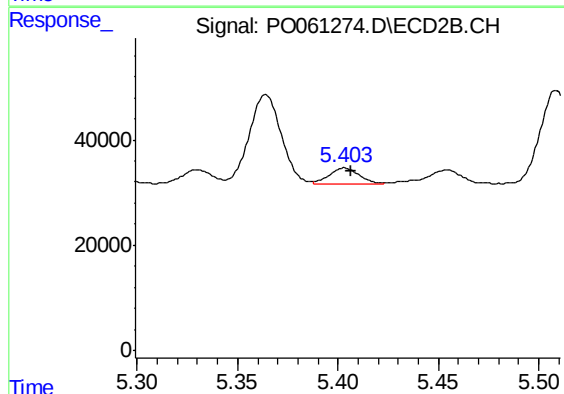


#25 AR-1248-5

R.T.: 5.403 min
Delta R.T.: -0.003 min
Response: 31197
Conc: 24.68 ng/ml

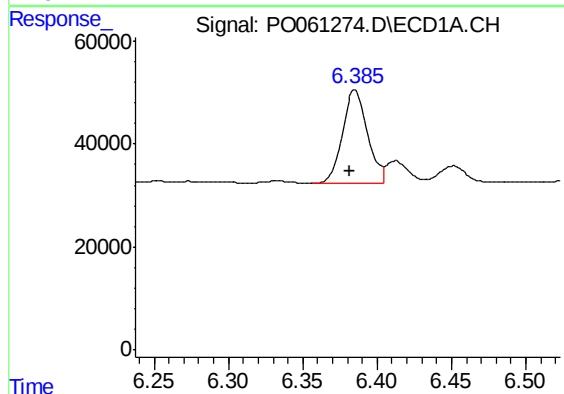


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: 0.003 min
Response: 213130
Conc: 110.62 ng/ml

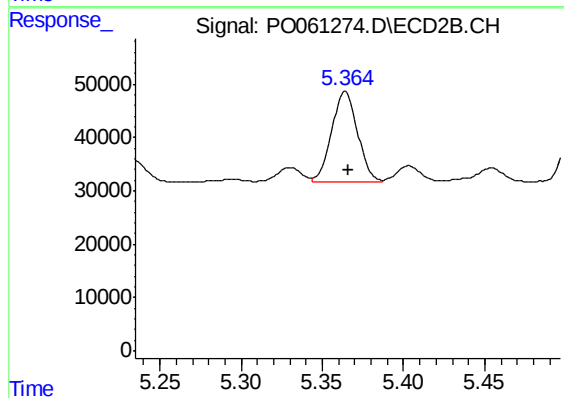

#26 AR-1254-1


R.T.: 5.364 min
Delta R.T.: -0.002 min
Response: 189124
Conc: 91.77 ng/ml



#27 AR-1254-2


R.T.: 6.603 min
Delta R.T.: 0.003 min
Response: 250243
Conc: 79.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

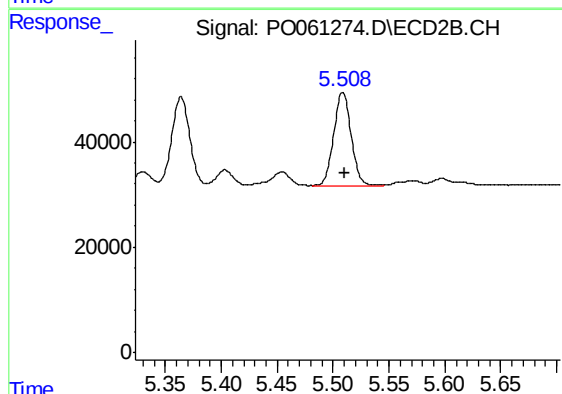


#27 AR-1254-2

R.T.: 5.509 min
Delta R.T.: -0.002 min
Response: 191556
Conc: 101.51 ng/ml

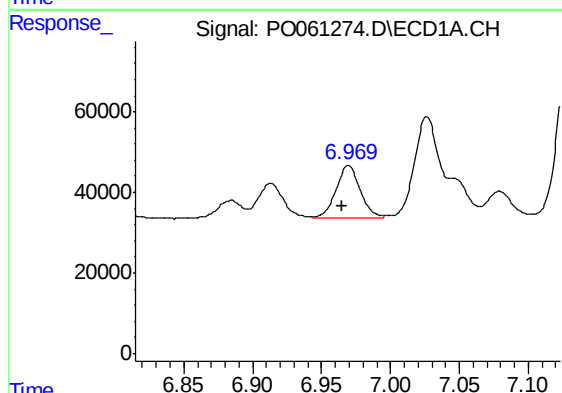


#28 AR-1254-3

R.T.: 6.970 min
Delta R.T.: 0.004 min
Response: 160216
Conc: 45.49 ng/ml

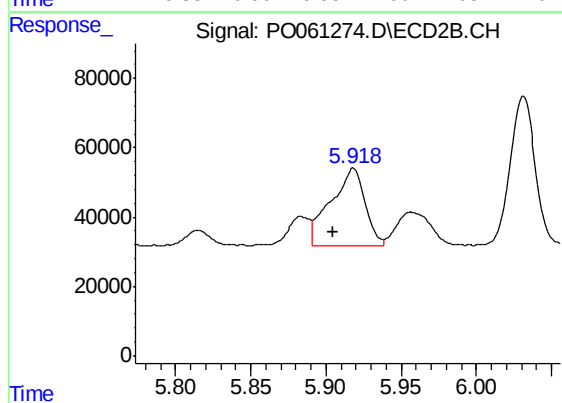

#28 AR-1254-3


R.T.: 5.918 min
Delta R.T.: 0.014 min
Response: 355170
Conc: 111.71 ng/ml

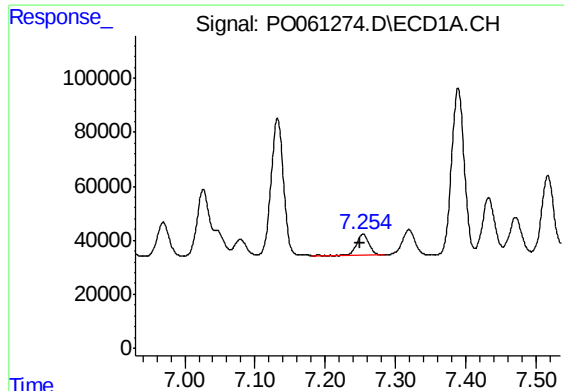

#29 AR-1254-4


R.T.: 7.254 min
Delta R.T.: 0.004 min
Response: 100140
Conc: 36.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

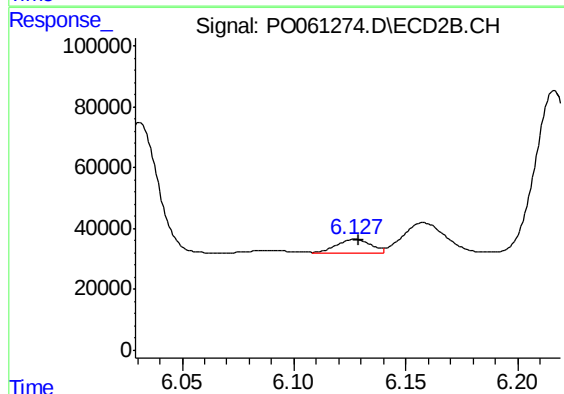


#29 AR-1254-4

R.T.: 6.127 min
Delta R.T.: -0.002 min
Response: 47748
Conc: 22.93 ng/ml

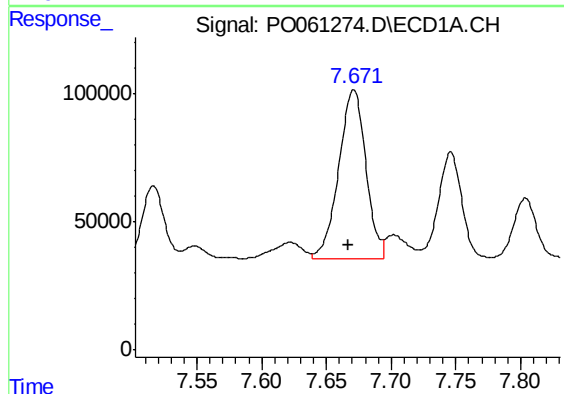


#30 AR-1254-5

R.T.: 7.671 min
Delta R.T.: 0.004 min
Response: 961617
Conc: 326.10 ng/ml

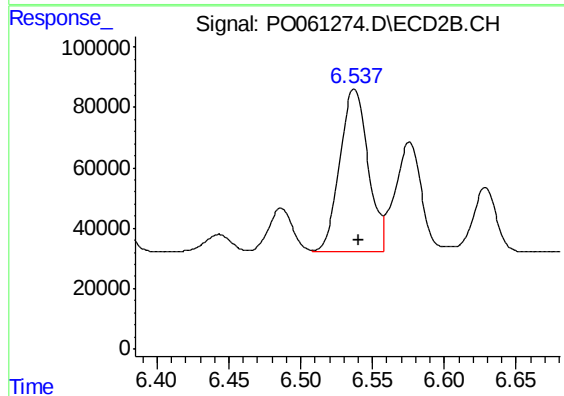

#30 AR-1254-5


R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 743938
Conc: 235.06 ng/ml



#31 AR-1260-1


R.T.: 7.132 min
Delta R.T.: 0.004 min
Response: 631838
Conc: 259.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#31 AR-1260-1

R.T.: 6.031 min
Delta R.T.: -0.003 min
Response: 496255
Conc: 235.93 ng/ml




#32 AR-1260-2

R.T.: 7.389 min
Delta R.T.: 0.004 min
Response: 770955
Conc: 255.00 ng/ml

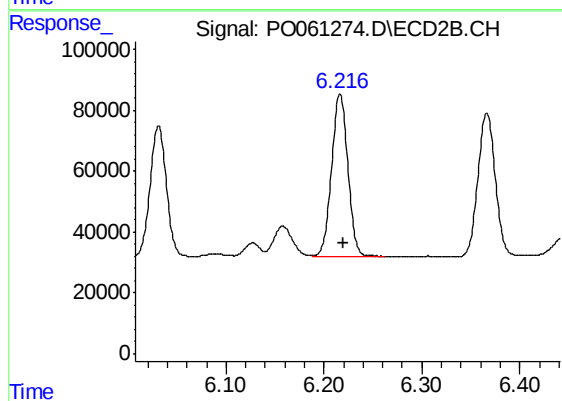

#32 AR-1260-2


R.T.: 6.216 min
Delta R.T.: -0.003 min
Response: 613959
Conc: 238.01 ng/ml



#33 AR-1260-3


R.T.: 7.746 min
Delta R.T.: 0.005 min
Response: 515262
Conc: 215.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#33 AR-1260-3

R.T.: 6.367 min
Delta R.T.: -0.003 min
Response: 579203
Conc: 240.53 ng/ml




#34 AR-1260-4

R.T.: 7.971 min
Delta R.T.: 0.006 min
Response: 647841
Conc: 231.56 ng/ml

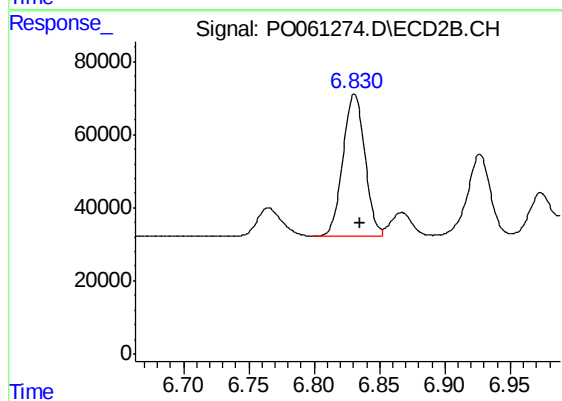

#34 AR-1260-4


R.T.: 6.831 min
Delta R.T.: -0.004 min
Response: 453177
Conc: 211.74 ng/ml

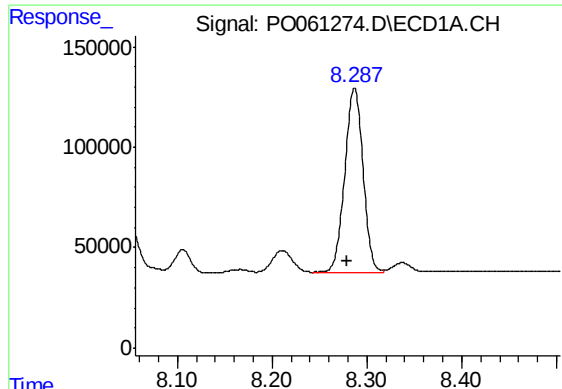

#35 AR-1260-5


R.T.: 8.287 min
Delta R.T.: 0.008 min
Response: 1239270
Conc: 227.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#35 AR-1260-5

R.T.: 7.070 min
Delta R.T.: -0.003 min
Response: 1040865
Conc: 215.39 ng/ml




#36 AR-1262-1

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 515262
Conc: 145.87 ng/ml

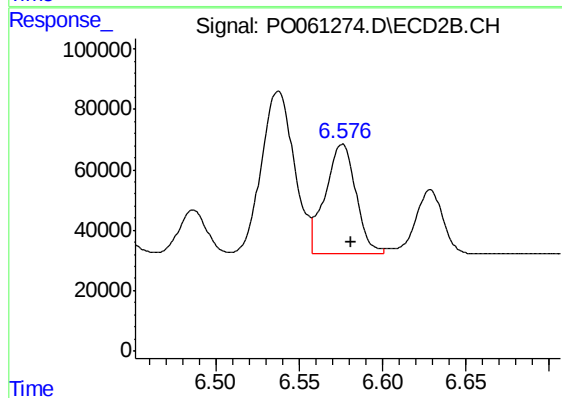

#36 AR-1262-1


R.T.: 6.576 min
Delta R.T.: -0.005 min
Response: 470341
Conc: 157.47 ng/ml



#37 AR-1262-2


R.T.: 8.287 min
Delta R.T.: 0.004 min
Response: 1239270
Conc: 198.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#37 AR-1262-2

R.T.: 7.070 min
Delta R.T.: -0.004 min
Response: 1040865
Conc: 200.19 ng/ml




#38 AR-1262-3

R.T.: 8.605 min
Delta R.T.: 0.018 min
Response: 815082
Conc: 191.29 ng/ml

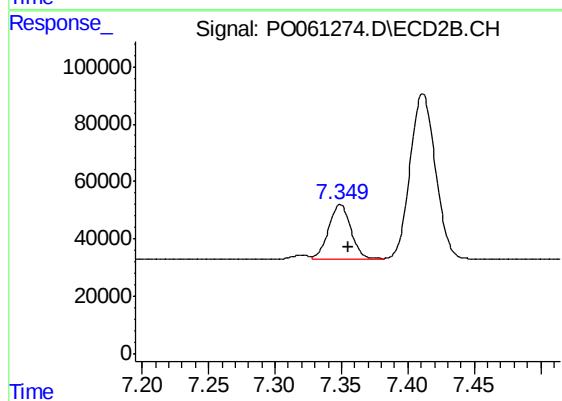

#38 AR-1262-3


R.T.: 7.349 min
Delta R.T.: -0.006 min
Response: 226187
Conc: 106.57 ng/ml

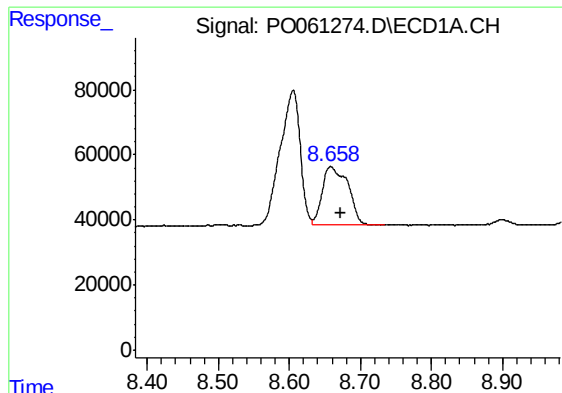

#39 AR-1262-4


R.T.: 8.658 min
Delta R.T.: -0.015 min
Response: 453956
Conc: 139.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

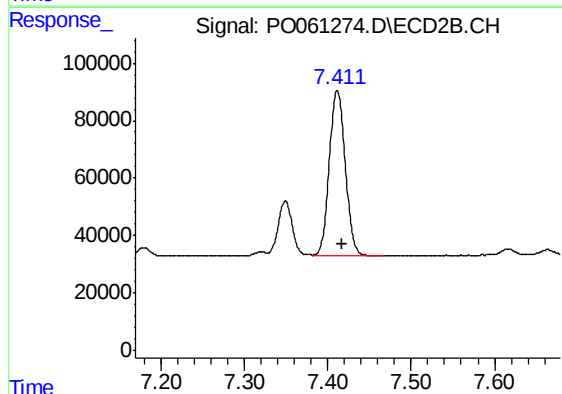


#39 AR-1262-4

R.T.: 7.411 min
Delta R.T.: -0.006 min
Response: 771125
Conc: 201.89 ng/ml

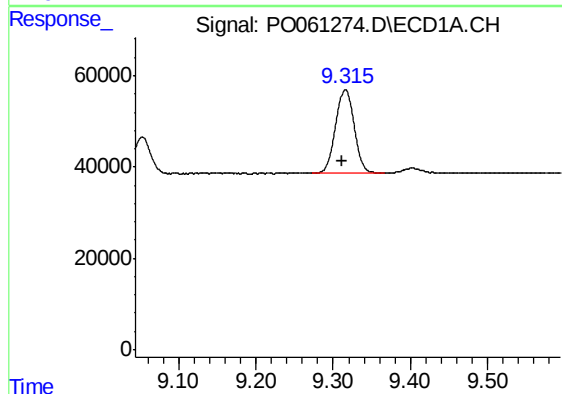


#40 AR-1262-5

R.T.: 9.316 min
Delta R.T.: 0.004 min
Response: 303454
Conc: 149.24 ng/ml

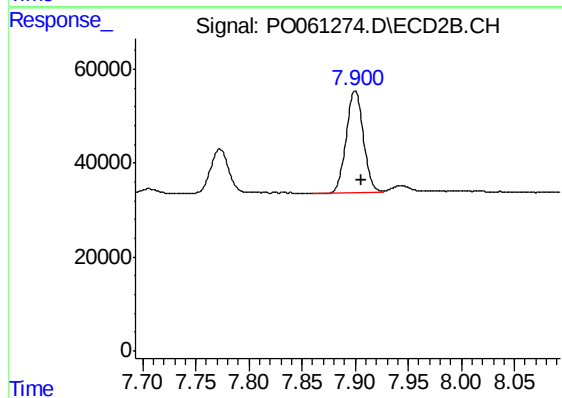

#40 AR-1262-5


R.T.: 7.900 min
Delta R.T.: -0.005 min
Response: 245778
Conc: 146.84 ng/ml

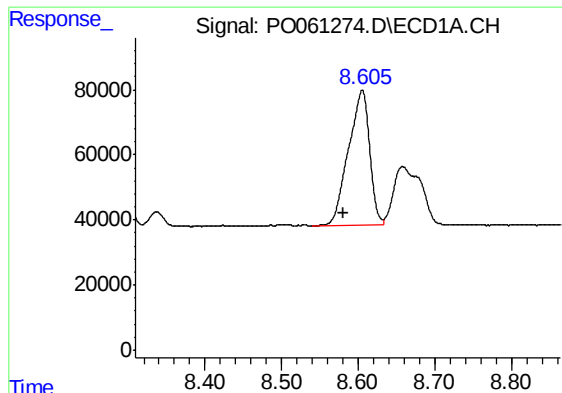

#41 AR-1268-1


R.T.: 8.605 min
Delta R.T.: 0.025 min
Response: 815082
Conc: 110.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

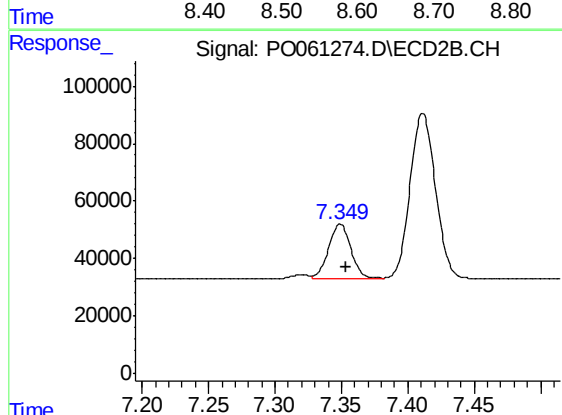


#41 AR-1268-1

R.T.: 7.349 min
Delta R.T.: -0.004 min
Response: 226187
Conc: 38.59 ng/ml

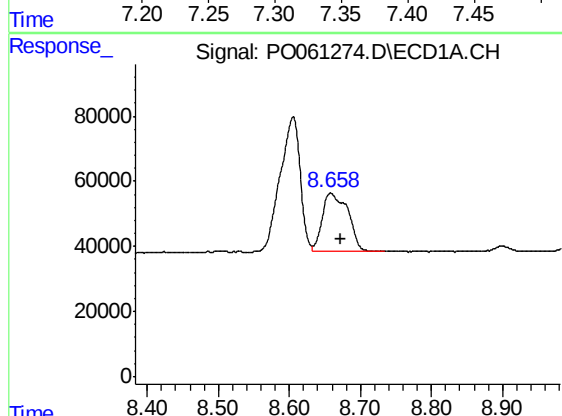


#42 AR-1268-2

R.T.: 8.658 min
Delta R.T.: -0.015 min
Response: 453956
Conc: 67.20 ng/ml

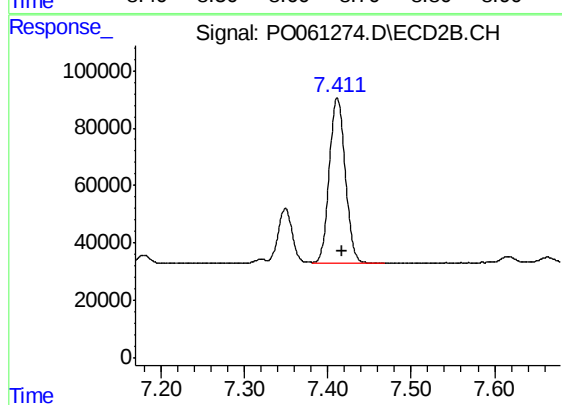

#42 AR-1268-2


R.T.: 7.411 min
Delta R.T.: -0.005 min
Response: 771125
Conc: 144.68 ng/ml



#43 AR-1268-3


R.T.: 8.900 min
Delta R.T.: 0.007 min
Response: 30629
Conc: 5.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD




#43 AR-1268-3

R.T.: 7.616 min
Delta R.T.: -0.005 min
Response: 26952
Conc: 6.08 ng/ml

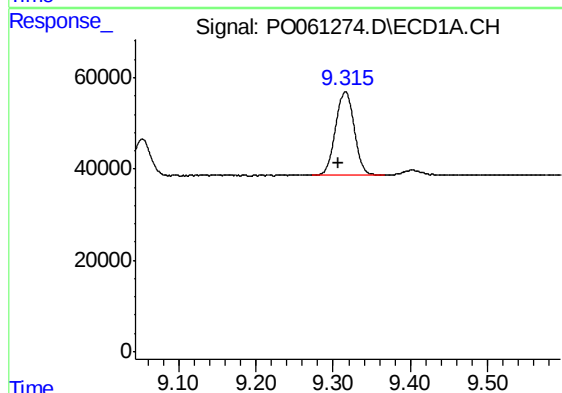


#44 AR-1268-4

R.T.: 9.316 min
Delta R.T.: 0.009 min
Response: 303454
Conc: 131.55 ng/ml

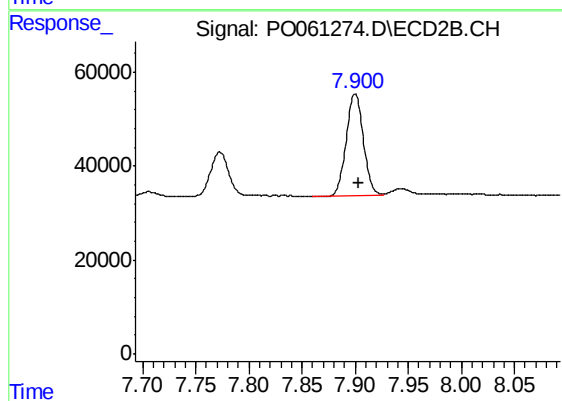

#44 AR-1268-4


R.T.: 7.900 min
Delta R.T.: -0.003 min
Response: 245778
Conc: 128.62 ng/ml

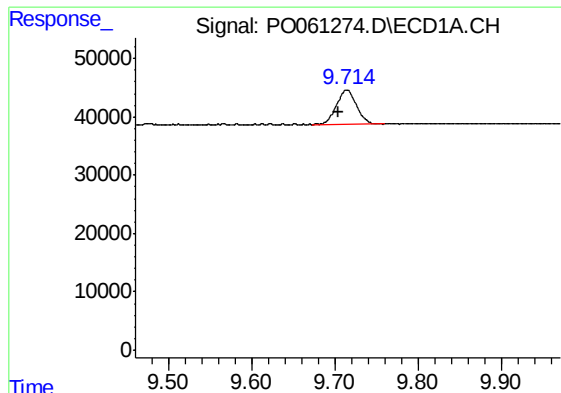

#45 AR-1268-5

R.T.: 9.715 min
Delta R.T.: 0.011 min
Response: 100891
Conc: 6.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-010-ABCDMSD

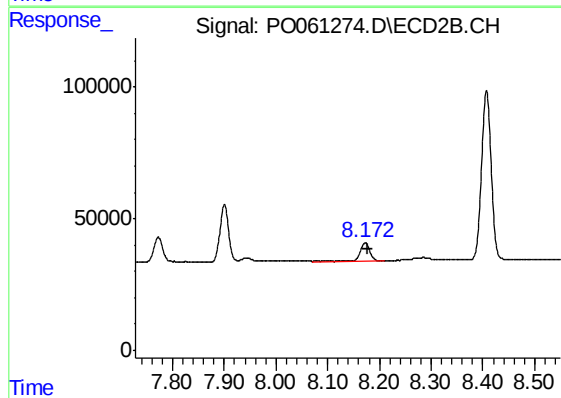

#45 AR-1268-5

R.T.: 8.172 min
Delta R.T.: -0.004 min
Response: 89653
Conc: 7.45 ng/ml