

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
 Data File : P0061295.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 1:59
 Operator : SM/AJ
 Sample : K5009-01 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-06

Manual Integrations
 APPROVED

Ankita
 9/24/2019 3:18:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 04:32:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.532	323787	213550	8.801m	7.648
2) SA Decachlor...	10.039	8.388	1358223	272754	29.561m	7.781m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 1:59
Operator : SM/AJ
Sample : K5009-01 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-06


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 04:32:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

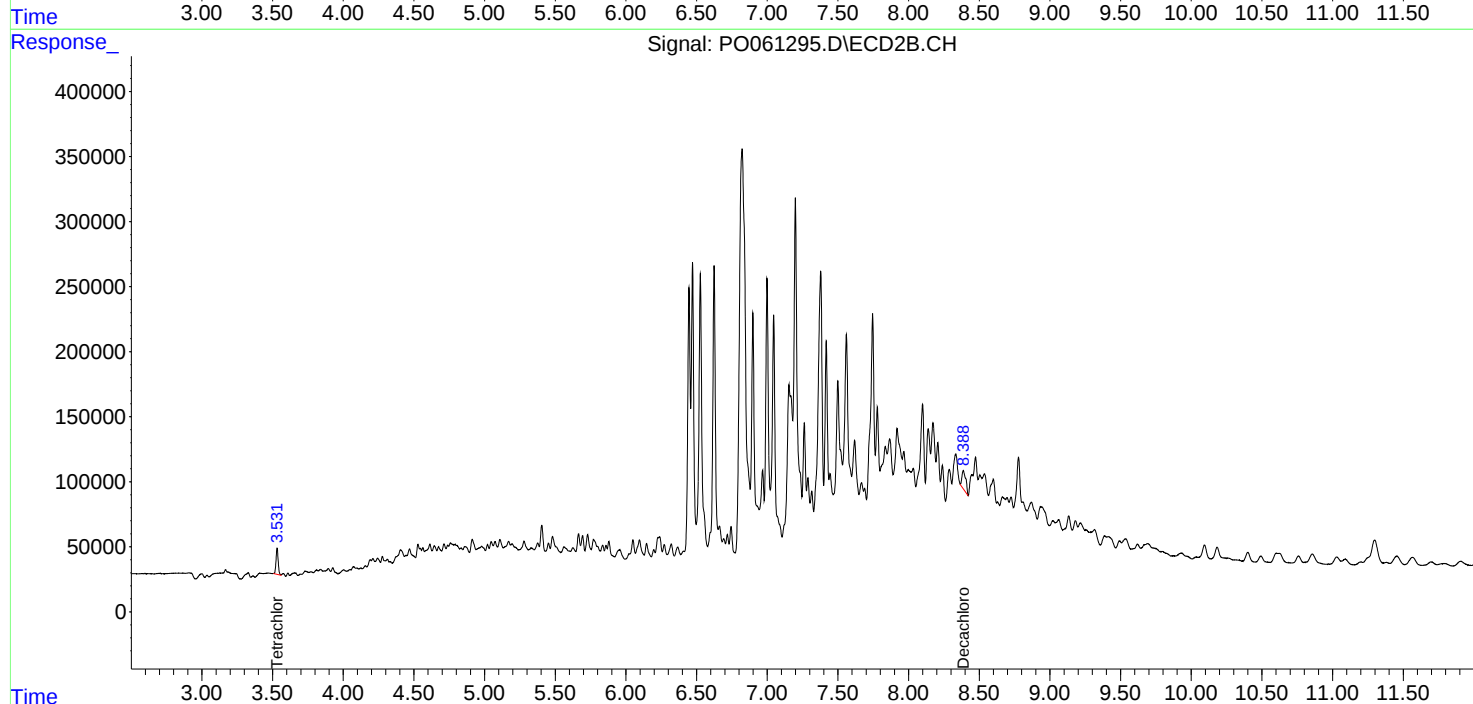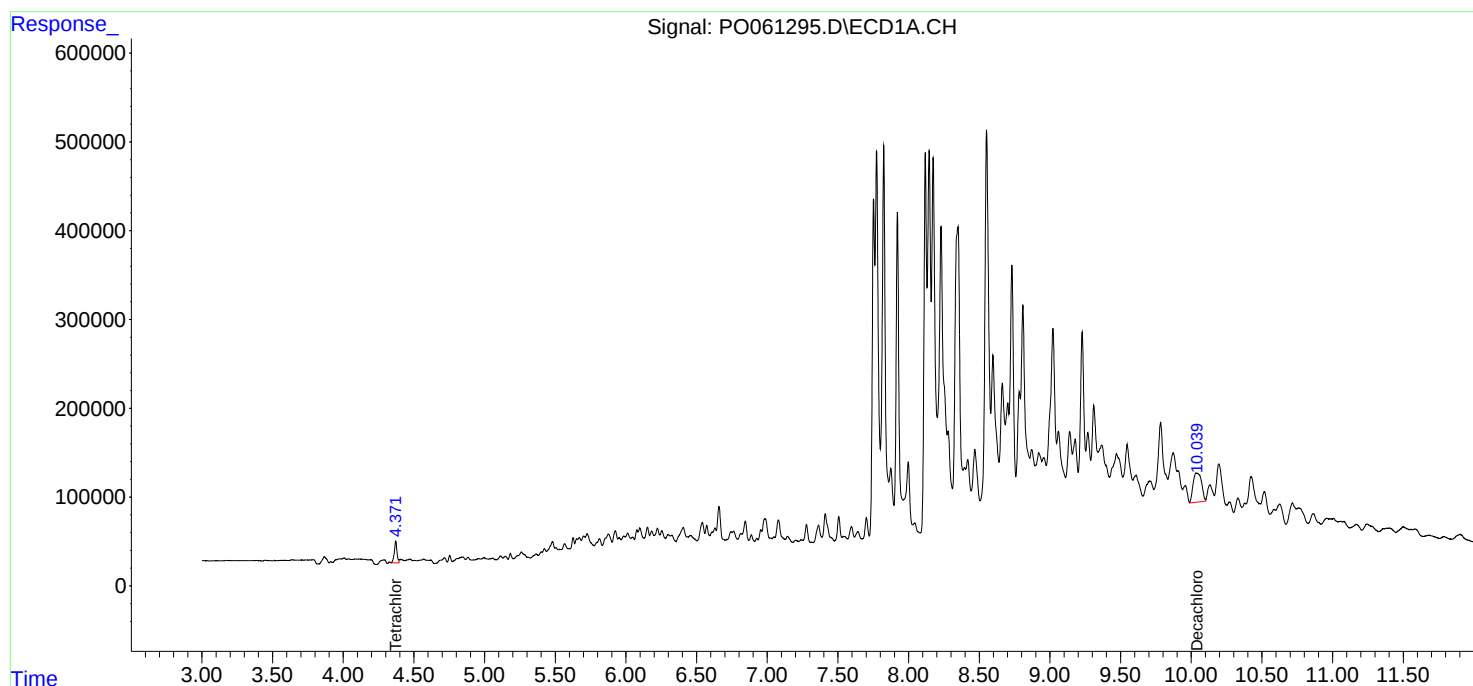

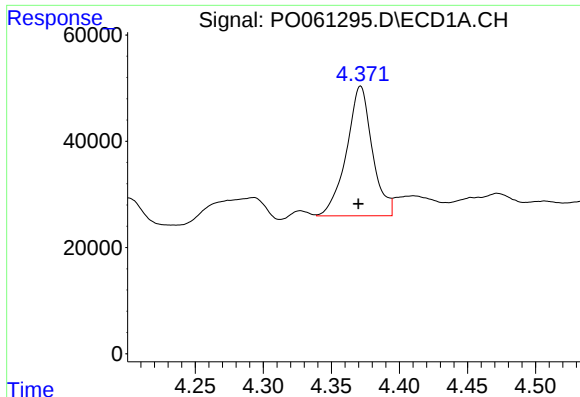


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.001 min
Response: 323787
Conc: 8.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-06


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:20 PM

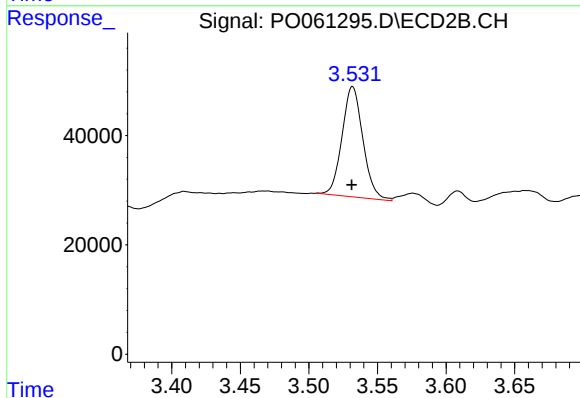


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 213550
Conc: 7.65 ng/ml

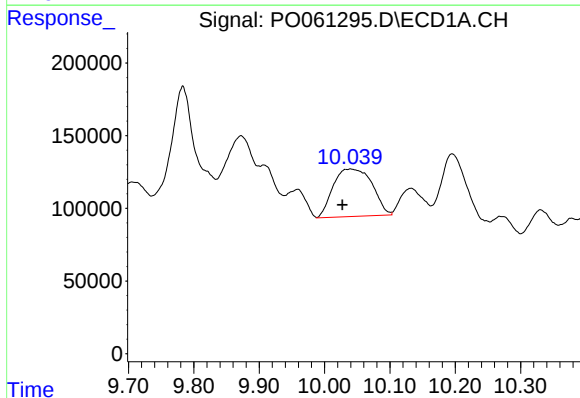

#2 Decachlorobiphenyl

R.T.: 10.039 min
Delta R.T.: 0.012 min
Response: 1358223
Conc: 29.56 ng/ml m

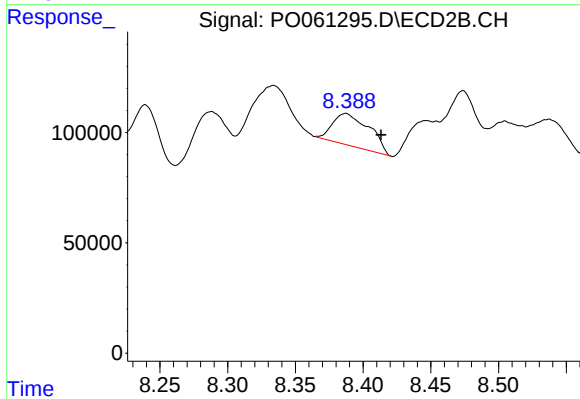

#2 Decachlorobiphenyl

R.T.: 8.388 min
Delta R.T.: -0.025 min
Response: 272754
Conc: 7.78 ng/ml m