

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 2:15
Operator : SM/AJ
Sample : K5009-02 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HA-07

Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 04:32:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.531	404889	206177	11.005m	7.384 #
2) SA Decachlor...	10.029	8.387	1895512	748327	41.255m	21.349m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 2:15
Operator : SM/AJ
Sample : K5009-02 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-07


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 04:32:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

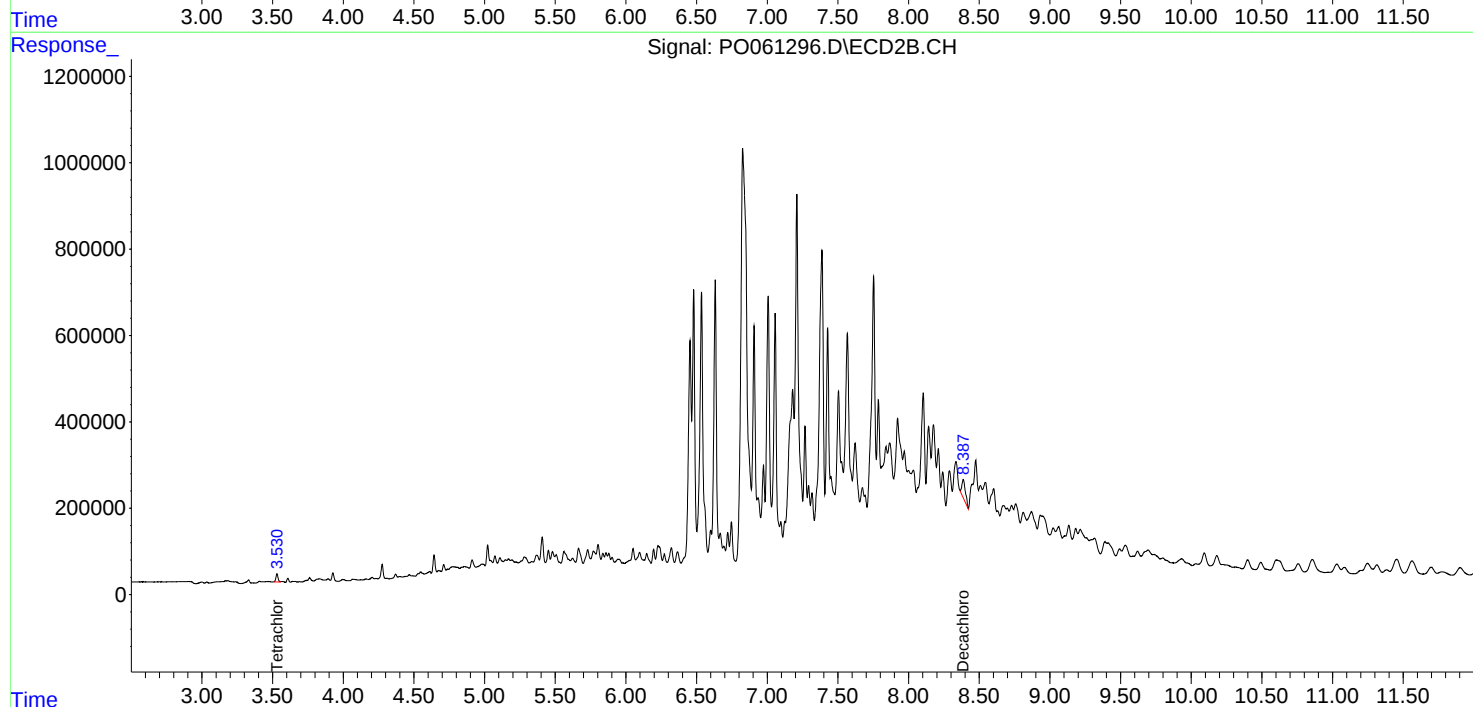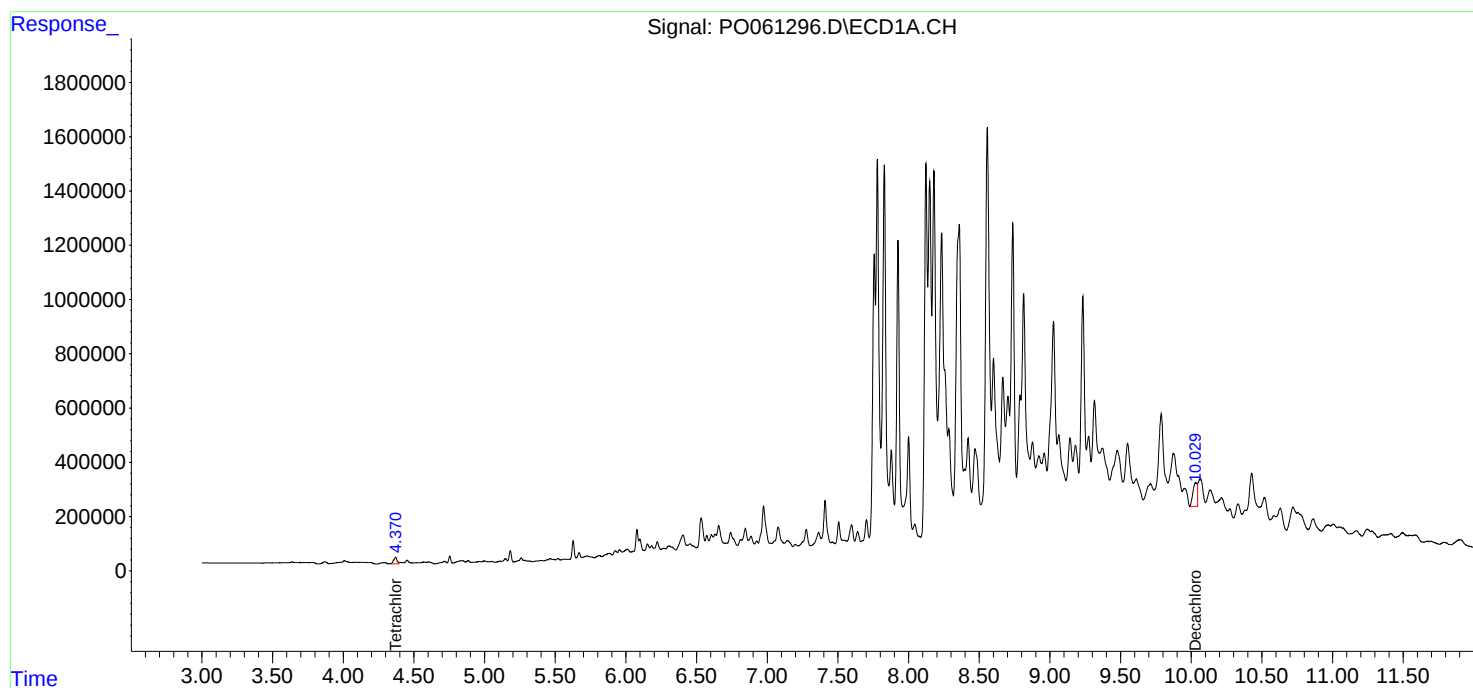

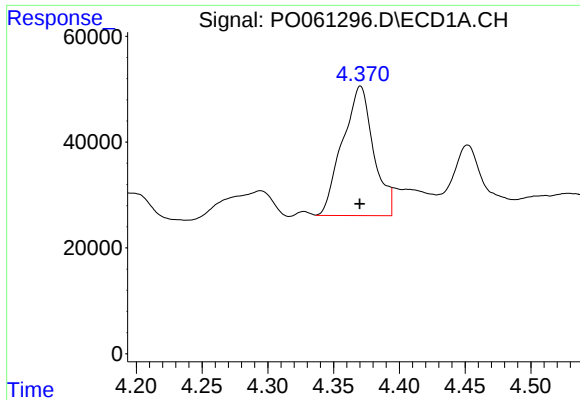


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 404889
Conc: 11.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-07


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:22 PM

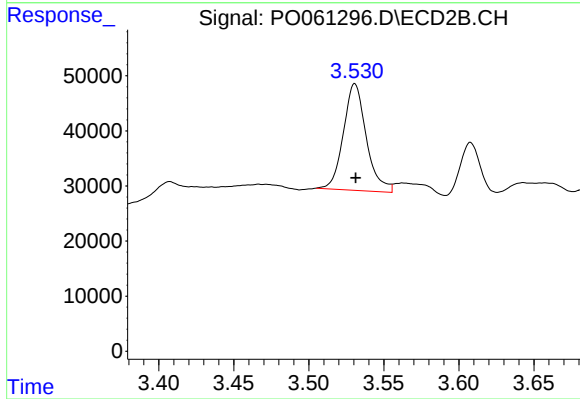


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 206177
Conc: 7.38 ng/ml

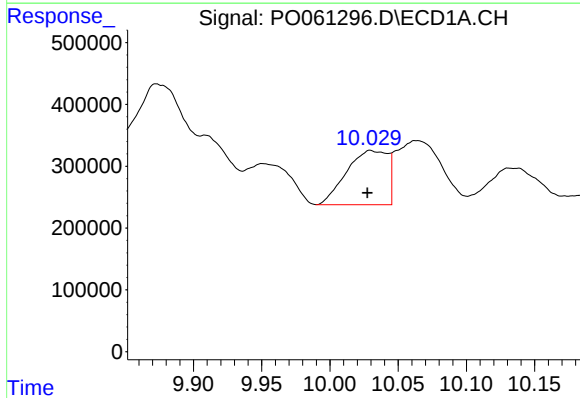

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: 0.001 min
Response: 1895512
Conc: 41.26 ng/ml m

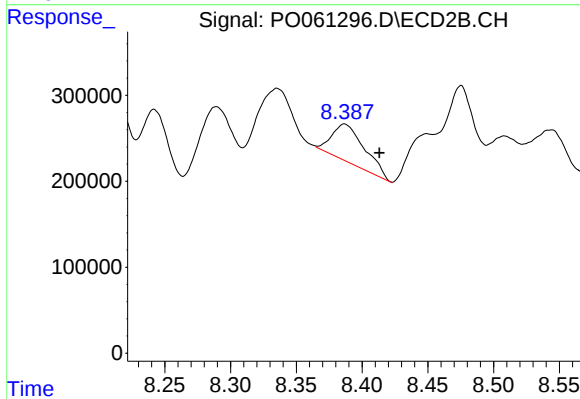

#2 Decachlorobiphenyl

R.T.: 8.387 min
Delta R.T.: -0.026 min
Response: 748327
Conc: 21.35 ng/ml m