

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
 Data File : P0061297.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 2:31
 Operator : SM/AJ
 Sample : K5009-03 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-08

Manual Integrations
 APPROVED

Ankita
 9/24/2019 3:18:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 04:32:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.531	192896	167131	5.243m	5.986
2) SA Decachlor...	10.039	8.405	143263	244159	3.118	6.966m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061297.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 2:31
Operator : SM/AJ
Sample : K5009-03 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-08


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 04:32:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

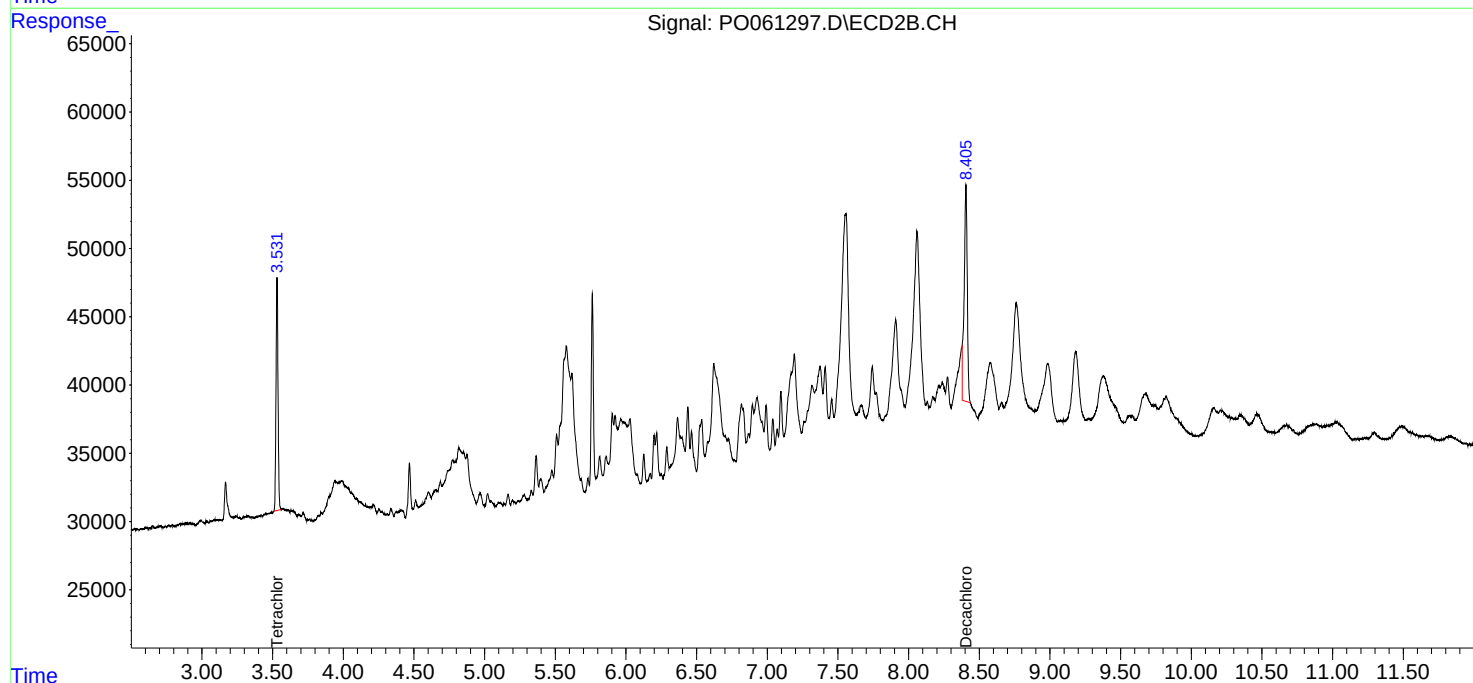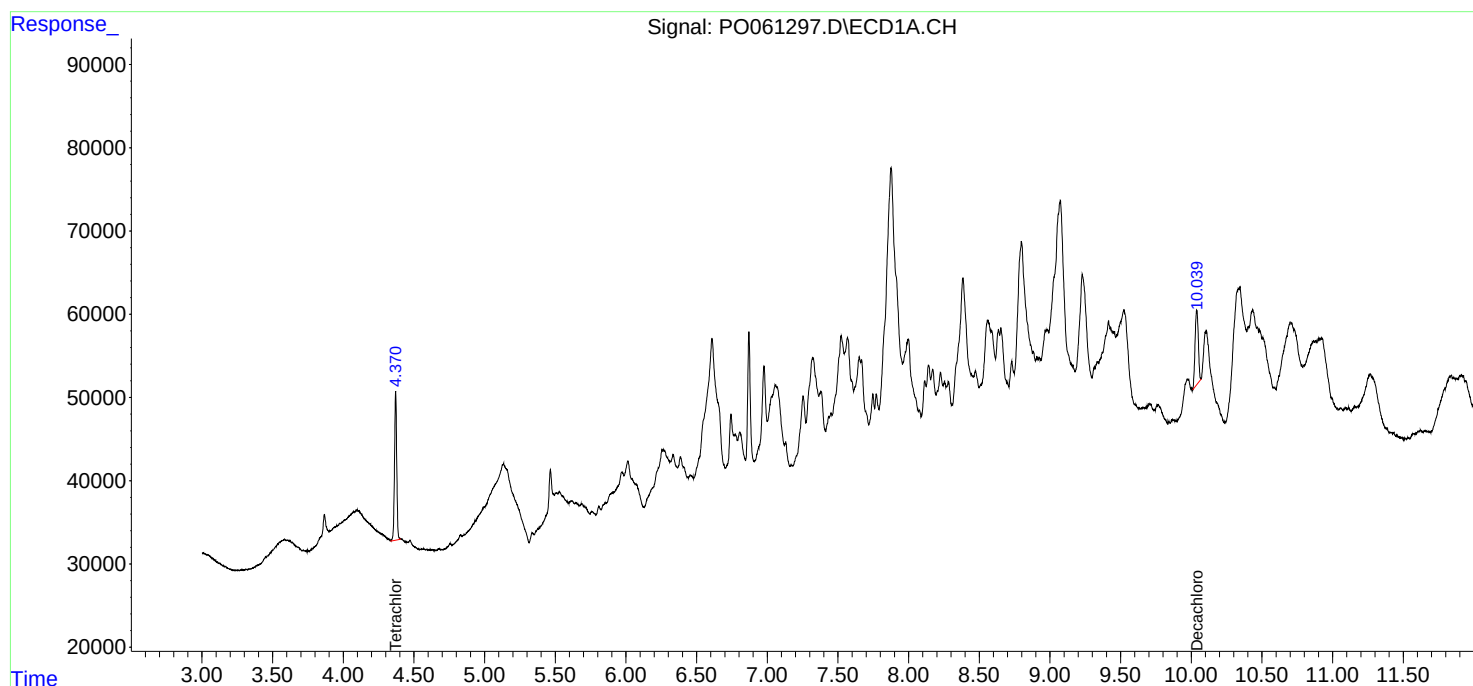

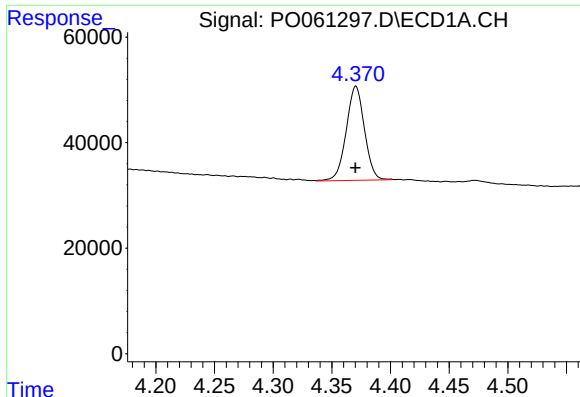


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 192896
Conc: 5.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-08


Manual Integrations
APPROVED

Ankita
9/24/2019 3:18:24 PM

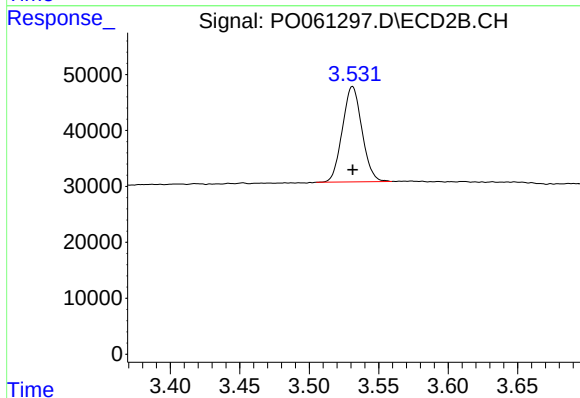


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 167131
Conc: 5.99 ng/ml

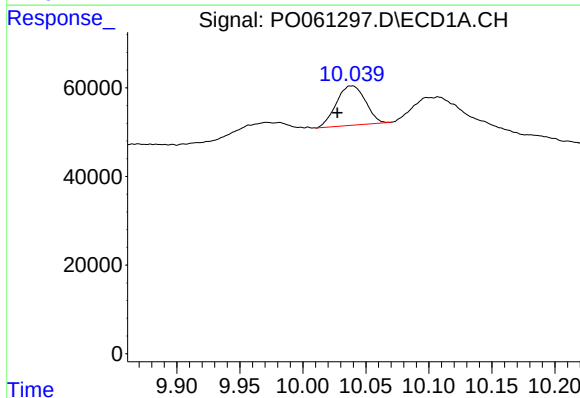

#2 Decachlorobiphenyl

R.T.: 10.039 min
Delta R.T.: 0.011 min
Response: 143263
Conc: 3.12 ng/ml

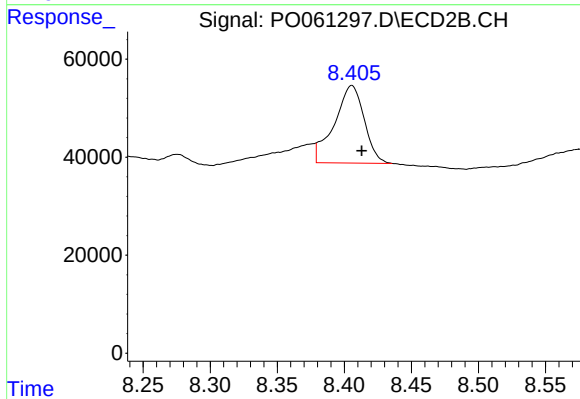

#2 Decachlorobiphenyl

R.T.: 8.405 min
Delta R.T.: -0.008 min
Response: 244159
Conc: 6.97 ng/ml m