

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
 Data File : P0061302.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 3:53
 Operator : SM/AJ
 Sample : K5009-08 5X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 04:35:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.531	207887	167356	5.651	5.994
2) SA Decachlor...	10.039	8.407	178662	163413	3.889	4.662

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092319\
Data File : P0061302.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 3:53
Operator : SM/AJ
Sample : K5009-08 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HA-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 04:35:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

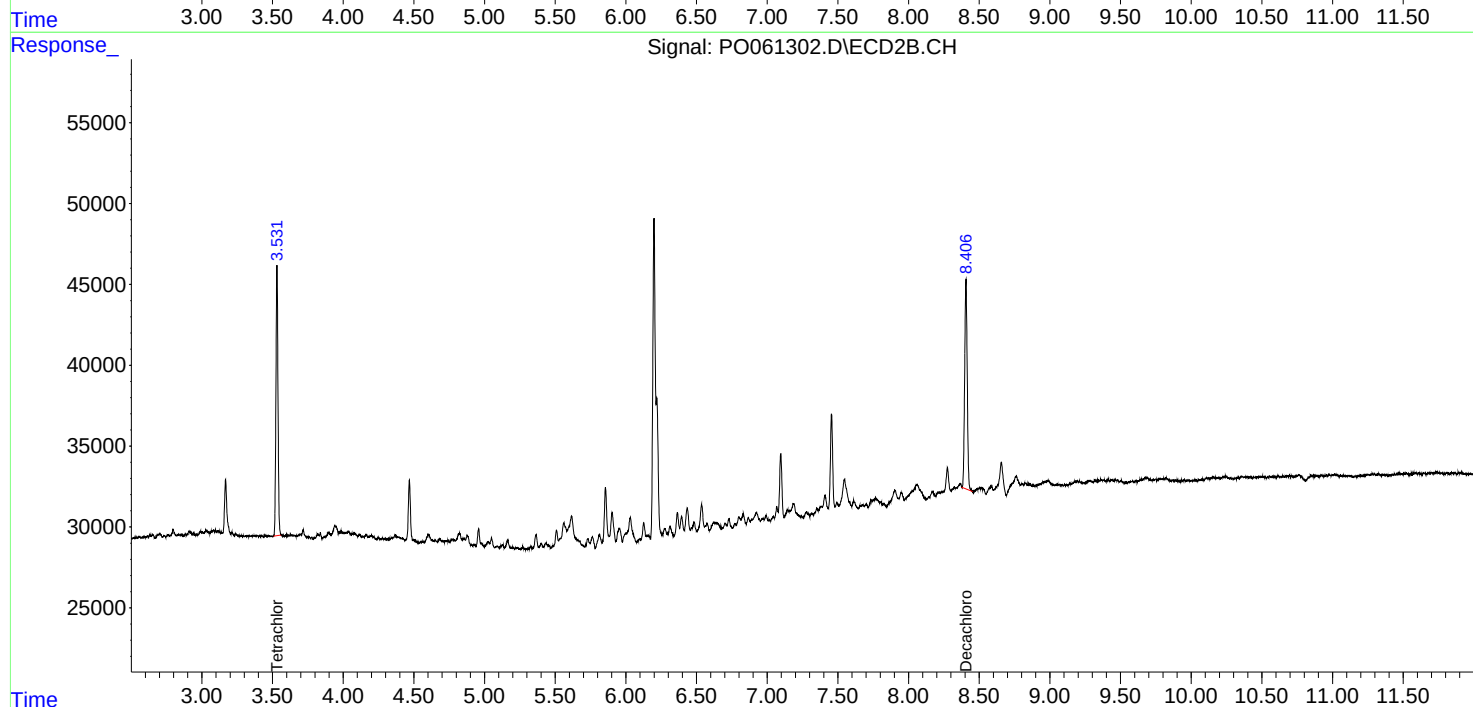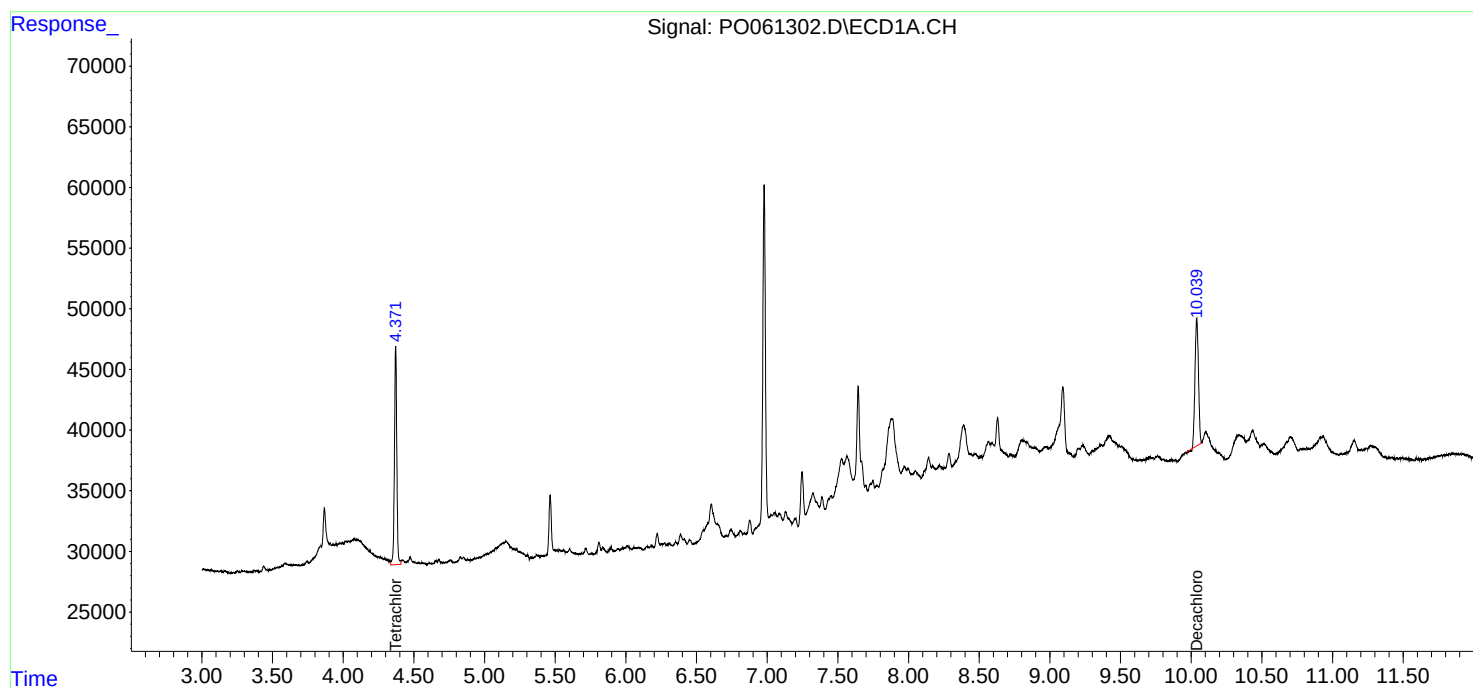


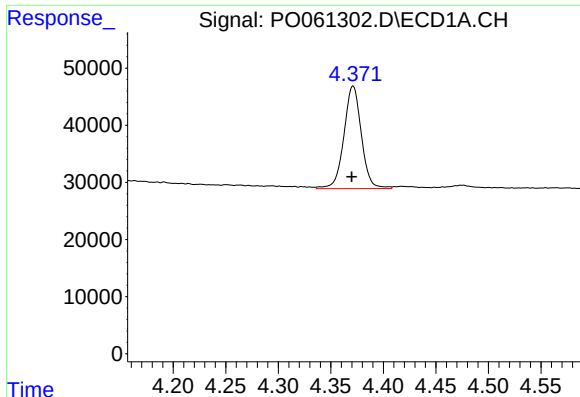

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.001 min
Response: 207887
Conc: 5.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-23

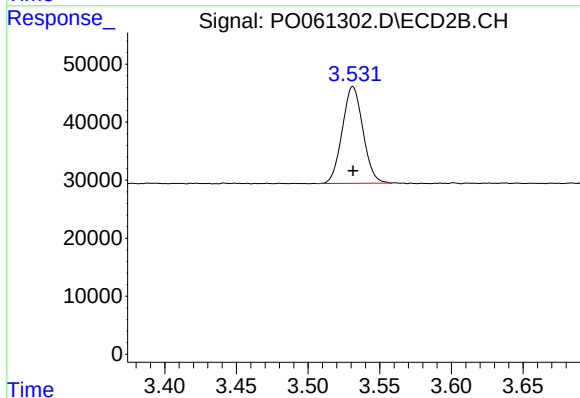


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 167356
Conc: 5.99 ng/ml

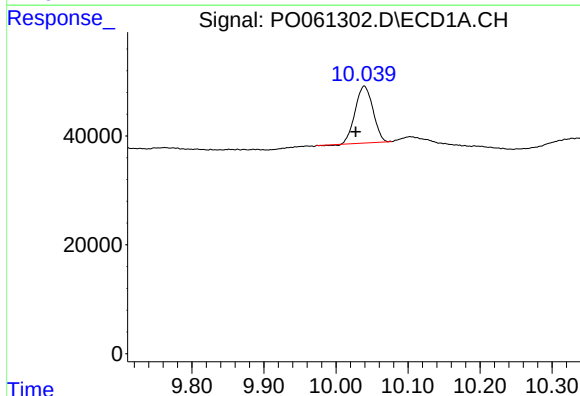

#2 Decachlorobiphenyl

R.T.: 10.039 min
Delta R.T.: 0.012 min
Response: 178662
Conc: 3.89 ng/ml

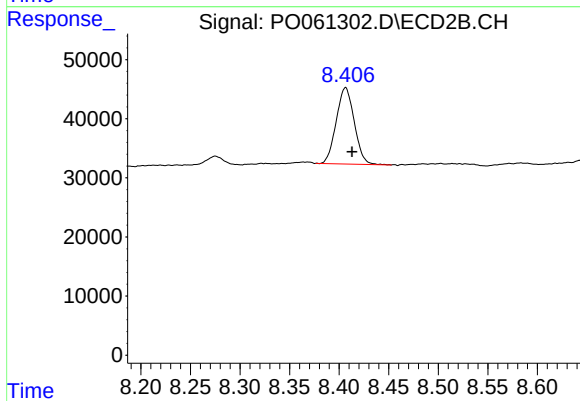

#2 Decachlorobiphenyl

R.T.: 8.407 min
Delta R.T.: -0.006 min
Response: 163413
Conc: 4.66 ng/ml