

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092320\
 Data File : P0071561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Sep 2020 9:47
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 10:26:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.339	3.522	1906982	940446	22.222	22.834
2)	SA Decachlor...	9.953	8.700	2560511	1354388	22.287	22.282

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092320\
Data File : PO071561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Sep 2020 9:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 10:26:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

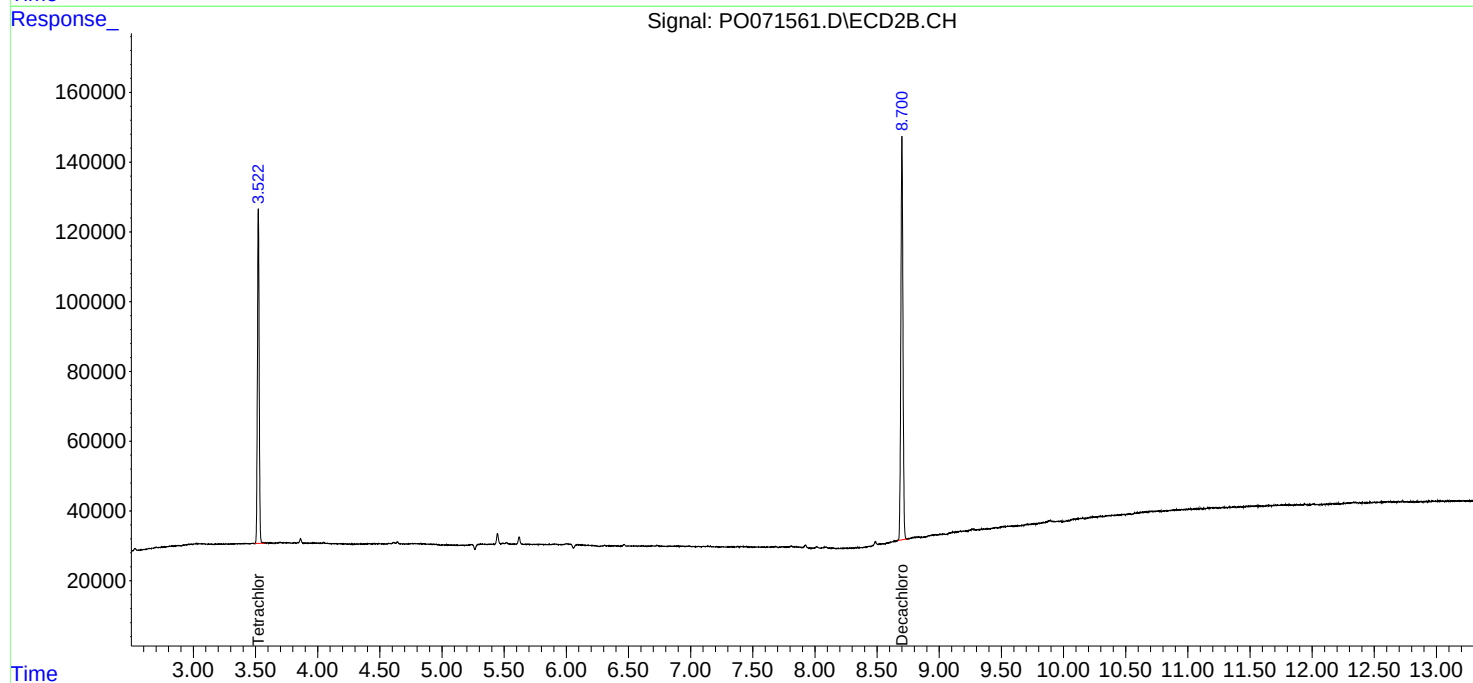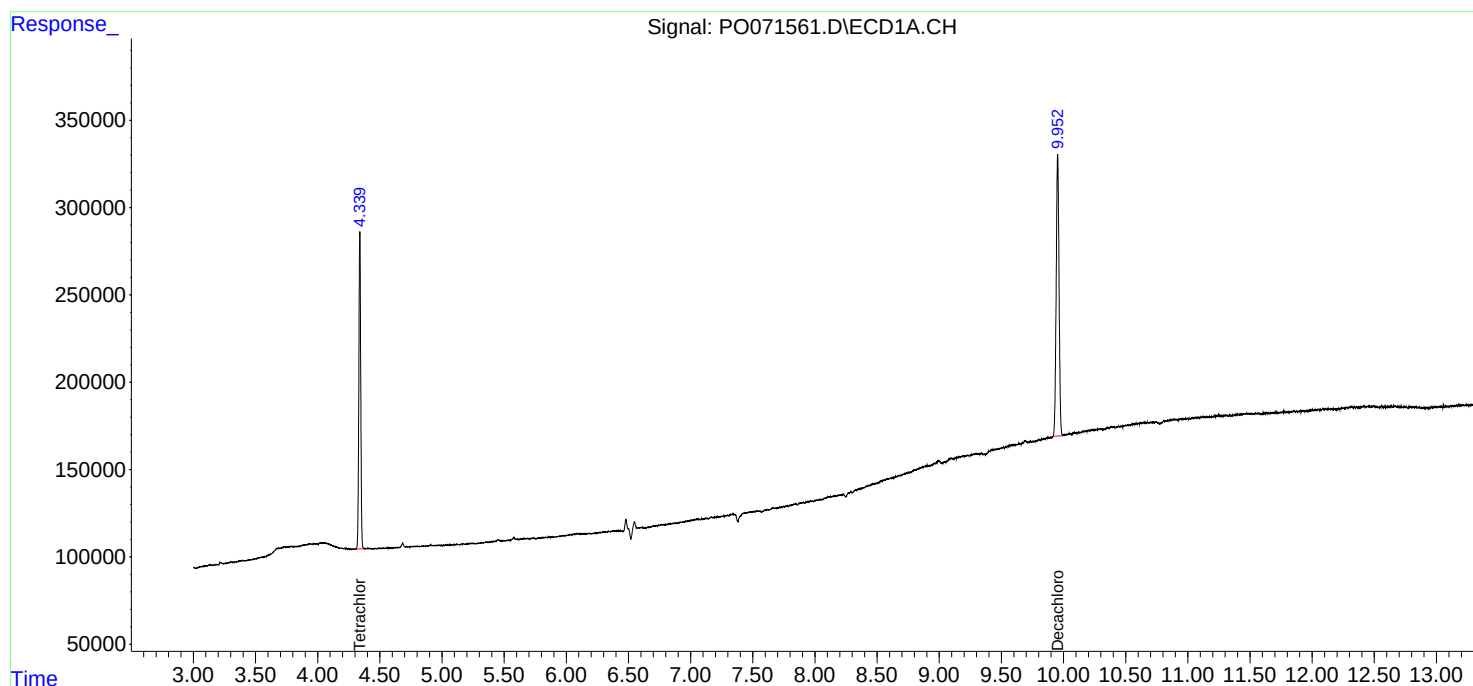


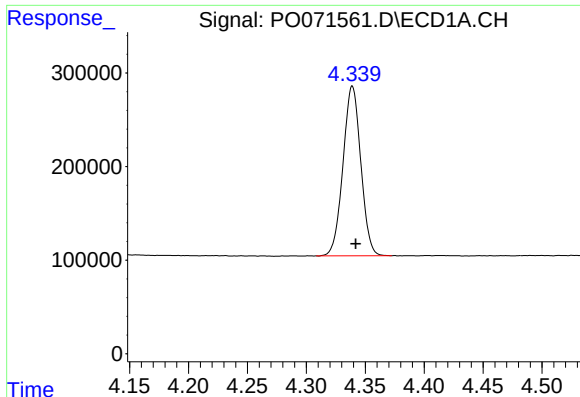

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.003 min
Response: 1906982
Conc: 22.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

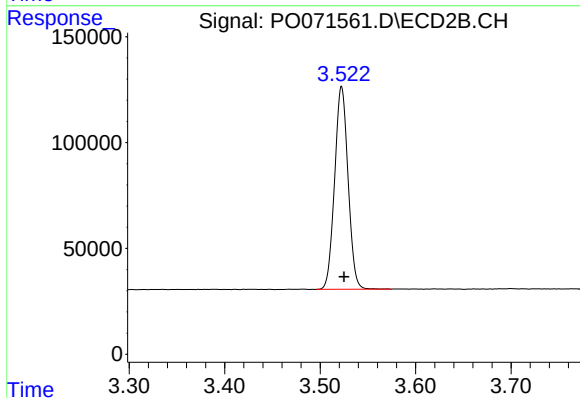


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.002 min
Response: 940446
Conc: 22.83 ng/ml

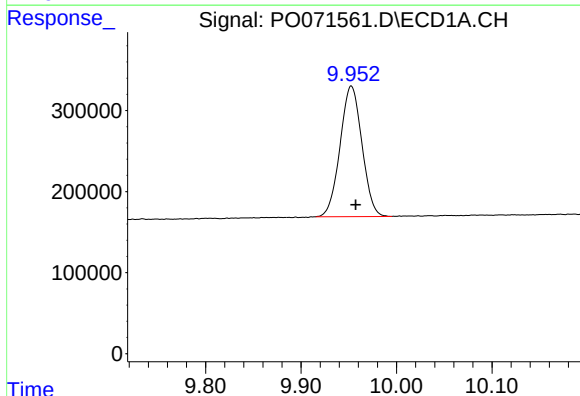

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.005 min
Response: 2560511
Conc: 22.29 ng/ml

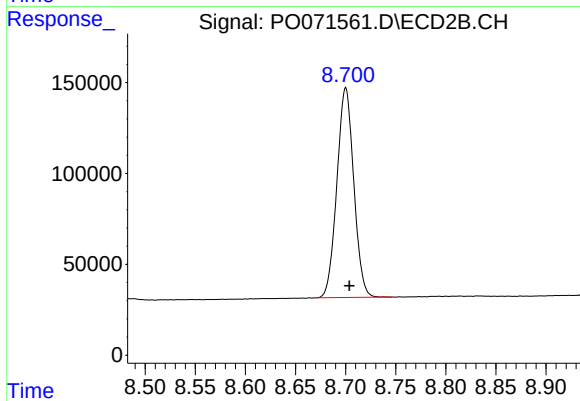

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.004 min
Response: 1354388
Conc: 22.28 ng/ml