

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092320\
 Data File : P0071583.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Sep 2020 17:02
 Operator : DD\AJ
 Sample : L4093-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KTS-GW-01-30

Manual Integrations
 APPROVED

Ankita
 9/24/2020 3:25:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 18:50:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.525	1286199	663704	14.988m	16.115
2) SA Decachlor...	9.952	8.701	886963	470826	7.720	7.746

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092320\
Data File : P0071583.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Sep 2020 17:02
Operator : DD\AJ
Sample : L4093-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KTS-GW-01-30


Manual Integrations
APPROVED

Ankita
9/24/2020 3:25:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 18:50:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

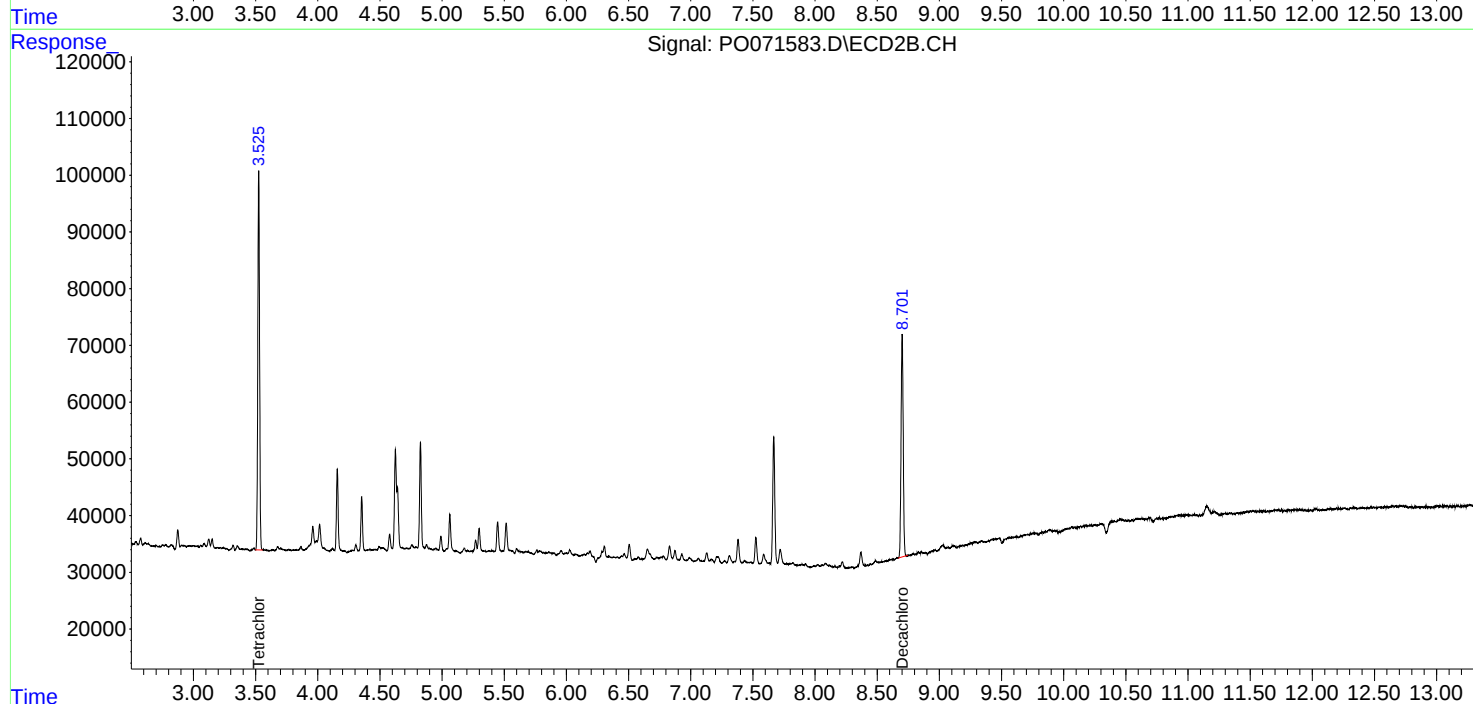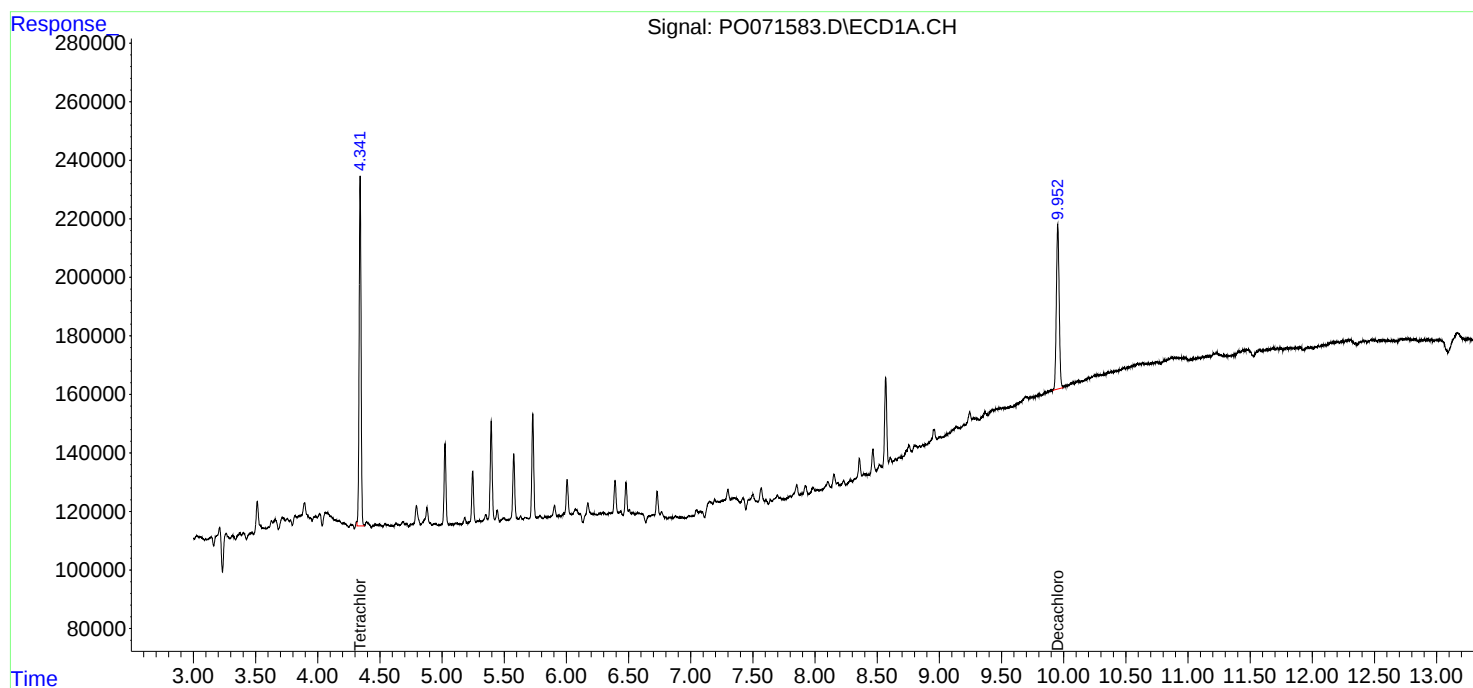

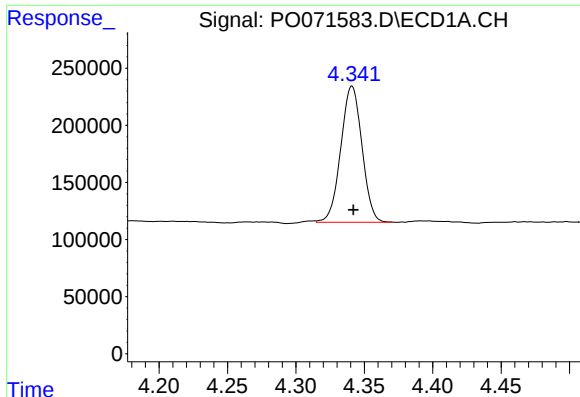


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: -0.001 min
Response: 1286199
Conc: 14.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KTS-GW-01-30


Manual Integrations
APPROVED

Ankita
9/24/2020 3:25:28 PM

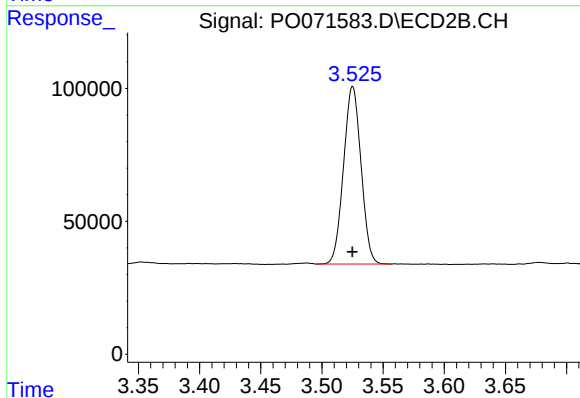


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 663704
Conc: 16.11 ng/ml

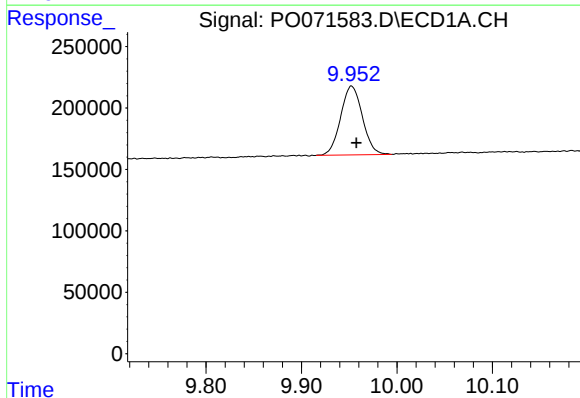

#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: -0.005 min
Response: 886963
Conc: 7.72 ng/ml

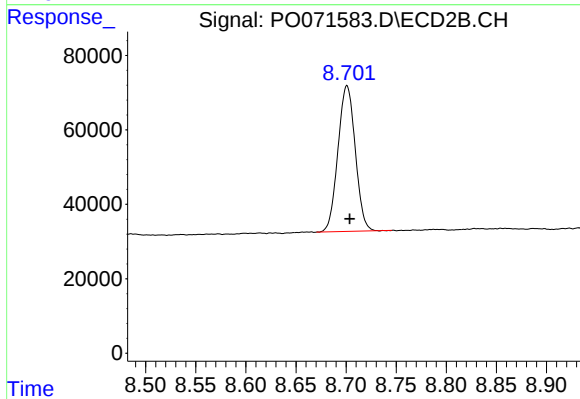

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.003 min
Response: 470826
Conc: 7.75 ng/ml