

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092320\
 Data File : P0071588.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Sep 2020 18:27
 Operator : DD\AJ
 Sample : L4107-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40AA-MH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 18:52:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.340	3.524	1252638	648263	14.597	15.740
2)	SA Decachlor...	9.953	8.700	1862307	952161	16.210	15.664

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092320\
Data File : P0071588.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Sep 2020 18:27
Operator : DD\AJ
Sample : L4107-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
40AA-MH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 18:52:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

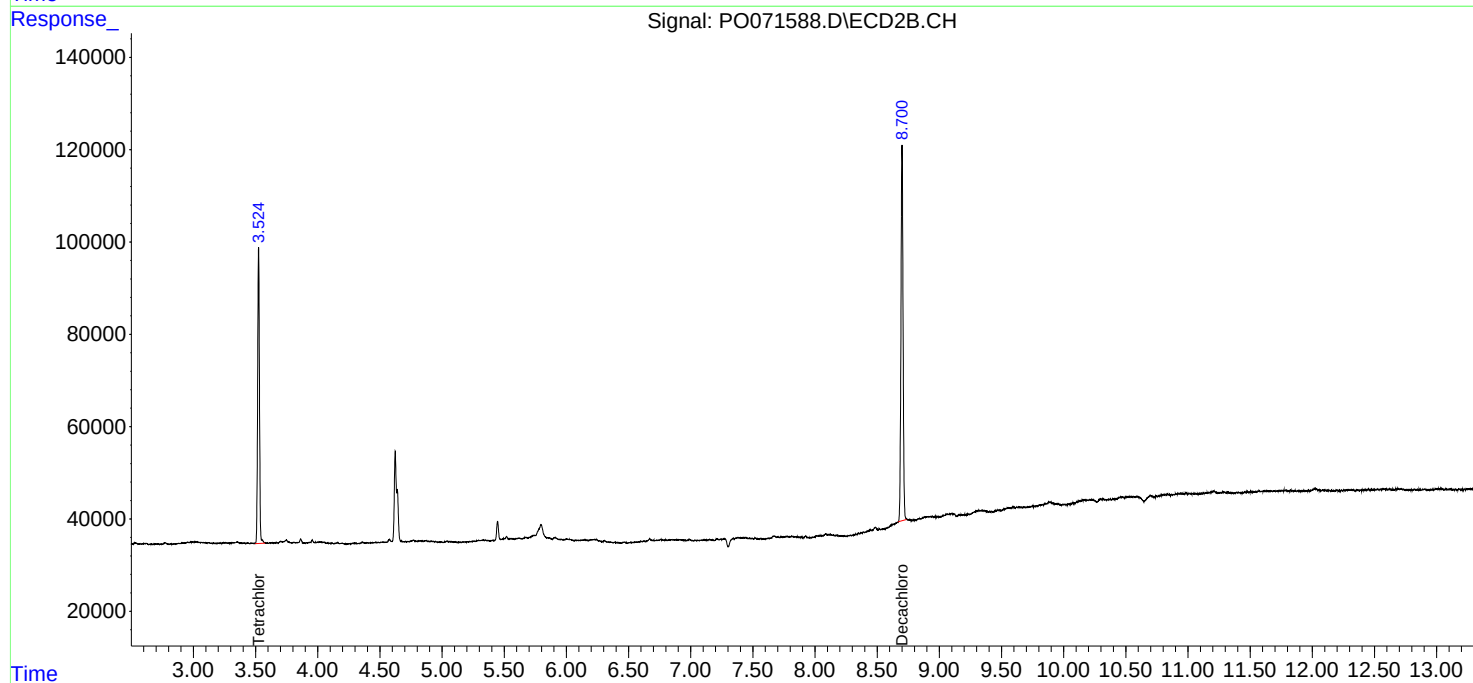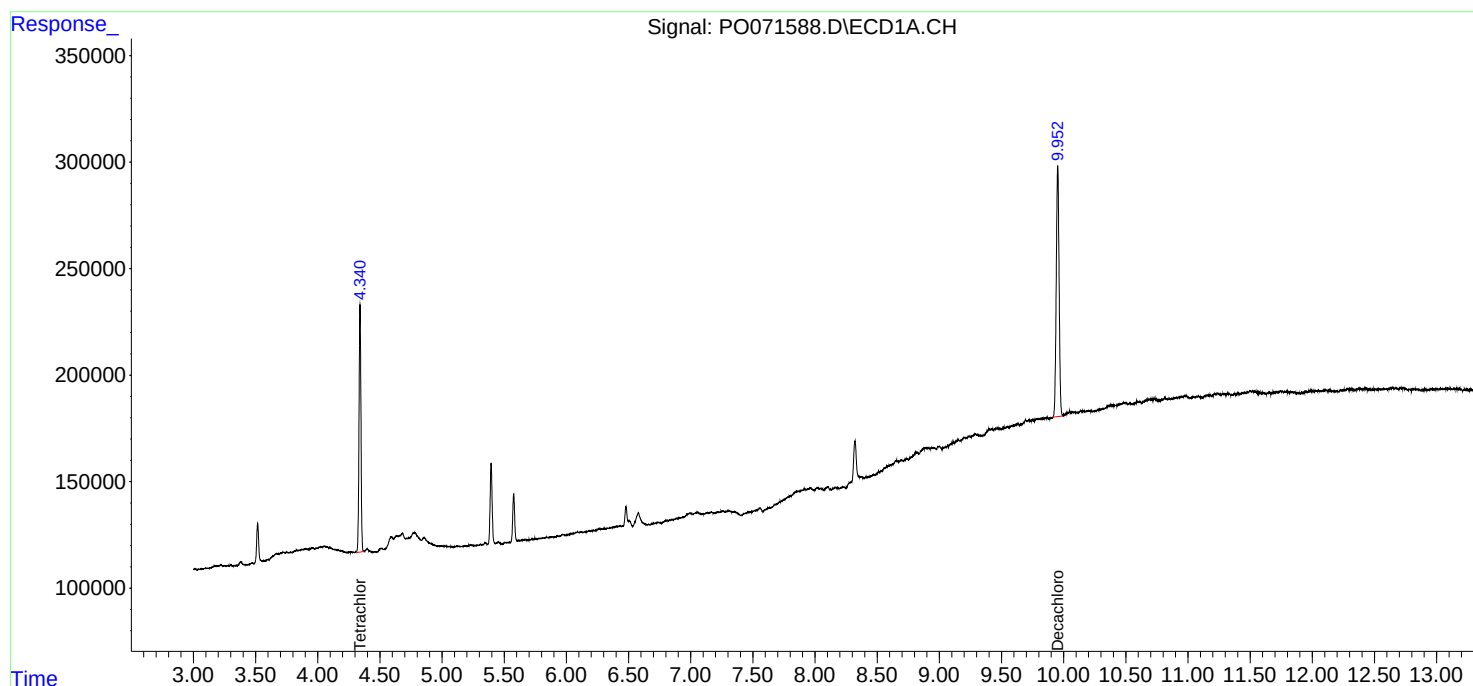


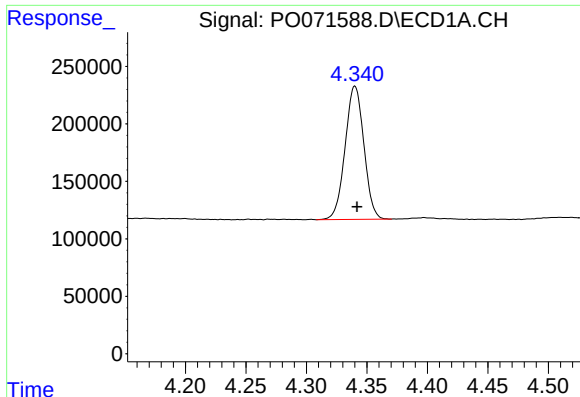

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: -0.002 min
Response: 1252638
Conc: 14.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
40AA-MH

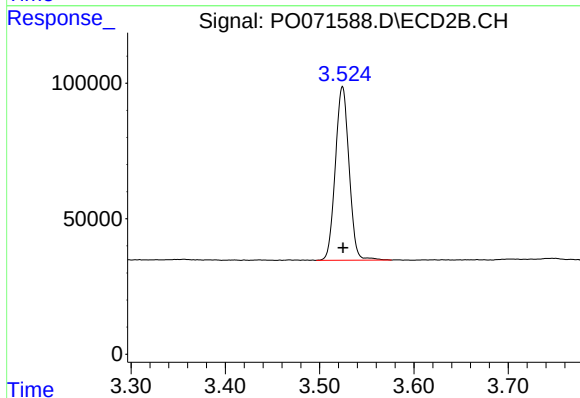


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 648263
Conc: 15.74 ng/ml

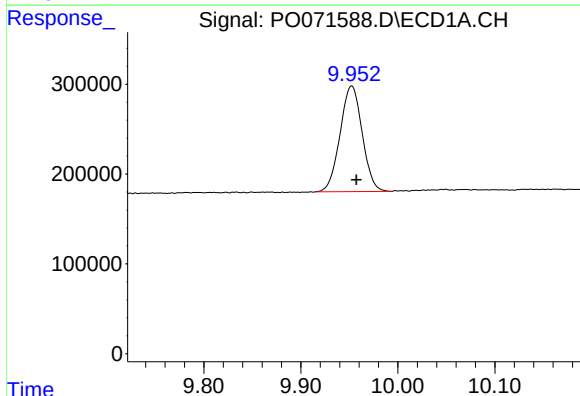

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.005 min
Response: 1862307
Conc: 16.21 ng/ml

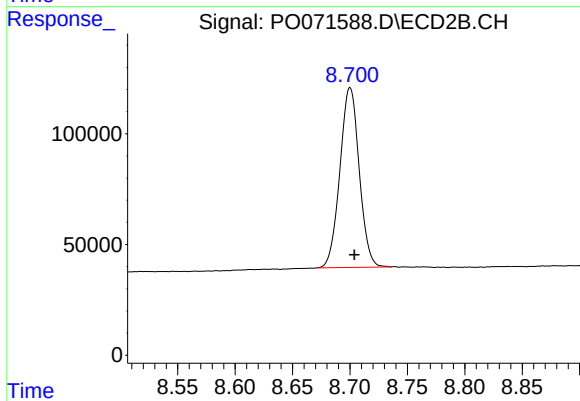

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.004 min
Response: 952161
Conc: 15.66 ng/ml