

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092324\
 Data File : P0106783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 14:14
 Operator : YP/AJ
 Sample : P4138-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LIBERTY-AVE-TP-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:44:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.709	148.8E6	56117658	19.837m	21.008
2) SA Decachlor...	10.193	8.733	79867318	37061017	16.158	18.528m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092324\
Data File : PO106783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 14:14
Operator : YP/AJ
Sample : P4138-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LIBERTY-AVE-TP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:44:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

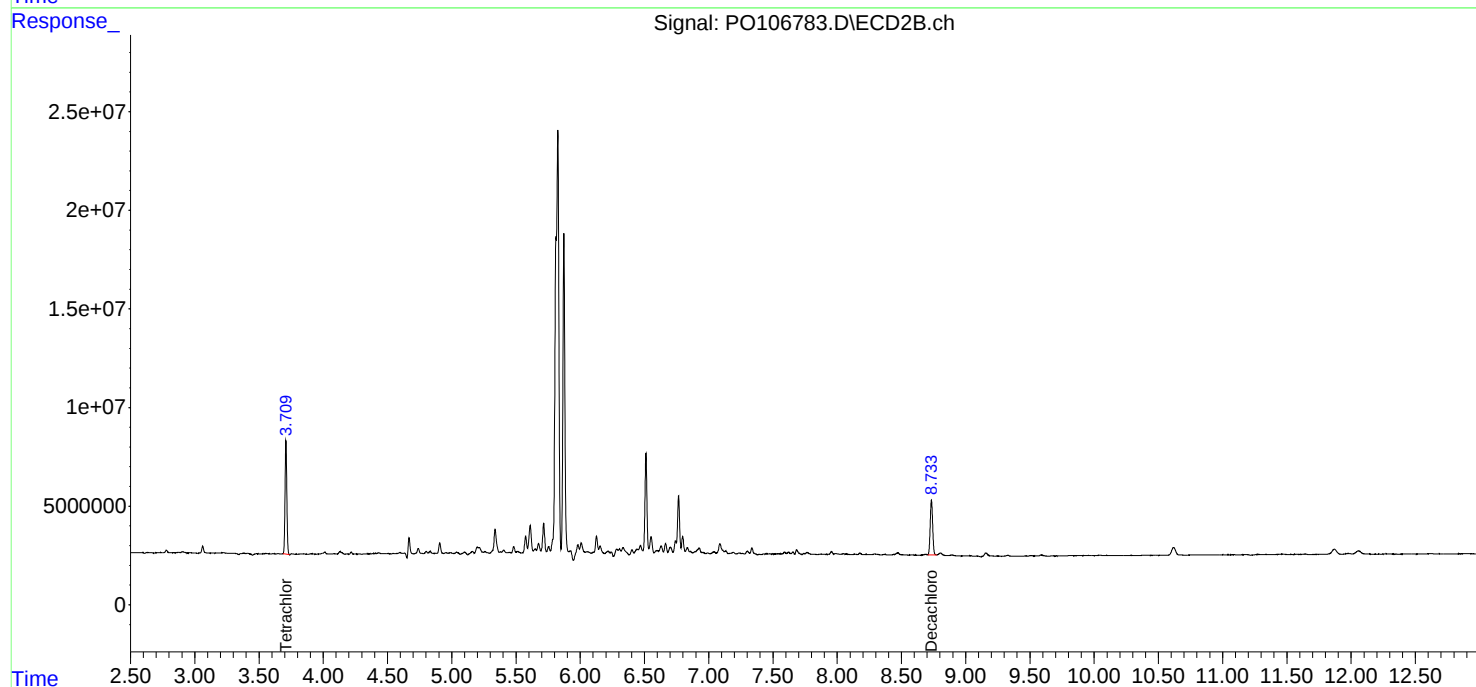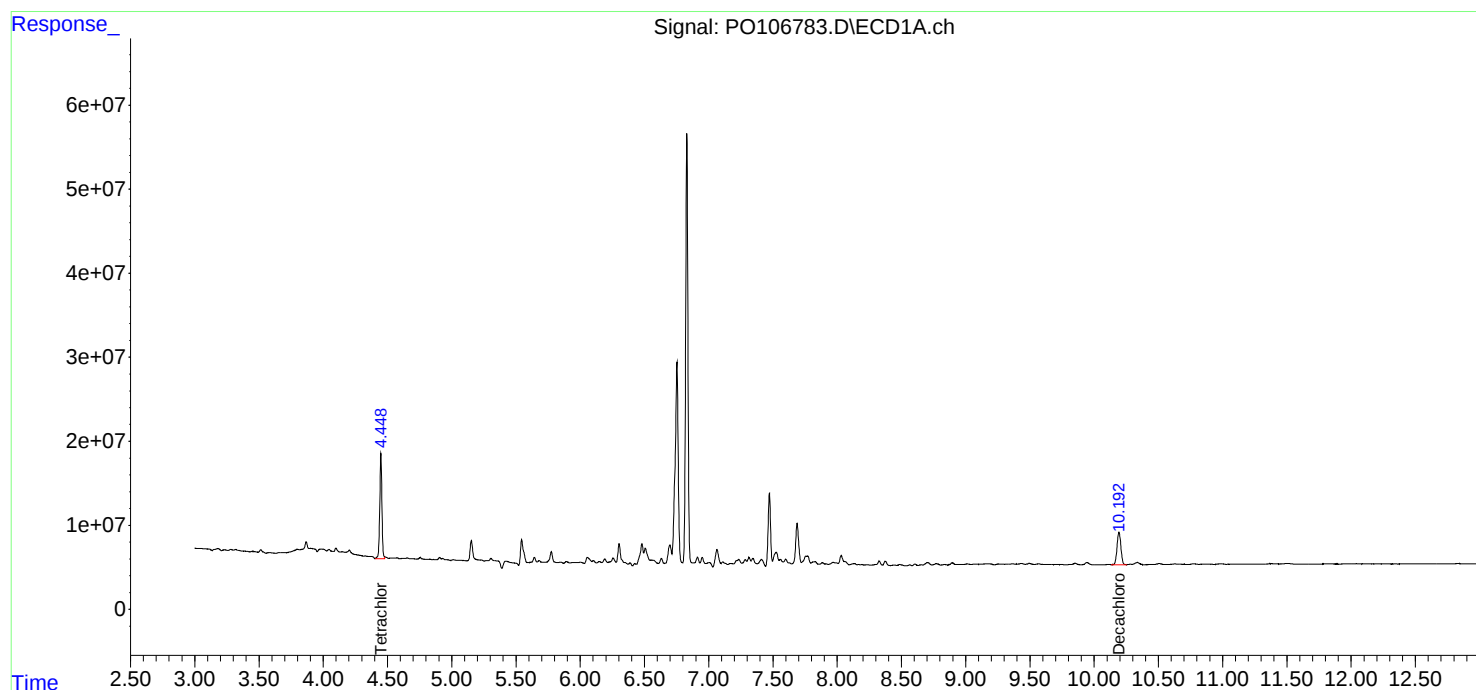

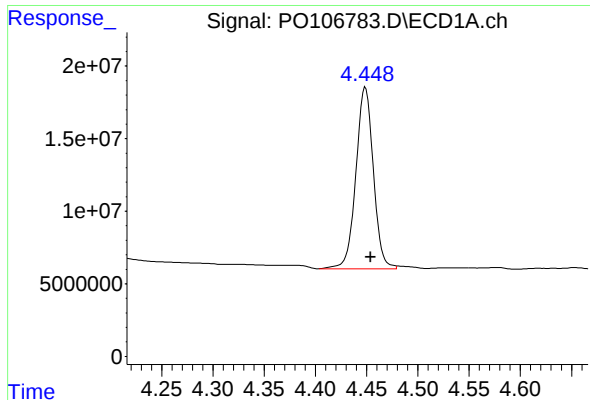


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.006 min
Response: 148805440
Conc: 19.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LIBERTY-AVE-TP-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

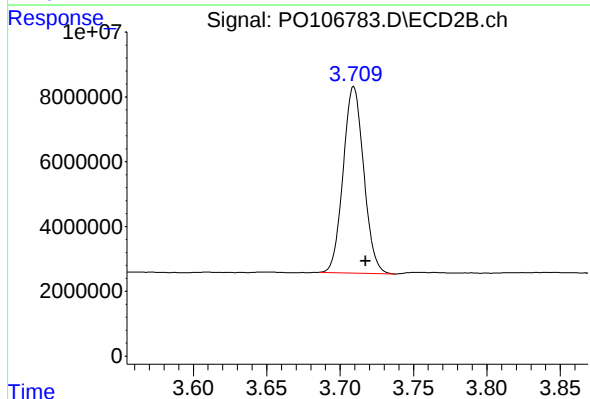


#1 Tetrachloro-m-xylene

R.T.: 3.709 min
Delta R.T.: -0.008 min
Response: 56117658
Conc: 21.01 ng/ml

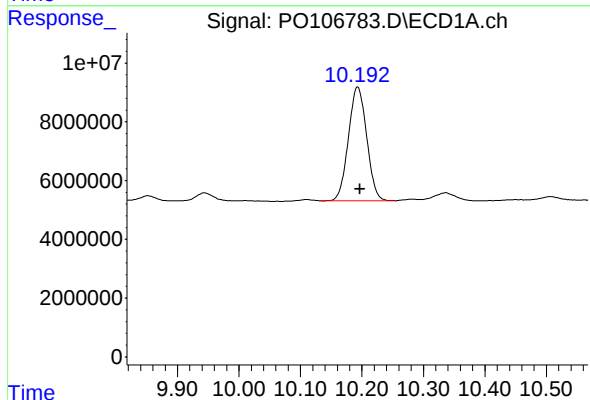

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.004 min
Response: 79867318
Conc: 16.16 ng/ml

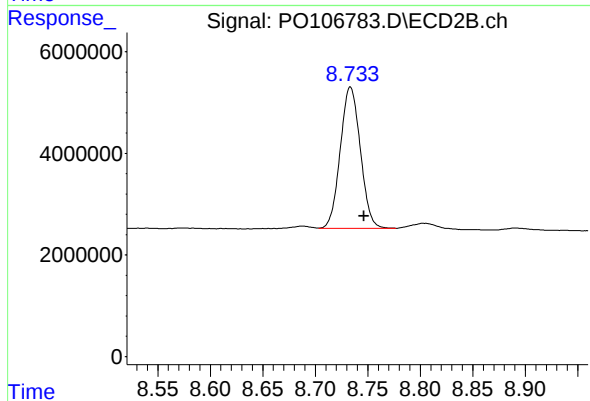

#2 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.013 min
Response: 37061017
Conc: 18.53 ng/ml m