

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092324\
 Data File : P0106786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 15:08
 Operator : YP/AJ
 Sample : P4140-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-23-00305

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:45:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.717	89020035	41854022	11.867	15.669 #
2) SA Decachlor...	10.211	8.749	75109080	30080189	15.196	15.038m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092324\
Data File : PO106786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 15:08
Operator : YP/AJ
Sample : P4140-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-23-00305


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:45:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

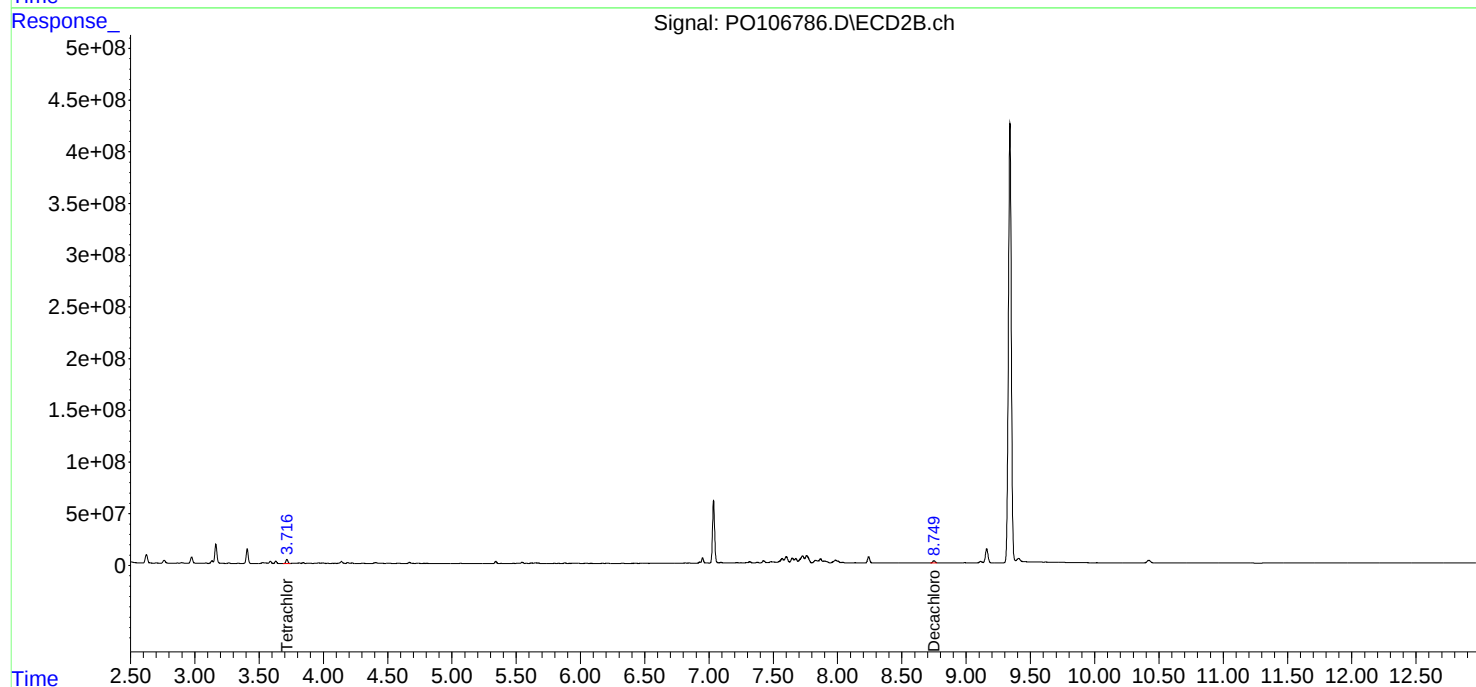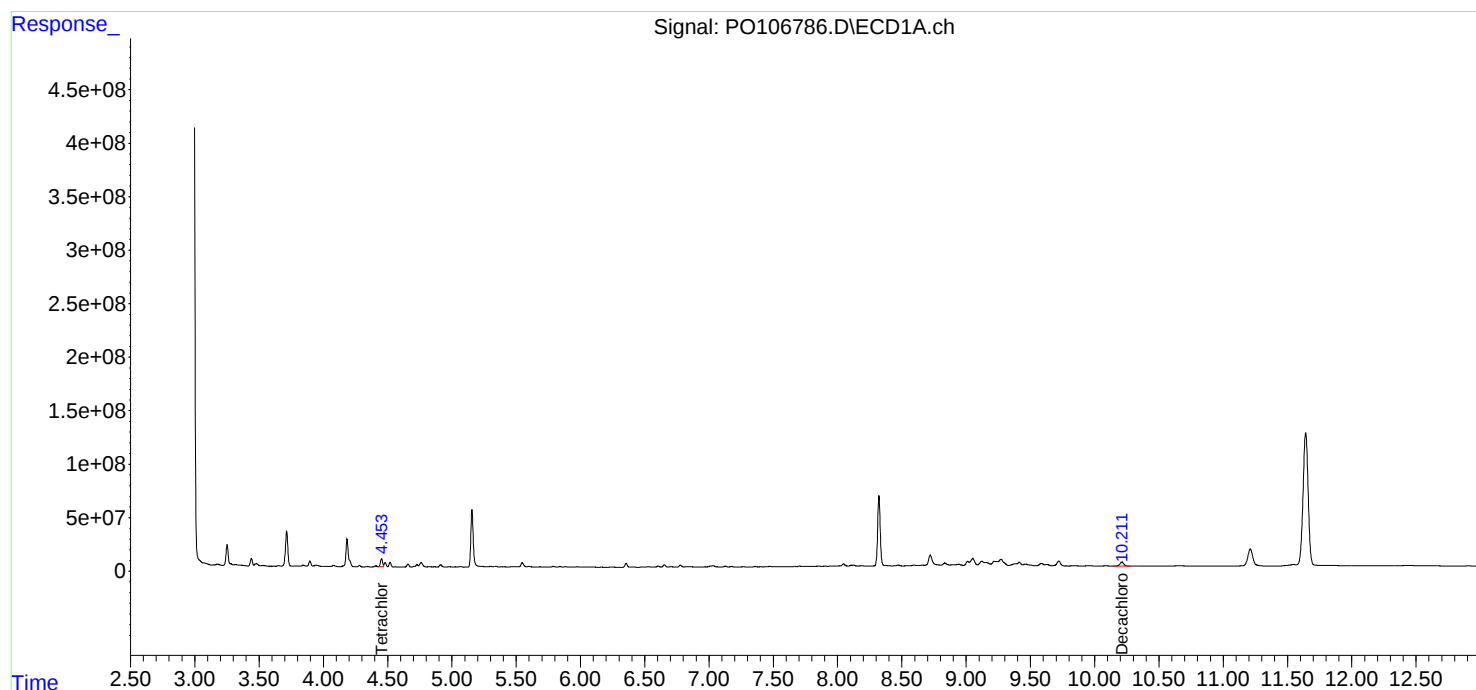

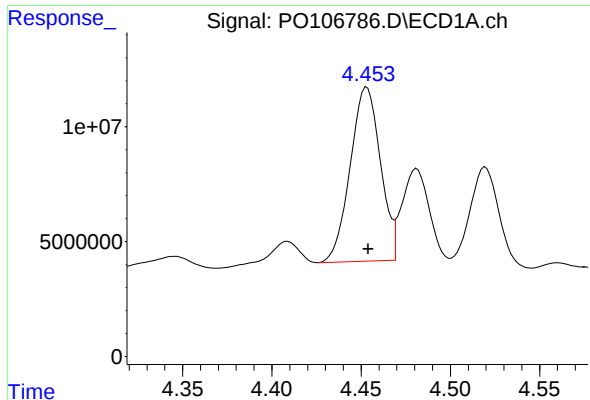


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 89020035
Conc: 11.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-23-00305


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

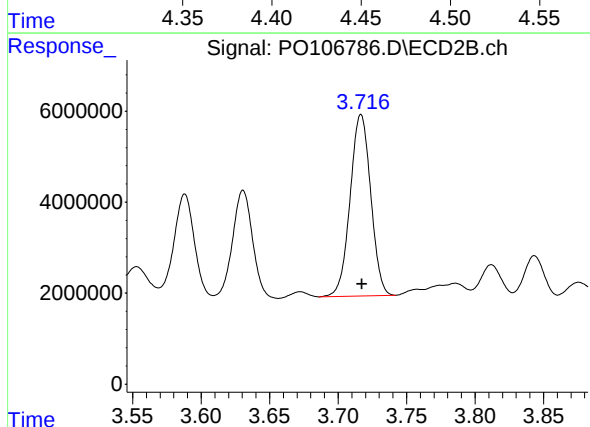


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: 0.000 min
Response: 41854022
Conc: 15.67 ng/ml

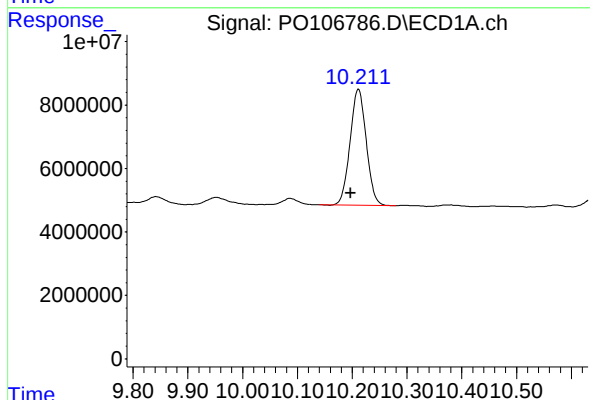

#2 Decachlorobiphenyl

R.T.: 10.211 min
Delta R.T.: 0.014 min
Response: 75109080
Conc: 15.20 ng/ml

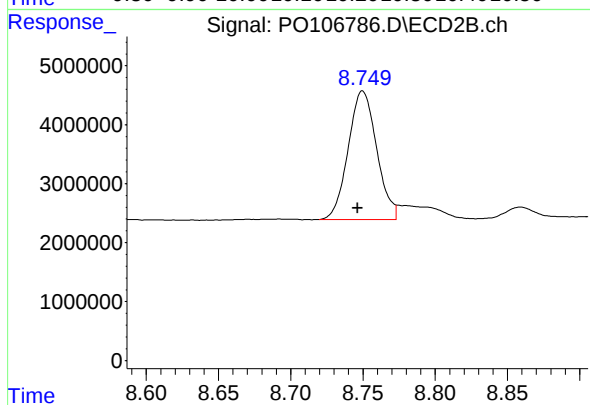

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: 0.003 min
Response: 30080189
Conc: 15.04 ng/ml m