

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092324\
 Data File : P0106810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 00:52
 Operator : YP/AJ
 Sample : P4141-01 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2307-0267-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:52:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.709	12332875	4571418	1.644m	1.711m
2) SA Decachlor...	10.194	8.736	8332602	3251463	1.686m	1.626m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092324\
Data File : PO106810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 00:52
Operator : YP/AJ
Sample : P4141-01 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2307-0267-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:52:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

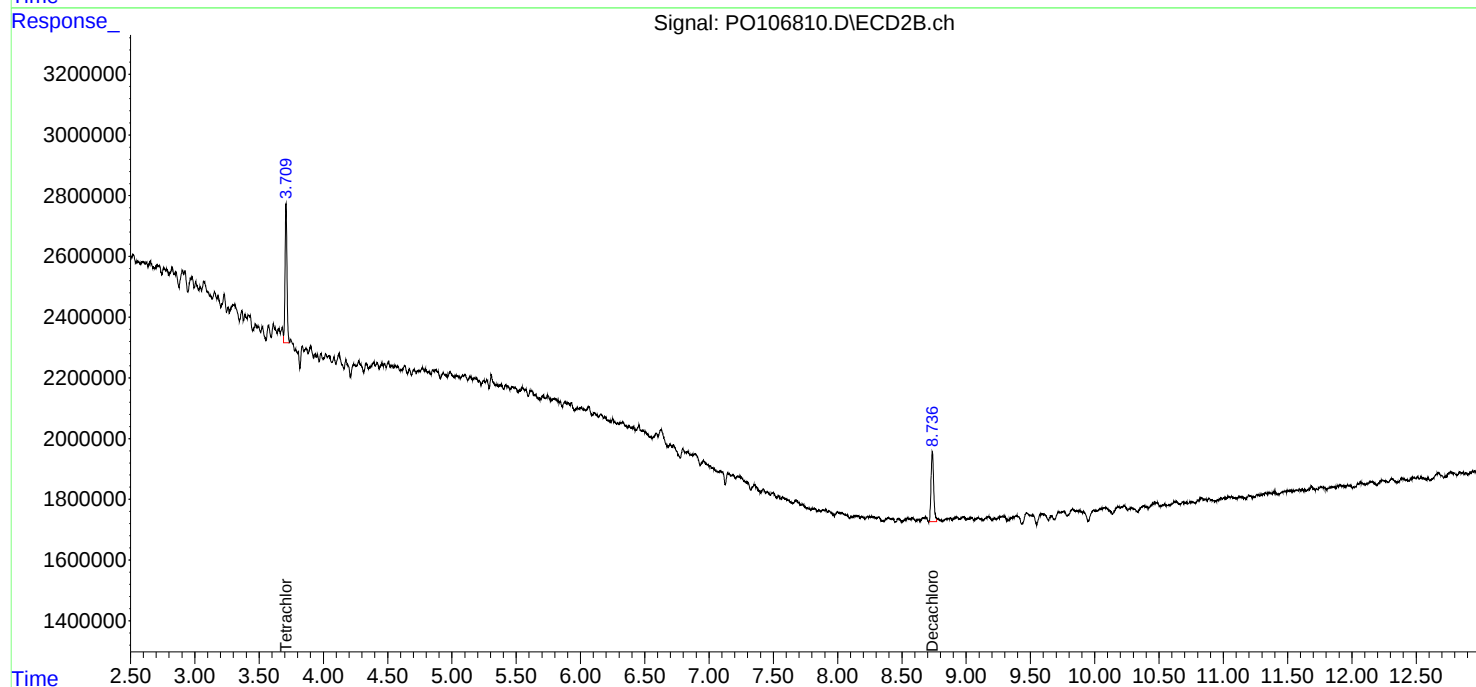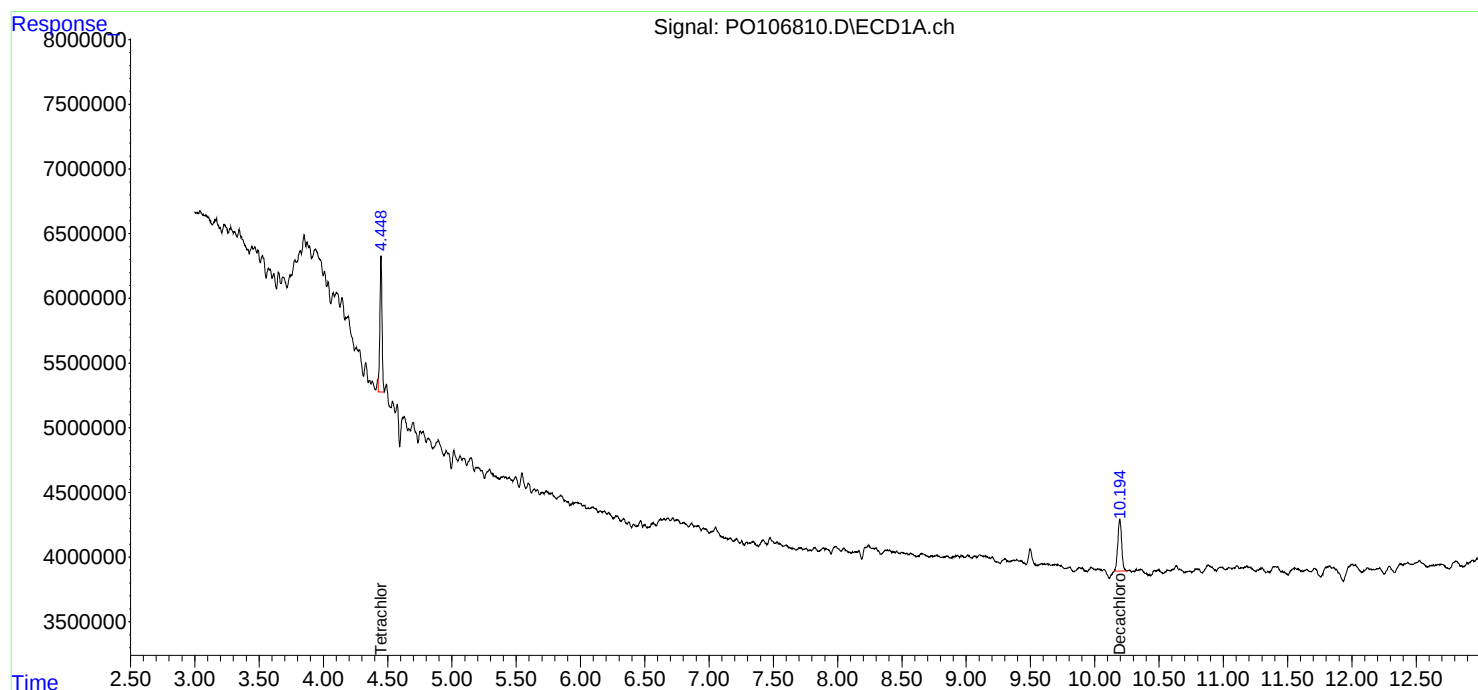

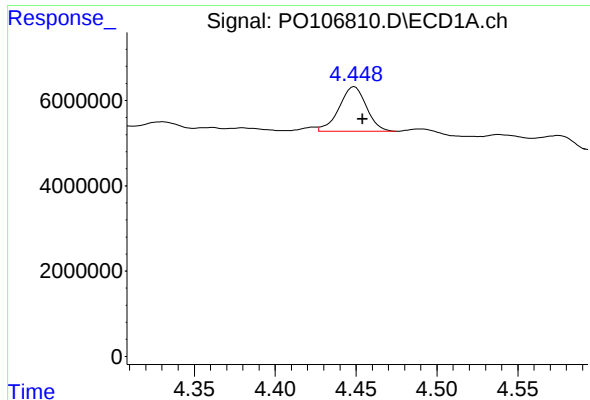


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.006 min
Response: 12332875
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2307-0267-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

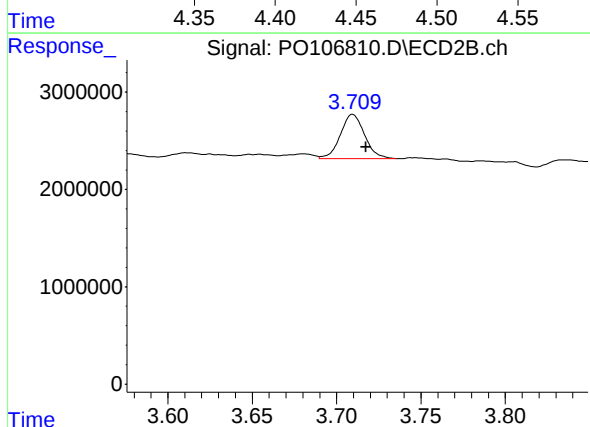


#1 Tetrachloro-m-xylene

R.T.: 3.709 min
Delta R.T.: -0.008 min
Response: 4571418
Conc: 1.71 ng/ml

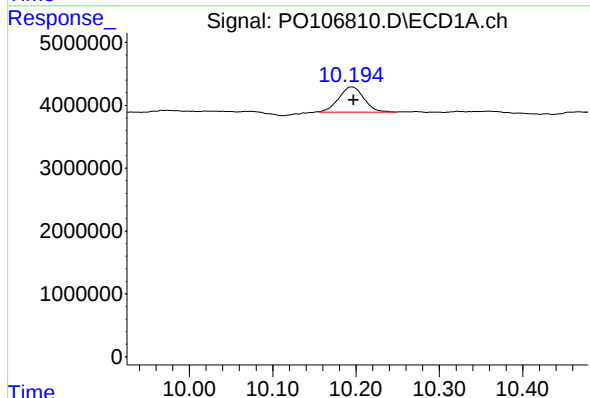

#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.003 min
Response: 8332602
Conc: 1.69 ng/ml

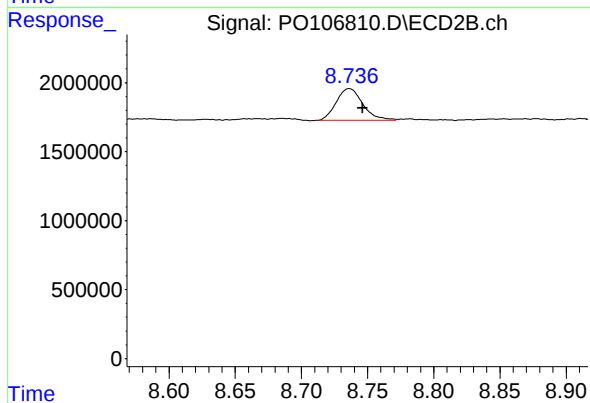

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.011 min
Response: 3251463
Conc: 1.63 ng/ml