

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092324\
 Data File : P0106811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 01:10
 Operator : YP/AJ
 Sample : P4141-02 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2307-0267-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 06:18:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0090924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 09:57:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.709	8786253	4580996	1.171	1.715m#
2) SA Decachlor...	10.192	8.735	8332961	3600474	1.686m	1.800m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092324\
Data File : PO106811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 01:10
Operator : YP/AJ
Sample : P4141-02 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2307-0267-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 06:18:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO090924.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 09:57:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

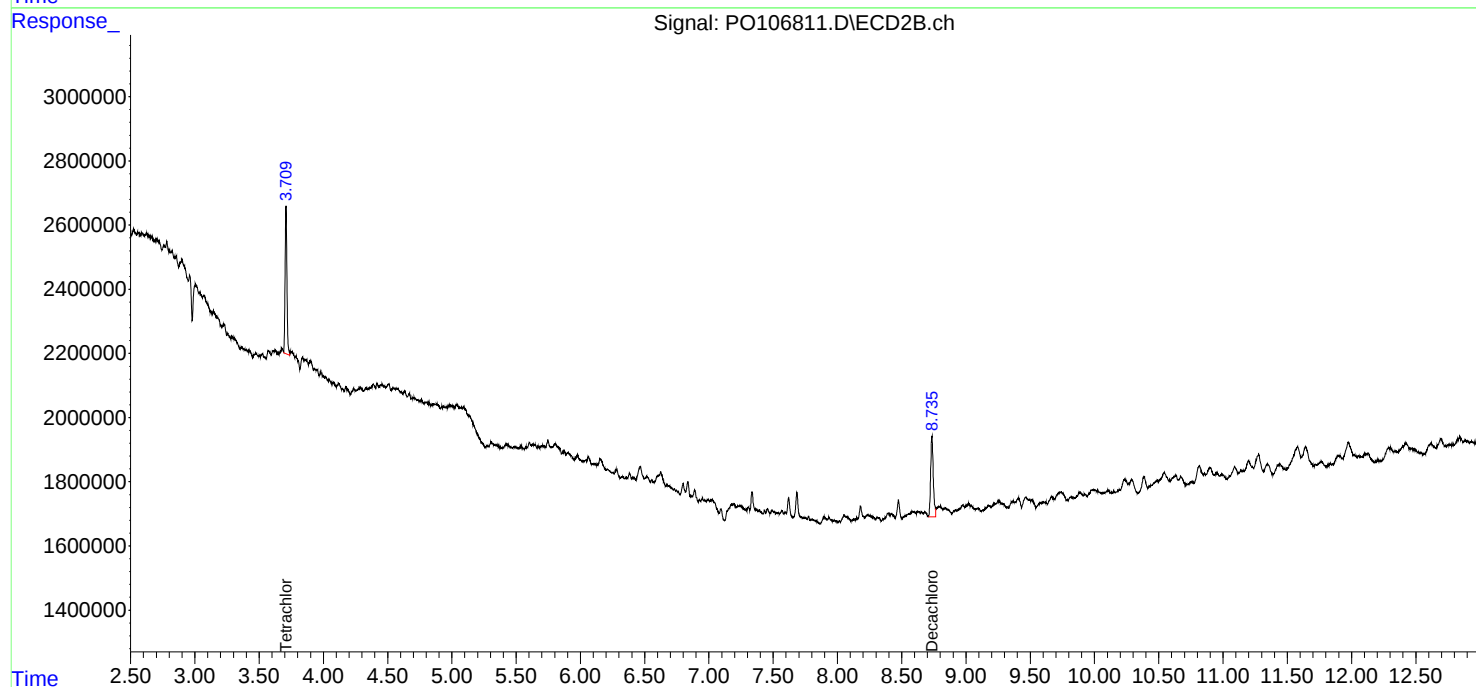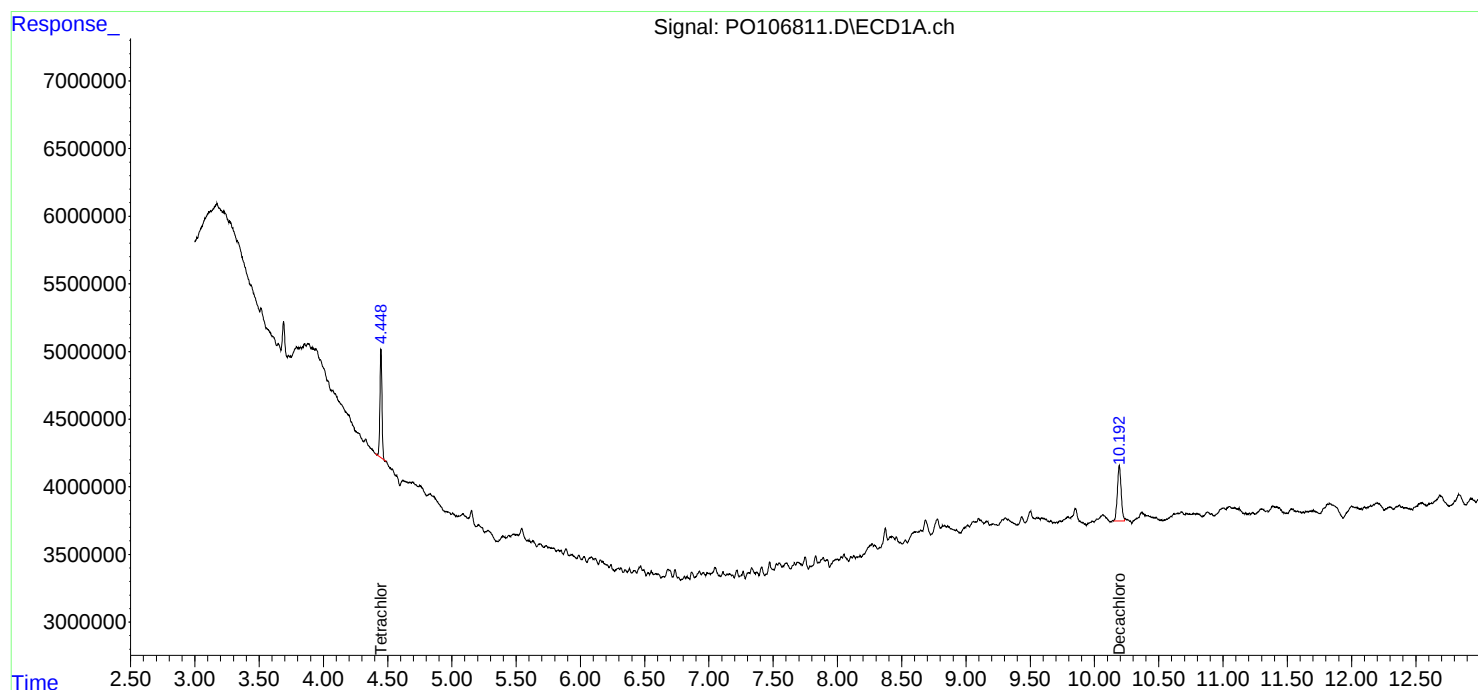

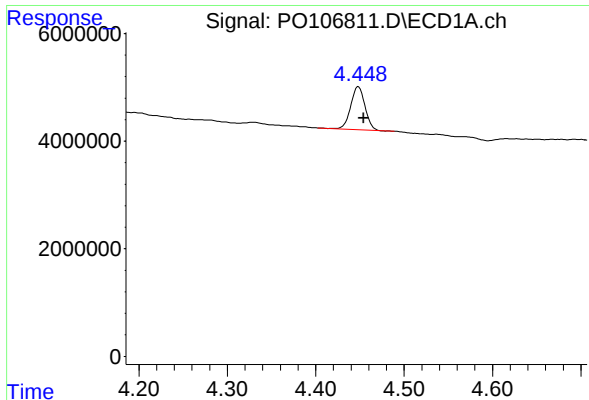


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.006 min
Response: 8786253
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2307-0267-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

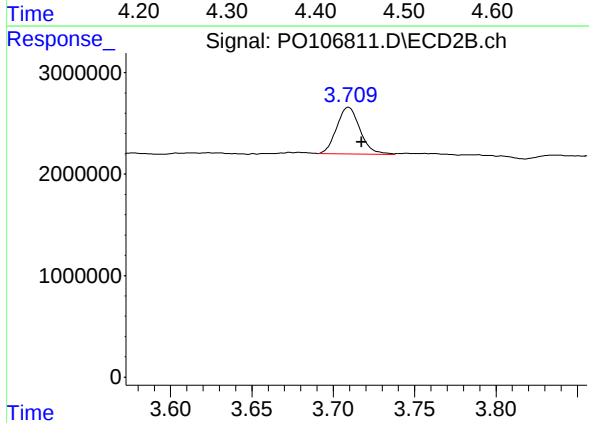


#1 Tetrachloro-m-xylene

R.T.: 3.709 min
Delta R.T.: -0.009 min
Response: 4580996
Conc: 1.71 ng/ml m

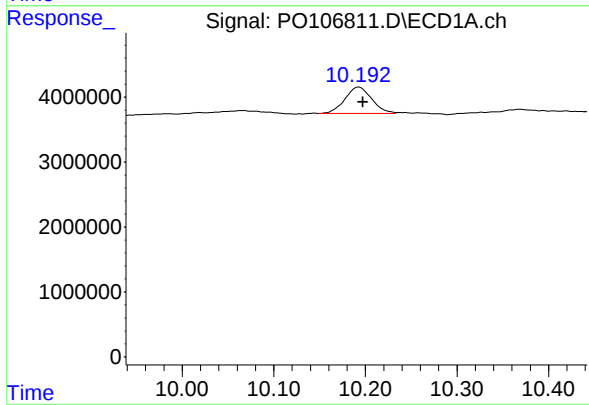

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.005 min
Response: 8332961
Conc: 1.69 ng/ml m

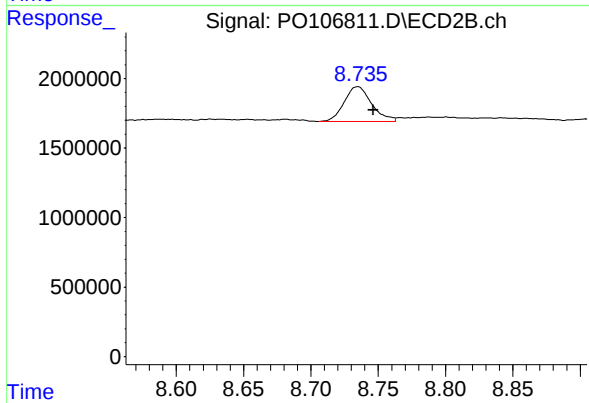

#2 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.011 min
Response: 3600474
Conc: 1.80 ng/ml m