

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092419\
 Data File : P0061311.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2019 11:15
 Operator : SM/AJ
 Sample : K4997-05RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-10-091919RE

Manual Integrations
 APPROVED

Ankita
 9/25/2019 8:45:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 02:34:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.529	925546	735961	25.157	26.358
2) SA Decachlor...	10.038	8.402	1165105	11154569	25.358	318.231m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092419\
Data File : P0061311.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2019 11:15
Operator : SM/AJ
Sample : K4997-05RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-10-091919RE


Manual Integrations
APPROVED

Ankita
9/25/2019 8:45:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 02:34:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

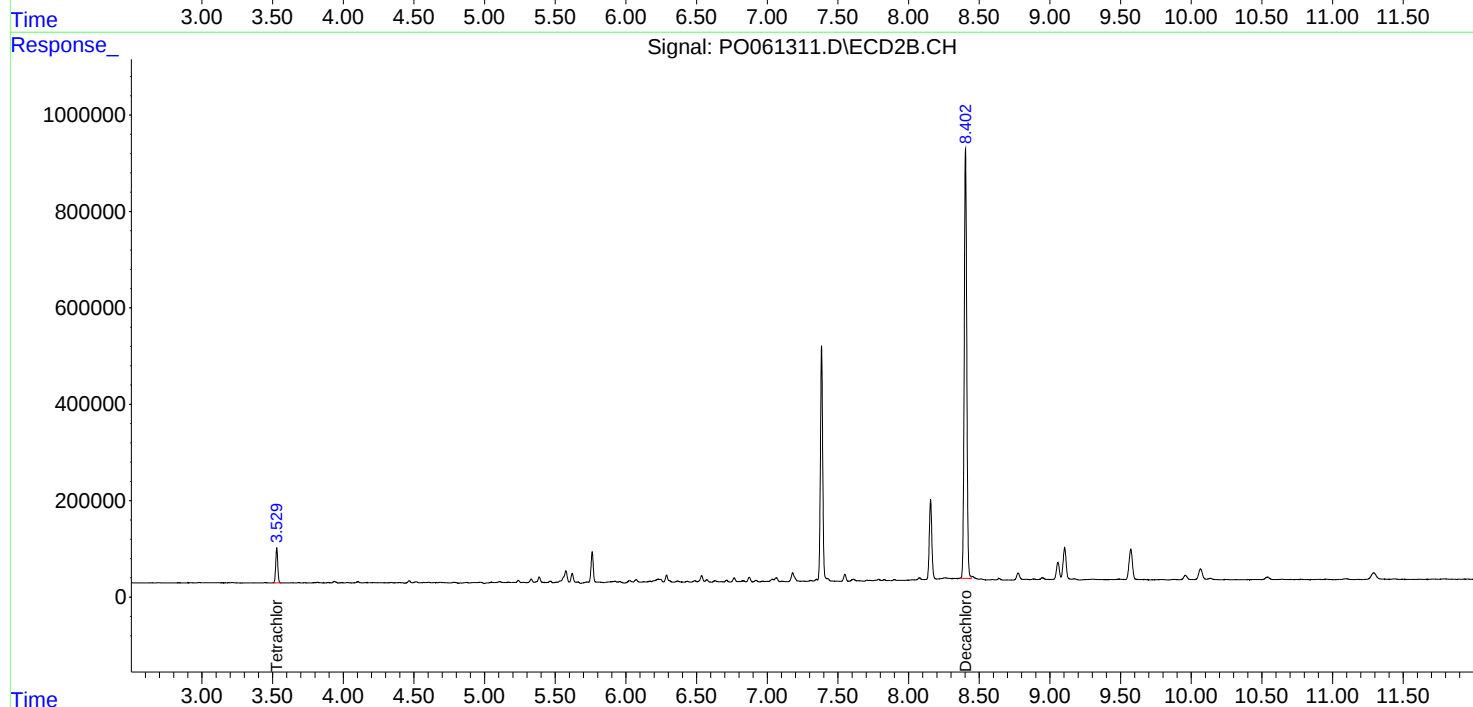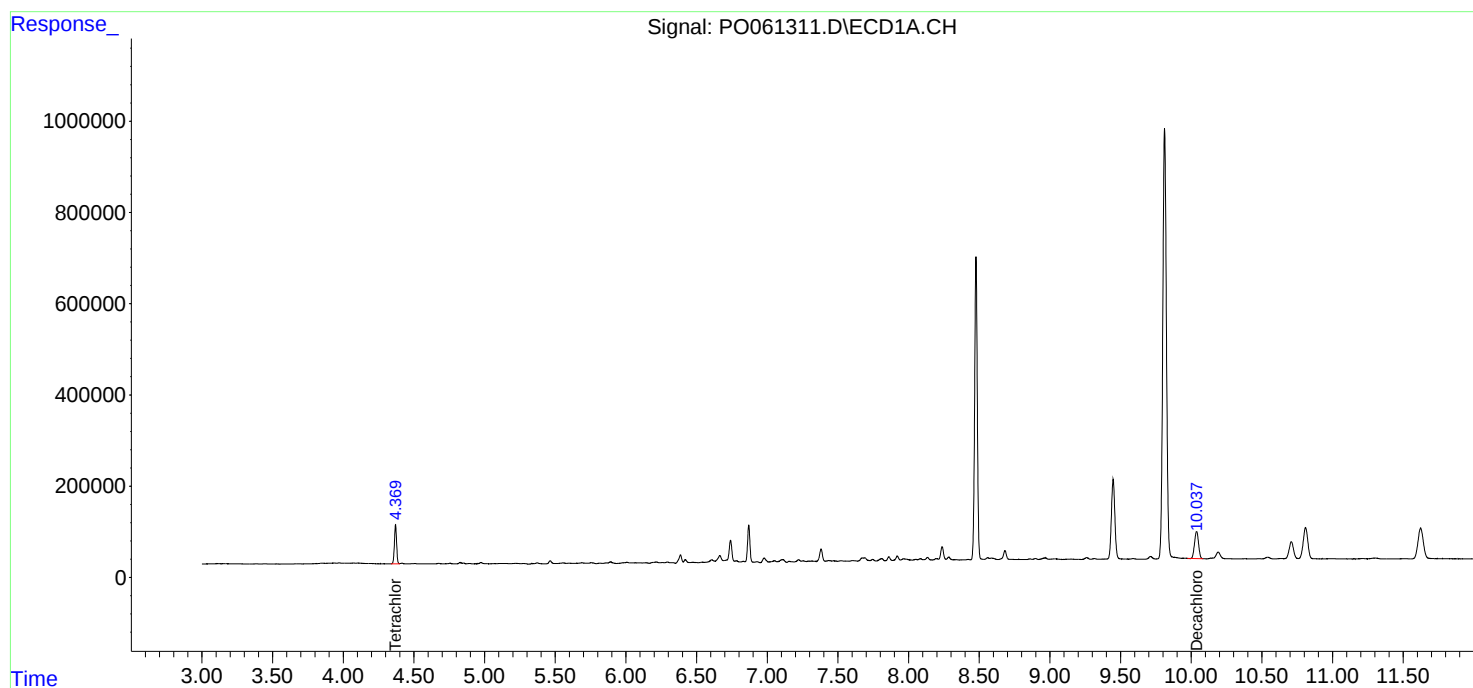

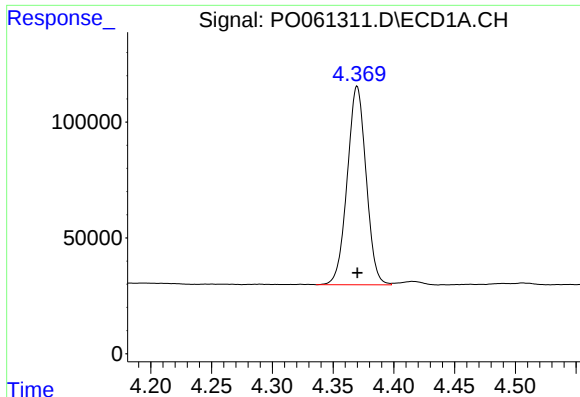


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 925546
Conc: 25.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-10-091919RE


Manual Integrations
APPROVED

Ankita
9/25/2019 8:45:56 AM

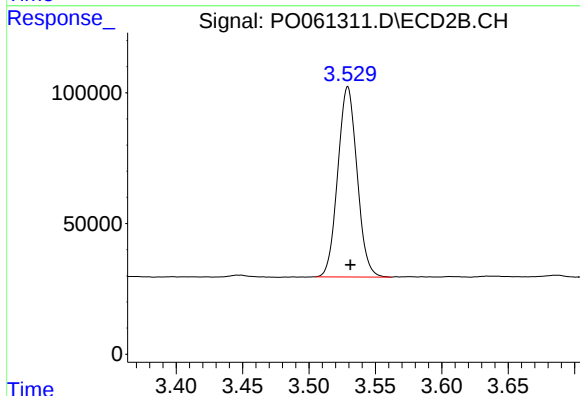


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.002 min
Response: 735961
Conc: 26.36 ng/ml

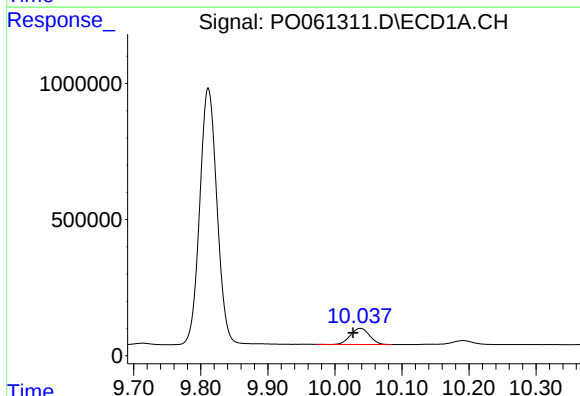

#2 Decachlorobiphenyl

R.T.: 10.038 min
Delta R.T.: 0.010 min
Response: 1165105
Conc: 25.36 ng/ml

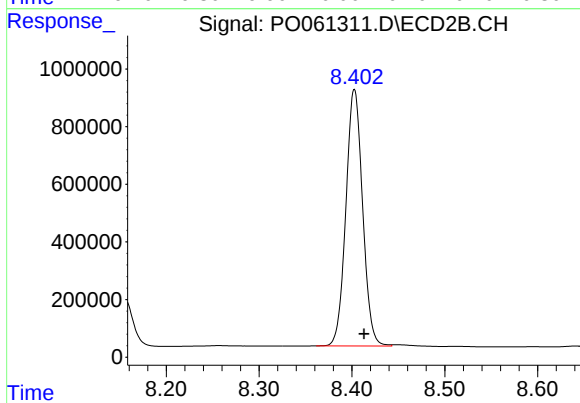

#2 Decachlorobiphenyl

R.T.: 8.402 min
Delta R.T.: -0.011 min
Response: 11154569
Conc: 318.23 ng/ml m