

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092420\
 Data File : P0071600.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2020 12:47
 Operator : DD\AJ
 Sample : L3871-25
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-092320

Manual Integrations
 APPROVED

Ankita
 9/25/2020 10:36:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 17:03:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.523	1891973	944312	22.047m	22.928
2) SA Decachlor...	9.952	8.699	2360594	1190736	20.547	19.589
Target Compounds						
31) L7 AR-1260-1	7.299	6.304	104150	29719	18.329	10.739m#
32) L7 AR-1260-2	7.569	6.505	108677	40082	12.518	11.340
33) L7 AR-1260-3	7.923	6.650	87769	38382	12.189	11.940m
34) L7 AR-1260-4	8.150	7.127	76007	30406	11.472	10.539
35) L7 AR-1260-5	8.464	7.379	157985	78359	10.477	10.594m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092420\
Data File : PO071600.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2020 12:47
Operator : DD\AJ
Sample : L3871-25
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TR-04-092320


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 17:03:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

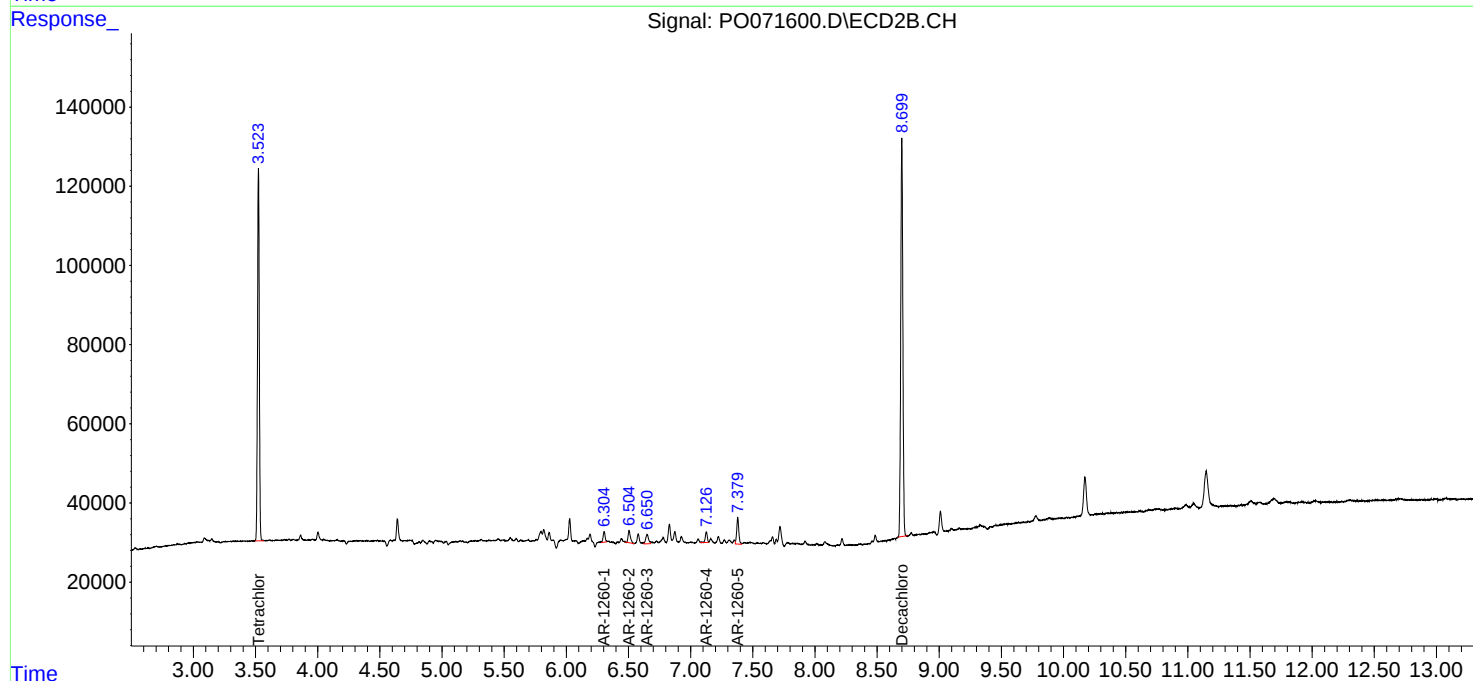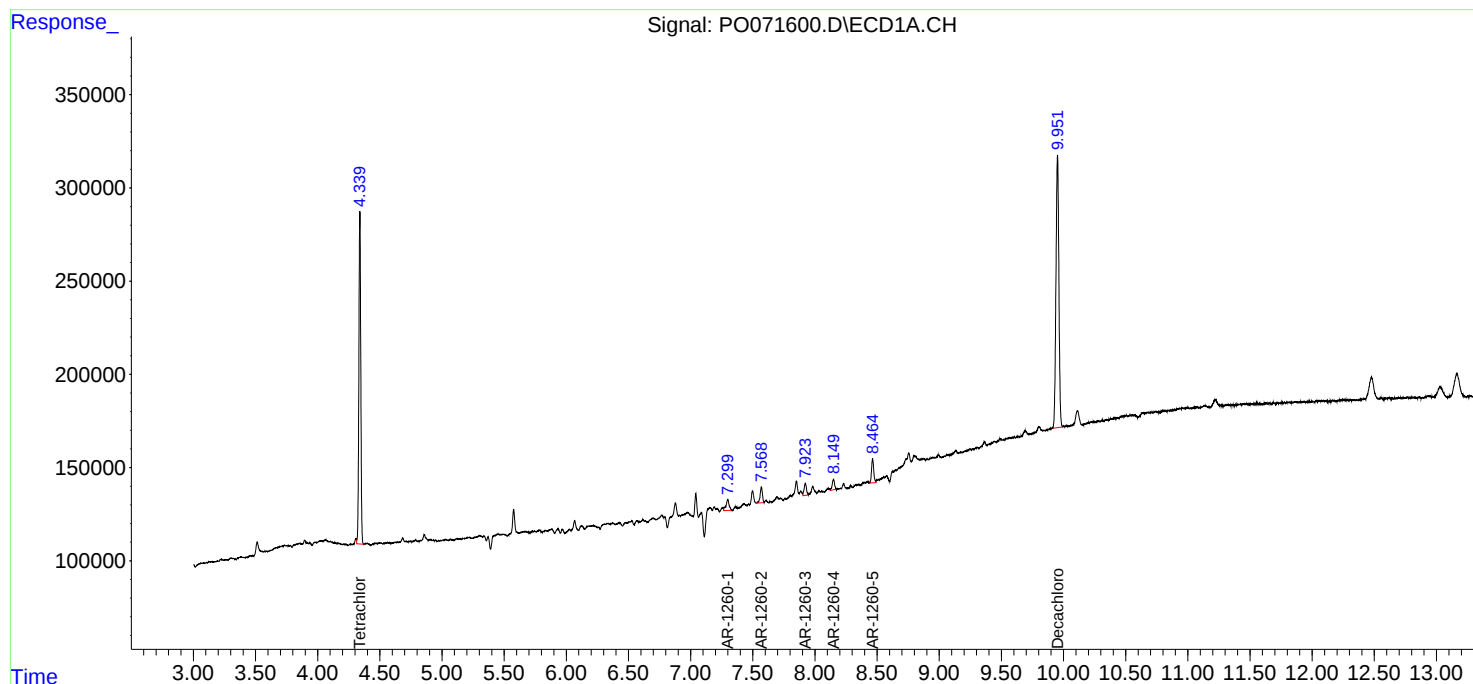

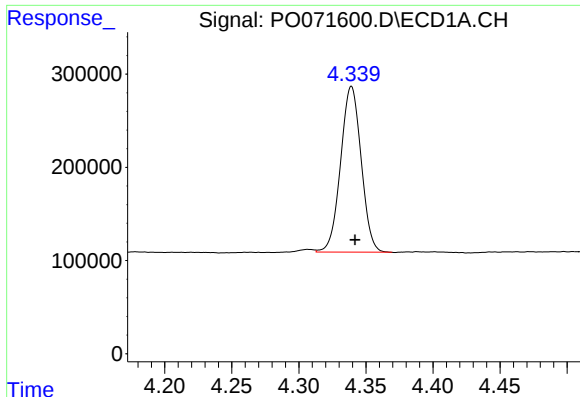


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.003 min
Response: 1891973
Conc: 22.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-04-092320


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:43 AM

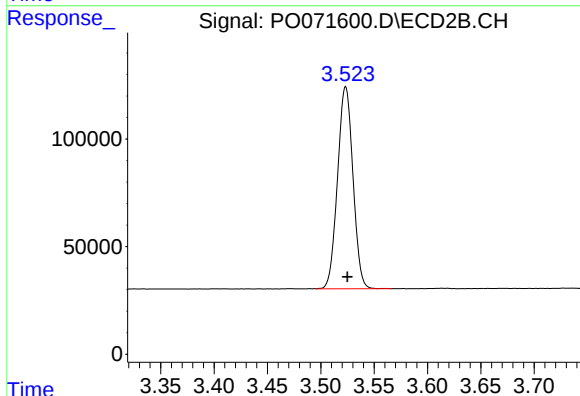


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.002 min
Response: 944312
Conc: 22.93 ng/ml

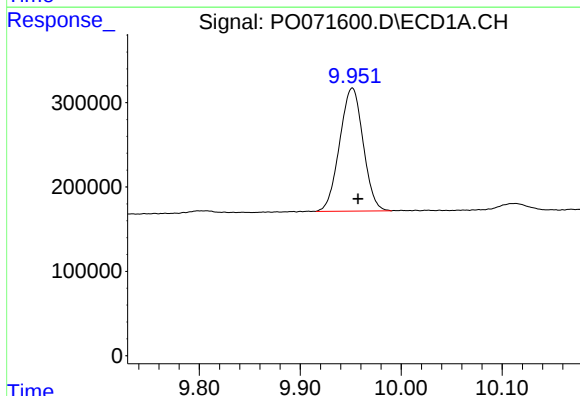


#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: -0.006 min
Response: 2360594
Conc: 20.55 ng/ml

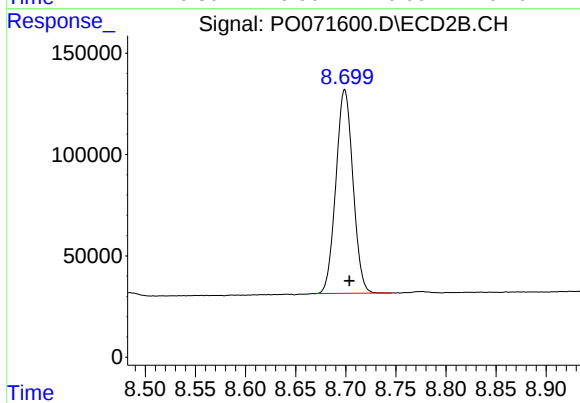

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.005 min
Response: 1190736
Conc: 19.59 ng/ml

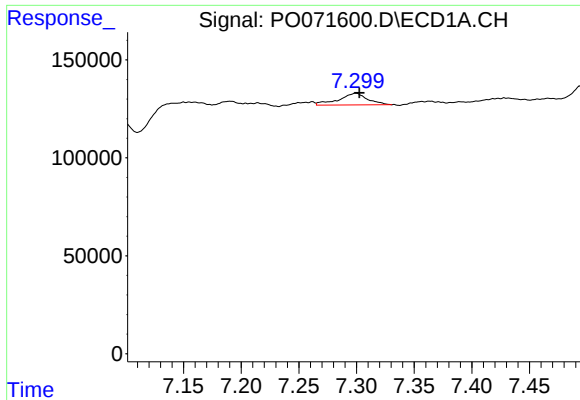


#31 AR-1260-1

R.T.: 7.299 min
Delta R.T.: -0.003 min
Response: 104150
Conc: 18.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-092320


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:43 AM

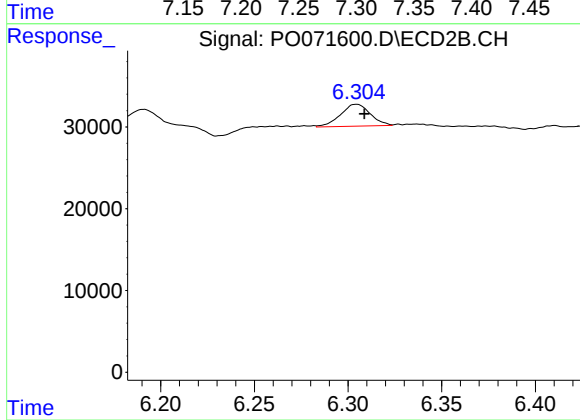


#31 AR-1260-1

R.T.: 6.304 min
Delta R.T.: -0.004 min
Response: 29719
Conc: 10.74 ng/ml m

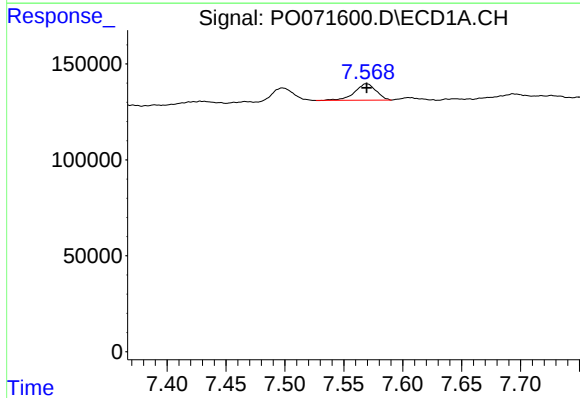


#32 AR-1260-2

R.T.: 7.569 min
Delta R.T.: 0.000 min
Response: 108677
Conc: 12.52 ng/ml

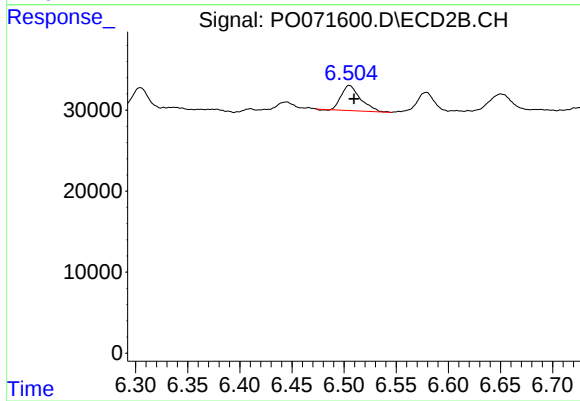

#32 AR-1260-2

R.T.: 6.505 min
Delta R.T.: -0.005 min
Response: 40082
Conc: 11.34 ng/ml

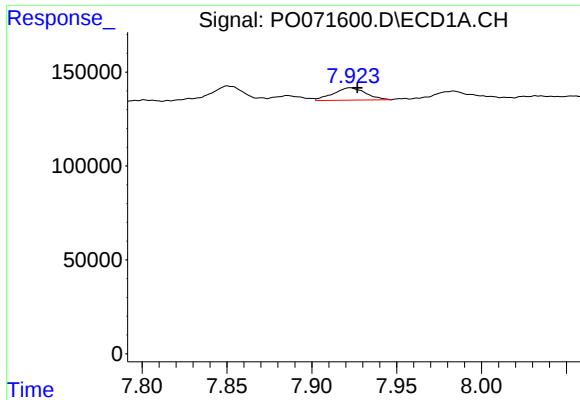


#33 AR-1260-3

R.T.: 7.923 min
Delta R.T.: -0.004 min
Response: 87769
Conc: 12.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-092320


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:43 AM

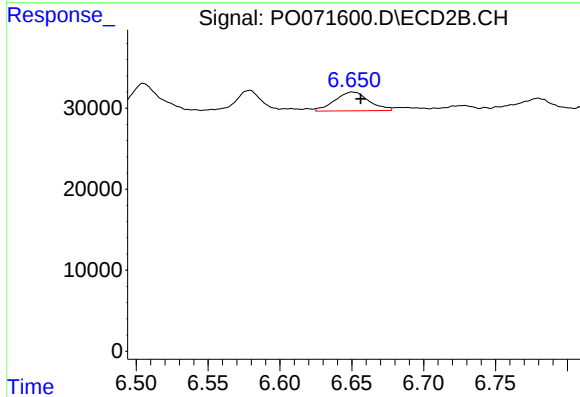


#33 AR-1260-3

R.T.: 6.650 min
Delta R.T.: -0.007 min
Response: 38382
Conc: 11.94 ng/ml m

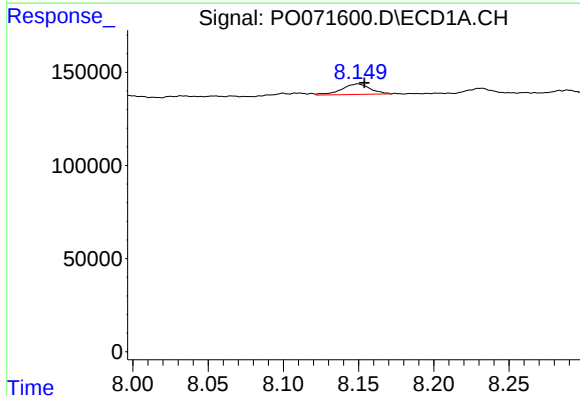


#34 AR-1260-4

R.T.: 8.150 min
Delta R.T.: -0.004 min
Response: 76007
Conc: 11.47 ng/ml

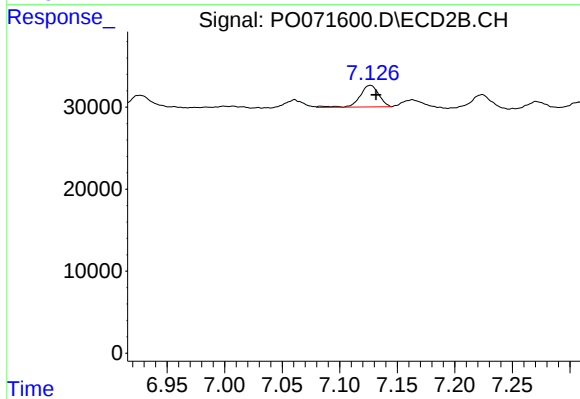

#34 AR-1260-4

R.T.: 7.127 min
Delta R.T.: -0.005 min
Response: 30406
Conc: 10.54 ng/ml

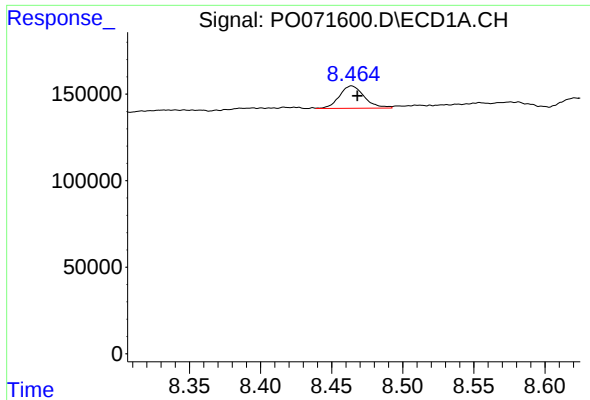


#35 AR-1260-5

R.T.: 8.464 min
Delta R.T.: -0.004 min
Response: 157985
Conc: 10.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-092320

Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:43 AM

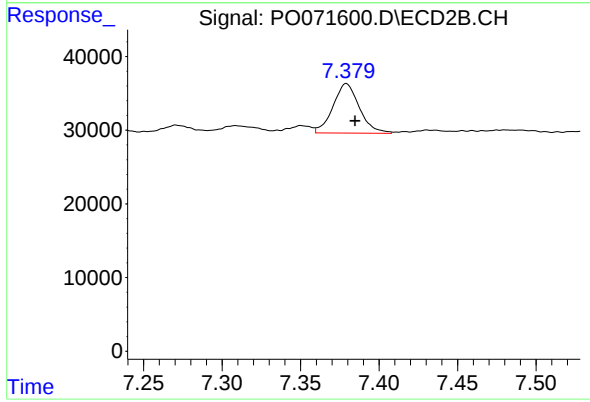

#35 AR-1260-5

R.T.: 7.379 min
Delta R.T.: -0.006 min
Response: 78359
Conc: 10.59 ng/ml m