

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092420\
 Data File : P0071616.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2020 17:37
 Operator : DD\AJ
 Sample : L4114-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 69-70-71-72

Manual Integrations
 APPROVED

Ankita
 9/25/2020 10:36:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 18:51:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 23 08:07:44 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.523	1053176	680819	12.273m	16.530m#
2) SA Decachlor...	9.949	8.698	1128345	582246	9.821	9.579

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092420\
Data File : PO071616.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2020 17:37
Operator : DD\AJ
Sample : L4114-11
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
69-70-71-72


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 18:51:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092320.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 23 08:07:44 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

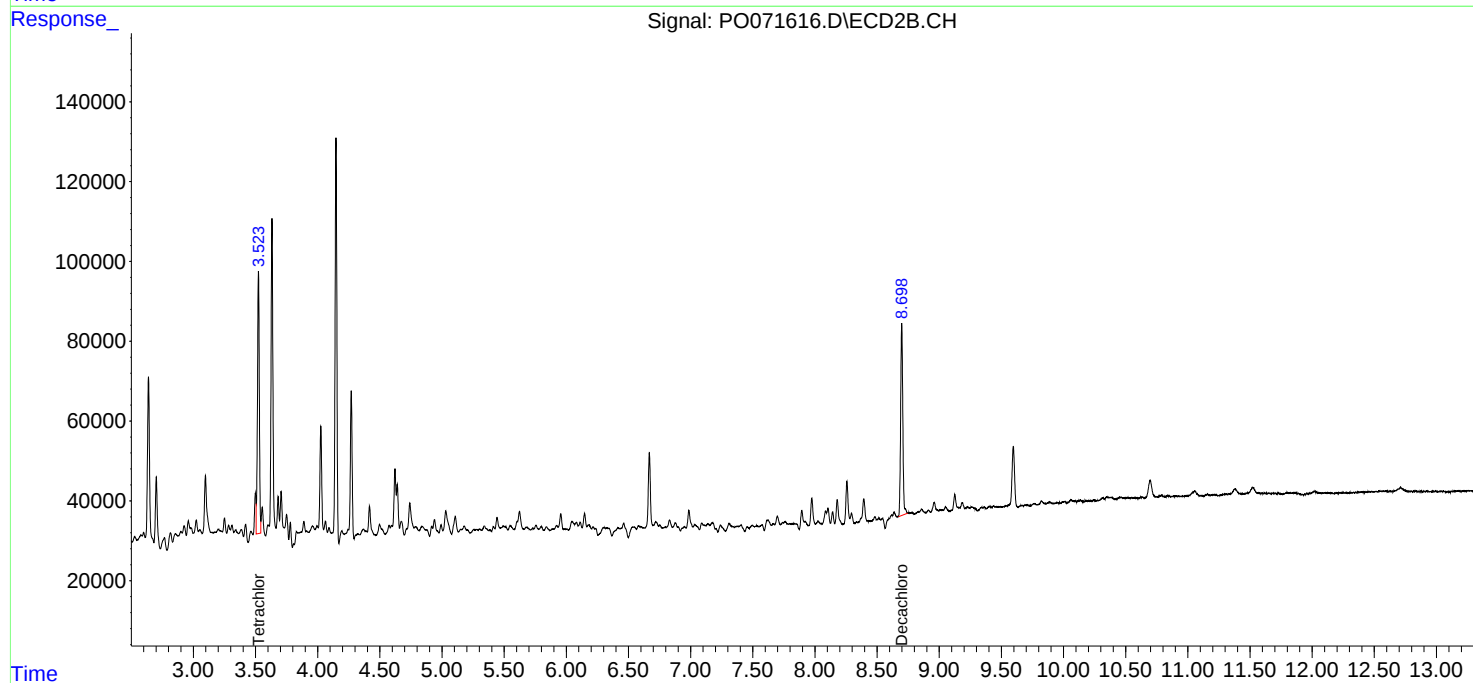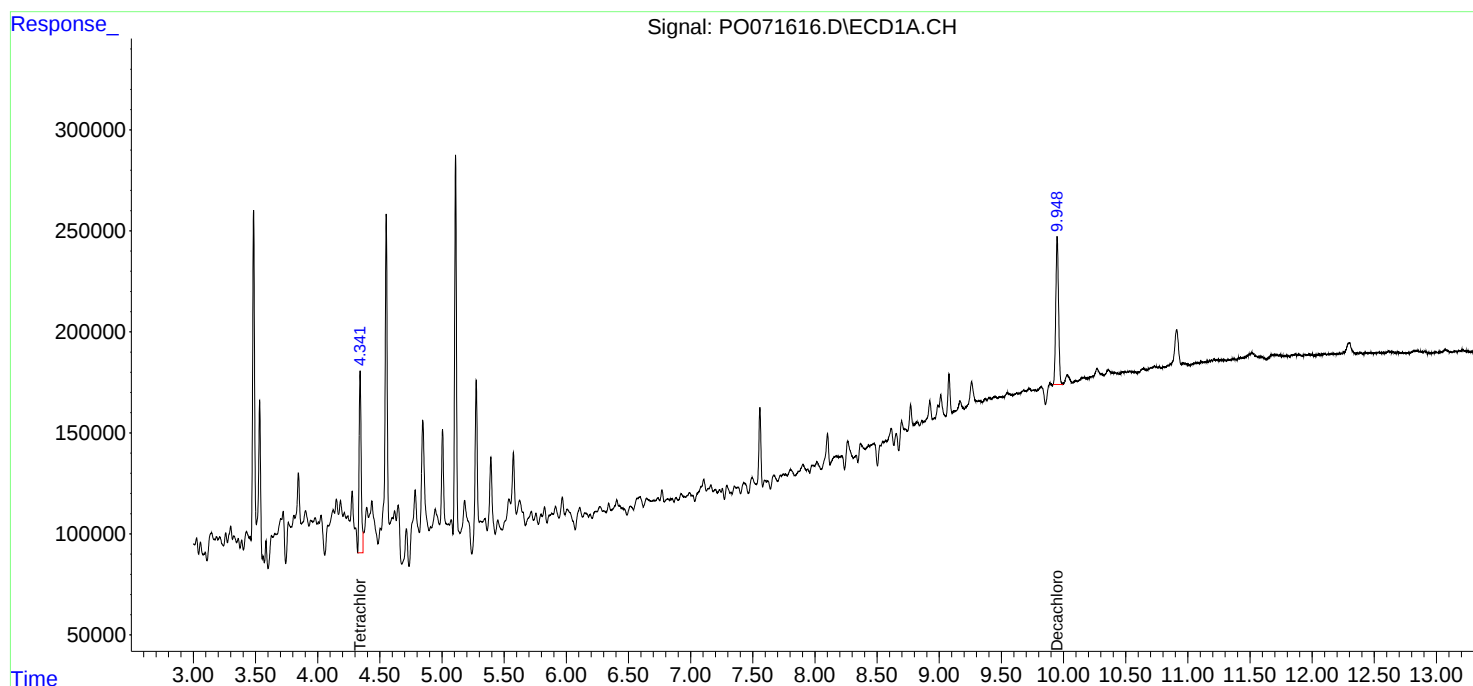

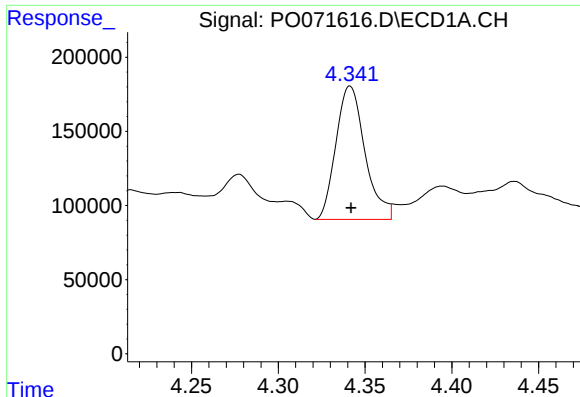


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: -0.001 min
Response: 1053176
Conc: 12.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
69-70-71-72


Manual Integrations
APPROVED

Ankita
9/25/2020 10:36:53 AM

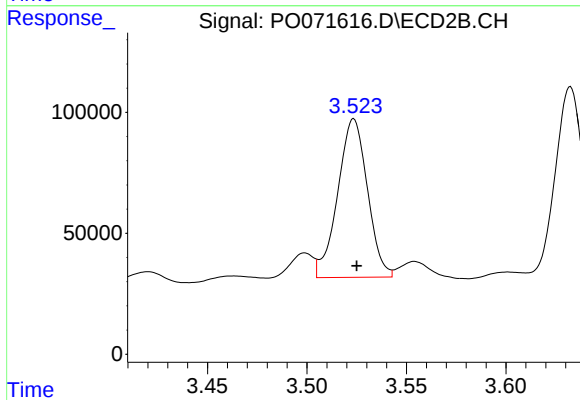


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.002 min
Response: 680819
Conc: 16.53 ng/ml m

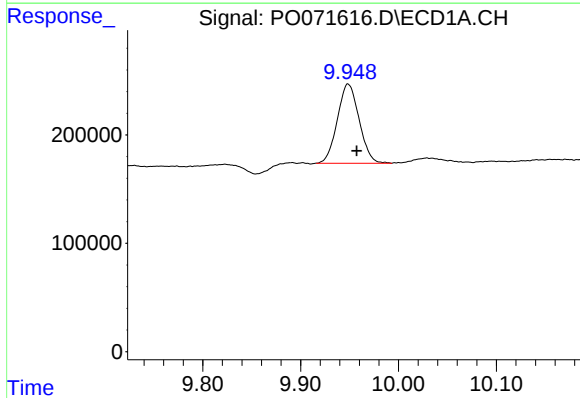

#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.009 min
Response: 1128345
Conc: 9.82 ng/ml

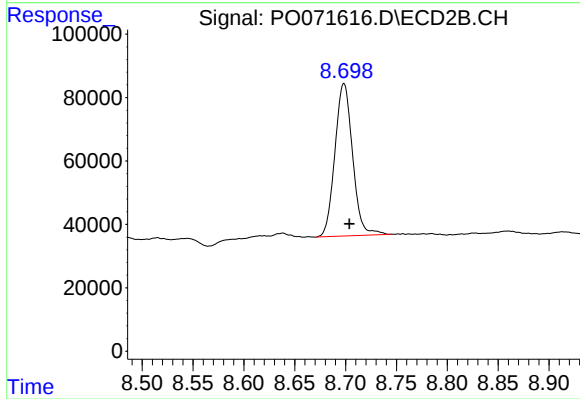

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.005 min
Response: 582246
Conc: 9.58 ng/ml