

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092421\
 Data File : P0081494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2021 16:54
 Operator : AJ\MA
 Sample : M3875-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20882

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:18:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.868	3.986	846349	319566	9.491m	11.995 #
2) SA Decachlor...	10.878	9.332	769188	260576	10.326	11.221

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092421\
Data File : PO081494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2021 16:54
Operator : AJ\MA
Sample : M3875-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20882

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:18:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

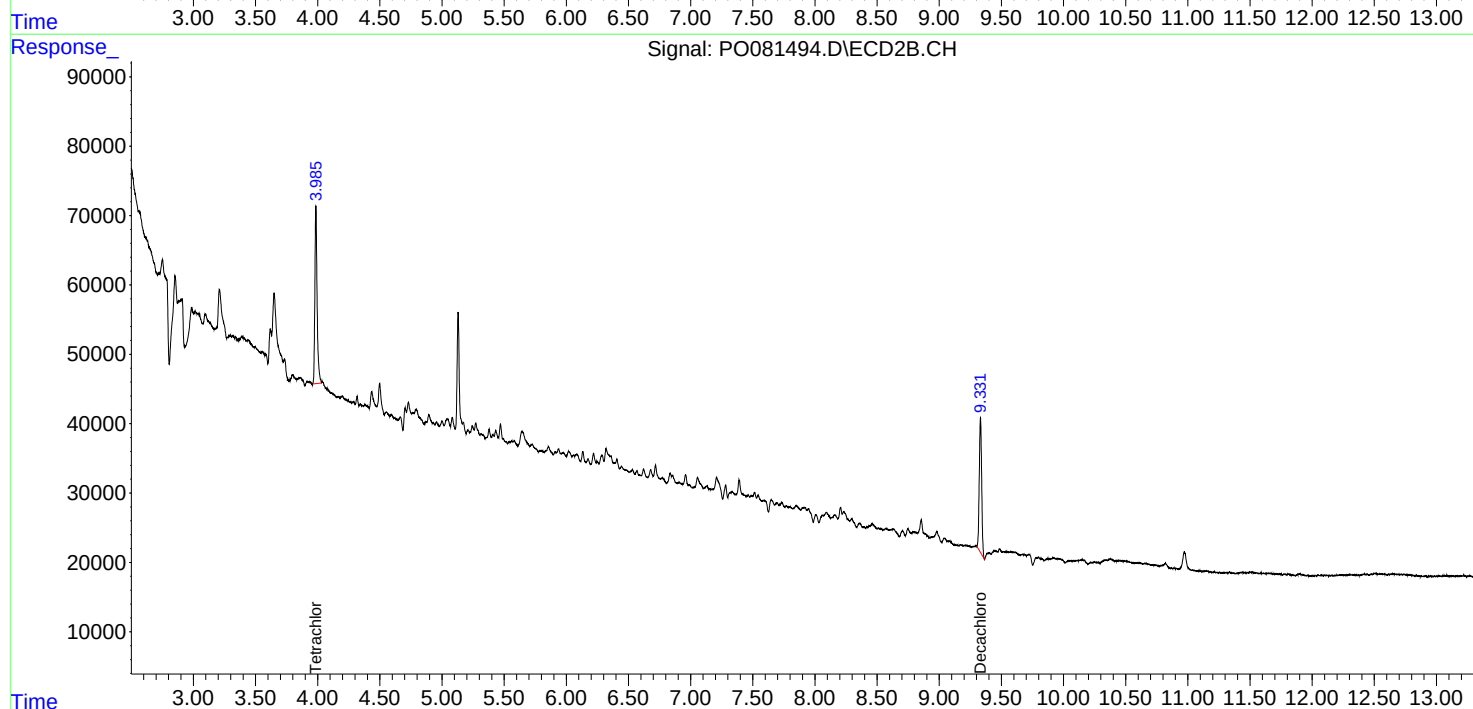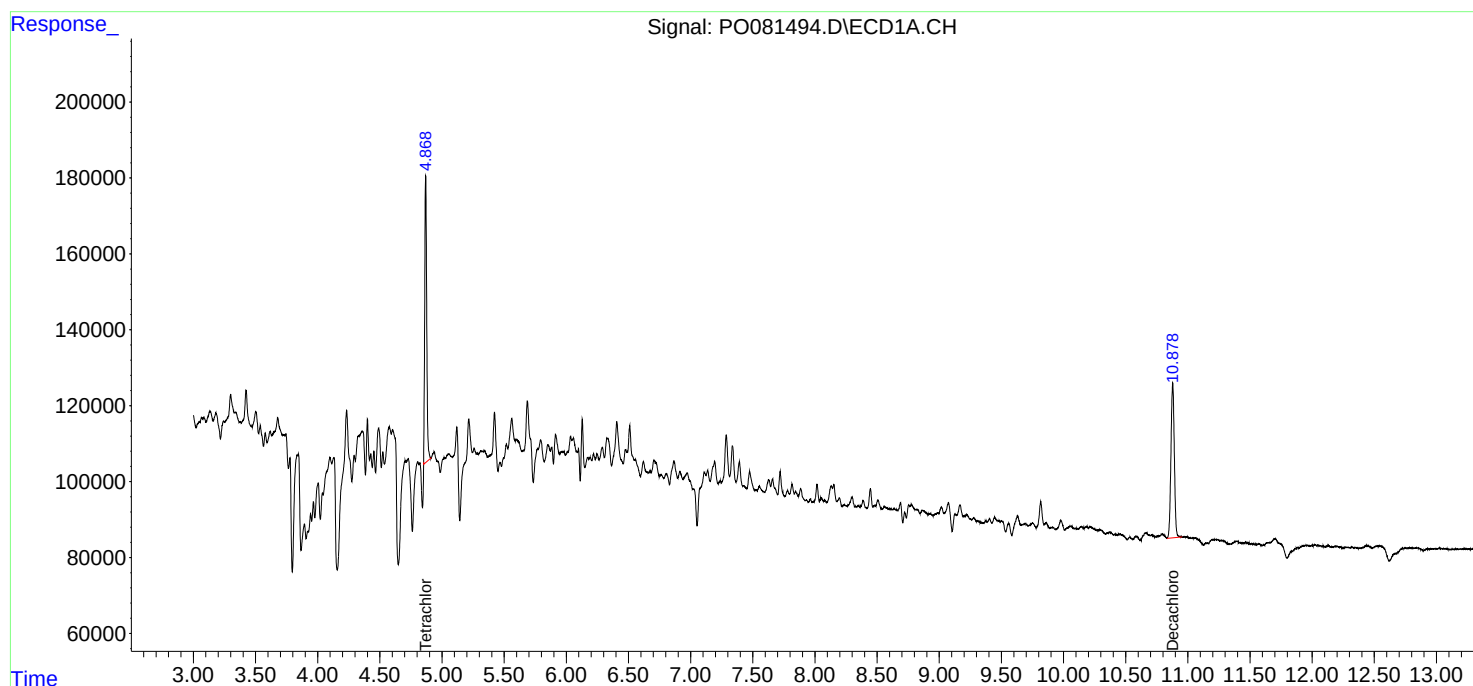


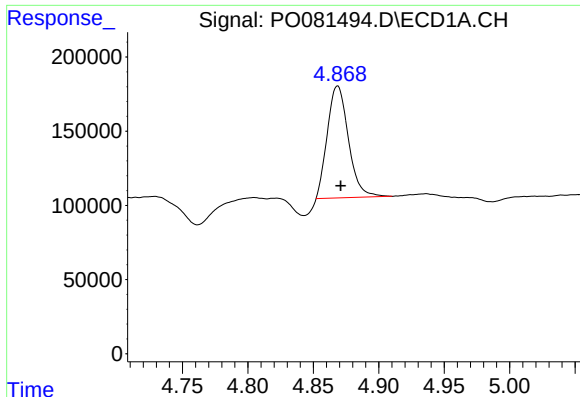

#1 Tetrachloro-m-xylene


R.T.: 4.868 min
Delta R.T.: -0.003 min
Response: 846349
Conc: 9.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
20882

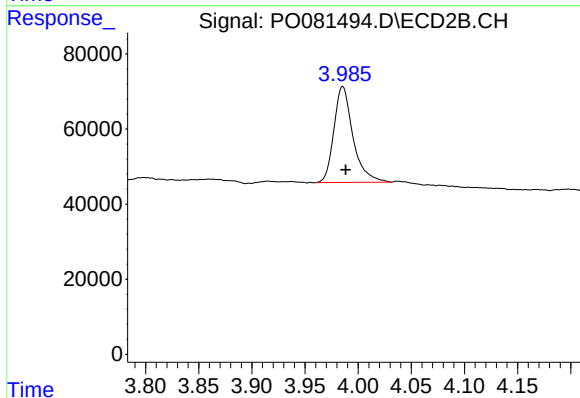


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: -0.003 min
Response: 319566
Conc: 11.99 ng/ml

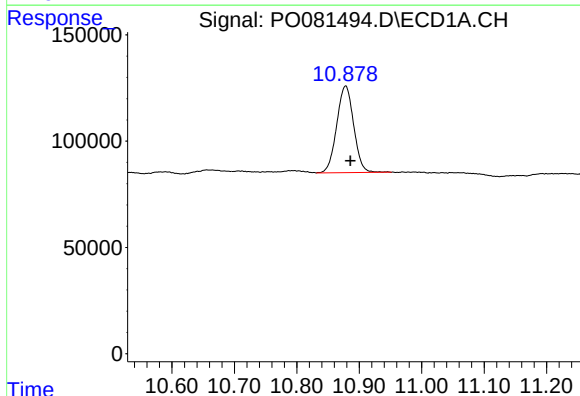

#2 Decachlorobiphenyl

R.T.: 10.878 min
Delta R.T.: -0.008 min
Response: 769188
Conc: 10.33 ng/ml

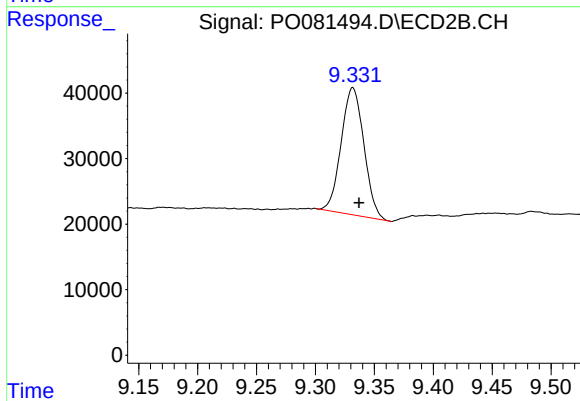

#2 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: -0.005 min
Response: 260576
Conc: 11.22 ng/ml