

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092421\
 Data File : P0081538.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2021 9:55
 Operator : AJ\MA
 Sample : M3846-09 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF580H-5-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 04:45:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.869	3.984	171829	45840	1.927	1.721
2) SA Decachlor...	10.880	9.329	145175	48756	1.949	2.099

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092421\
Data File : P0081538.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2021 9:55
Operator : AJ\MA
Sample : M3846-09 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEF580H-5-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 04:45:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

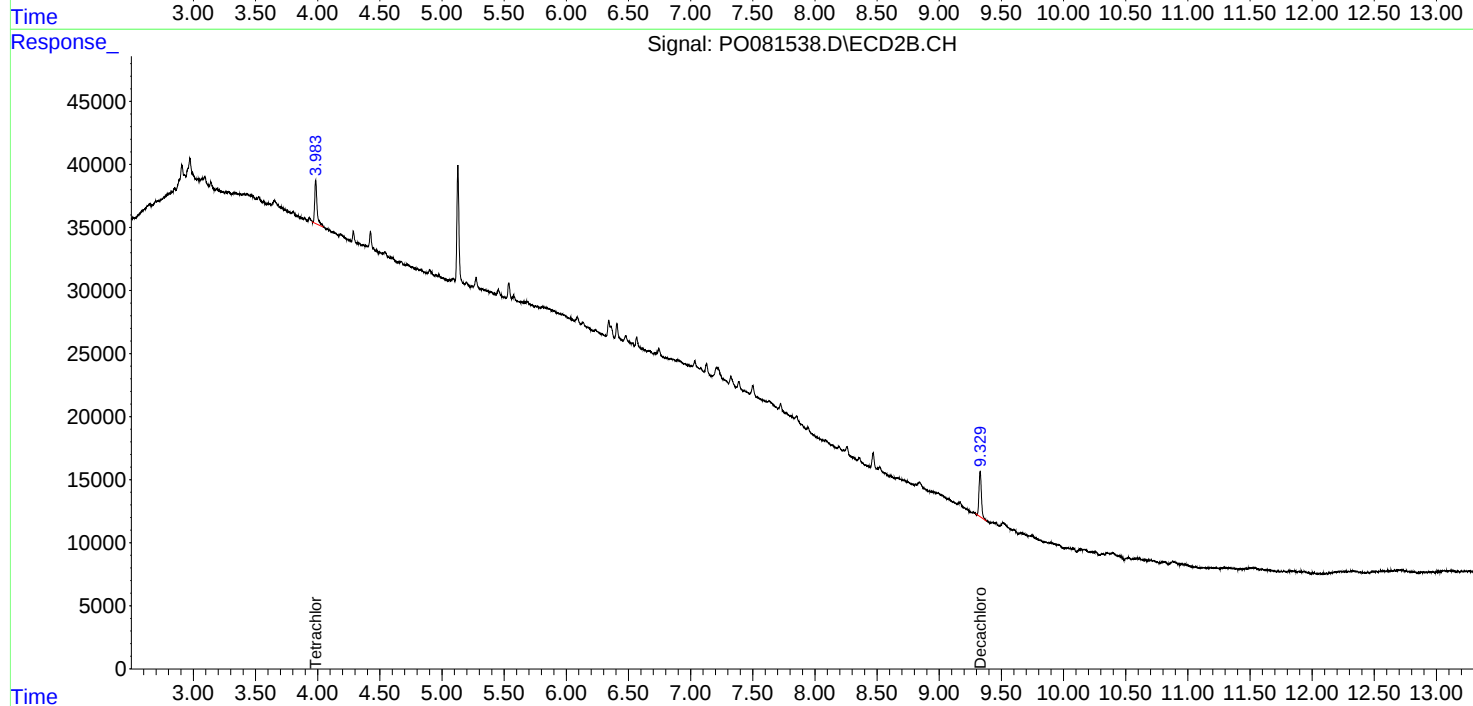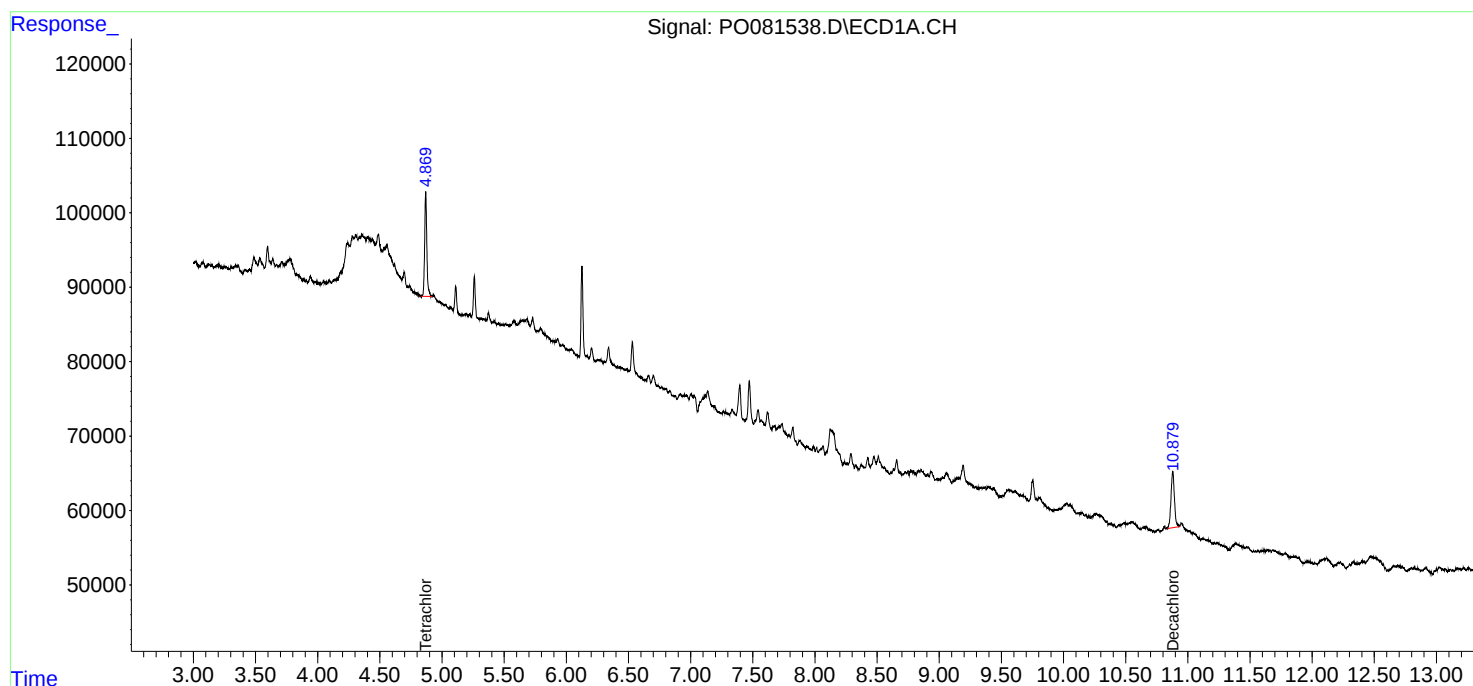


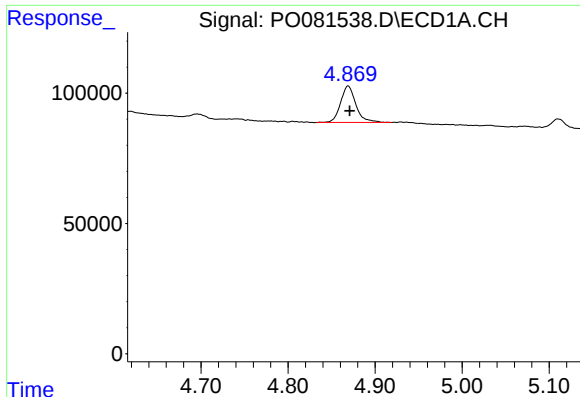

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 171829
Conc: 1.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF580H-5-1

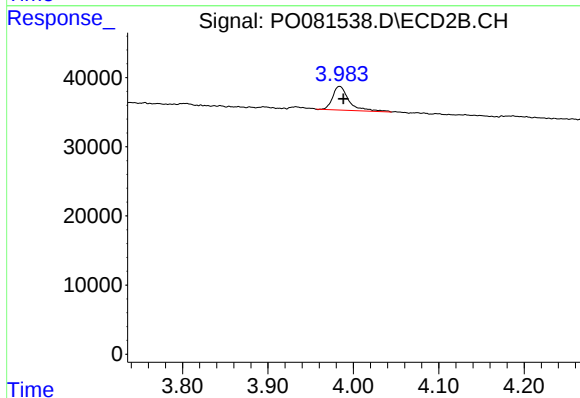


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.004 min
Response: 45840
Conc: 1.72 ng/ml

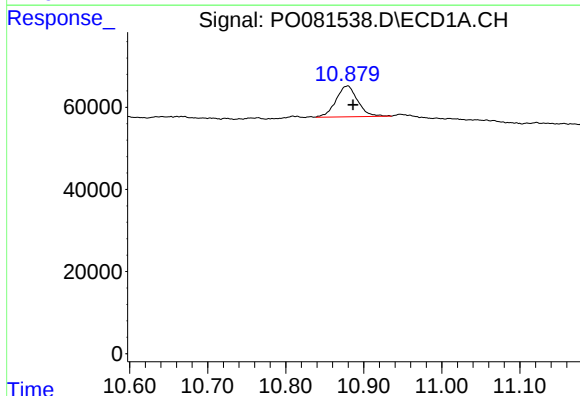

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 145175
Conc: 1.95 ng/ml

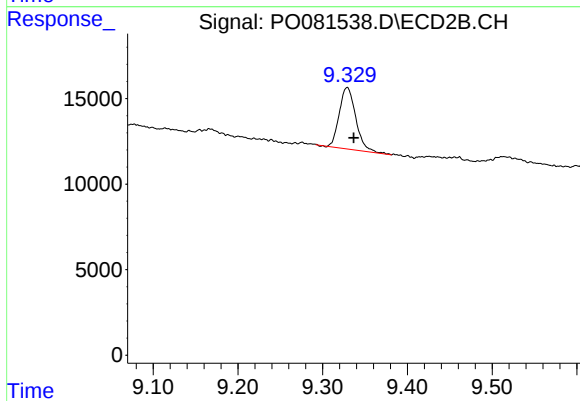

#2 Decachlorobiphenyl

R.T.: 9.329 min
Delta R.T.: -0.008 min
Response: 48756
Conc: 2.10 ng/ml