

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092421\
 Data File : P0081553.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2021 15:41
 Operator : AJ\MA
 Sample : M3846-03 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEF580H-2-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:32:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 02:21:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.871	3.986	196416	46204	2.203	1.734
2) SA Decachlor...	10.882	9.333	179811	53457	2.414	2.302

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092421\
Data File : PO081553.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2021 15:41
Operator : AJ\MA
Sample : M3846-03 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEF580H-2-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:32:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 02:21:54 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

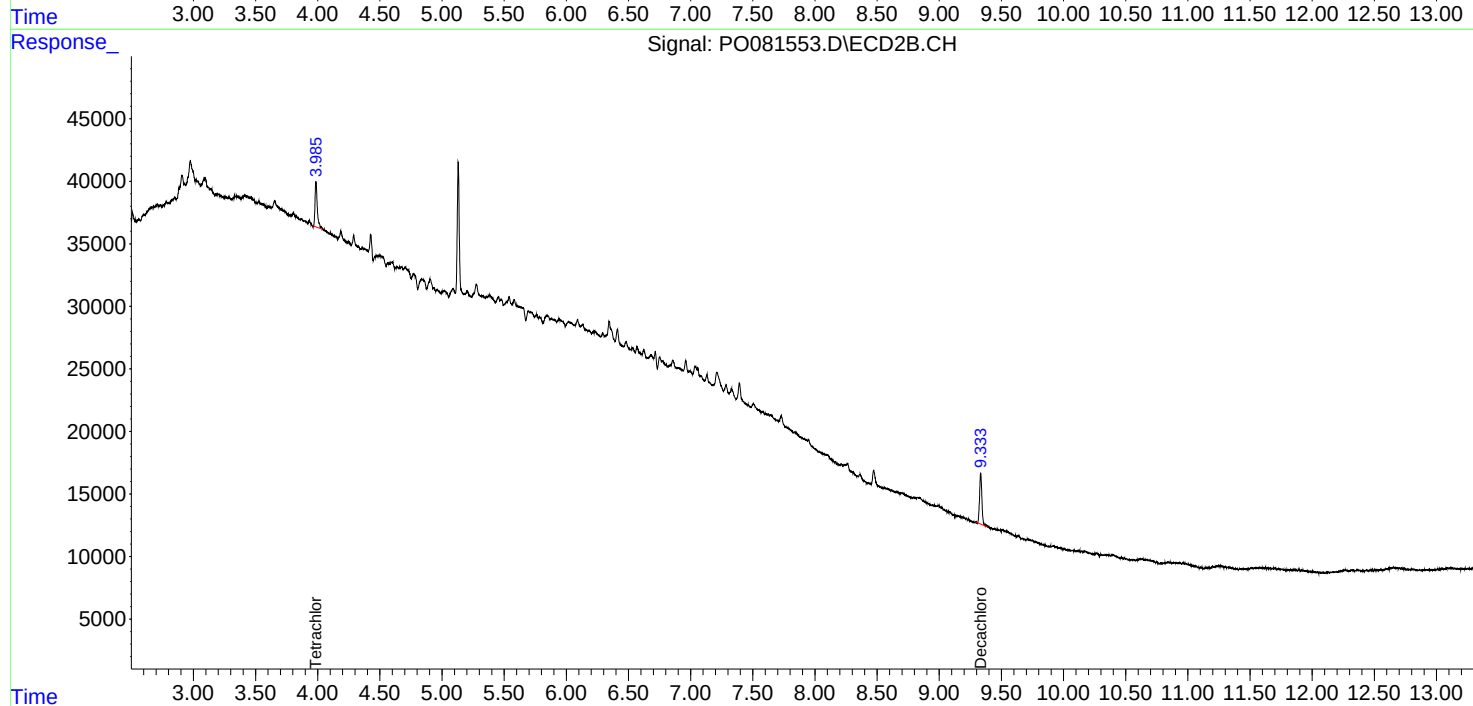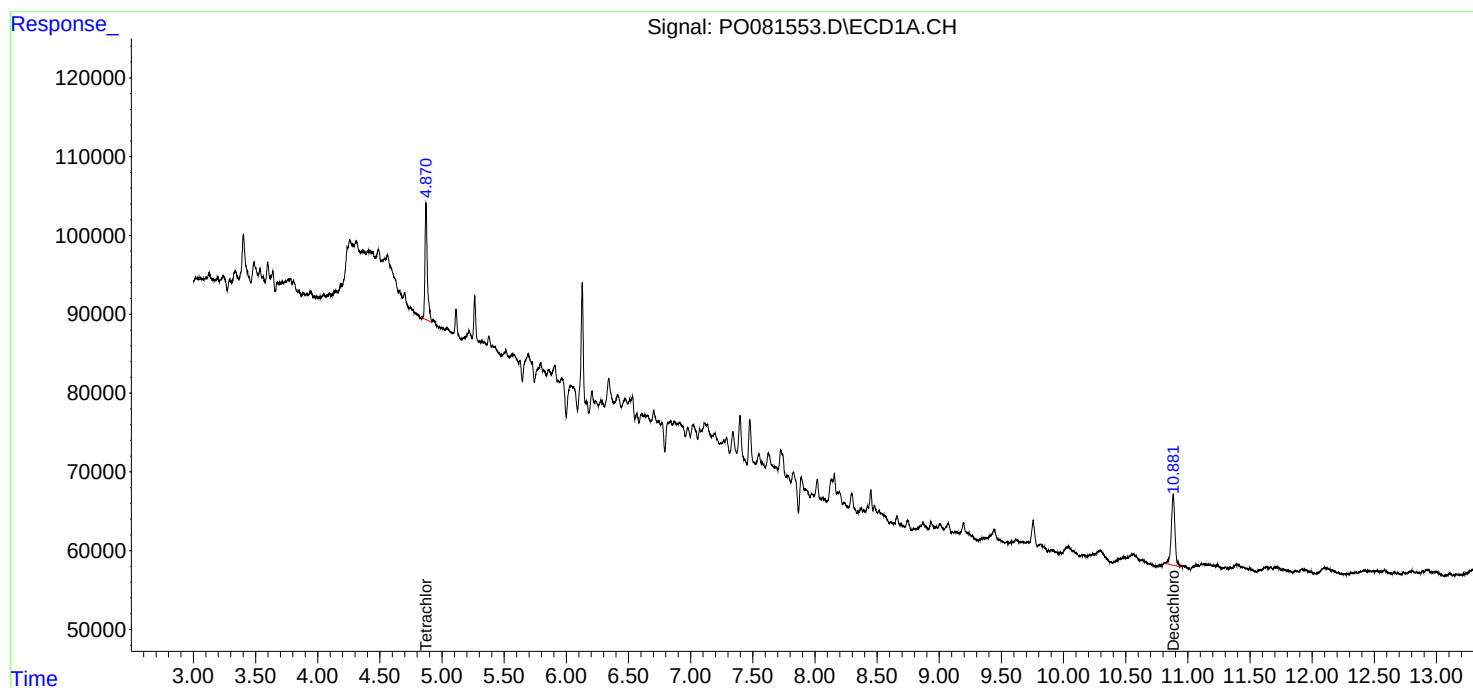


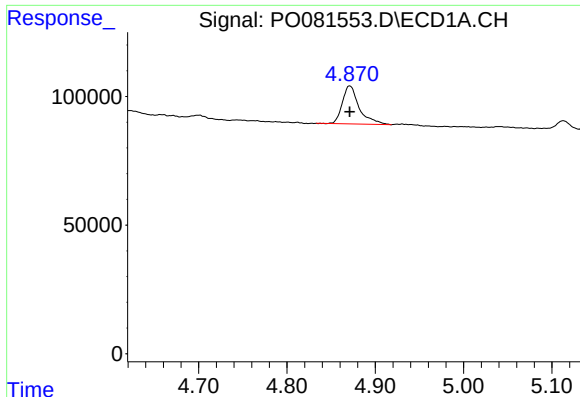

#1 Tetrachloro-m-xylene


R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 196416
Conc: 2.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEF580H-2-1

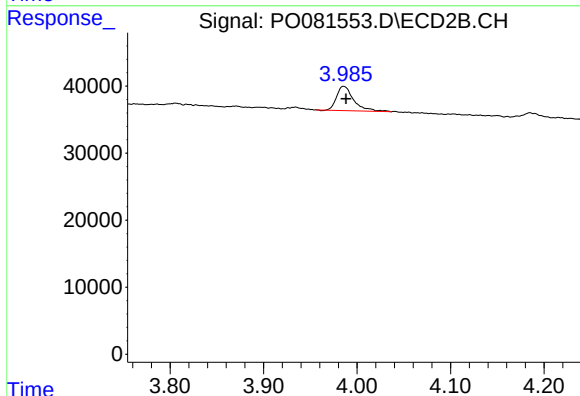


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: -0.003 min
Response: 46204
Conc: 1.73 ng/ml

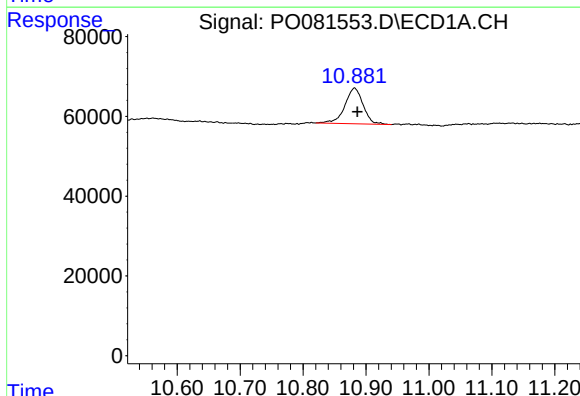

#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.004 min
Response: 179811
Conc: 2.41 ng/ml

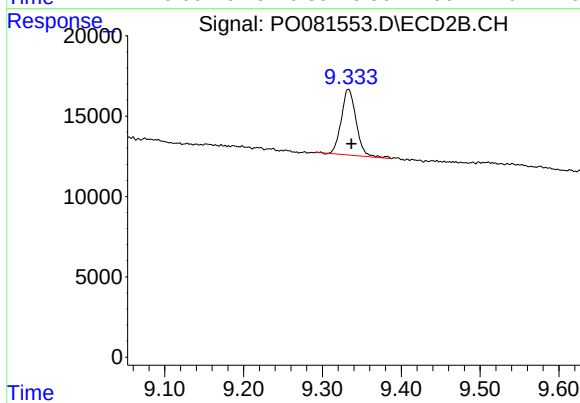

#2 Decachlorobiphenyl

R.T.: 9.333 min
Delta R.T.: -0.004 min
Response: 53457
Conc: 2.30 ng/ml