

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092425\
 Data File : P0114012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 23:15
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 08:08:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.706f	3.654	109988	32482	0.012	0.006 #
2)	SA Decachlor...	8.662	8.620	550807	105605	0.082	0.051 #
Target Compounds							
3)	L1 AR-1016-1	4.749	4.725	1408212	202336	4.640	1.110 #
4)	L1 AR-1016-2	4.749	4.732	1408212	227204	3.095	0.821 #
5)	L1 AR-1016-3	4.802	4.917	881703	2180633	2.947	14.601 #
6)	L1 AR-1016-4	4.931	4.962	1712378	3139752	7.124	26.011 #
7)	L1 AR-1016-5	5.217	5.173	39232078	1531078	163.398	10.203 #
8)	L2 AR-1221-1	3.886	3.858	80982	45638	0.836	0.674
9)	L2 AR-1221-2	3.951	3.953	205197	292827	2.854	5.746 #
10)	L2 AR-1221-3	4.043	4.031	265448	182471	1.121	1.165
11)	L3 AR-1232-1	4.043	4.031	265448	182471	1.516	1.541
12)	L3 AR-1232-2	4.488	4.732	994080	227204	10.360	1.850 #
13)	L3 AR-1232-3	4.749	4.917	1408212	2180633	7.147	32.769 #
14)	L3 AR-1232-4	4.931	4.999	1712378	2455048	17.343	41.866 #
15)	L3 AR-1232-5	4.946	5.166	4876045	4557799	74.718	74.069
16)	L4 AR-1242-1	4.749	4.725	1408212	202336	6.338	1.483 #
17)	L4 AR-1242-2	4.749	4.732	1408212	227204	4.190	1.096 #
18)	L4 AR-1242-3	4.802	4.917	881703	2180633	4.101	18.797 #
19)	L4 AR-1242-4	4.931	4.999	1712378	2455048	9.790	21.349 #
20)	L4 AR-1242-5	5.606	5.502	34114595	4660317	162.935	32.854 #
21)	L5 AR-1248-1	4.749	4.725	1408212	202336	7.812	1.851 #
22)	L5 AR-1248-2	4.946	4.962	4876045	3139752	20.048	19.925
23)	L5 AR-1248-3	5.217	4.999	39232078	2455048	120.906	14.708 #
24)	L5 AR-1248-4	5.529	5.166	17152172	4557799	34.282	23.459 #
25)	L5 AR-1248-5	5.567	5.565	23756193	3088972	70.245	15.233 #
26)	L6 AR-1254-1	5.529	5.502	17152172	4660317	31.459	15.411 #
27)	L6 AR-1254-2	5.713	5.683	60557319	21800425	119.105	82.553 #
28)	L6 AR-1254-3	6.113	6.078	53167402	15439406	67.980	39.862 #
29)	L6 AR-1254-4	6.341	6.306	3712244	1199251	6.788	5.052 #
30)	L6 AR-1254-5	6.740	6.703	6116.4E6	2369.1E6	8217.280	7717.502
31)	L7 AR-1260-1	6.229	6.195	4871776	2366144	9.938	9.416
32)	L7 AR-1260-2	6.419	6.383	11721639	6126129	15.306	18.530
33)	L7 AR-1260-3	6.740f	6.510	6116.4E6	-10536522	9090.838	N.D. #
34)	L7 AR-1260-4	7.045	7.006	393007	98552	0.908	0.515 #
35)	L7 AR-1260-5	7.274	7.252	1397718	72942	1.234	0.171 #
36)	L8 AR-1262-1	6.740f	6.703f	6116.4E6	2369.1E6	6163.161	6470.142
37)	L8 AR-1262-2	7.274	7.252	1397718	72942	0.882	0.160 #
38)	L8 AR-1262-3	7.566	7.541	613358	1320073	1.097	7.578 #
39)	L8 AR-1262-4	7.627	7.593	1097607	145128	1.097	0.522 #
40)	L8 AR-1262-5	8.126	8.075	624713	201744	1.565	1.775
41)	L9 AR-1268-1	7.566	7.541	613358	1320073	0.346	2.704 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092425\
 Data File : P0114012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 23:15
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 08:08:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.627	7.593	1097607	145128	0.737	0.364 #
43) L9	AR-1268-3	7.827	7.804	762369	60824	0.623	0.186 #
44) L9	AR-1268-4	8.126	8.075	624713	201744	1.374	1.591
45) L9	AR-1268-5	8.417	8.365	107698	148994	0.035	0.169 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092425\
Data File : PO114012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2025 23:15
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 08:08:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

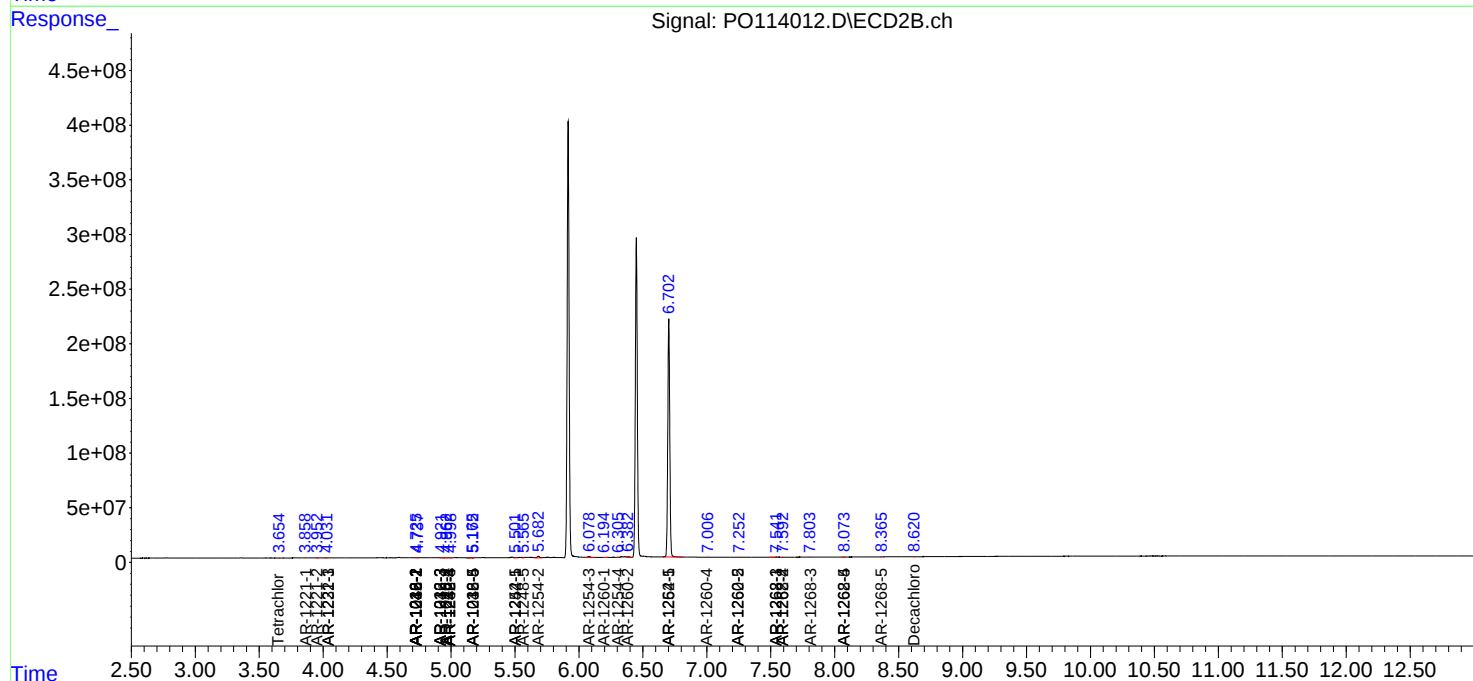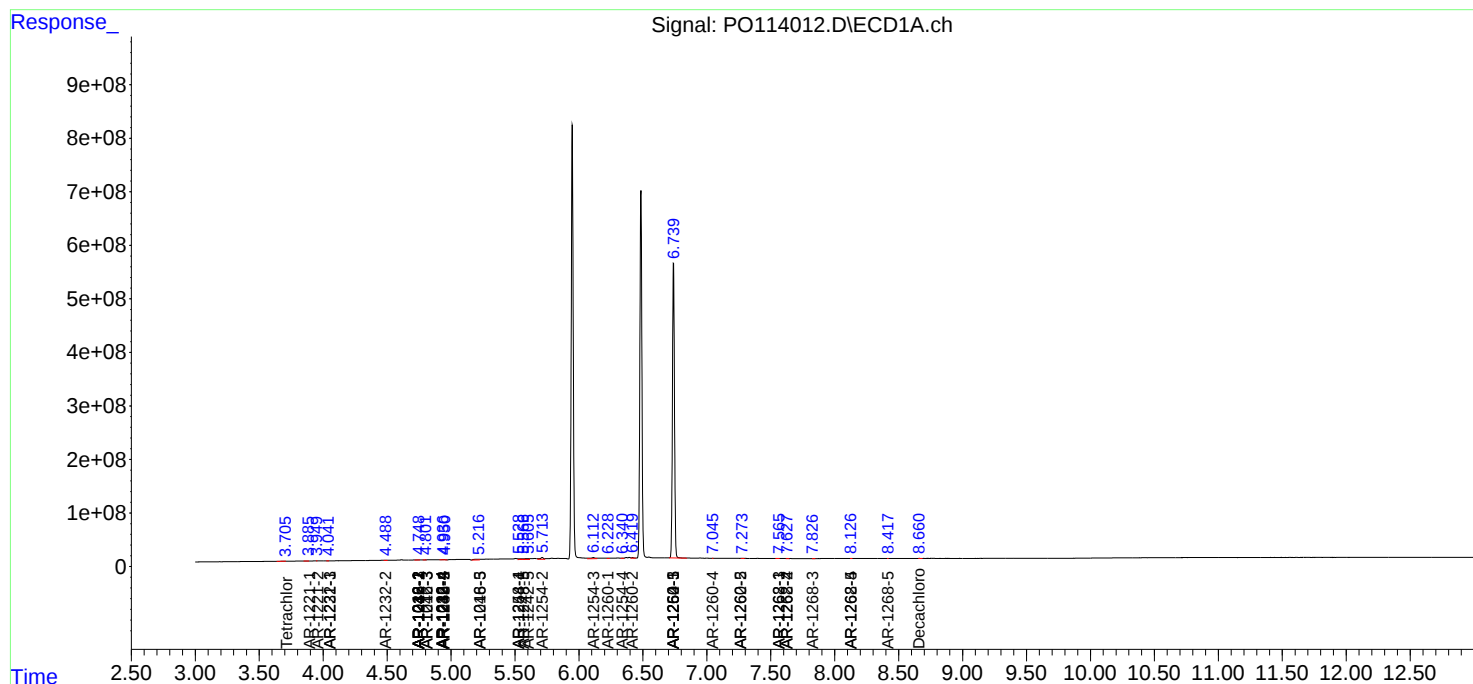


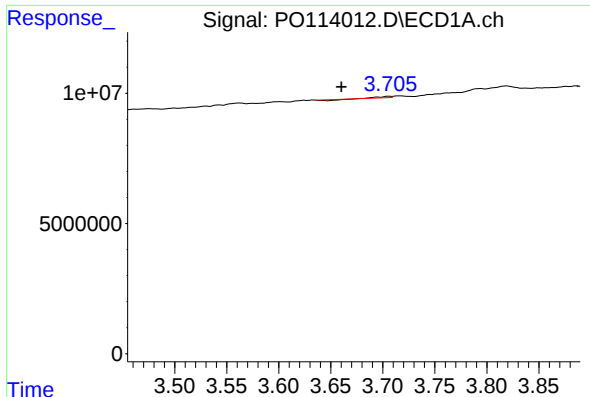

#1 Tetrachloro-m-xylene


R.T.: 3.706 min
Delta R.T.: 0.046 min
Response: 109988
Conc: 0.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

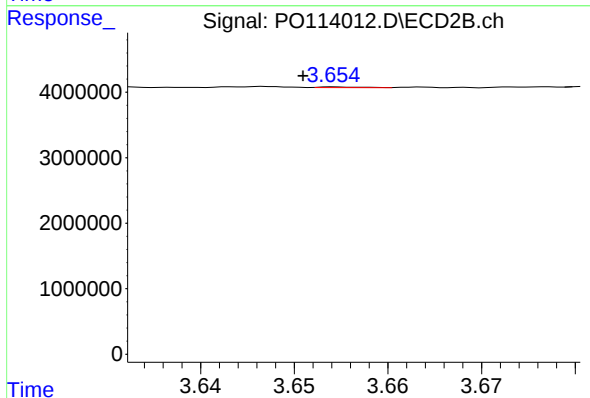


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: 0.003 min
Response: 32482
Conc: 0.01 ng/ml

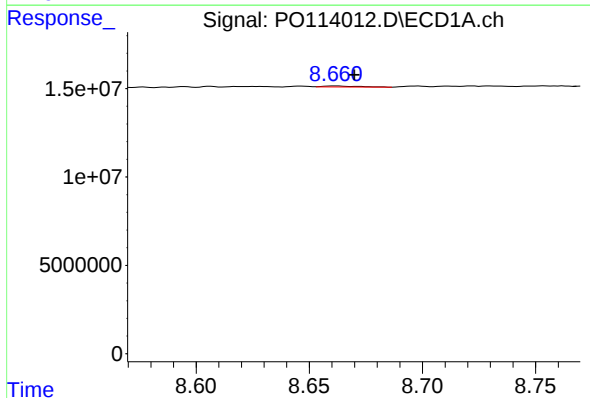


#2 Decachlorobiphenyl

R.T.: 8.662 min
Delta R.T.: -0.008 min
Response: 550807
Conc: 0.08 ng/ml

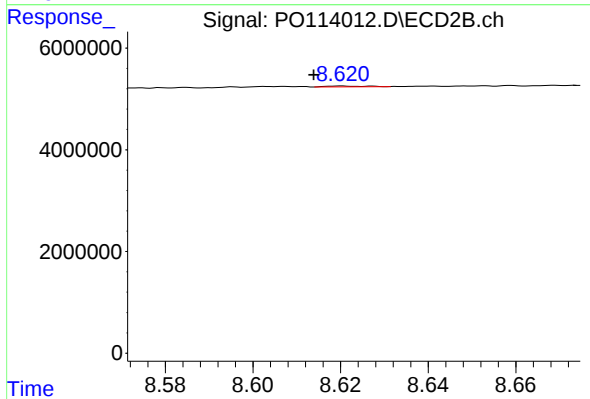

#2 Decachlorobiphenyl


R.T.: 8.620 min
Delta R.T.: 0.006 min
Response: 105605
Conc: 0.05 ng/ml

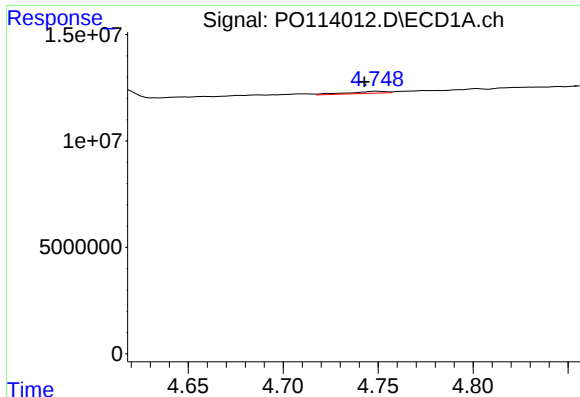

#3 AR-1016-1


R.T.: 4.749 min
Delta R.T.: 0.006 min
Response: 1408212
Conc: 4.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

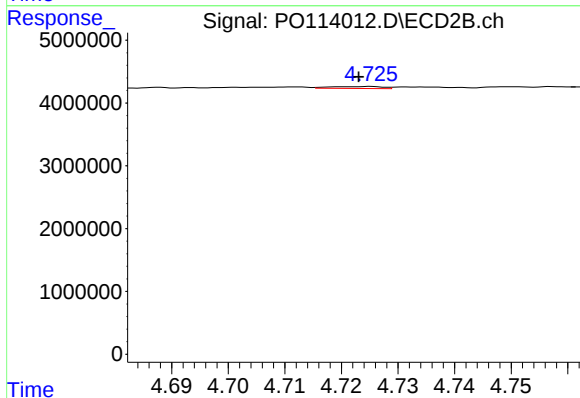


#3 AR-1016-1

R.T.: 4.725 min
Delta R.T.: 0.002 min
Response: 202336
Conc: 1.11 ng/ml

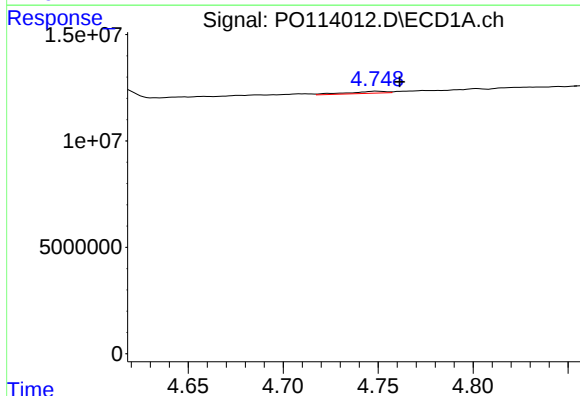


#4 AR-1016-2

R.T.: 4.749 min
Delta R.T.: -0.012 min
Response: 1408212
Conc: 3.09 ng/ml

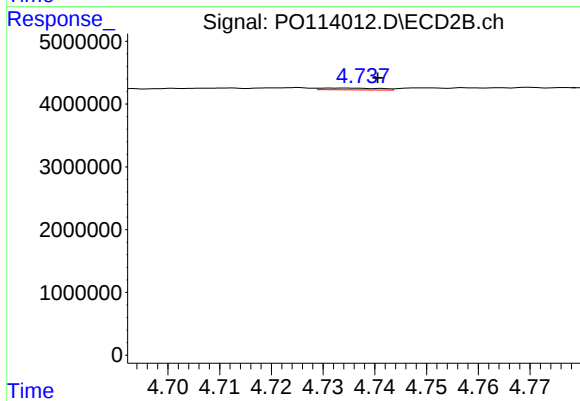

#4 AR-1016-2


R.T.: 4.732 min
Delta R.T.: -0.009 min
Response: 227204
Conc: 0.82 ng/ml

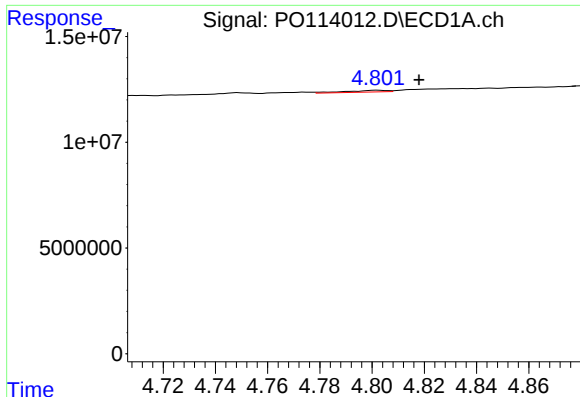

#5 AR-1016-3


R.T.: 4.802 min
Delta R.T.: -0.016 min
Response: 881703
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

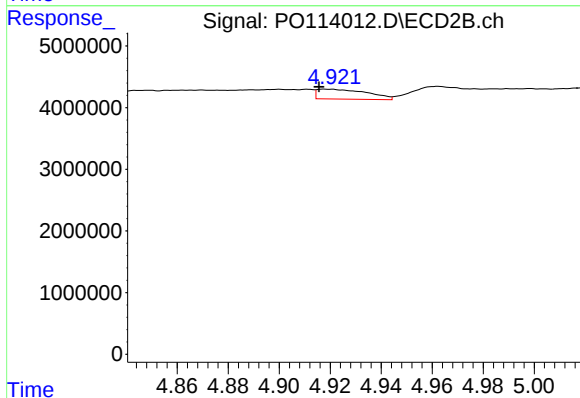


#5 AR-1016-3

R.T.: 4.917 min
Delta R.T.: 0.002 min
Response: 2180633
Conc: 14.60 ng/ml

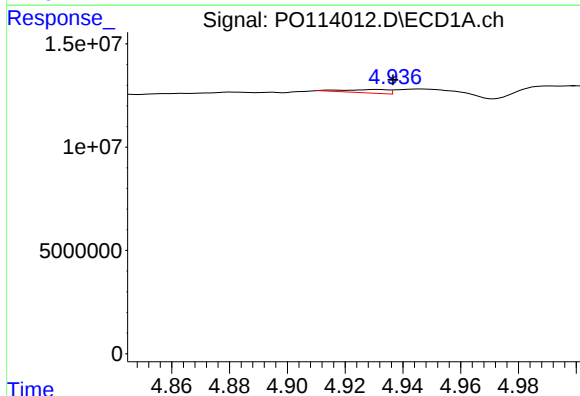


#6 AR-1016-4

R.T.: 4.931 min
Delta R.T.: -0.005 min
Response: 1712378
Conc: 7.12 ng/ml

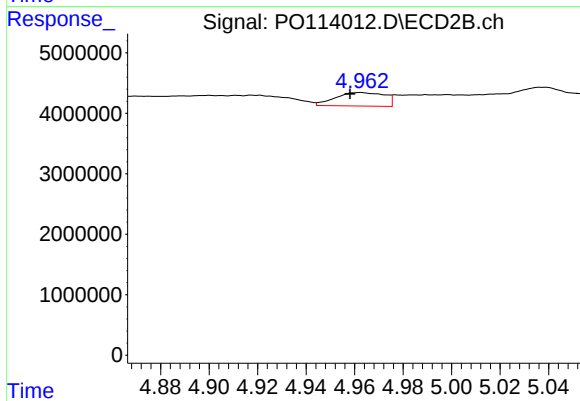

#6 AR-1016-4


R.T.: 4.962 min
Delta R.T.: 0.004 min
Response: 3139752
Conc: 26.01 ng/ml

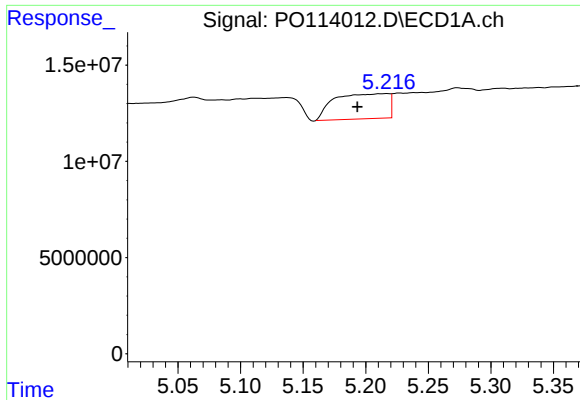

#7 AR-1016-5


R.T.: 5.217 min
Delta R.T.: 0.024 min
Response: 39232078
Conc: 163.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

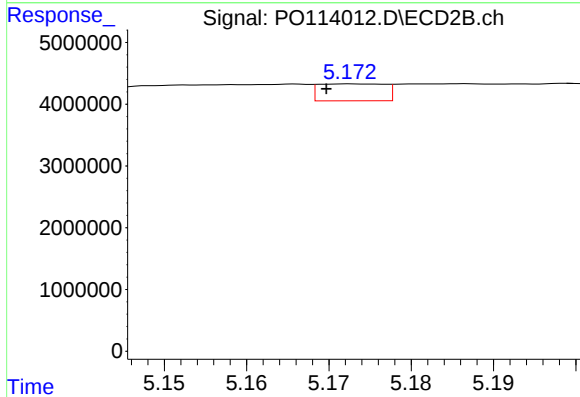


#7 AR-1016-5

R.T.: 5.173 min
Delta R.T.: 0.003 min
Response: 1531078
Conc: 10.20 ng/ml

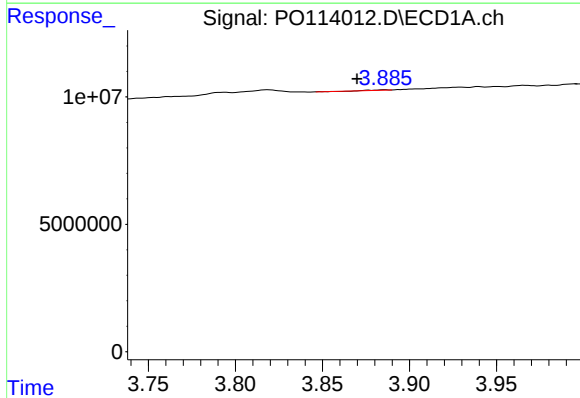


#8 AR-1221-1

R.T.: 3.886 min
Delta R.T.: 0.016 min
Response: 80982
Conc: 0.84 ng/ml

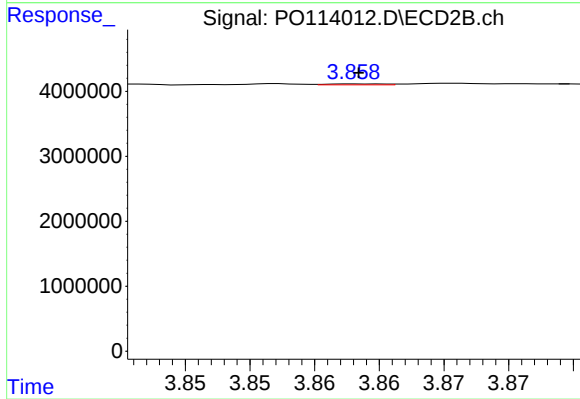

#8 AR-1221-1


R.T.: 3.858 min
Delta R.T.: 0.000 min
Response: 45638
Conc: 0.67 ng/ml

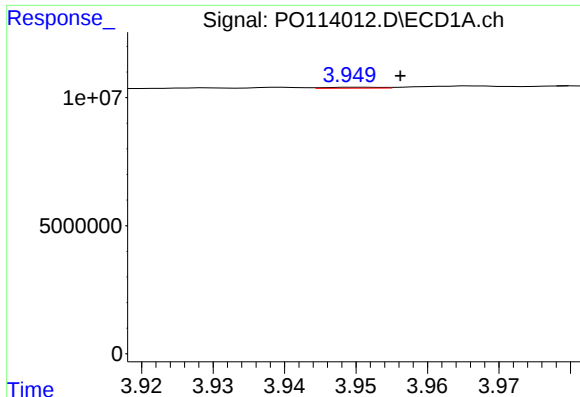

#9 AR-1221-2


R.T.: 3.951 min
Delta R.T.: -0.006 min
Response: 205197
Conc: 2.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

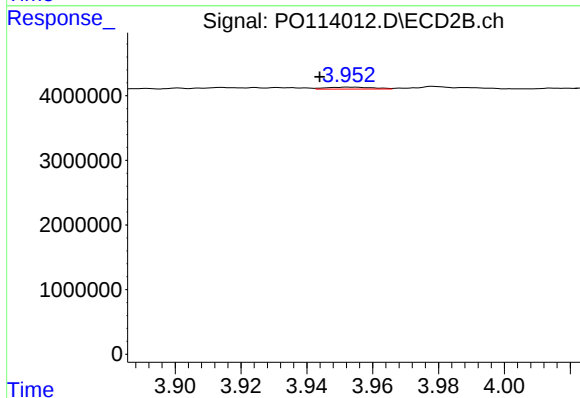


#9 AR-1221-2

R.T.: 3.953 min
Delta R.T.: 0.009 min
Response: 292827
Conc: 5.75 ng/ml

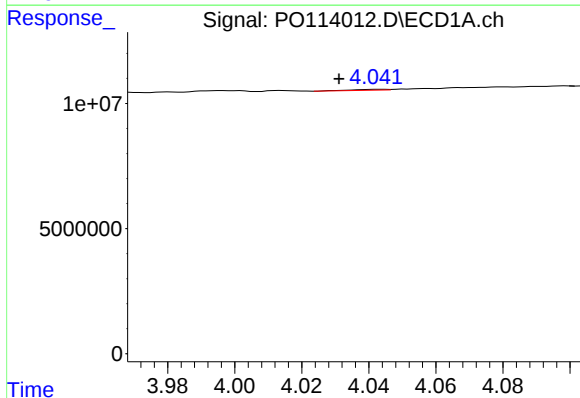


#10 AR-1221-3

R.T.: 4.043 min
Delta R.T.: 0.012 min
Response: 265448
Conc: 1.12 ng/ml

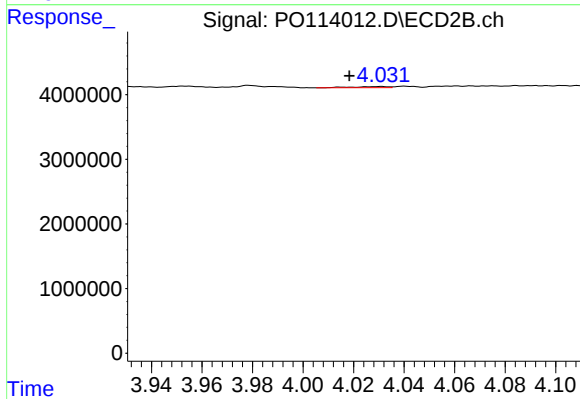

#10 AR-1221-3


R.T.: 4.031 min
Delta R.T.: 0.013 min
Response: 182471
Conc: 1.17 ng/ml

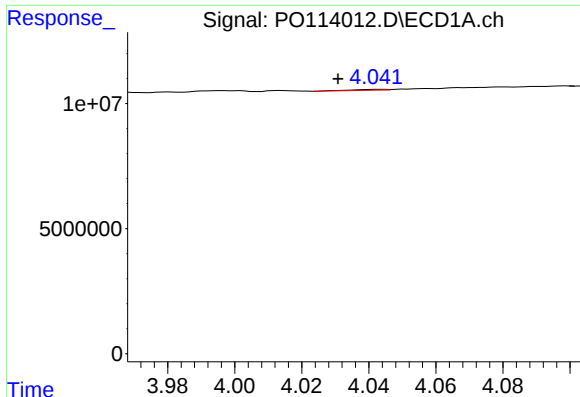

#11 AR-1232-1


R.T.: 4.043 min
Delta R.T.: 0.012 min
Response: 265448
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

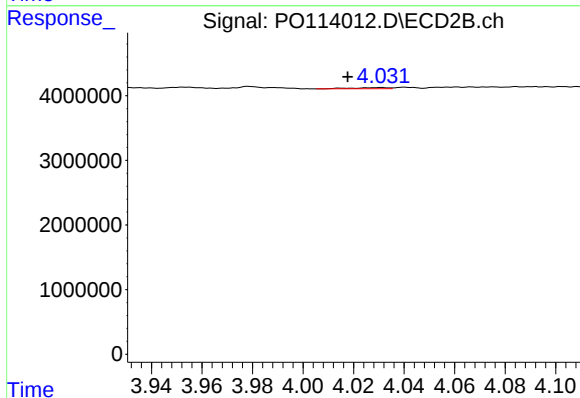


#11 AR-1232-1

R.T.: 4.031 min
Delta R.T.: 0.013 min
Response: 182471
Conc: 1.54 ng/ml

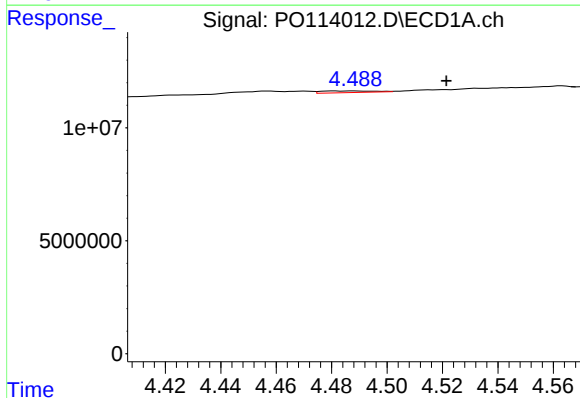


#12 AR-1232-2

R.T.: 4.488 min
Delta R.T.: -0.033 min
Response: 994080
Conc: 10.36 ng/ml

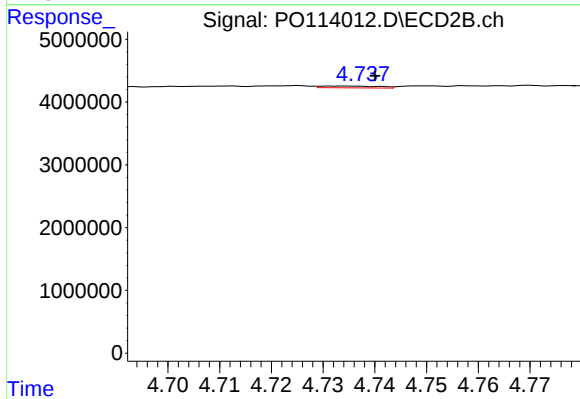

#12 AR-1232-2


R.T.: 4.732 min
Delta R.T.: -0.008 min
Response: 227204
Conc: 1.85 ng/ml

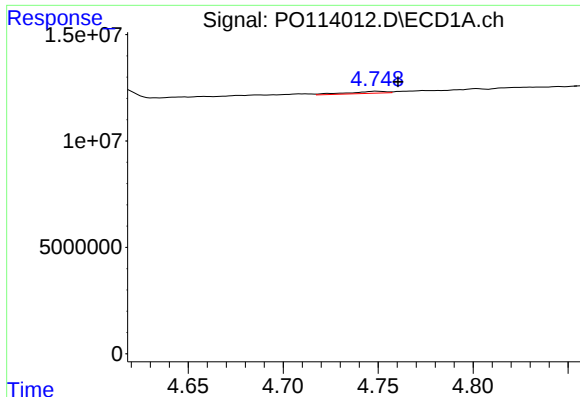

#13 AR-1232-3


R.T.: 4.749 min
Delta R.T.: -0.011 min
Response: 1408212
Conc: 7.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

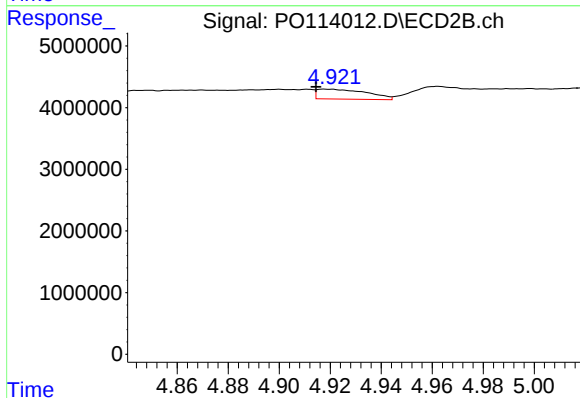


#13 AR-1232-3

R.T.: 4.917 min
Delta R.T.: 0.003 min
Response: 2180633
Conc: 32.77 ng/ml

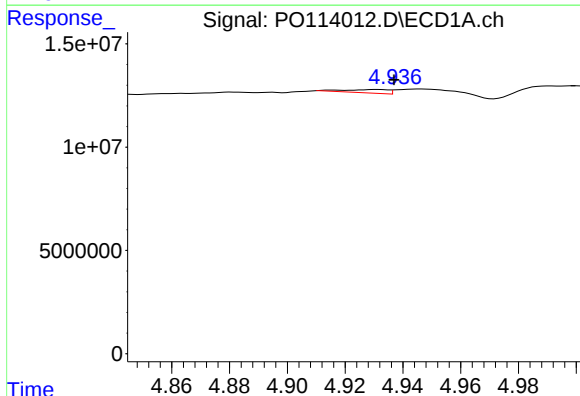


#14 AR-1232-4

R.T.: 4.931 min
Delta R.T.: -0.006 min
Response: 1712378
Conc: 17.34 ng/ml

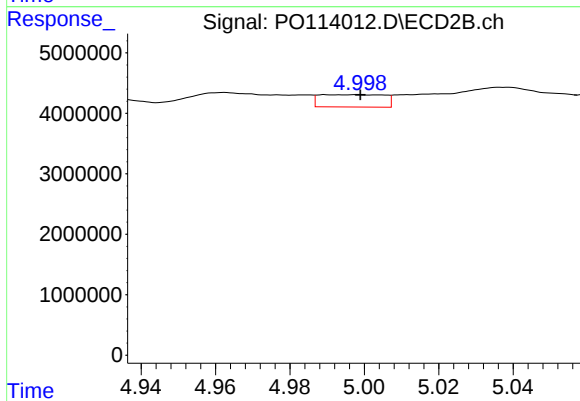

#14 AR-1232-4


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 2455048
Conc: 41.87 ng/ml

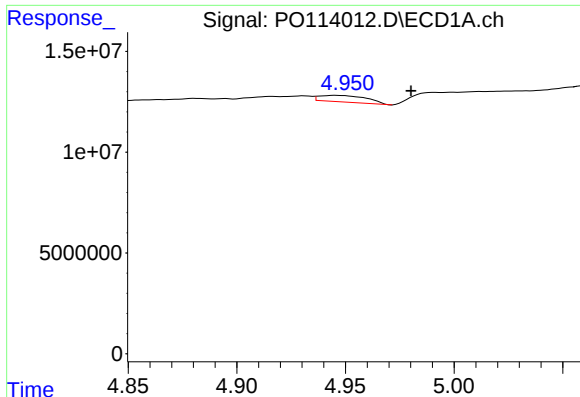

#15 AR-1232-5


R.T.: 4.946 min
Delta R.T.: -0.034 min
Response: 4876045
Conc: 74.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

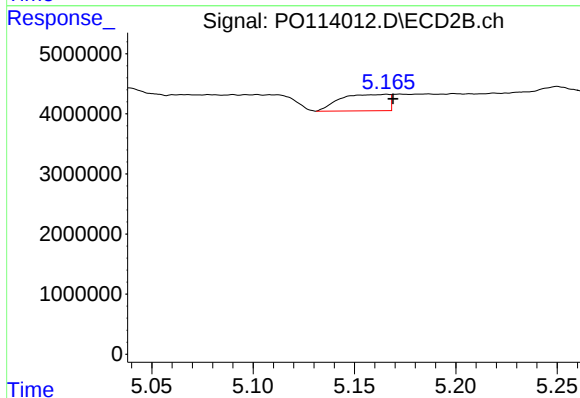


#15 AR-1232-5

R.T.: 5.166 min
Delta R.T.: -0.003 min
Response: 4557799
Conc: 74.07 ng/ml

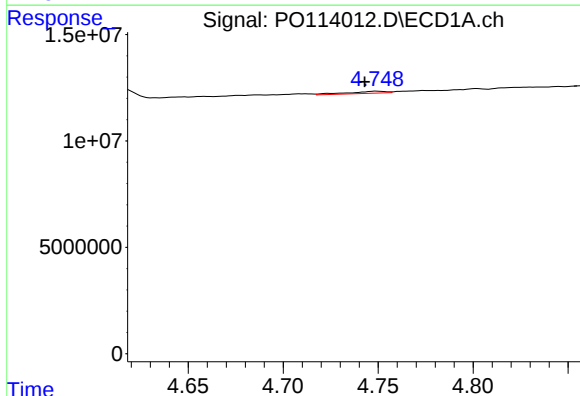


#16 AR-1242-1

R.T.: 4.749 min
Delta R.T.: 0.006 min
Response: 1408212
Conc: 6.34 ng/ml

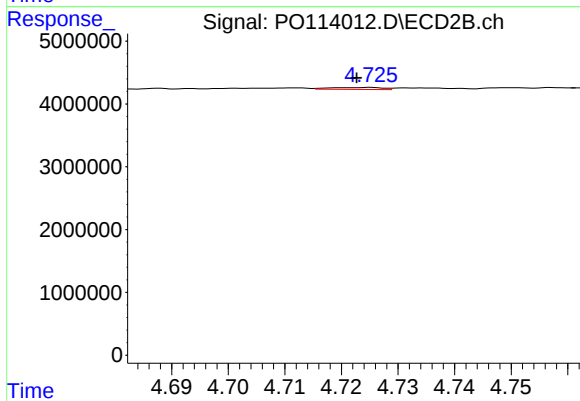

#16 AR-1242-1


R.T.: 4.725 min
Delta R.T.: 0.002 min
Response: 202336
Conc: 1.48 ng/ml

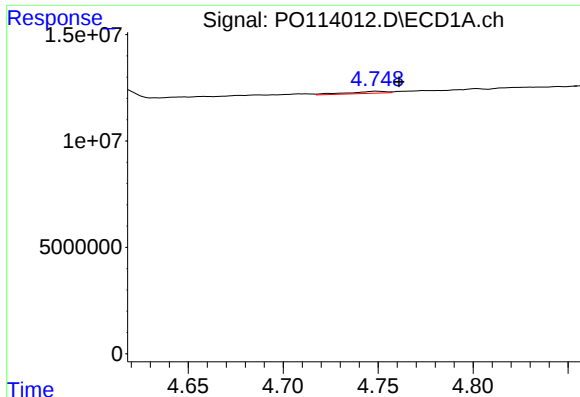

#17 AR-1242-2


R.T.: 4.749 min
Delta R.T.: -0.012 min
Response: 1408212
Conc: 4.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

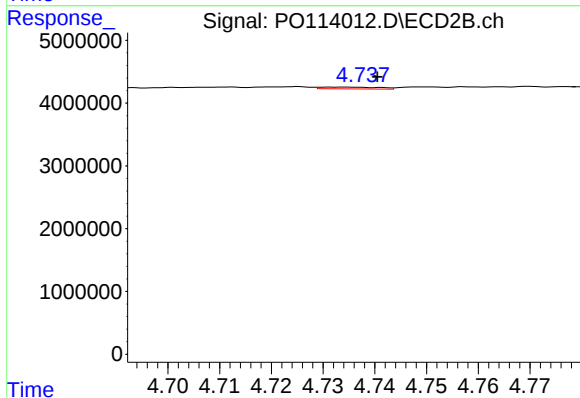


#17 AR-1242-2

R.T.: 4.732 min
Delta R.T.: -0.009 min
Response: 227204
Conc: 1.10 ng/ml

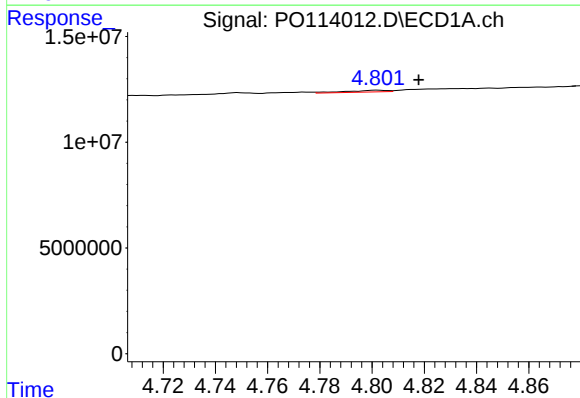


#18 AR-1242-3

R.T.: 4.802 min
Delta R.T.: -0.016 min
Response: 881703
Conc: 4.10 ng/ml

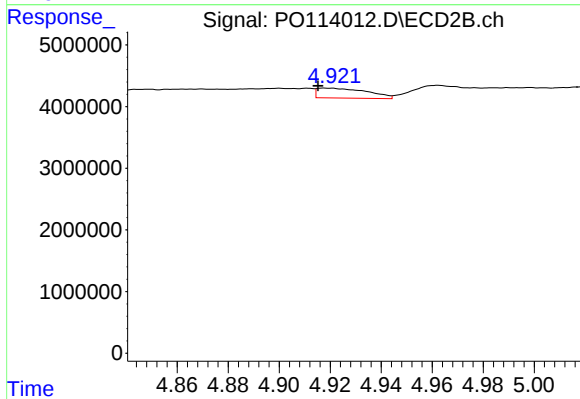

#18 AR-1242-3


R.T.: 4.917 min
Delta R.T.: 0.002 min
Response: 2180633
Conc: 18.80 ng/ml

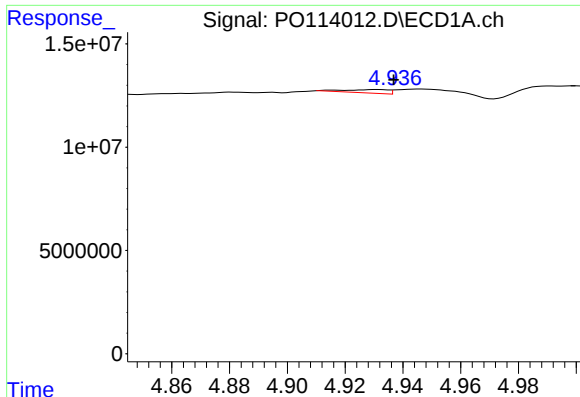

#19 AR-1242-4


R.T.: 4.931 min
Delta R.T.: -0.006 min
Response: 1712378
Conc: 9.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

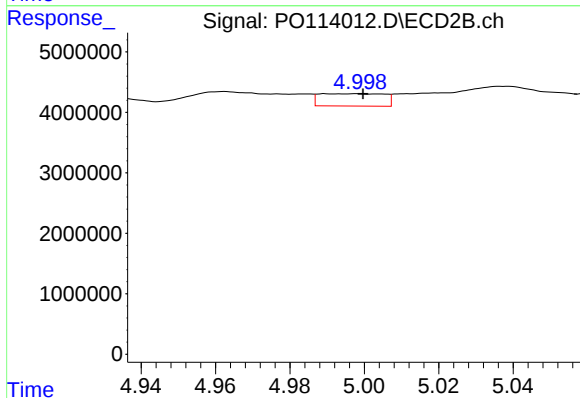


#19 AR-1242-4

R.T.: 4.999 min
Delta R.T.: -0.001 min
Response: 2455048
Conc: 21.35 ng/ml

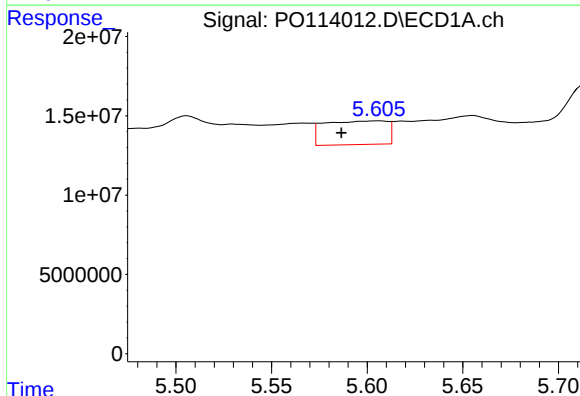


#20 AR-1242-5

R.T.: 5.606 min
Delta R.T.: 0.020 min
Response: 34114595
Conc: 162.94 ng/ml

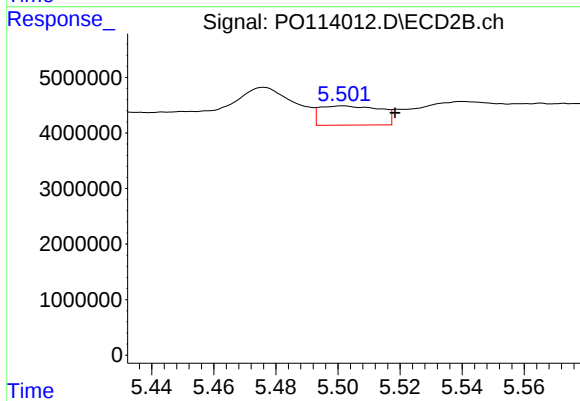

#20 AR-1242-5


R.T.: 5.502 min
Delta R.T.: -0.017 min
Response: 4660317
Conc: 32.85 ng/ml

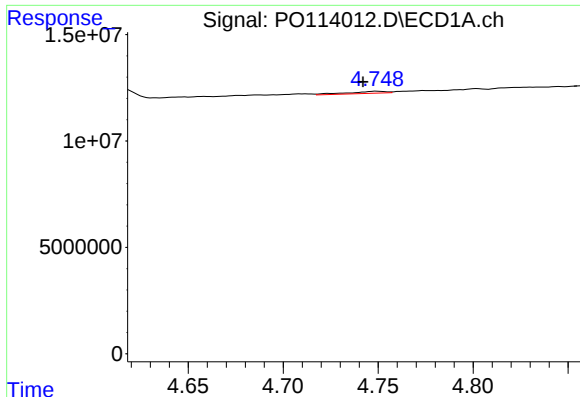

#21 AR-1248-1


R.T.: 4.749 min
Delta R.T.: 0.007 min
Response: 1408212
Conc: 7.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

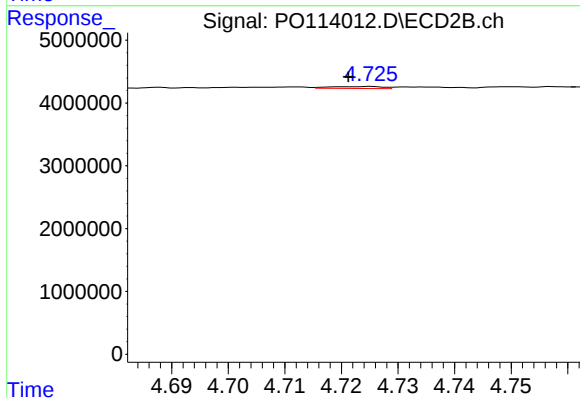


#21 AR-1248-1

R.T.: 4.725 min
Delta R.T.: 0.004 min
Response: 202336
Conc: 1.85 ng/ml

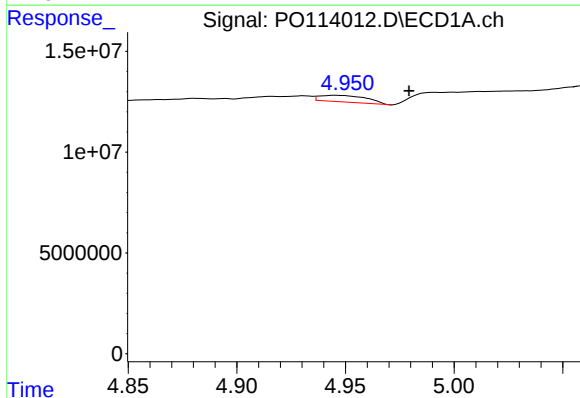


#22 AR-1248-2

R.T.: 4.946 min
Delta R.T.: -0.033 min
Response: 4876045
Conc: 20.05 ng/ml

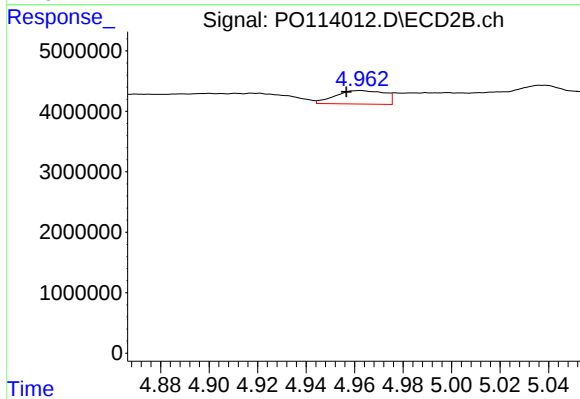

#22 AR-1248-2


R.T.: 4.962 min
Delta R.T.: 0.006 min
Response: 3139752
Conc: 19.93 ng/ml

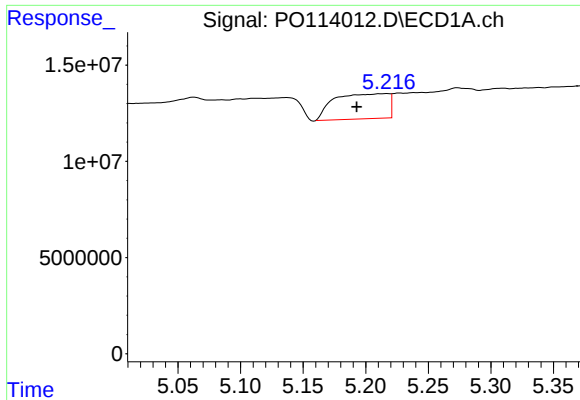

#23 AR-1248-3


R.T.: 5.217 min
Delta R.T.: 0.024 min
Response: 39232078
Conc: 120.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

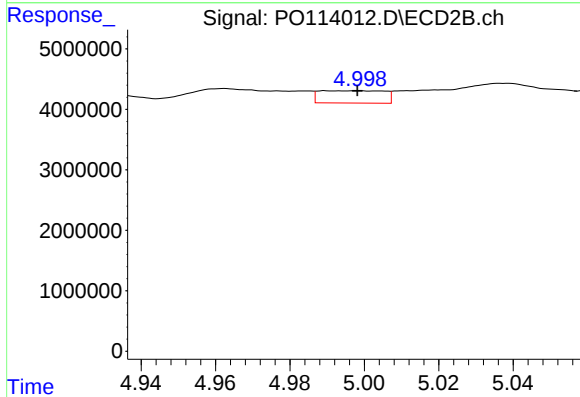


#23 AR-1248-3

R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 2455048
Conc: 14.71 ng/ml

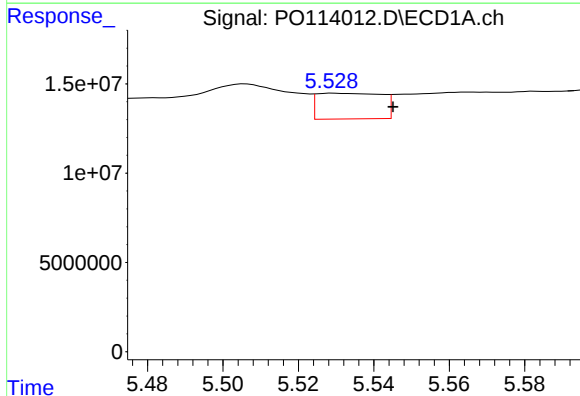


#24 AR-1248-4

R.T.: 5.529 min
Delta R.T.: -0.016 min
Response: 17152172
Conc: 34.28 ng/ml

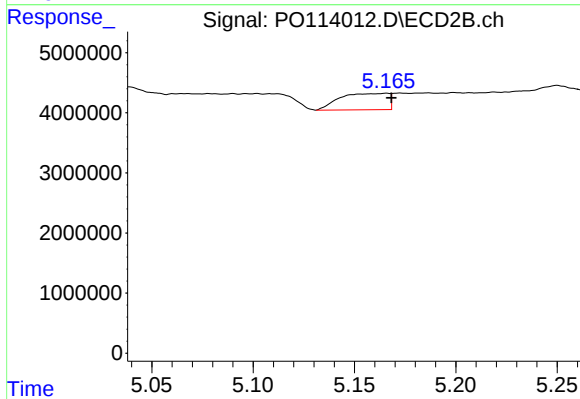

#24 AR-1248-4


R.T.: 5.166 min
Delta R.T.: -0.002 min
Response: 4557799
Conc: 23.46 ng/ml

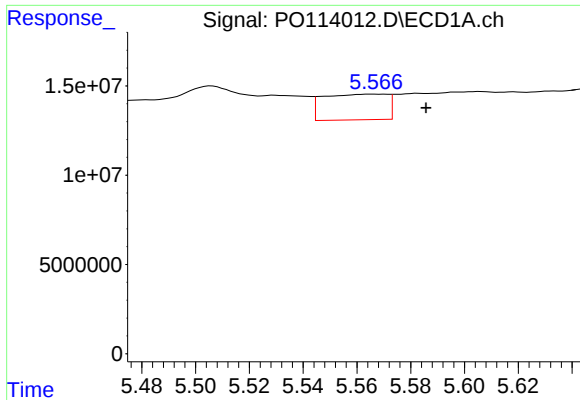

#25 AR-1248-5


R.T.: 5.567 min
Delta R.T.: -0.019 min
Response: 23756193
Conc: 70.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

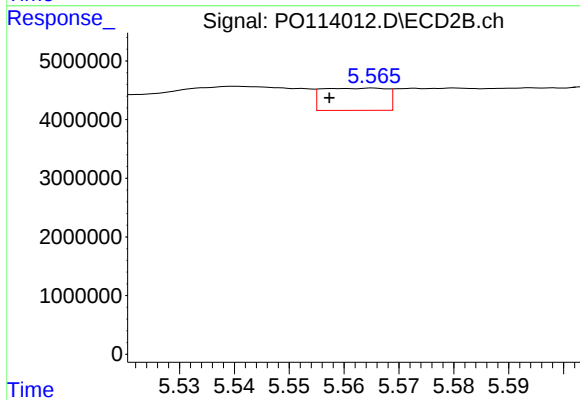


#25 AR-1248-5

R.T.: 5.565 min
Delta R.T.: 0.008 min
Response: 3088972
Conc: 15.23 ng/ml

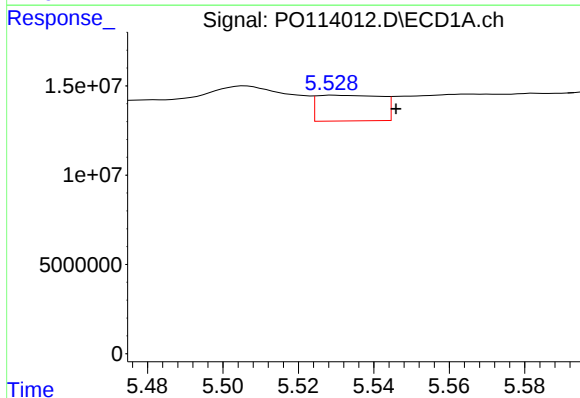


#26 AR-1254-1

R.T.: 5.529 min
Delta R.T.: -0.016 min
Response: 17152172
Conc: 31.46 ng/ml

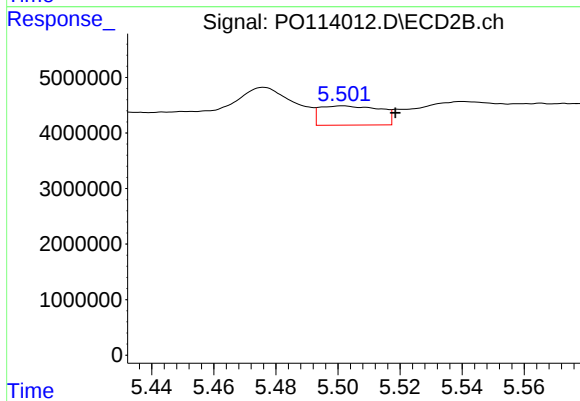

#26 AR-1254-1


R.T.: 5.502 min
Delta R.T.: -0.017 min
Response: 4660317
Conc: 15.41 ng/ml

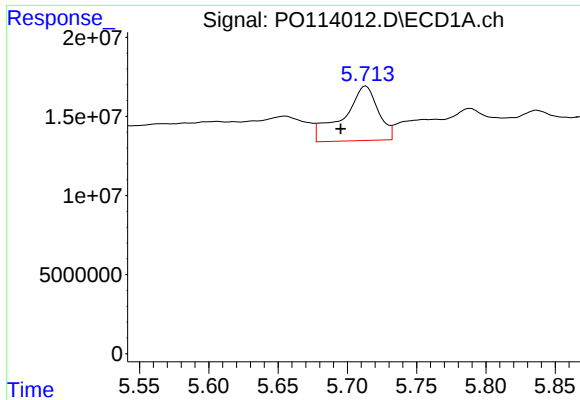

#27 AR-1254-2


R.T.: 5.713 min
Delta R.T.: 0.018 min
Response: 60557319
Conc: 119.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

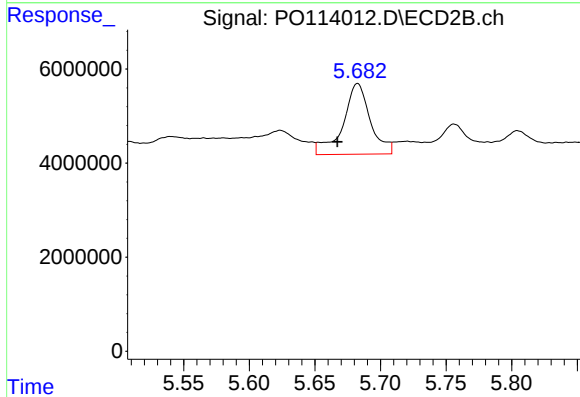


#27 AR-1254-2

R.T.: 5.683 min
Delta R.T.: 0.016 min
Response: 21800425
Conc: 82.55 ng/ml

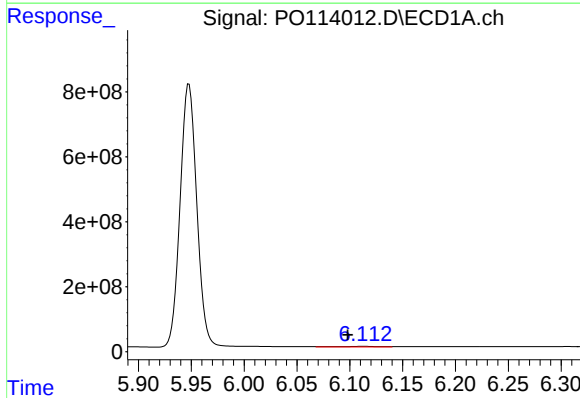


#28 AR-1254-3

R.T.: 6.113 min
Delta R.T.: 0.015 min
Response: 53167402
Conc: 67.98 ng/ml

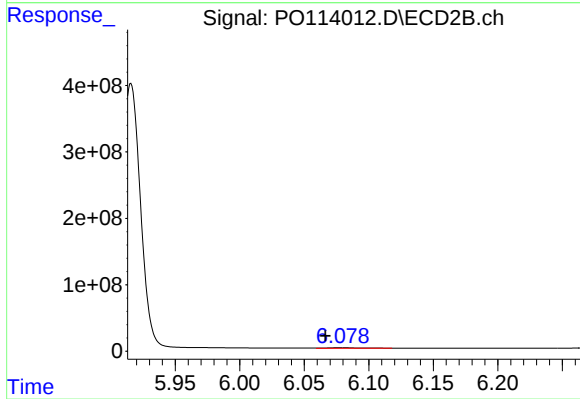

#28 AR-1254-3


R.T.: 6.078 min
Delta R.T.: 0.012 min
Response: 15439406
Conc: 39.86 ng/ml

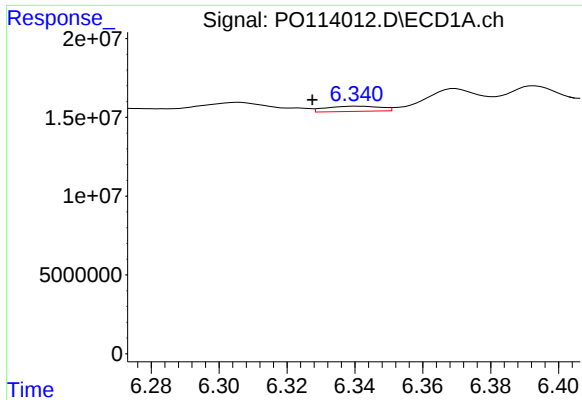

#29 AR-1254-4


R.T.: 6.341 min
Delta R.T.: 0.013 min
Response: 3712244
Conc: 6.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

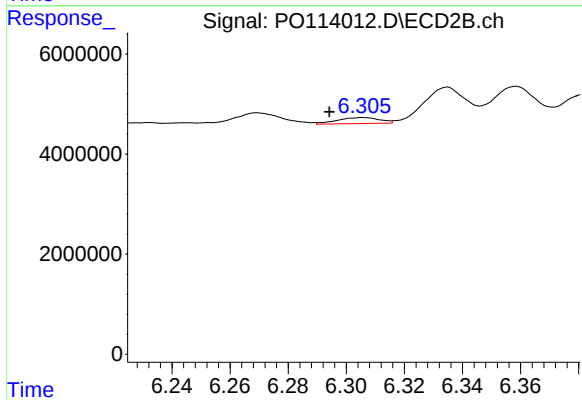


#29 AR-1254-4

R.T.: 6.306 min
Delta R.T.: 0.012 min
Response: 1199251
Conc: 5.05 ng/ml

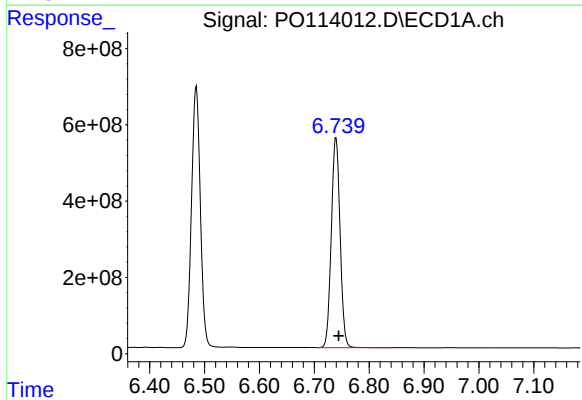


#30 AR-1254-5

R.T.: 6.740 min
Delta R.T.: -0.005 min
Response: 6116423313
Conc: 8217.28 ng/ml

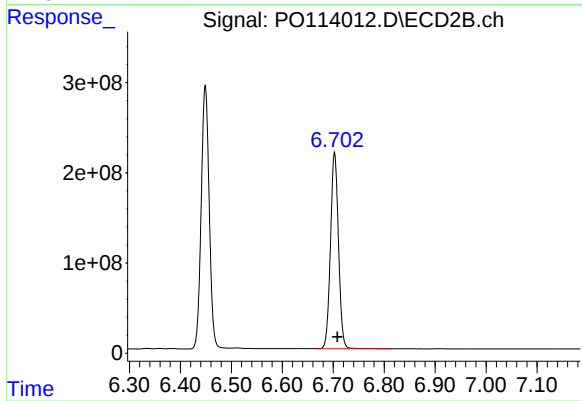

#30 AR-1254-5


R.T.: 6.703 min
Delta R.T.: -0.006 min
Response: 2369057771
Conc: 7717.50 ng/ml

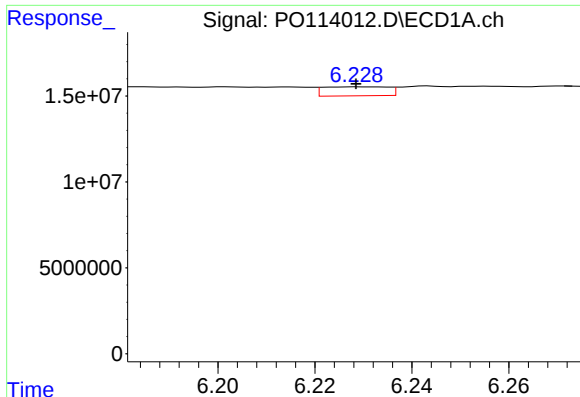

#31 AR-1260-1


R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 4871776
Conc: 9.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

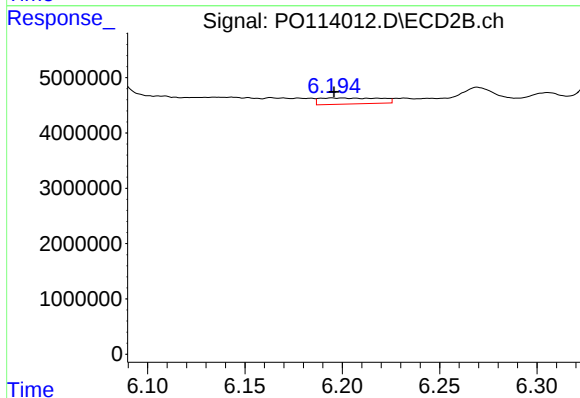


#31 AR-1260-1

R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 2366144
Conc: 9.42 ng/ml

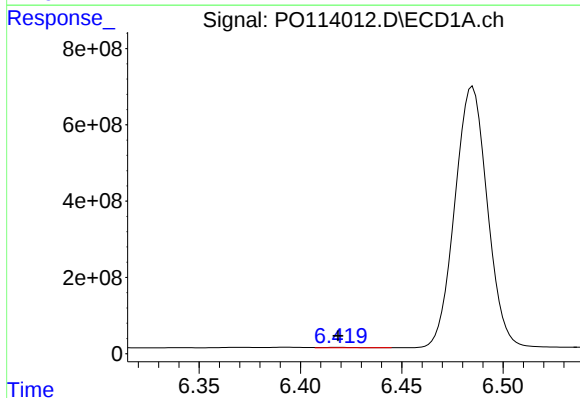


#32 AR-1260-2

R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 11721639
Conc: 15.31 ng/ml

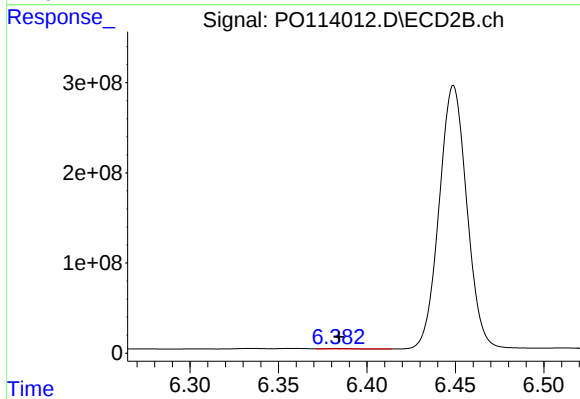

#32 AR-1260-2


R.T.: 6.383 min
Delta R.T.: -0.001 min
Response: 6126129
Conc: 18.53 ng/ml

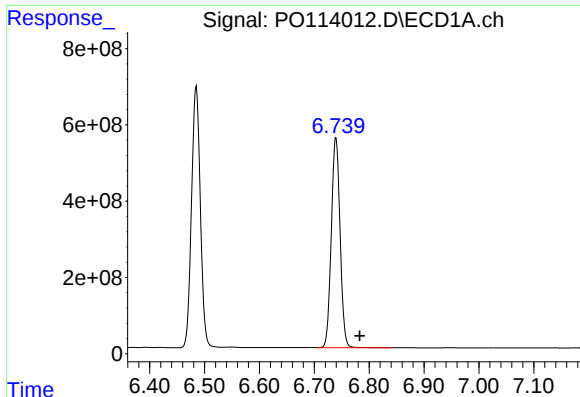

#33 AR-1260-3


R.T.: 6.740 min
Delta R.T.: -0.043 min
Response: 6116423313
Conc: 9090.84 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

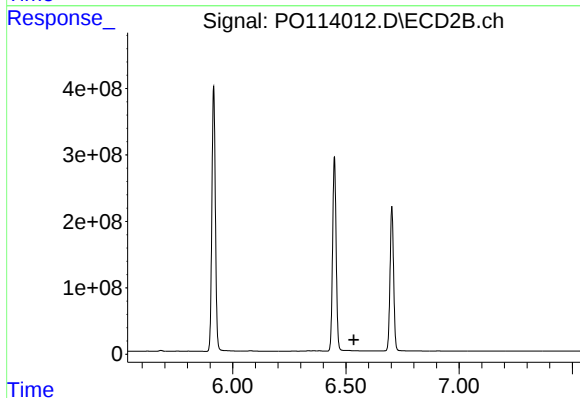


#33 AR-1260-3

R.T.: 6.510 min
Delta R.T.: -0.025 min
Response: -10536522
Conc: N.D.

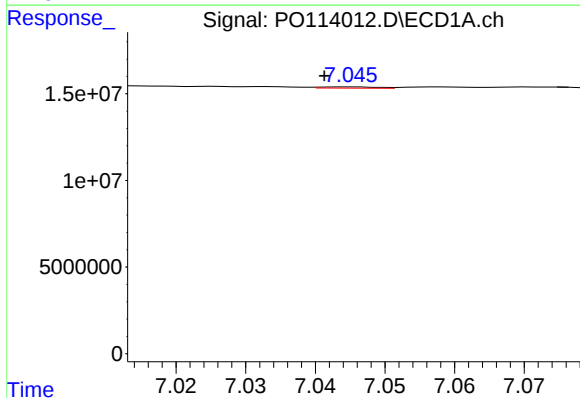


#34 AR-1260-4

R.T.: 7.045 min
Delta R.T.: 0.004 min
Response: 393007
Conc: 0.91 ng/ml

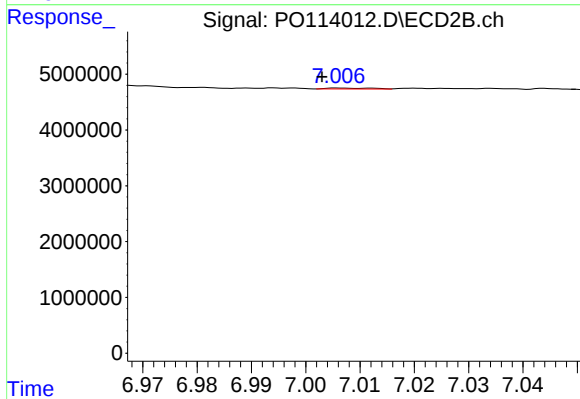

#34 AR-1260-4


R.T.: 7.006 min
Delta R.T.: 0.003 min
Response: 98552
Conc: 0.52 ng/ml

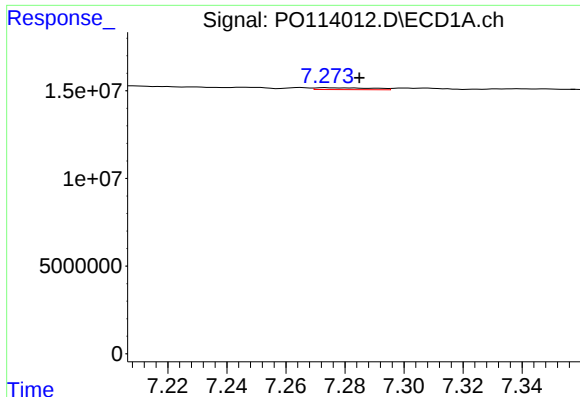

#35 AR-1260-5


R.T.: 7.274 min
Delta R.T.: -0.011 min
Response: 1397718
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

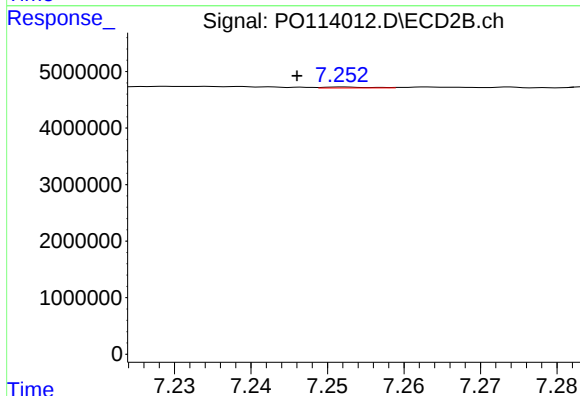


#35 AR-1260-5

R.T.: 7.252 min
Delta R.T.: 0.006 min
Response: 72942
Conc: 0.17 ng/ml

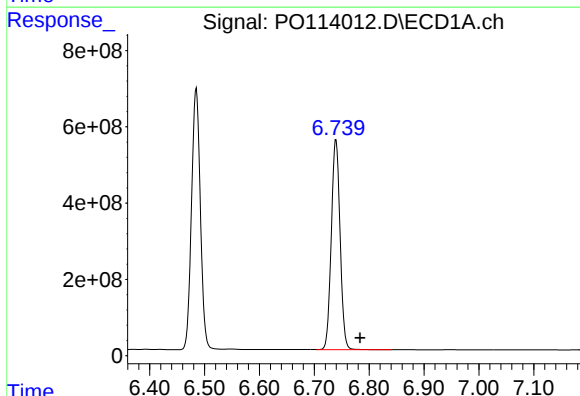


#36 AR-1262-1

R.T.: 6.740 min
Delta R.T.: -0.044 min
Response: 6116423313
Conc: 6163.16 ng/ml

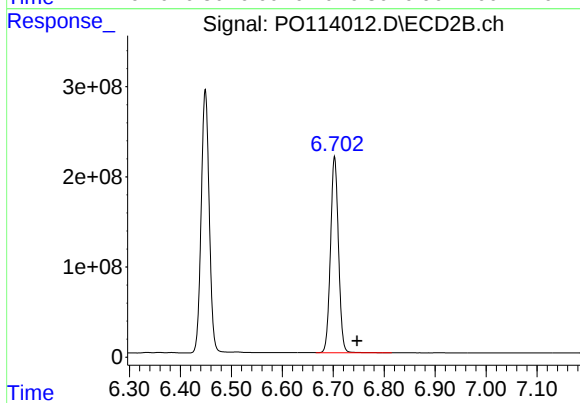

#36 AR-1262-1


R.T.: 6.703 min
Delta R.T.: -0.044 min
Response: 2369057771
Conc: 6470.14 ng/ml

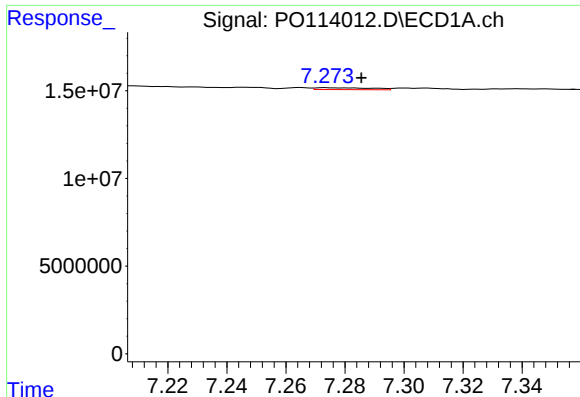

#37 AR-1262-2


R.T.: 7.274 min
Delta R.T.: -0.012 min
Response: 1397718
Conc: 0.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

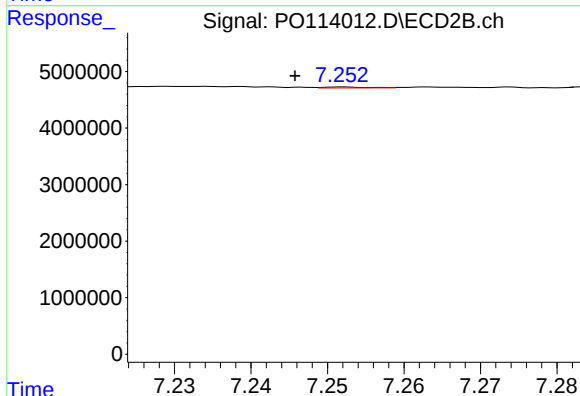


#37 AR-1262-2

R.T.: 7.252 min
Delta R.T.: 0.006 min
Response: 72942
Conc: 0.16 ng/ml

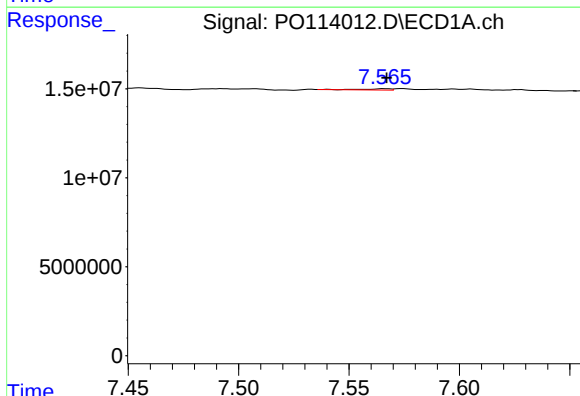


#38 AR-1262-3

R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 613358
Conc: 1.10 ng/ml

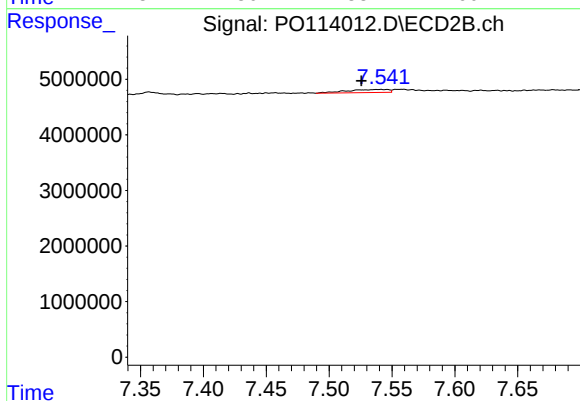

#38 AR-1262-3


R.T.: 7.541 min
Delta R.T.: 0.015 min
Response: 1320073
Conc: 7.58 ng/ml

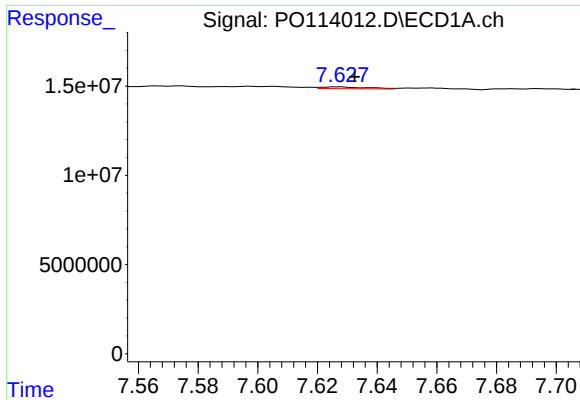

#39 AR-1262-4


R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 1097607
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

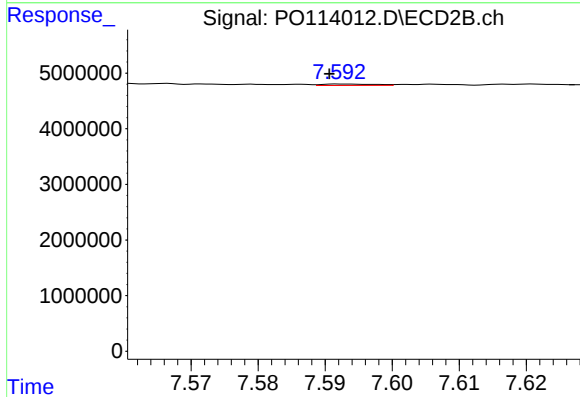


#39 AR-1262-4

R.T.: 7.593 min
Delta R.T.: 0.002 min
Response: 145128
Conc: 0.52 ng/ml

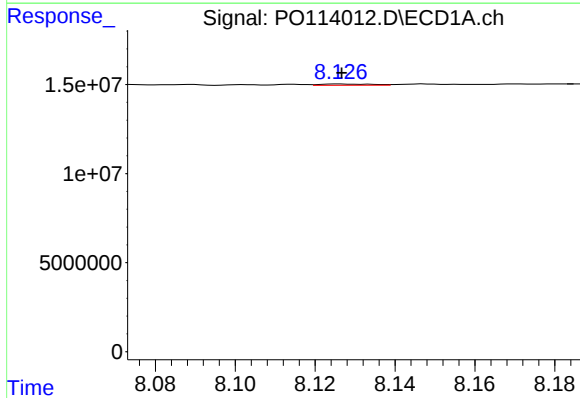


#40 AR-1262-5

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 624713
Conc: 1.57 ng/ml

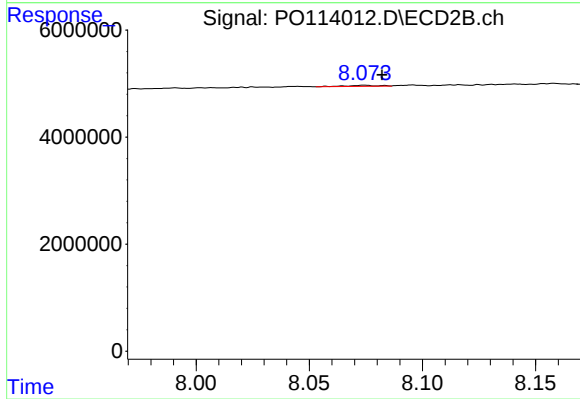

#40 AR-1262-5


R.T.: 8.075 min
Delta R.T.: -0.008 min
Response: 201744
Conc: 1.77 ng/ml

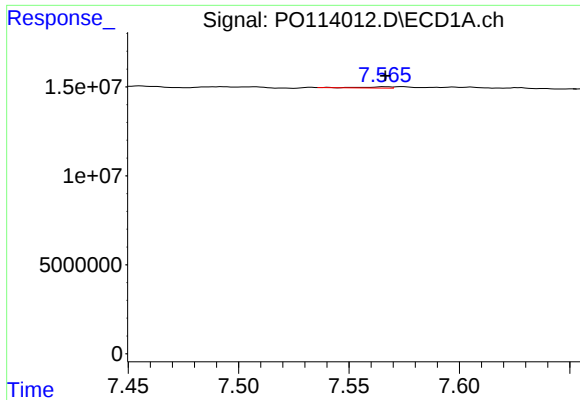

#41 AR-1268-1


R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 613358
Conc: 0.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

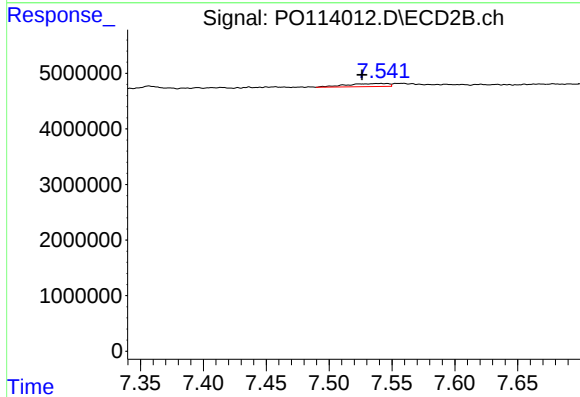


#41 AR-1268-1

R.T.: 7.541 min
Delta R.T.: 0.014 min
Response: 1320073
Conc: 2.70 ng/ml

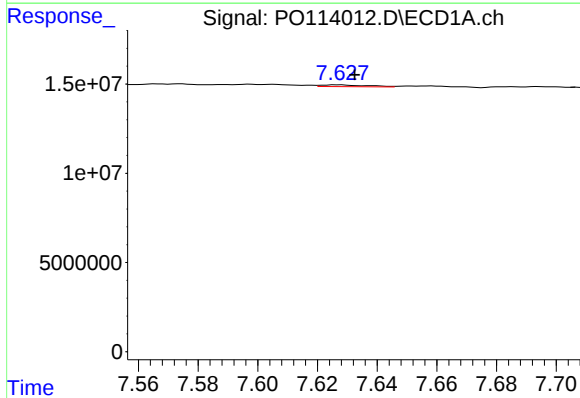


#42 AR-1268-2

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 1097607
Conc: 0.74 ng/ml

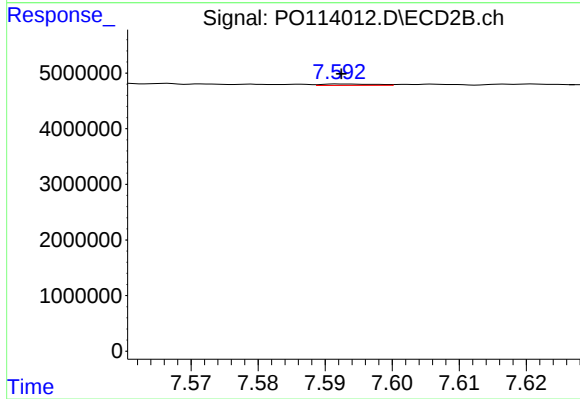

#42 AR-1268-2


R.T.: 7.593 min
Delta R.T.: 0.000 min
Response: 145128
Conc: 0.36 ng/ml

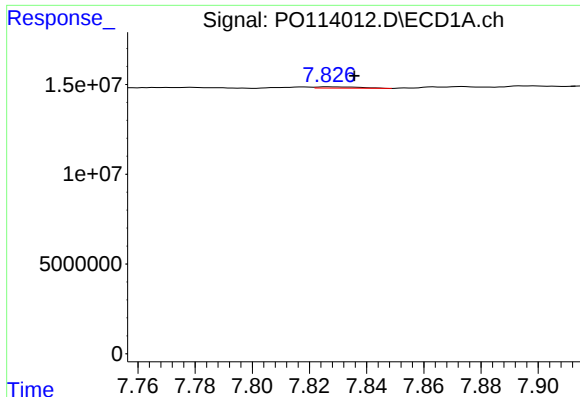

#43 AR-1268-3


R.T.: 7.827 min
Delta R.T.: -0.009 min
Response: 762369
Conc: 0.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

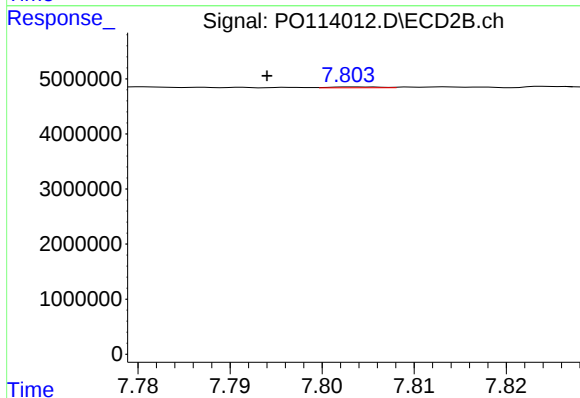


#43 AR-1268-3

R.T.: 7.804 min
Delta R.T.: 0.010 min
Response: 60824
Conc: 0.19 ng/ml

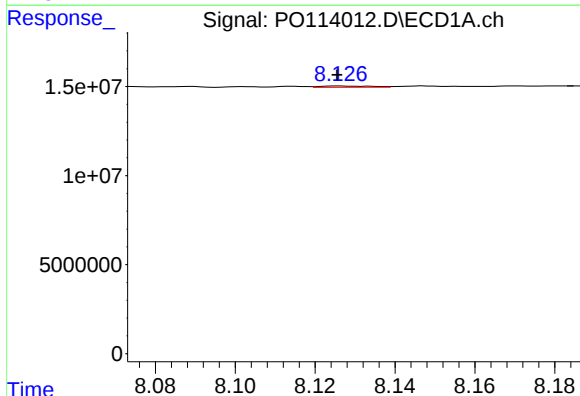


#44 AR-1268-4

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 624713
Conc: 1.37 ng/ml

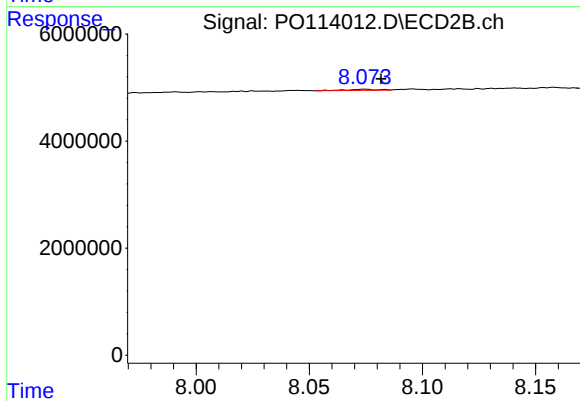

#44 AR-1268-4


R.T.: 8.075 min
Delta R.T.: -0.007 min
Response: 201744
Conc: 1.59 ng/ml

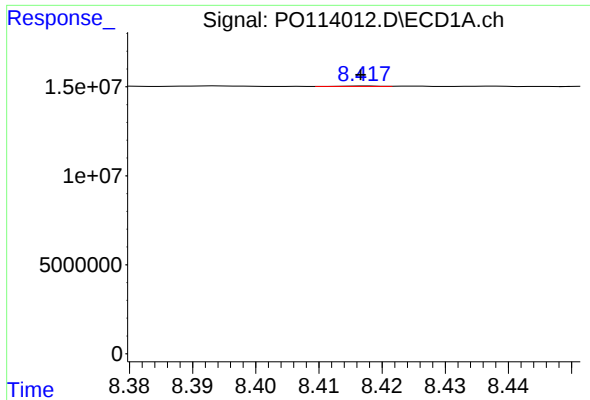

#45 AR-1268-5

R.T.: 8.417 min
Delta R.T.: 0.000 min
Response: 107698
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

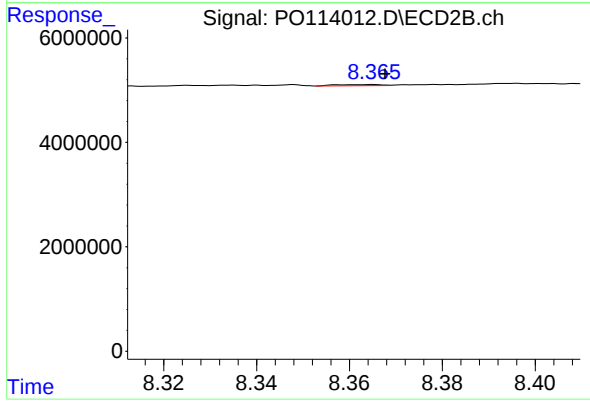

#45 AR-1268-5

R.T.: 8.365 min
Delta R.T.: -0.003 min
Response: 148994
Conc: 0.17 ng/ml