

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092425\
 Data File : P0114005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 19:52
 Operator : YP/AJ
 Sample : Q3169-07DL 50X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CT#3DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/25/2025
 Supervised By :mohammad ahmed 09/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 08:06:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 02:49:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
26)	L6	AR-1254-1	5.543	5.515	476.5E6	252.7E6	874.033	835.709
27)	L6	AR-1254-2	5.692	5.663	437.3E6	220.3E6	859.993	834.328
28)	L6	AR-1254-3	6.093	6.062	559.8E6	296.6E6	715.801	765.884
29)	L6	AR-1254-4	6.323	6.289	409.2E6	187.5E6	748.362	789.736
30)	L6	AR-1254-5	6.741	6.705	554.8E6	235.6E6	745.429	767.650

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092425\
Data File : PO114005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2025 19:52
Operator : YP/AJ
Sample : Q3169-07DL 50X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CT#3DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2025
Supervised By :mohammad ahmed 09/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 08:06:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO091525.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 02:49:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

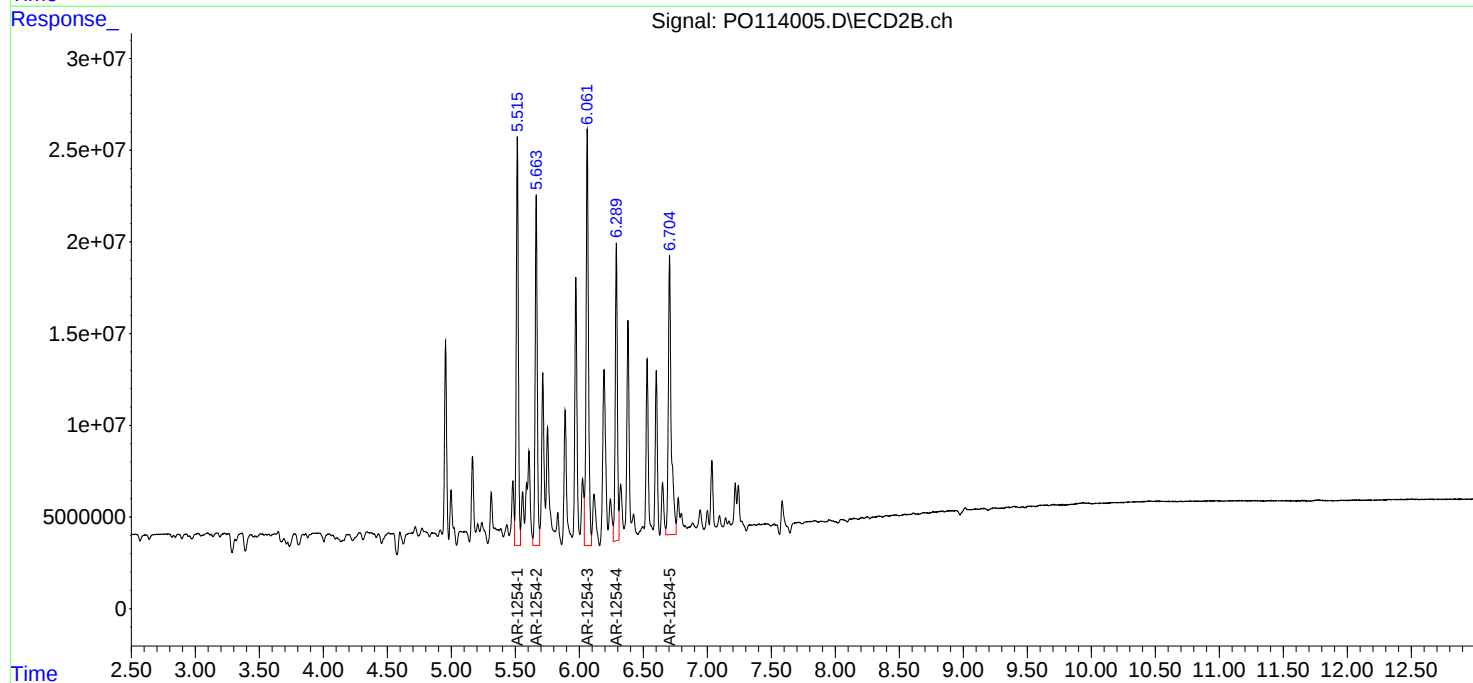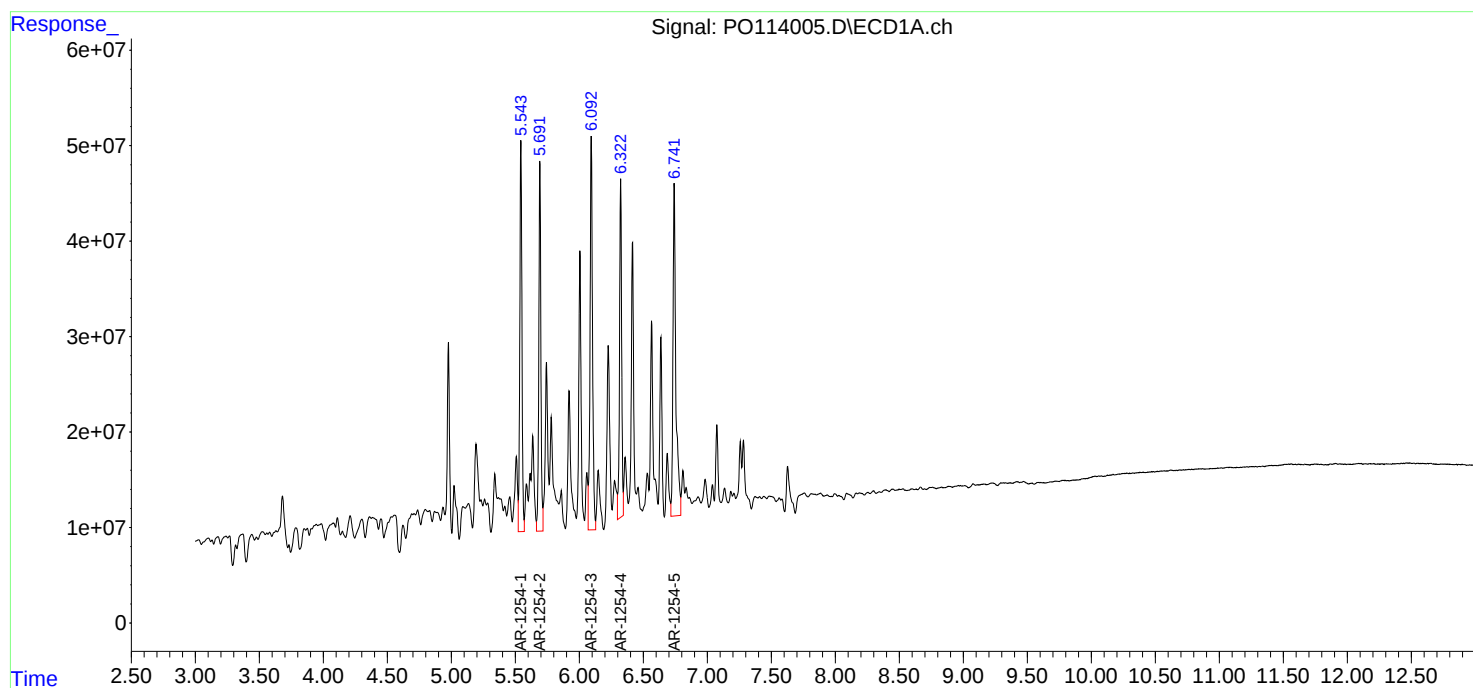

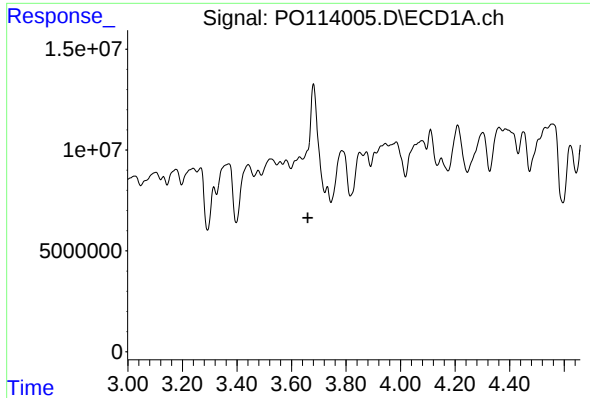


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CT#3DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2025
Supervised By :mohammad ahmed 09/26/2025

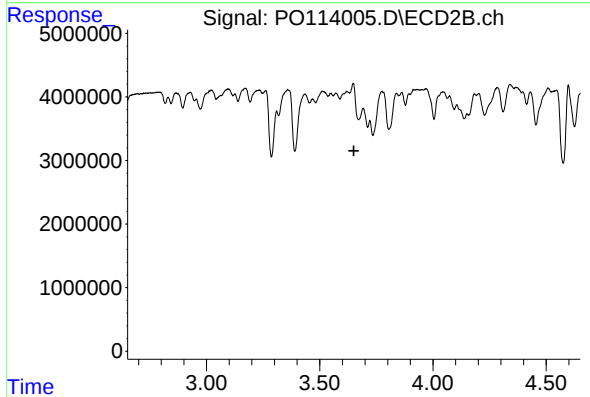


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.651 min
Response: 0
Conc: N.D.

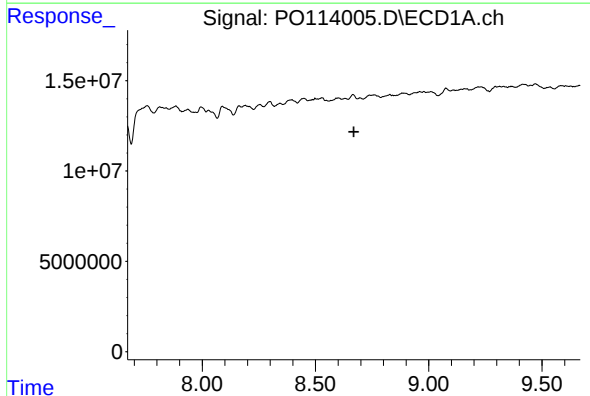


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.670 min
Response: 0
Conc: N.D.

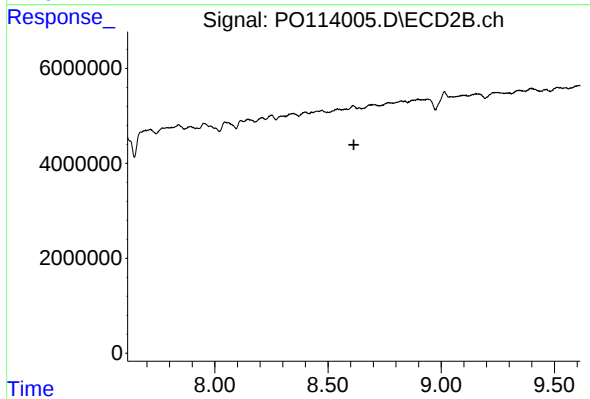

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.614 min
Response: 0
Conc: N.D.

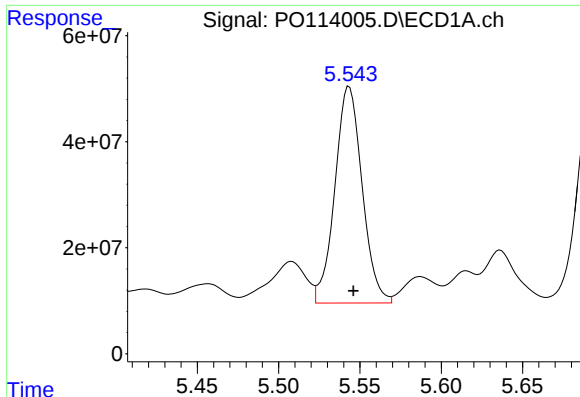


#26 AR-1254-1

R.T.: 5.543 min
Delta R.T.: -0.002 min
Response: 476539450
Conc: 874.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CT#3DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2025
Supervised By :mohammad ahmed 09/26/2025

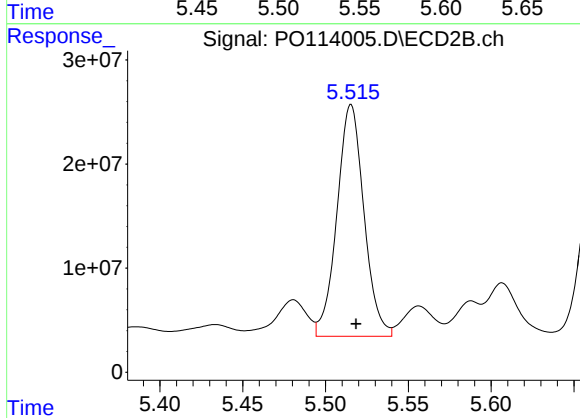


#26 AR-1254-1

R.T.: 5.515 min
Delta R.T.: -0.003 min
Response: 252716709
Conc: 835.71 ng/ml

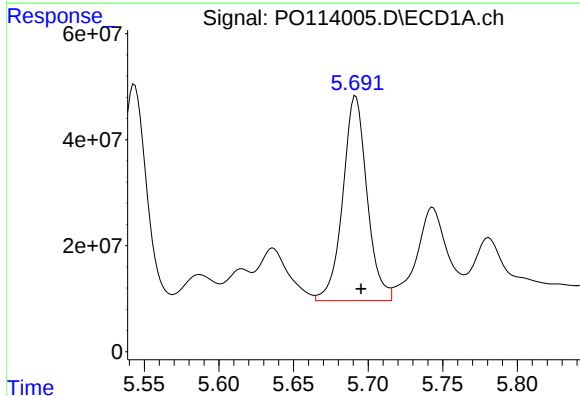


#27 AR-1254-2

R.T.: 5.692 min
Delta R.T.: -0.003 min
Response: 437253399
Conc: 859.99 ng/ml

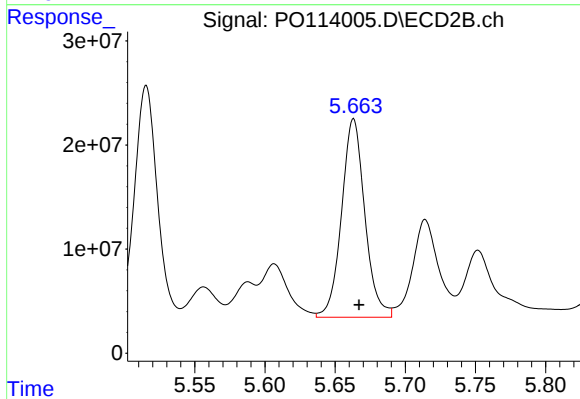

#27 AR-1254-2

R.T.: 5.663 min
Delta R.T.: -0.004 min
Response: 220328693
Conc: 834.33 ng/ml

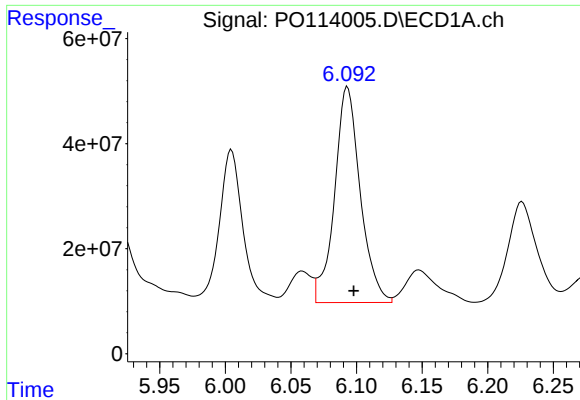


#28 AR-1254-3

R.T.: 6.093 min
Delta R.T.: -0.005 min
Response: 559832082
Conc: 715.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CT#3DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2025
Supervised By :mohammad ahmed 09/26/2025

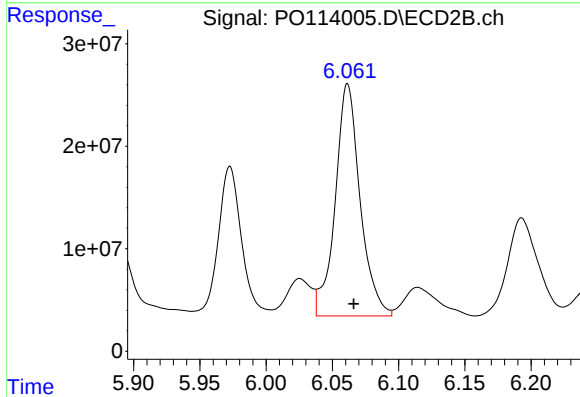


#28 AR-1254-3

R.T.: 6.062 min
Delta R.T.: -0.005 min
Response: 296640399
Conc: 765.88 ng/ml

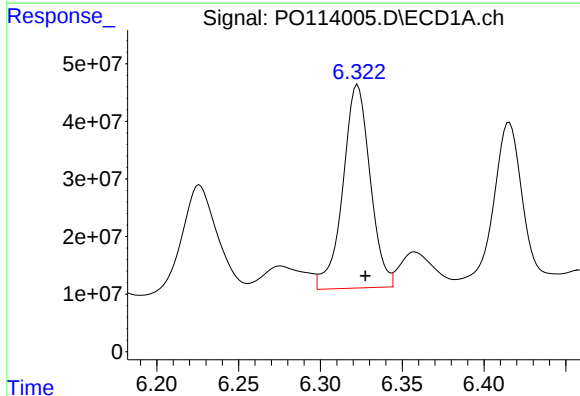


#29 AR-1254-4

R.T.: 6.323 min
Delta R.T.: -0.005 min
Response: 409244661
Conc: 748.36 ng/ml

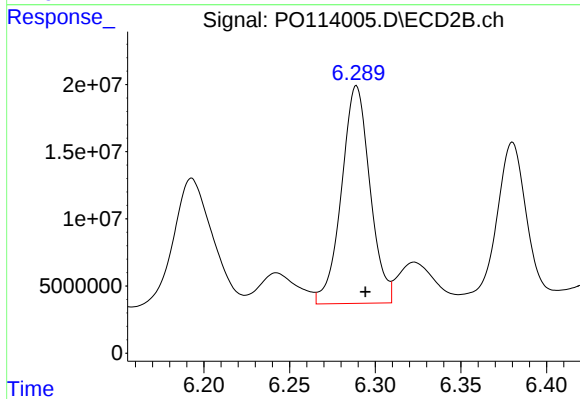

#29 AR-1254-4

R.T.: 6.289 min
Delta R.T.: -0.005 min
Response: 187477045
Conc: 789.74 ng/ml

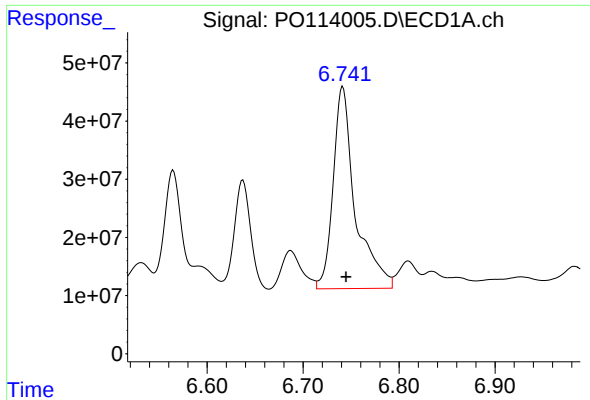


#30 AR-1254-5

R.T.: 6.741 min
Delta R.T.: -0.003 min
Response: 554849971
Conc: 745.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
CT#3DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2025
Supervised By :mohammad ahmed 09/26/2025

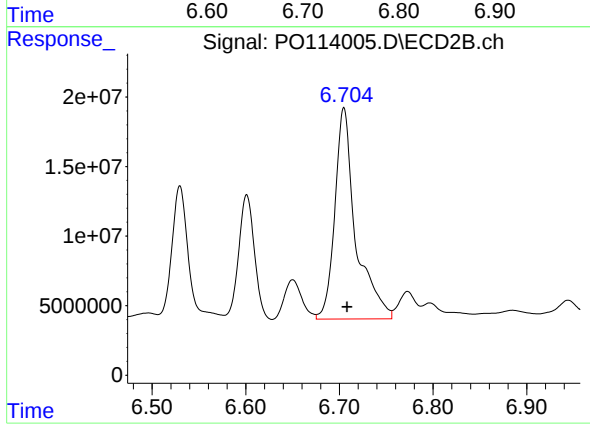

#30 AR-1254-5

R.T.: 6.705 min
Delta R.T.: -0.003 min
Response: 235646990
Conc: 767.65 ng/ml