

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
 Data File : P0061351.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2019 14:57
 Operator : SM/AJ
 Sample : K4657-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BU-03-092419

Manual Integrations
 APPROVED

Ankita
 9/26/2019 5:03:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:21:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.362	3.521	873516	677597	23.743	24.267m
2) SA Decachlor...	10.028	8.395	1012549	704254	22.038	20.092m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
Data File : P0061351.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2019 14:57
Operator : SM/AJ
Sample : K4657-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BU-03-092419


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:21:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

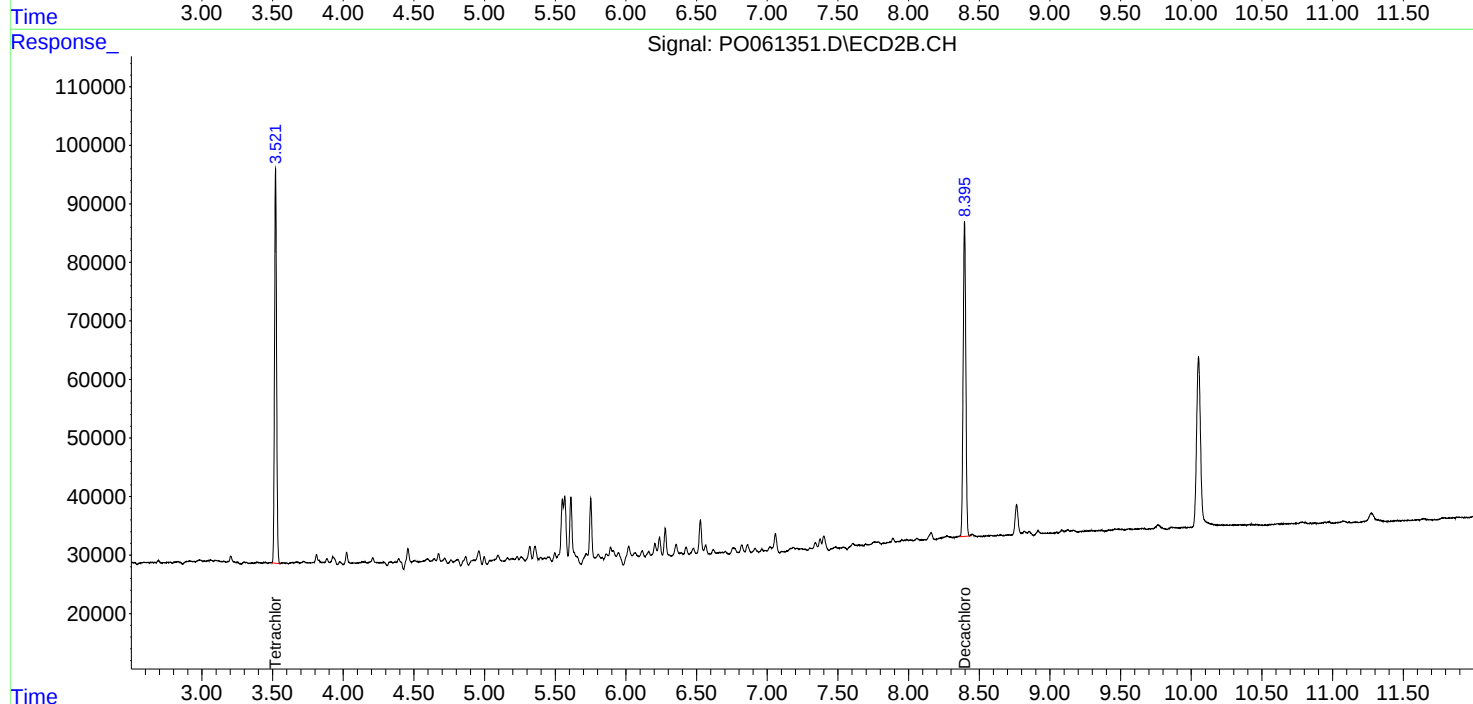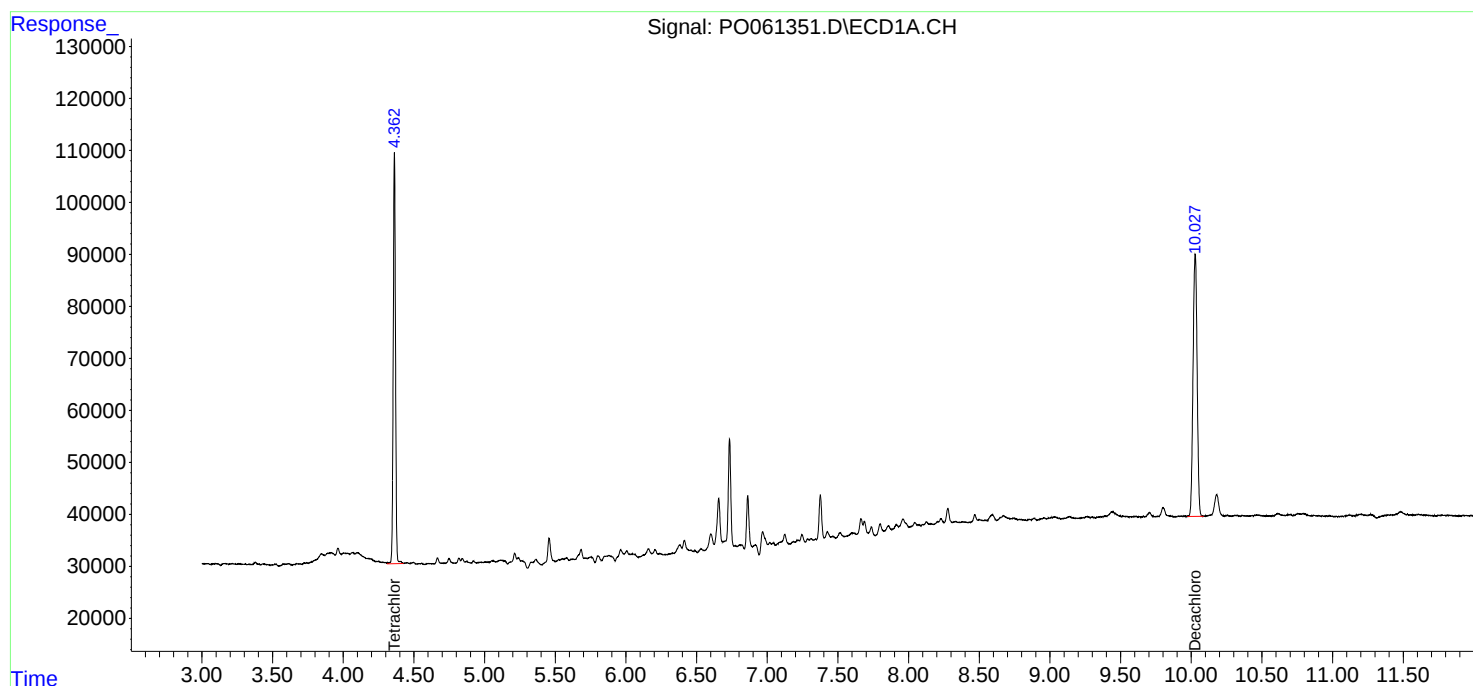

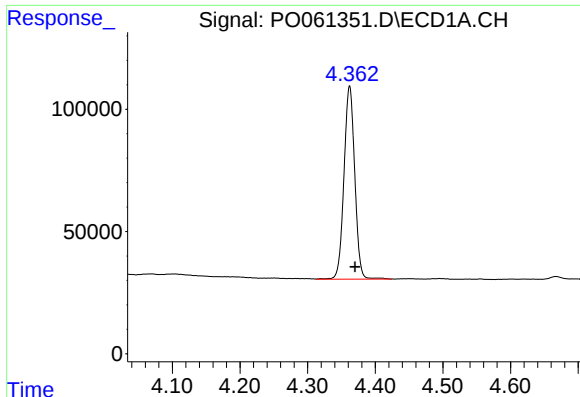


#1 Tetrachloro-m-xylene

R.T.: 4.362 min
Delta R.T.: -0.008 min
Response: 873516
Conc: 23.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
BU-03-092419


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:00 PM

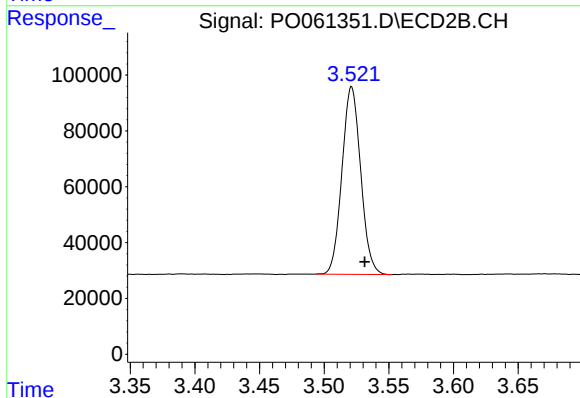


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: -0.011 min
Response: 677597
Conc: 24.27 ng/ml m

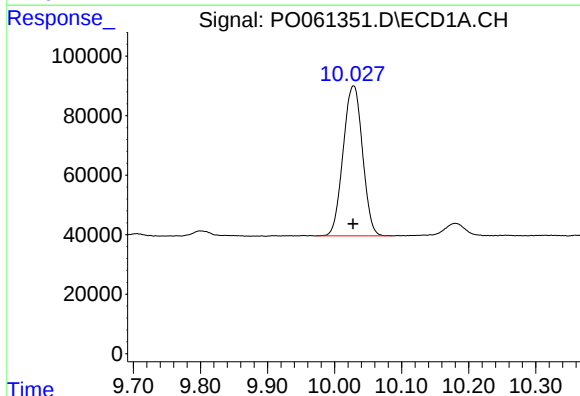

#2 Decachlorobiphenyl

R.T.: 10.028 min
Delta R.T.: 0.000 min
Response: 1012549
Conc: 22.04 ng/ml

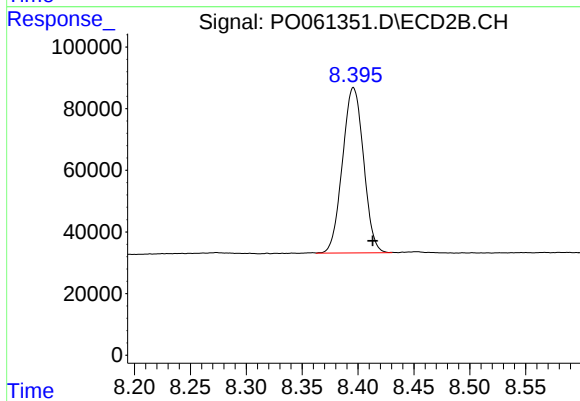

#2 Decachlorobiphenyl

R.T.: 8.395 min
Delta R.T.: -0.018 min
Response: 704254
Conc: 20.09 ng/ml m