

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
 Data File : P0061352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2019 15:14
 Operator : SM/AJ
 Sample : K4663-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-092419

Manual Integrations
 APPROVED

Ankita
 9/26/2019 5:03:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:21:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.364	3.522	942078	727237	25.606	26.045m
2) SA Decachlor...	10.030	8.397	933797	617152	20.324	17.607m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
Data File : P0061352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2019 15:14
Operator : SM/AJ
Sample : K4663-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-092419


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:21:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

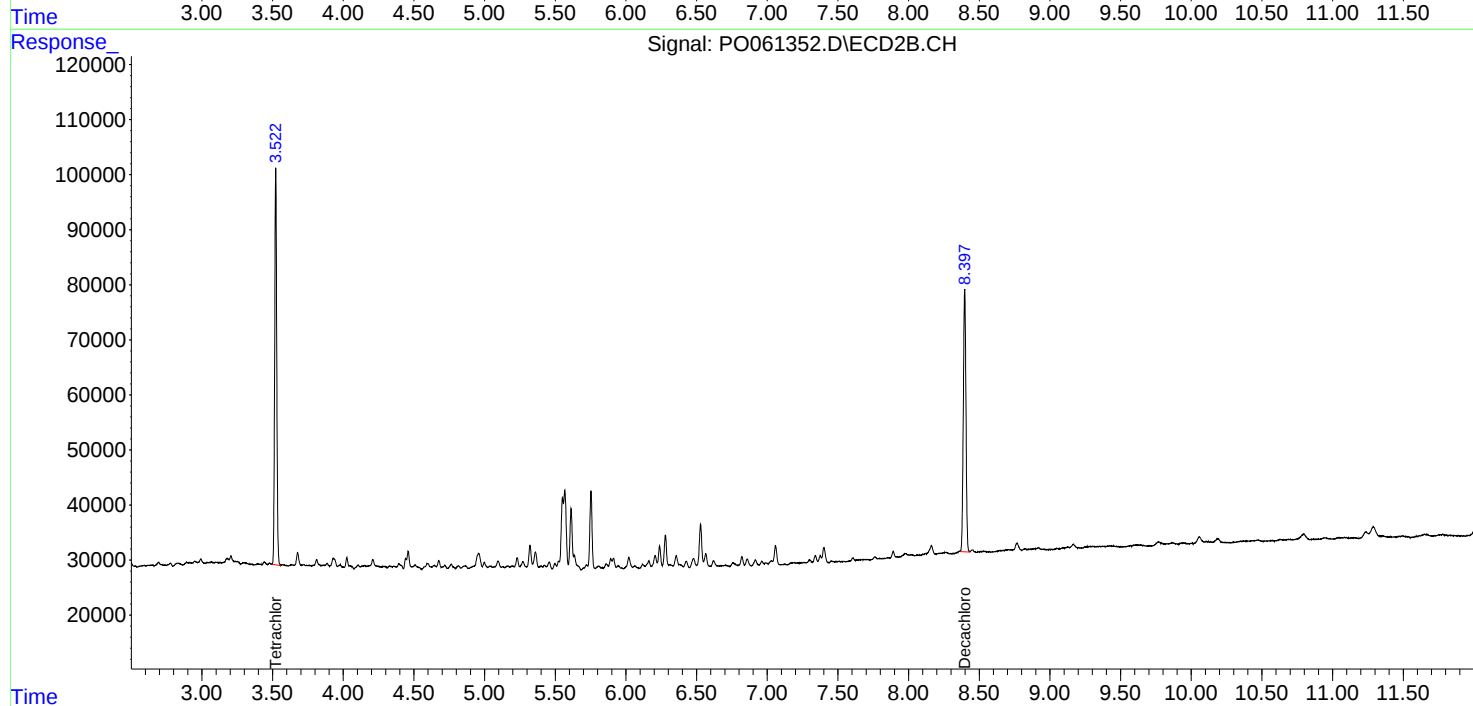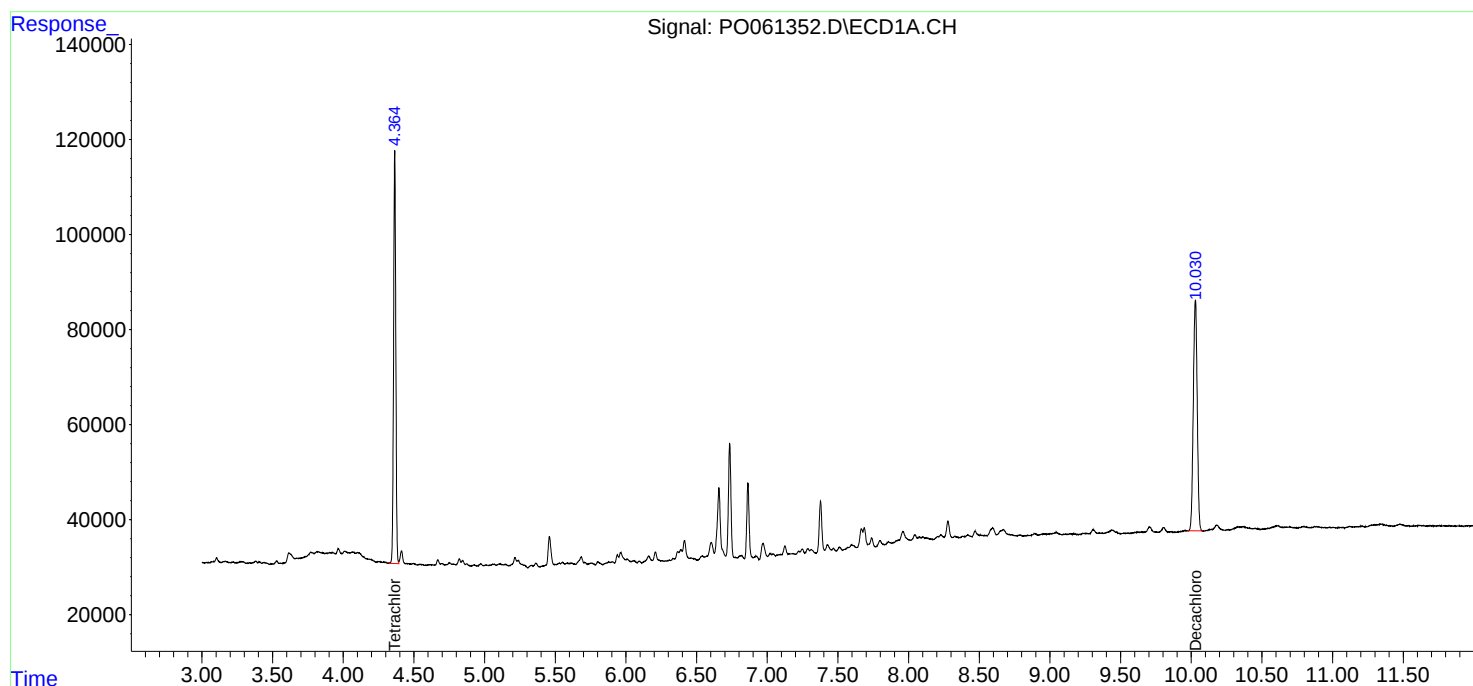

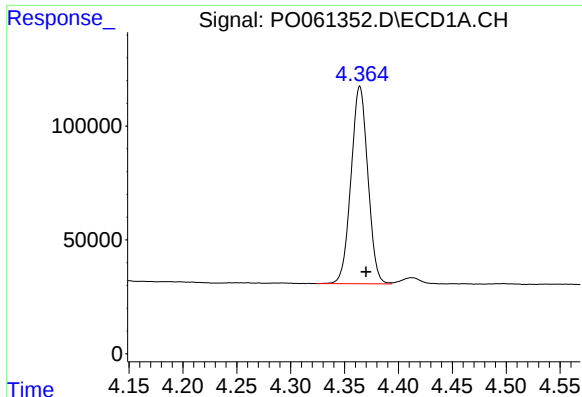


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: -0.006 min
Response: 942078
Conc: 25.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-092419


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:02 PM

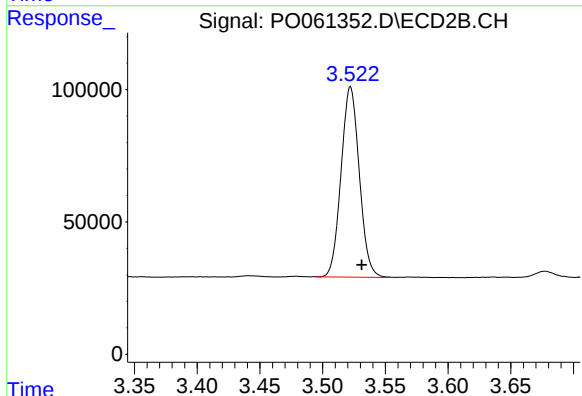


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.010 min
Response: 727237
Conc: 26.05 ng/ml m

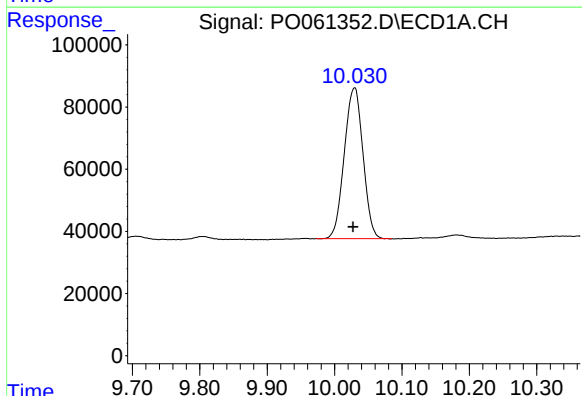

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.002 min
Response: 933797
Conc: 20.32 ng/ml

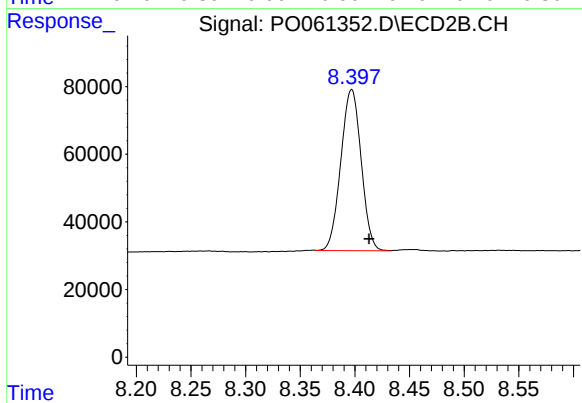

#2 Decachlorobiphenyl

R.T.: 8.397 min
Delta R.T.: -0.016 min
Response: 617152
Conc: 17.61 ng/ml m