

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
 Data File : P0061359.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Sep 2019 18:13
 Operator : SM/AJ
 Sample : K5021-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RT-1488-RBR200031-RBR200036

Manual Integrations
 APPROVED

Ankita
 9/26/2019 5:03:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:24:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359	3.519	793252	607044	21.561	21.741m
2) SA Decachlor...	10.023	8.394	959362	677925	20.880	19.341m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092519\
Data File : P0061359.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Sep 2019 18:13
Operator : SM/AJ
Sample : K5021-01
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
RT-1488-RBR200031-RBR200036


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:24:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

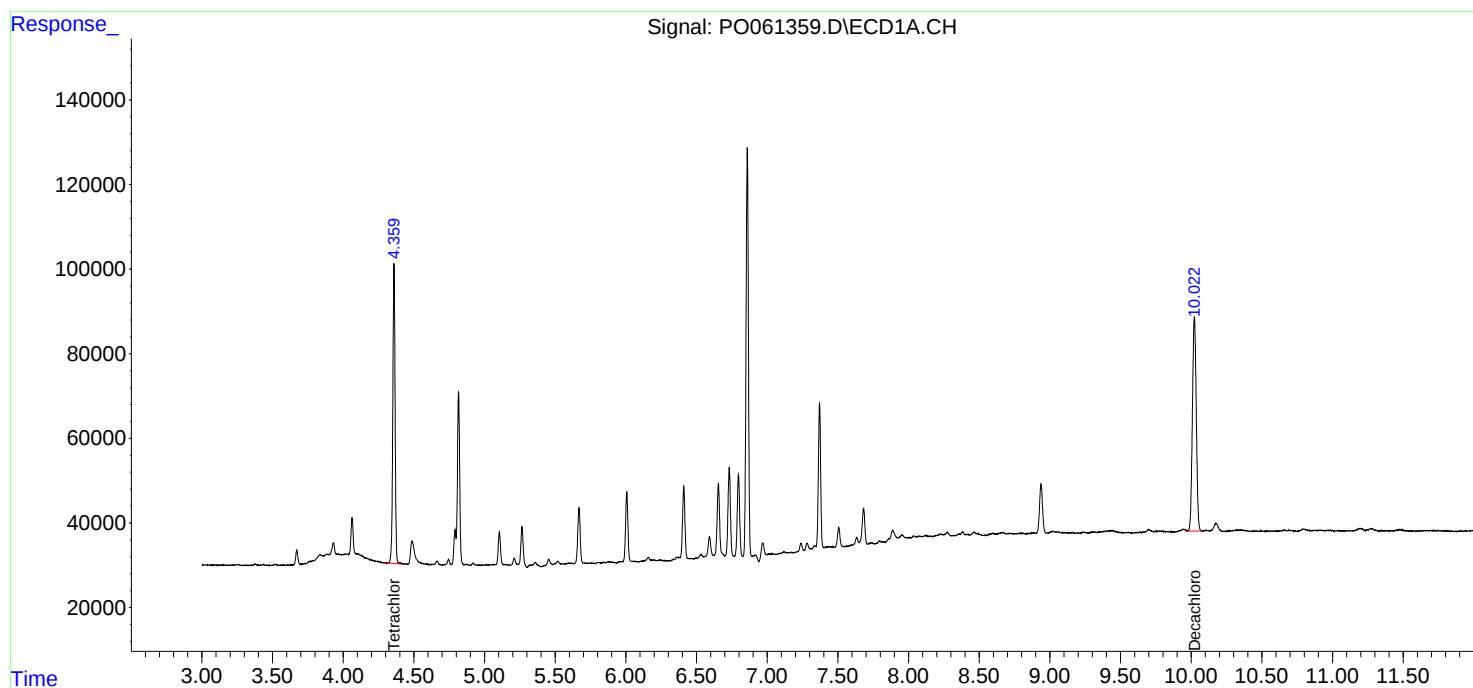

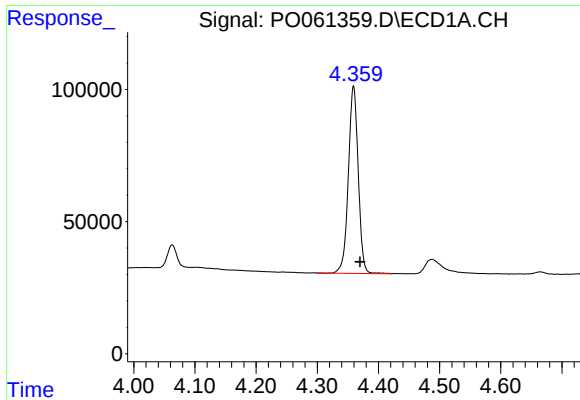


#1 Tetrachloro-m-xylene

R.T.: 4.359 min
Delta R.T.: -0.011 min
Response: 793252
Conc: 21.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-1488-RBR200031-RBR200036


Manual Integrations
APPROVED

Ankita
9/26/2019 5:03:15 PM

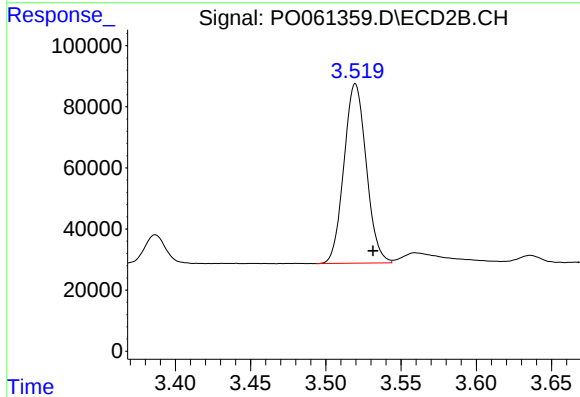


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.012 min
Response: 607044
Conc: 21.74 ng/ml m

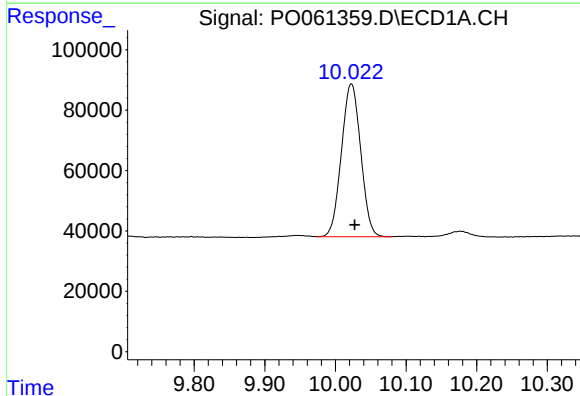

#2 Decachlorobiphenyl

R.T.: 10.023 min
Delta R.T.: -0.005 min
Response: 959362
Conc: 20.88 ng/ml

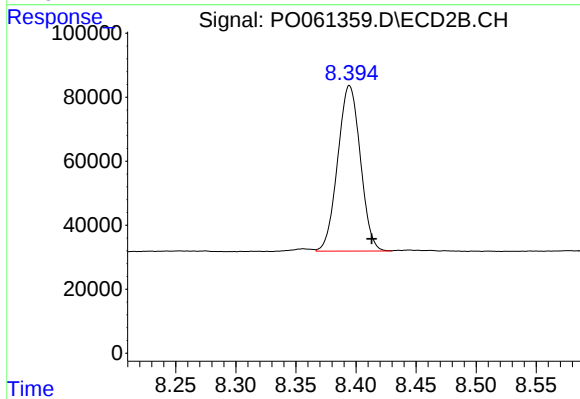

#2 Decachlorobiphenyl

R.T.: 8.394 min
Delta R.T.: -0.019 min
Response: 677925
Conc: 19.34 ng/ml m