

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092618\
 Data File : P0049336.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Sep 2018 14:16
 Operator : SM/SJ
 Sample : J4923-01RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BS-PAINT-CHIPSRE

Manual Integrations
 APPROVED

Sohil
 9/27/2018 4:10:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 01:00:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 20 02:02:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.524	6068314	6834696	32.682m	33.073
2) SA Decachlor...	10.114	8.458	10241323	8834940	37.257	43.157

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092618\
Data File : P0049336.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Sep 2018 14:16
Operator : SM/SJ
Sample : J4923-01RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BS-PAINT-CHIPSRE


Manual Integrations
APPROVED

Sohil
9/27/2018 4:10:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 01:00:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 20 02:02:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

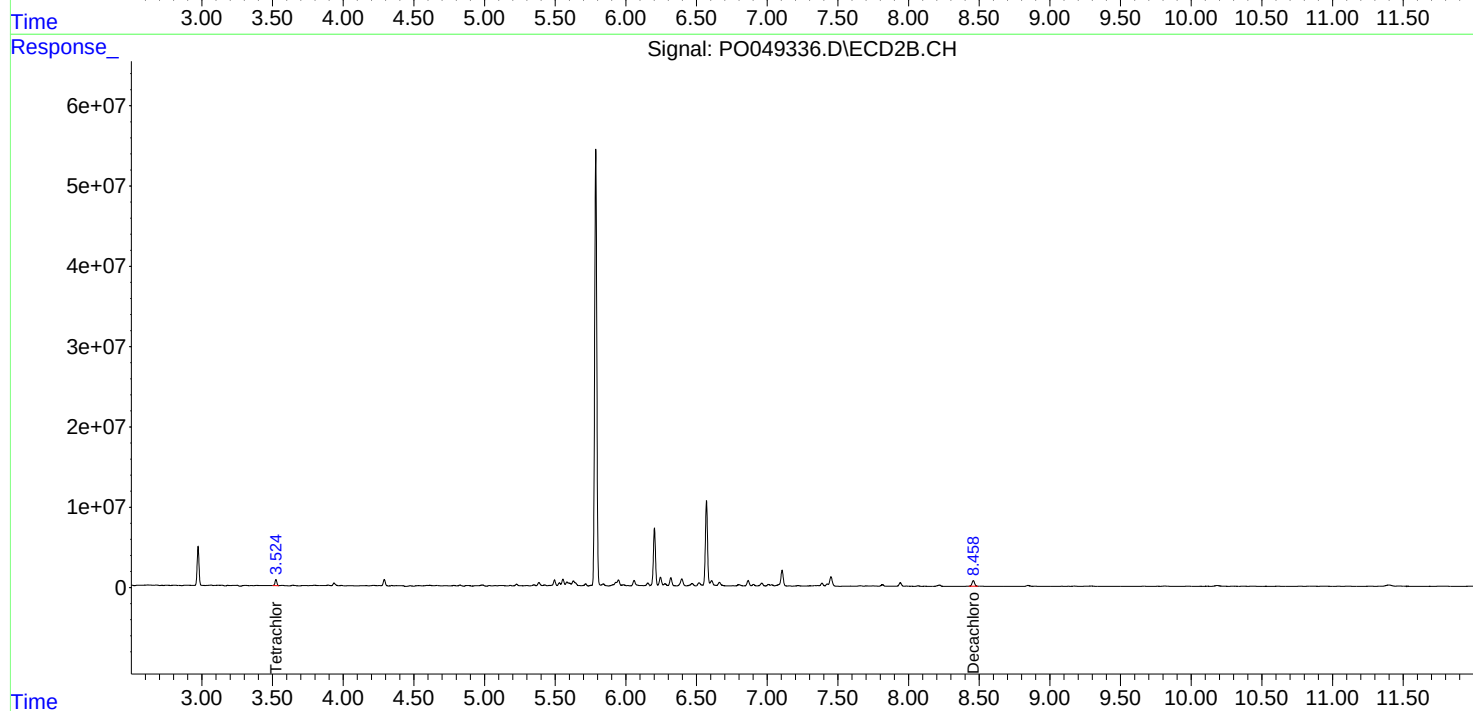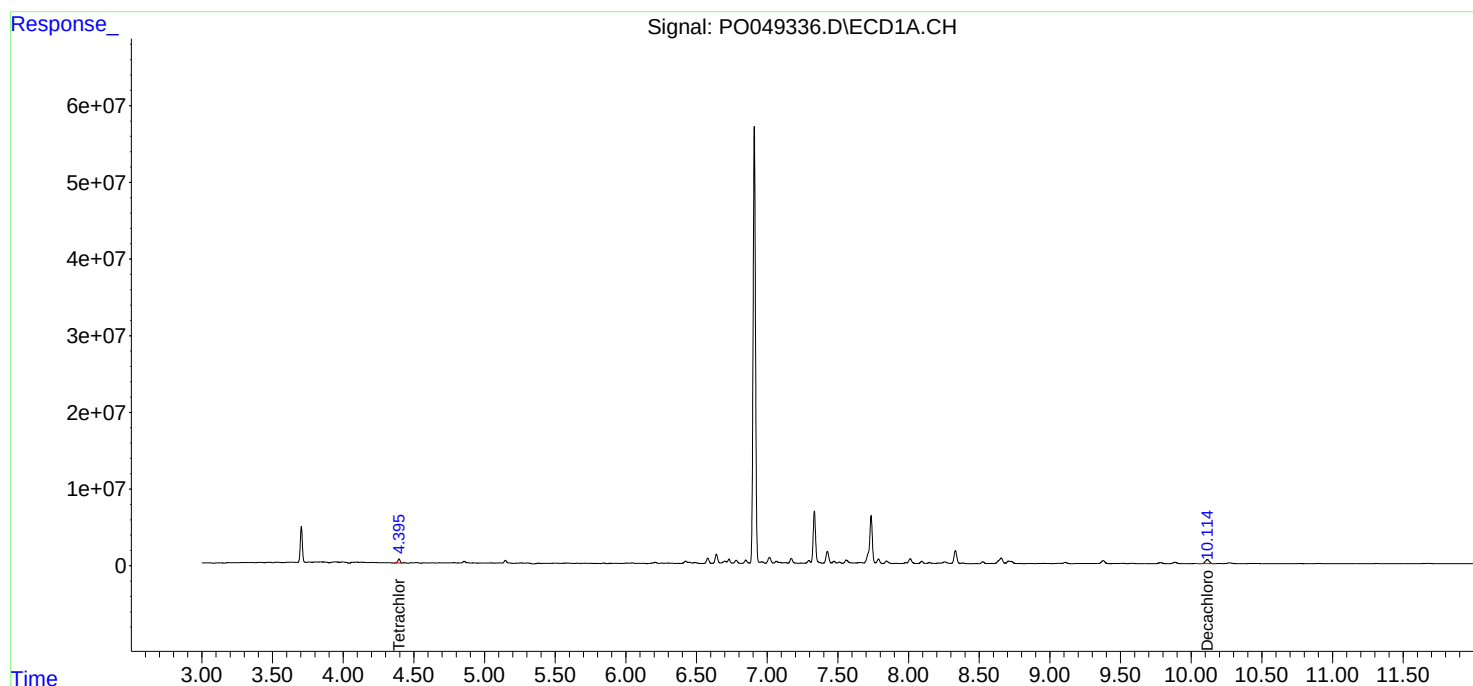

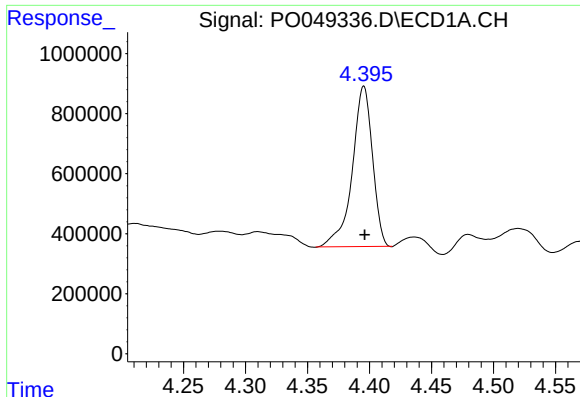


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 6068314
Conc: 32.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BS-PAINT-CHIPSRE


Manual Integrations
APPROVED

Sohil
9/27/2018 4:10:39 PM

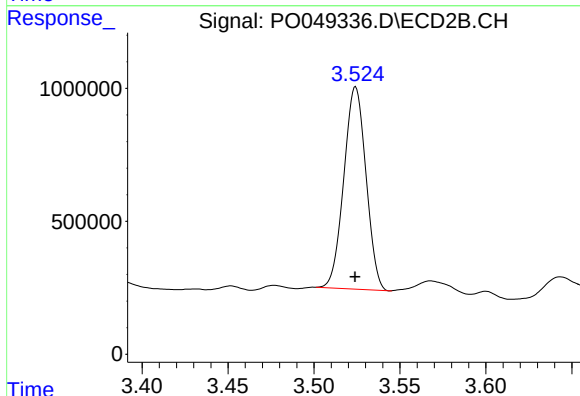


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 6834696
Conc: 33.07 ng/ml

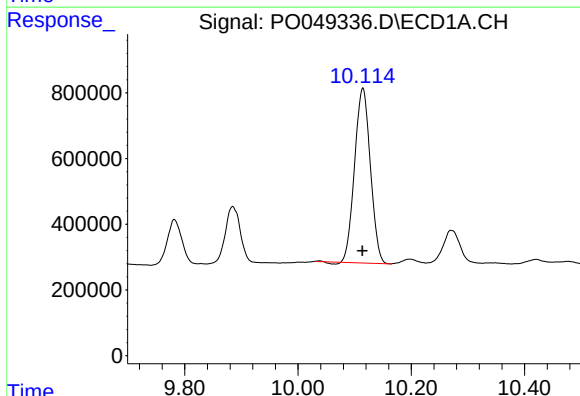

#2 Decachlorobiphenyl

R.T.: 10.114 min
Delta R.T.: 0.000 min
Response: 10241323
Conc: 37.26 ng/ml

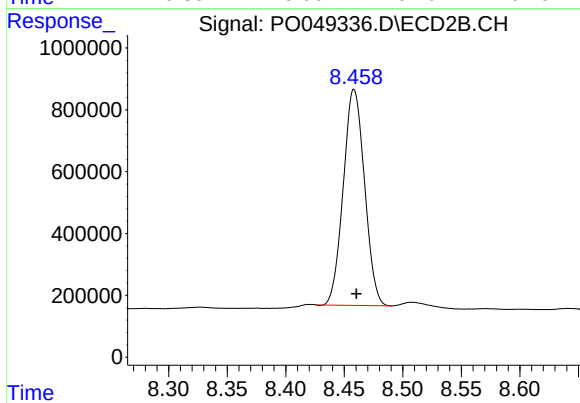

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.002 min
Response: 8834940
Conc: 43.16 ng/ml