

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0092623\
 Data File : P0098271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 15:32
 Operator : YP/AJ
 Sample : 04605-02 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 KMA872E-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 15:56:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0092523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 26 09:03:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.638	2713958	1236497	1.422	1.629m
2) SA Decachlor...	10.292	8.658	3107837	692569	3.866	1.799 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092623\
Data File : PO098271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 15:32
Operator : YP/AJ
Sample : 04605-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA872E-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 15:56:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092523.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 26 09:03:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

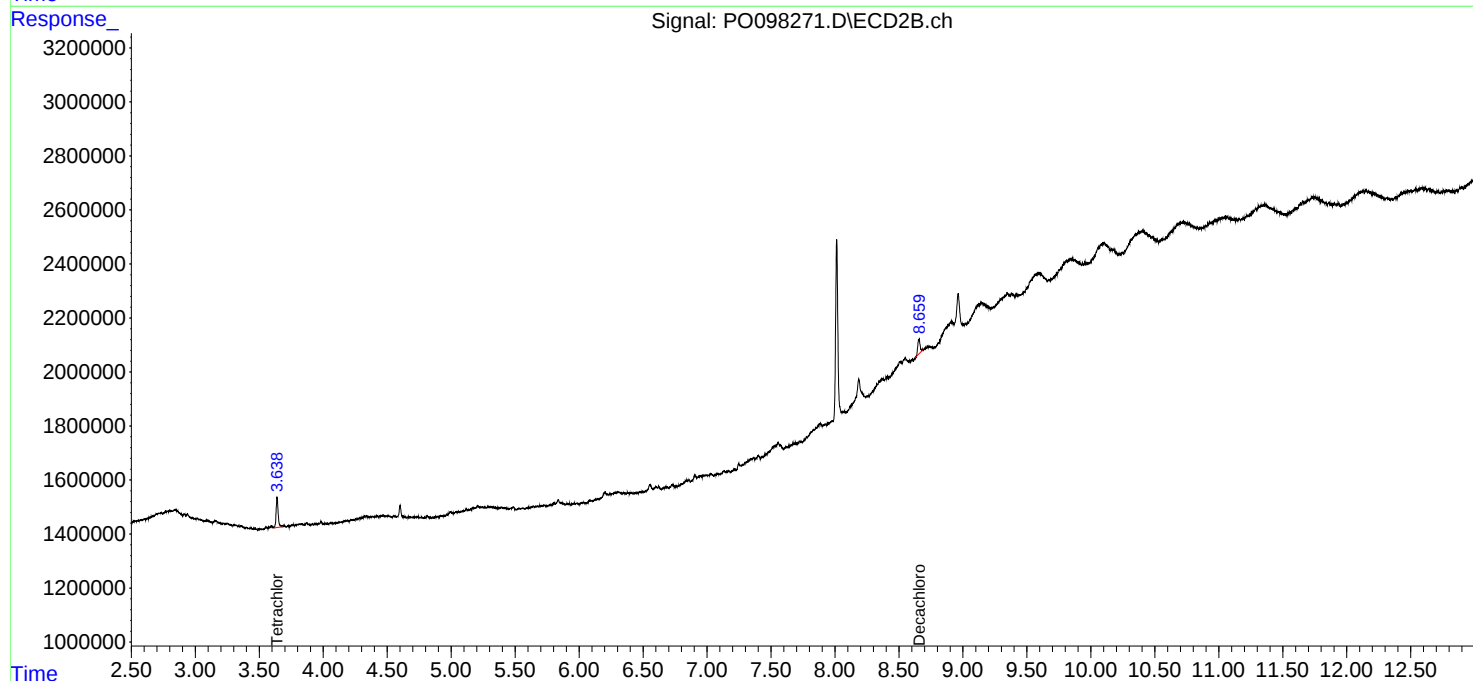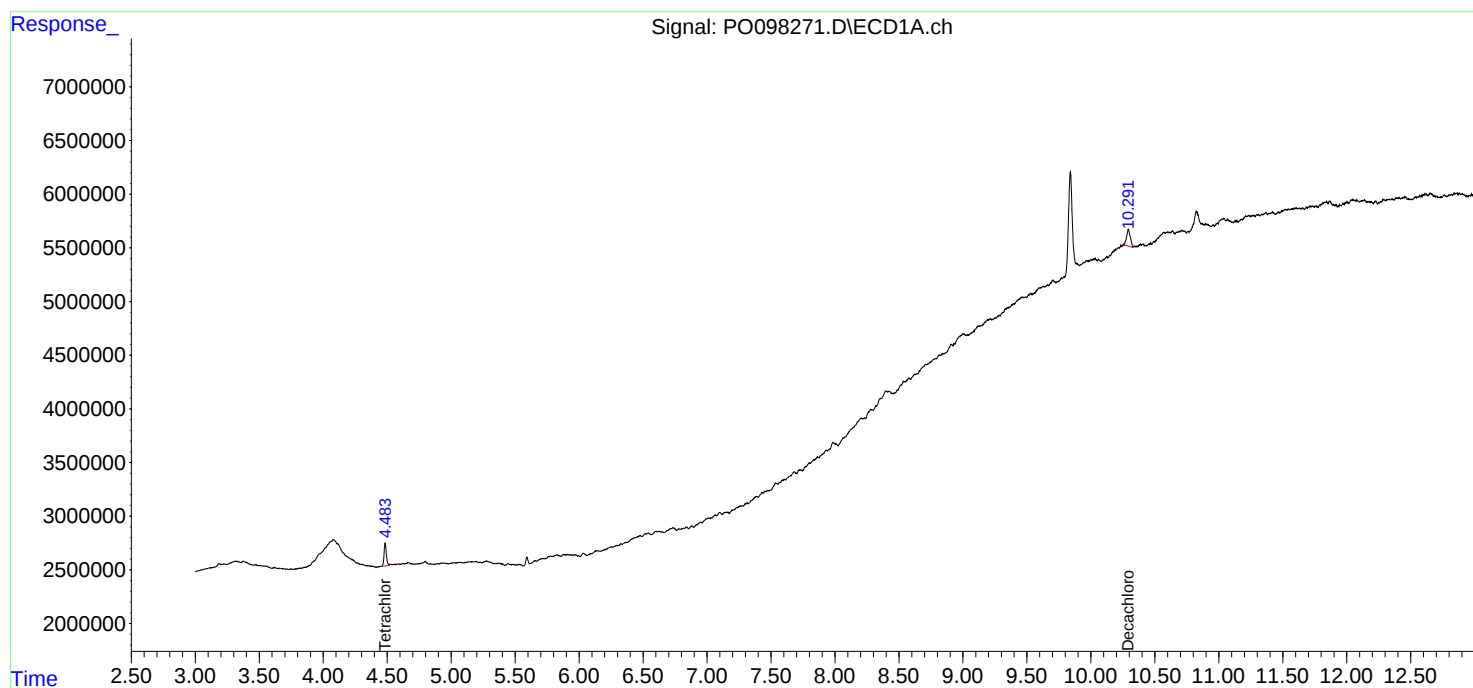

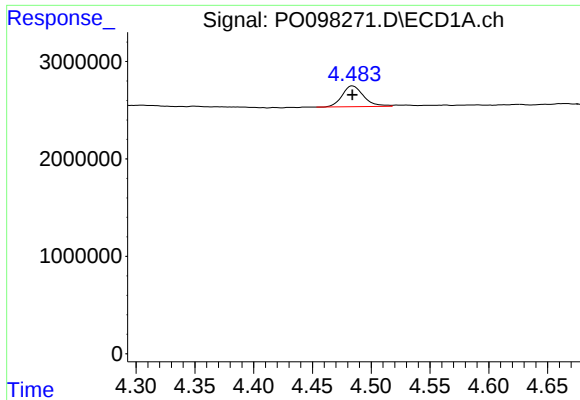


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.000 min
Response: 2713958
Conc: 1.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA872E-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

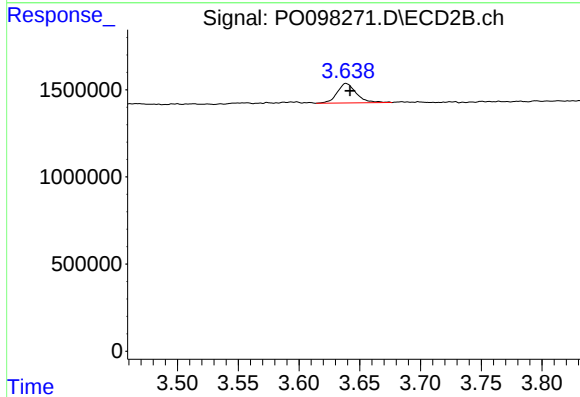


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.004 min
Response: 1236497
Conc: 1.63 ng/ml m

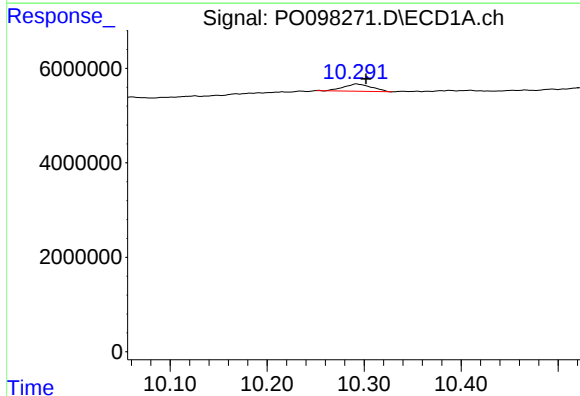

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.010 min
Response: 3107837
Conc: 3.87 ng/ml

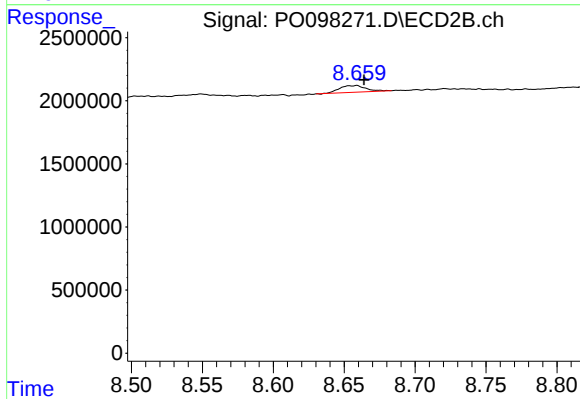

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.006 min
Response: 692569
Conc: 1.80 ng/ml