

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0092623\
 Data File : P0098296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2023 23:03
 Operator : YP/AJ
 Sample : PB155834BSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 PB155834BSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 00:53:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0092523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 26 09:03:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.639	46007987	19018429	24.100	25.055m
2) SA Decachlor...	10.297	8.652	30511575	15756645	37.958	40.918m
Target Compounds						
26) L6 AR-1254-1	6.516	5.527	11342683	6429271	207.567m	190.432m
27) L6 AR-1254-2	6.735	5.675	16560317	6606914	210.446m	226.728m
28) L6 AR-1254-3	7.104	6.080	32699593	15876801	449.029	372.047m
29) L6 AR-1254-4	7.390	6.310	27202240	11988180	662.990	575.011
30) L6 AR-1254-5	7.809	6.728	59493729	37376850	1228.287	1136.947

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092623\
Data File : PO098296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2023 23:03
Operator : YP/AJ
Sample : PB155834BSD
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB155834BSD


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 09/27/2023
Supervised By : Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 00:53:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092523.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 26 09:03:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

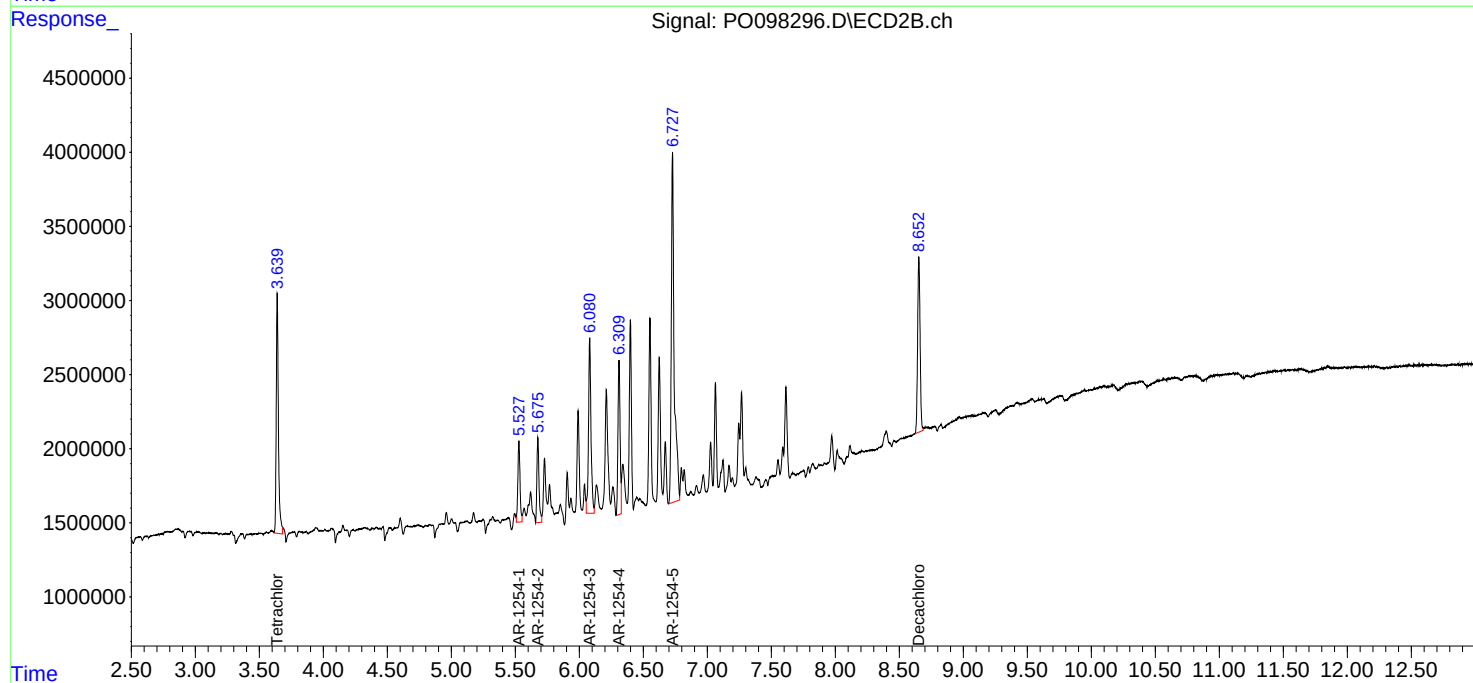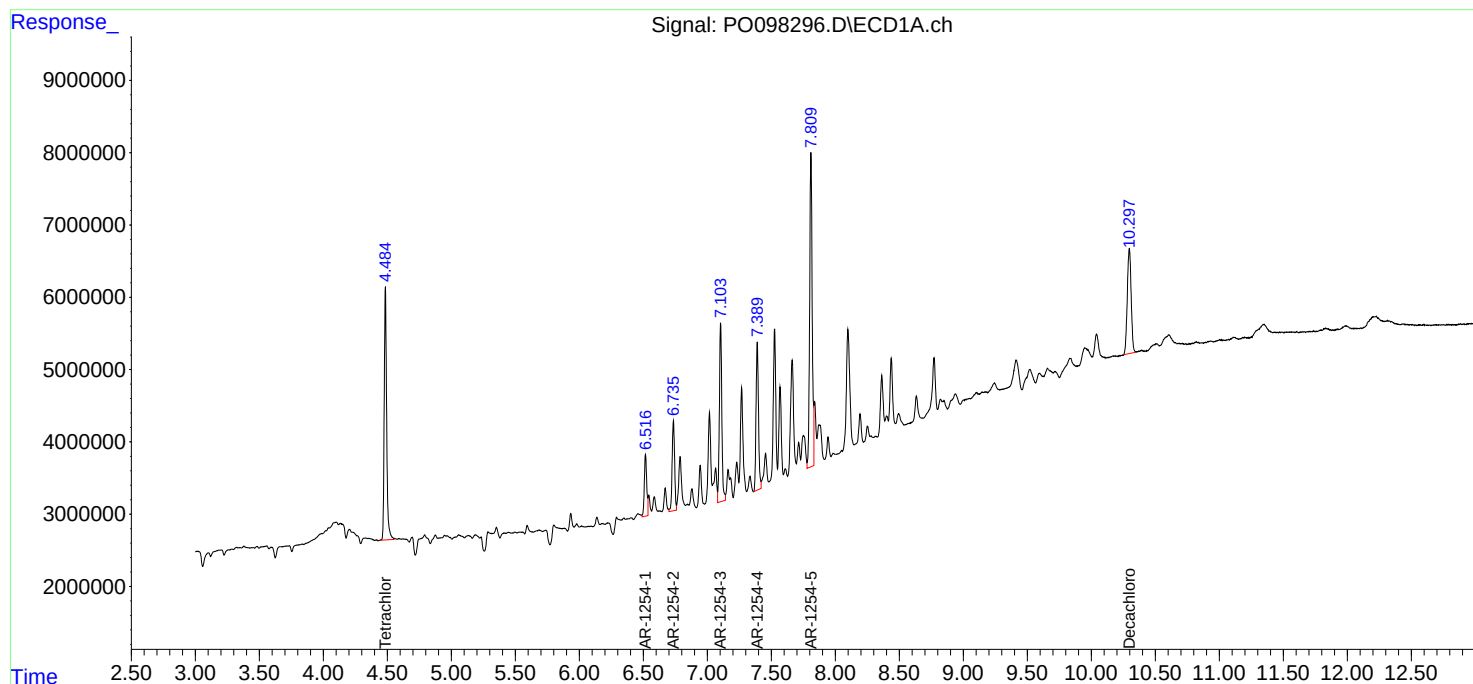

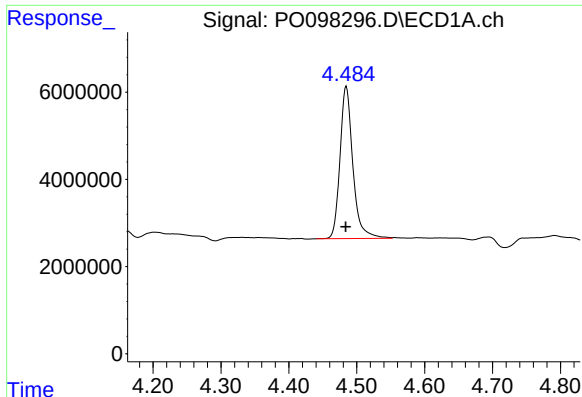


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: 0.000 min
Response: 46007987
Conc: 24.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB155834BSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

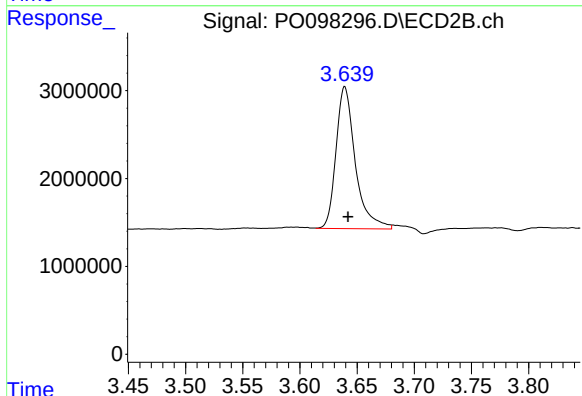


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.003 min
Response: 19018429
Conc: 25.06 ng/ml m

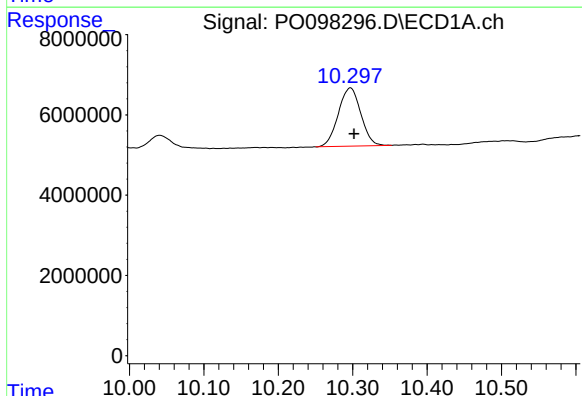


#2 Decachlorobiphenyl

R.T.: 10.297 min
Delta R.T.: -0.005 min
Response: 30511575
Conc: 37.96 ng/ml

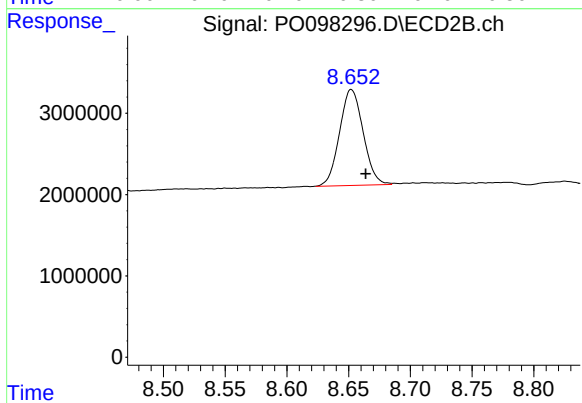

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.012 min
Response: 15756645
Conc: 40.92 ng/ml m

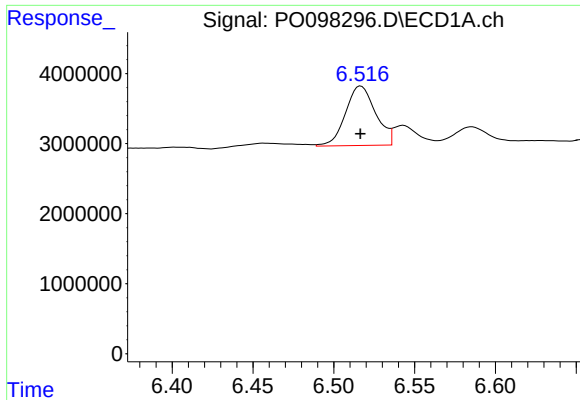


#26 AR-1254-1

R.T.: 6.516 min
Delta R.T.: 0.000 min
Response: 11342683
Conc: 207.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB155834BSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

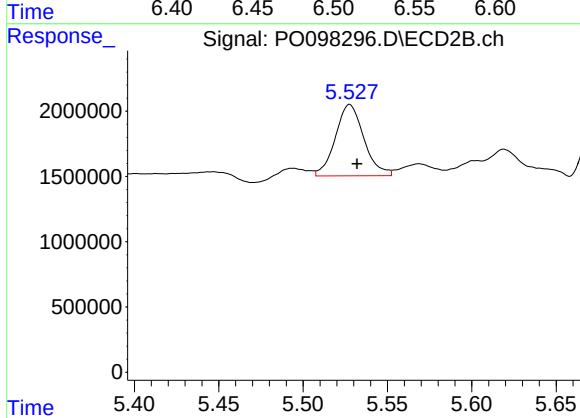


#26 AR-1254-1

R.T.: 5.527 min
Delta R.T.: -0.005 min
Response: 6429271
Conc: 190.43 ng/ml m

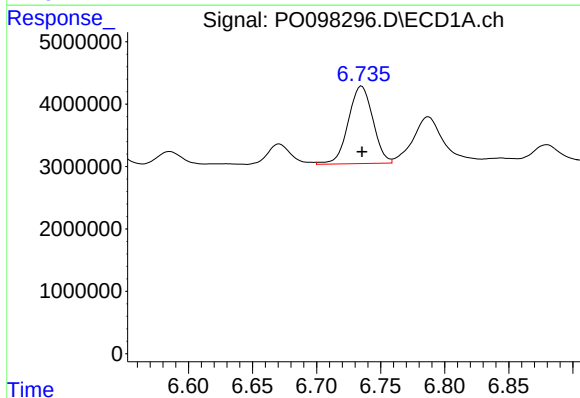


#27 AR-1254-2

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 16560317
Conc: 210.45 ng/ml m

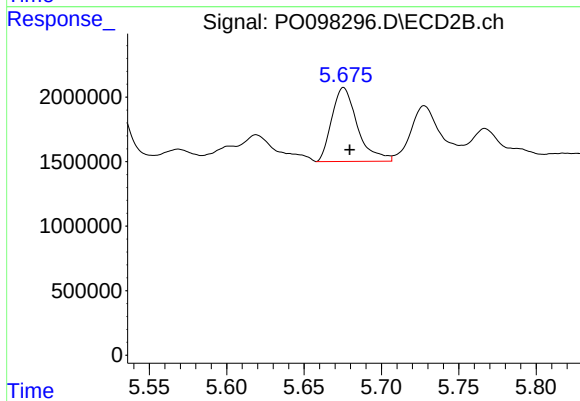

#27 AR-1254-2

R.T.: 5.675 min
Delta R.T.: -0.004 min
Response: 6606914
Conc: 226.73 ng/ml m

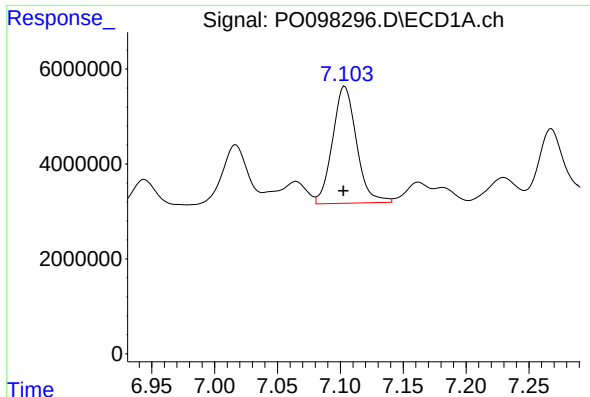


#28 AR-1254-3

R.T.: 7.104 min
Delta R.T.: 0.001 min
Response: 32699593
Conc: 449.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB155834BSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

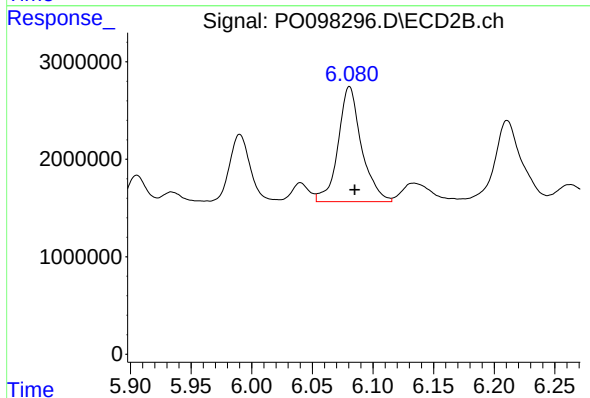


#28 AR-1254-3

R.T.: 6.080 min
Delta R.T.: -0.005 min
Response: 15876801
Conc: 372.05 ng/ml m

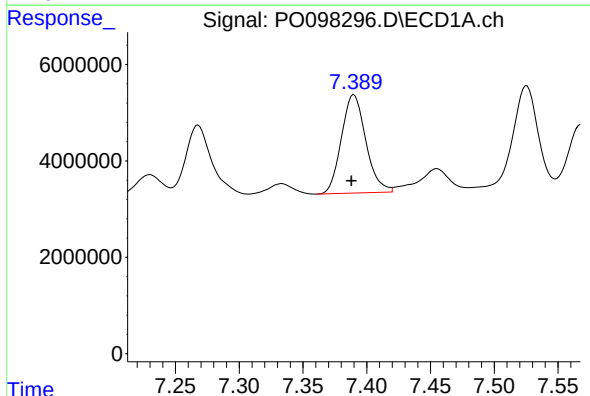


#29 AR-1254-4

R.T.: 7.390 min
Delta R.T.: 0.002 min
Response: 27202240
Conc: 662.99 ng/ml

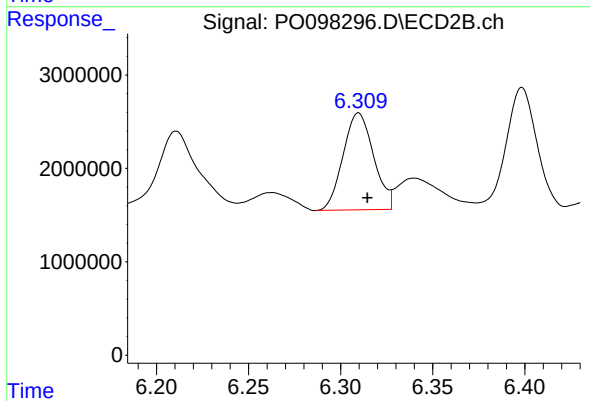

#29 AR-1254-4

R.T.: 6.310 min
Delta R.T.: -0.005 min
Response: 11988180
Conc: 575.01 ng/ml

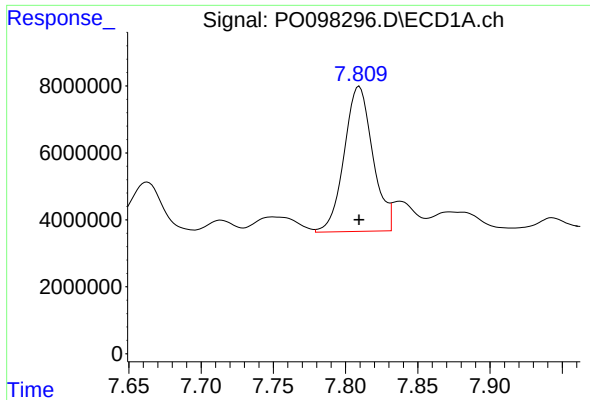


#30 AR-1254-5

R.T.: 7.809 min
Delta R.T.: 0.000 min
Response: 59493729
Conc: 1228.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB155834BSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

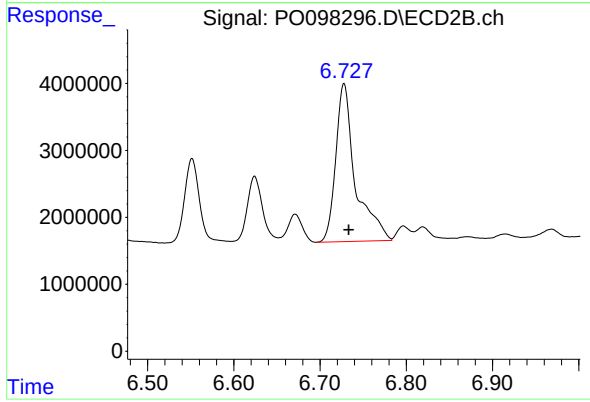

#30 AR-1254-5

R.T.: 6.728 min
Delta R.T.: -0.005 min
Response: 37376850
Conc: 1136.95 ng/ml