

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092623\
 Data File : P0098312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 03:48
 Operator : YP/AJ
 Sample : 04612-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 07-A-07-B-07-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 03:58:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 26 09:03:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.485	3.639	39226838	15737388	20.548	20.733m
2) SA Decachlor...	10.296	8.653	25675753	9657782	31.942	25.080m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092623\
Data File : PO098312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 03:48
Operator : YP/AJ
Sample : 04612-07
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
07-A-07-B-07-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 03:58:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092523.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 26 09:03:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

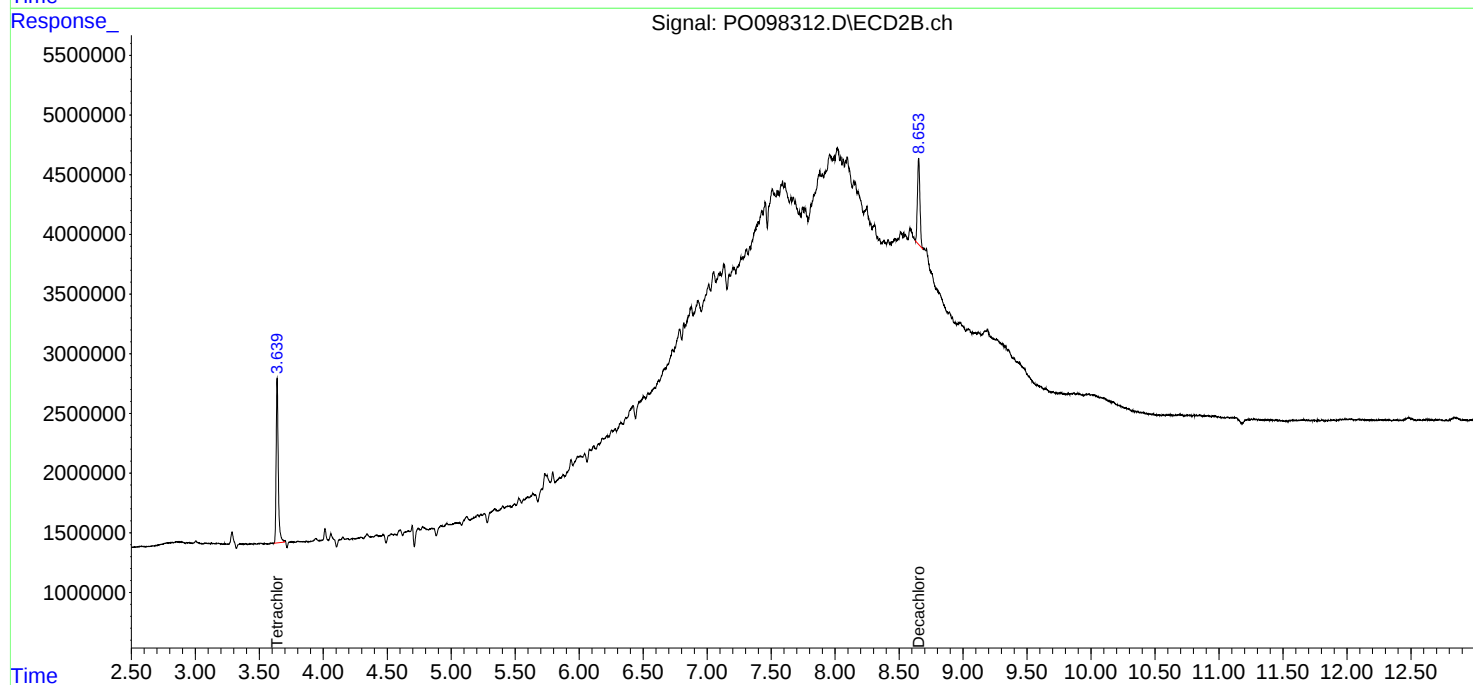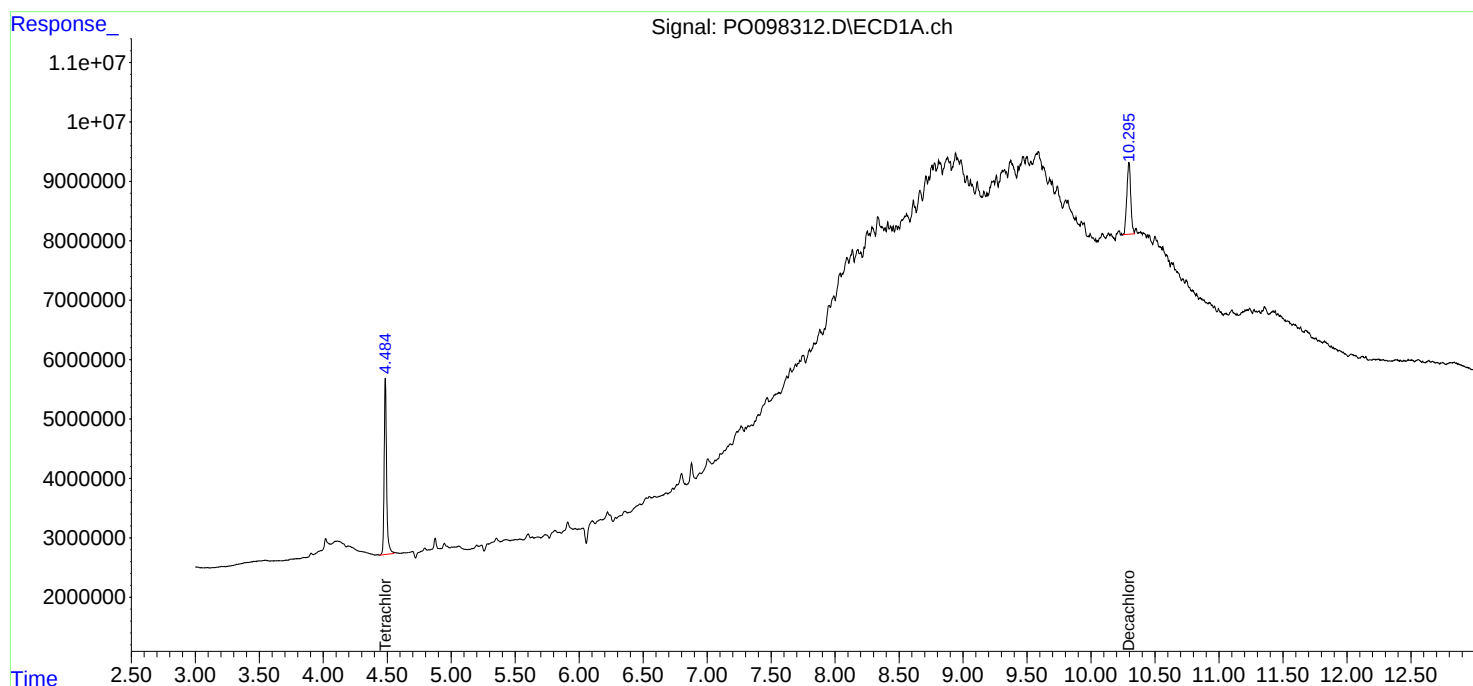

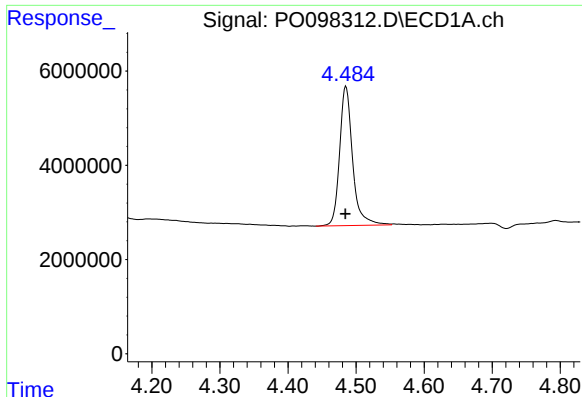


#1 Tetrachloro-m-xylene

R.T.: 4.485 min
Delta R.T.: 0.001 min
Response: 39226838
Conc: 20.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
07-A-07-B-07-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

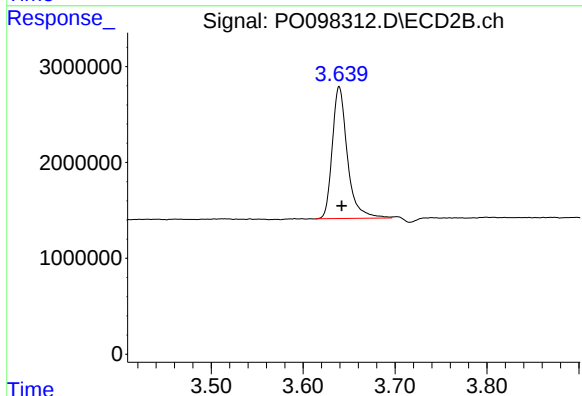


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.003 min
Response: 15737388
Conc: 20.73 ng/ml m

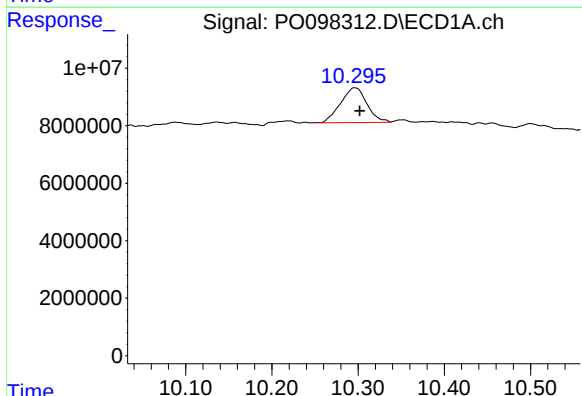

#2 Decachlorobiphenyl

R.T.: 10.296 min
Delta R.T.: -0.005 min
Response: 25675753
Conc: 31.94 ng/ml

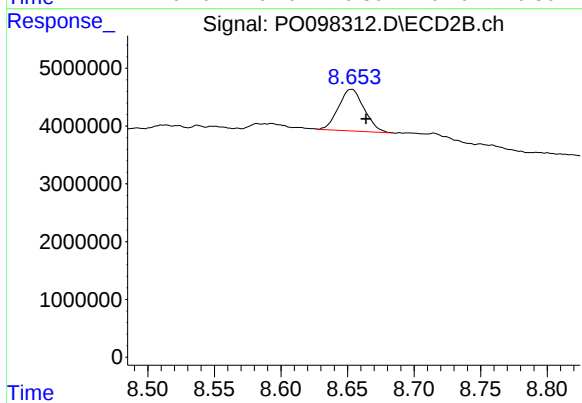

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.011 min
Response: 9657782
Conc: 25.08 ng/ml m