

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092623\
 Data File : P0098313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 04:04
 Operator : YP/AJ
 Sample : 04612-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 08-A-08-B-08-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 04:23:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 26 09:03:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.484	3.639	40323669	15933913	21.122	20.991m
2) SA Decachlor...	10.292	8.652	25399973	9940130	31.599	25.813m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO092623\
Data File : PO098313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 04:04
Operator : YP/AJ
Sample : 04612-08
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
08-A-08-B-08-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 04:23:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092523.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 26 09:03:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

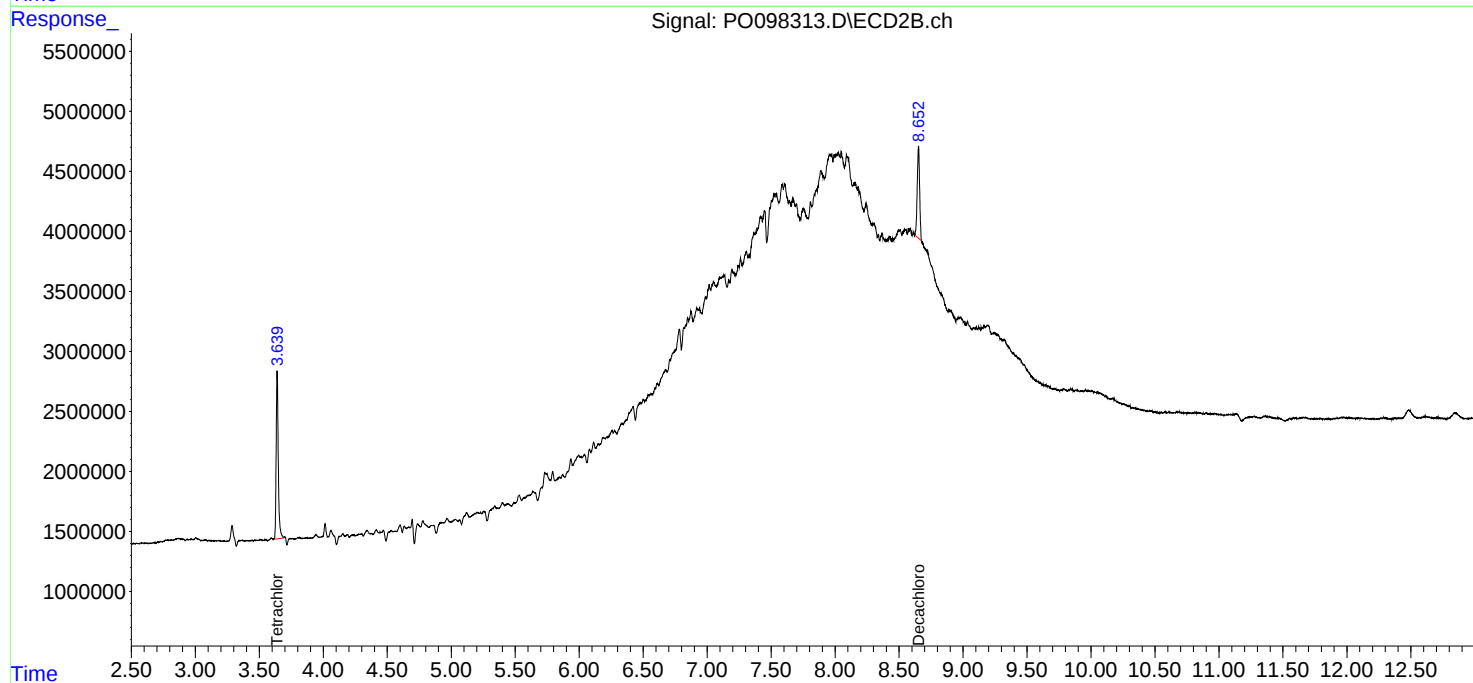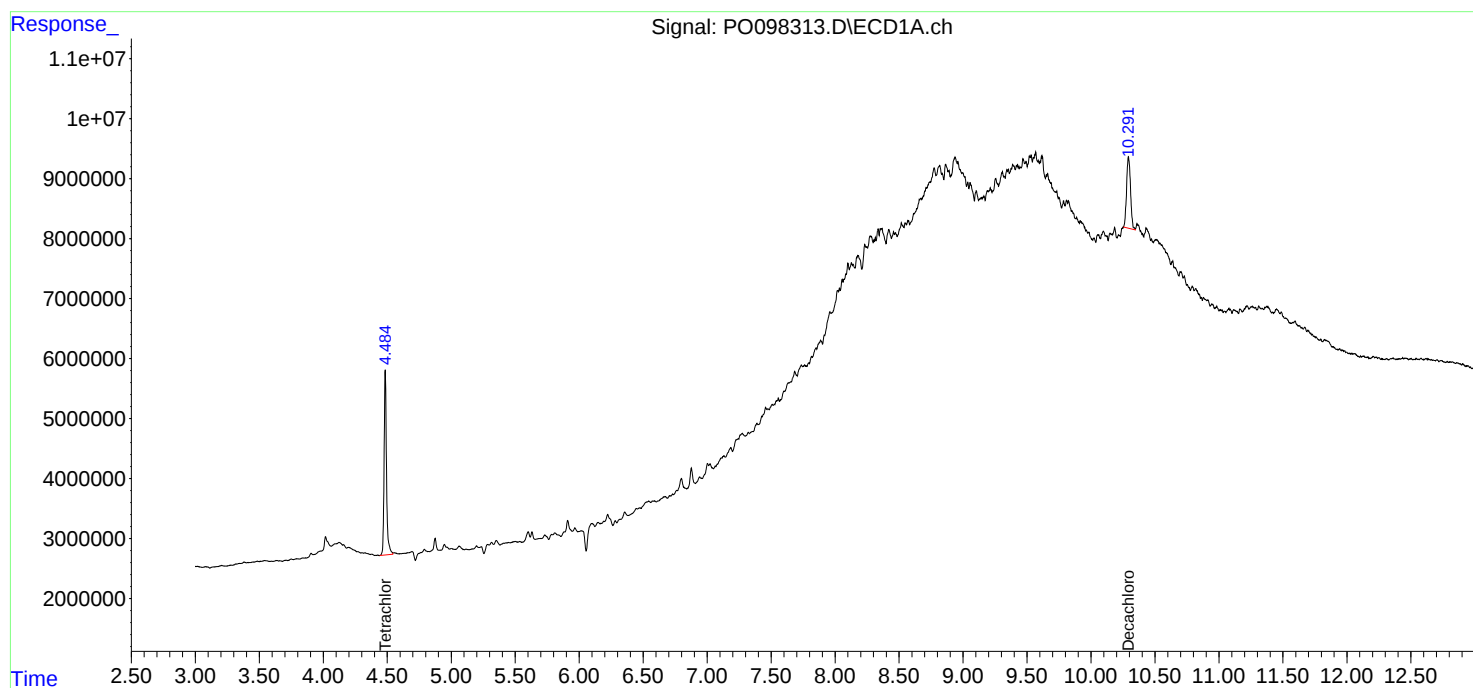

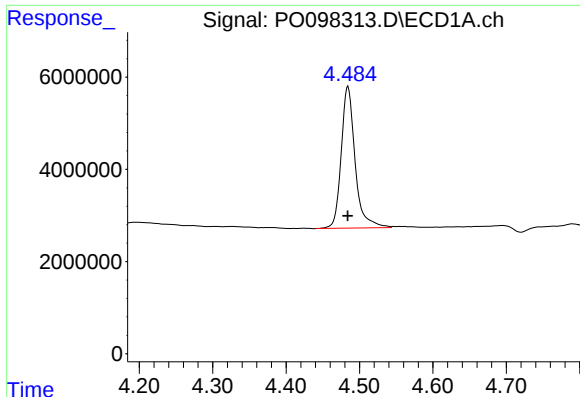


#1 Tetrachloro-m-xylene

R.T.: 4.484 min
Delta R.T.: 0.000 min
Response: 40323669
Conc: 21.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
08-A-08-B-08-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :Ankita Jodhani 09/27/2023

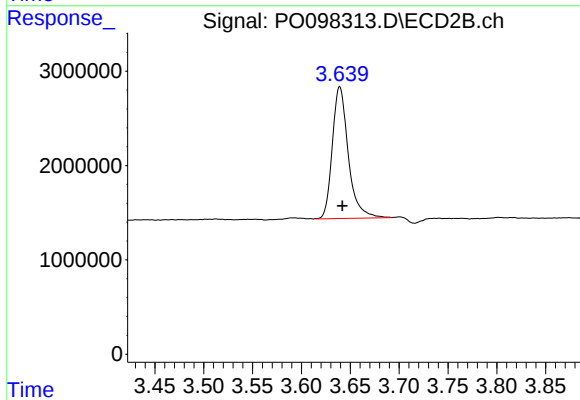


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.003 min
Response: 15933913
Conc: 20.99 ng/ml m

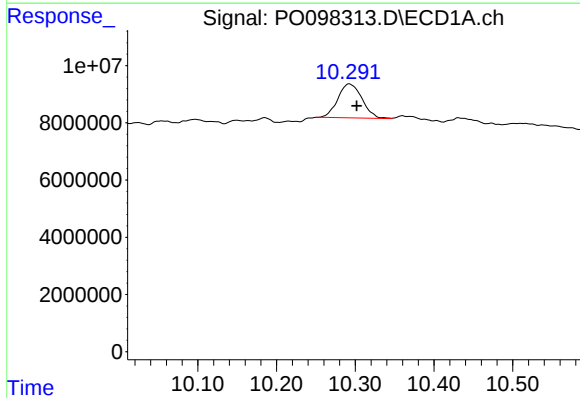

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.010 min
Response: 25399973
Conc: 31.60 ng/ml

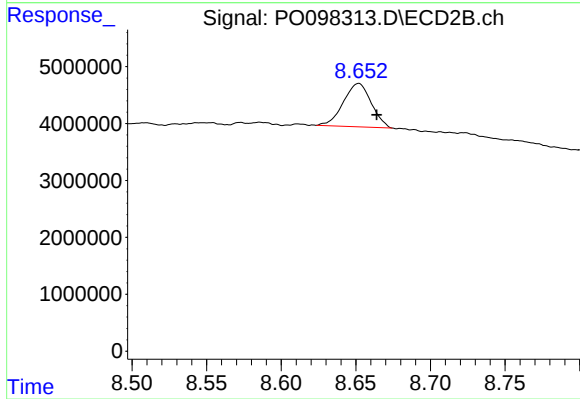

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.012 min
Response: 9940130
Conc: 25.81 ng/ml m