

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 18:51
 Operator : HP/AJ
 Sample : K5060-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-060

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:56:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.367	3.526	866836	696541	23.561	24.946
2)	SA Decachlor...	10.030	8.398	623712	400657	13.575	11.430
Target Compounds							
3)	L1 AR-1016-1	5.602	0.000	4176	0	2.613	N.D. #
4)	L1 AR-1016-2	5.602	0.000	4176	0	1.824	N.D. #
5)	L1 AR-1016-3	5.602	4.773	4176	3775	2.909	3.893 #
6)	L1 AR-1016-4	5.688	4.813	26379	4002	22.364	4.889 #
7)	L1 AR-1016-5	0.000	4.964	0	29900	N.D.	28.548 #
9)	L2 AR-1221-2	4.671	3.815	12775	13221	37.401	47.044 #
10)	L2 AR-1221-3	4.753	3.889	90987	84022	85.901	101.223
11)	L3 AR-1232-1	4.753	3.889	90987	84022	77.982	92.196
12)	L3 AR-1232-2	5.267	0.000	6975	0	10.757	N.D. #
13)	L3 AR-1232-3	5.602	4.773	4176	3775	3.118	6.726 #
14)	L3 AR-1232-4	5.688	4.873	26379	3392	38.390	6.496 #
15)	L3 AR-1232-5	5.804	4.964	6347	29900	11.591	52.834 #
16)	L4 AR-1242-1	5.602	0.000	4176	0	3.499	N.D. #
17)	L4 AR-1242-2	5.602	0.000	4176	0	2.444	N.D. #
18)	L4 AR-1242-3	5.602	4.773	4176	3775	3.857	5.282 #
19)	L4 AR-1242-4	5.688	4.873	26379	3392	29.881	4.658 #
20)	L4 AR-1242-5	6.472	5.364	12640	47209	11.279	47.691 #
21)	L5 AR-1248-1	5.602	0.000	4176	0	4.536	N.D. #
22)	L5 AR-1248-2	5.804	4.813	6347	4002	4.746	4.142
23)	L5 AR-1248-3	0.000	4.873	0	3392	N.D.	3.368 #
24)	L5 AR-1248-4	6.417	4.964	70323	29900	38.599	24.898 #
25)	L5 AR-1248-5	6.472	5.364	12640	47209	7.224	37.345 #
26)	L6 AR-1254-1	6.393	5.364	56745	47209	29.453	22.907
27)	L6 AR-1254-2	6.608	5.500	188741	5213	59.976	2.762 #
28)	L6 AR-1254-3	6.972	5.896	31982	4477	9.081	1.408 #
29)	L6 AR-1254-4	7.250	6.128	12184	7959	4.501	3.823
30)	L6 AR-1254-5	7.666	6.531	9961	16402	3.378	5.182 #
31)	L7 AR-1260-1	7.128	6.025	7942	6598	3.262	3.137
32)	L7 AR-1260-2	7.380	6.208	74388	10151	24.605	3.935 #
33)	L7 AR-1260-3	7.796	6.359	8687	10321	3.640	4.286
34)	L7 AR-1260-4	7.963	6.825	58722	6296	20.989	2.942 #
35)	L7 AR-1260-5	8.280	7.061	58320	8428	10.710	1.744 #
36)	L8 AR-1262-1	7.796	6.531	8687	16402	2.459	5.491 #
37)	L8 AR-1262-2	8.280	7.061	58320	8428	9.355	1.621 #
38)	L8 AR-1262-3	0.000	7.379	0	4052	N.D.	1.909 #
39)	L8 AR-1262-4	8.677	7.379	46383	4052	14.226	1.061 #
40)	L8 AR-1262-5	9.271	7.894	23899	2484	11.753	1.484 #
41)	L9 AR-1268-1	8.513	7.379	12649	4052	1.714	0.691 #
42)	L9 AR-1268-2	8.677	7.379	46383	4052	6.866	0.760 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 18:51
 Operator : HP/AJ
 Sample : K5060-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-060

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:56:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.889	7.627	5236	567	0.932	0.128 #
44) L9	AR-1268-4	9.271	7.894	23899	2484	10.360	1.300 #
45) L9	AR-1268-5	0.000	8.164	0	24054	N.D.	1.999 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061435.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 18:51
Operator : HP/AJ
Sample : K5060-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:56:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

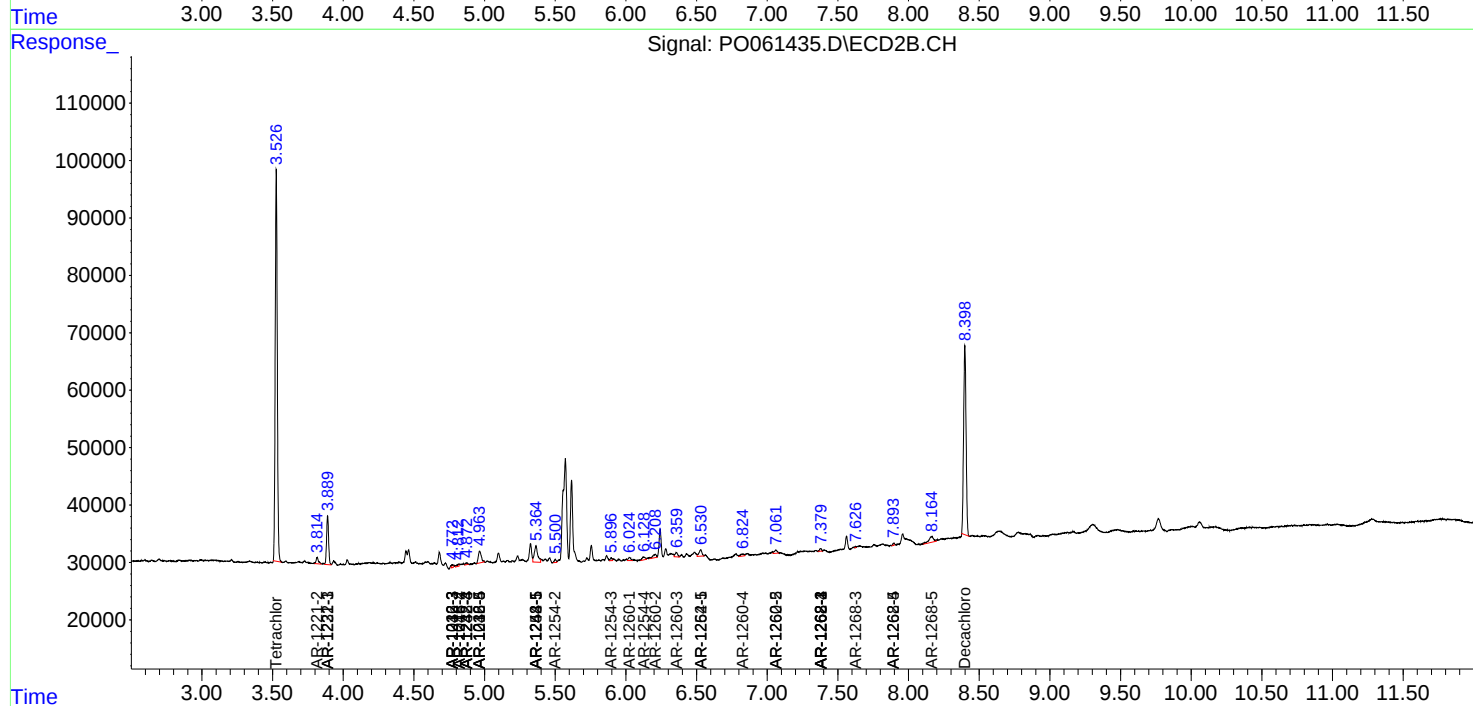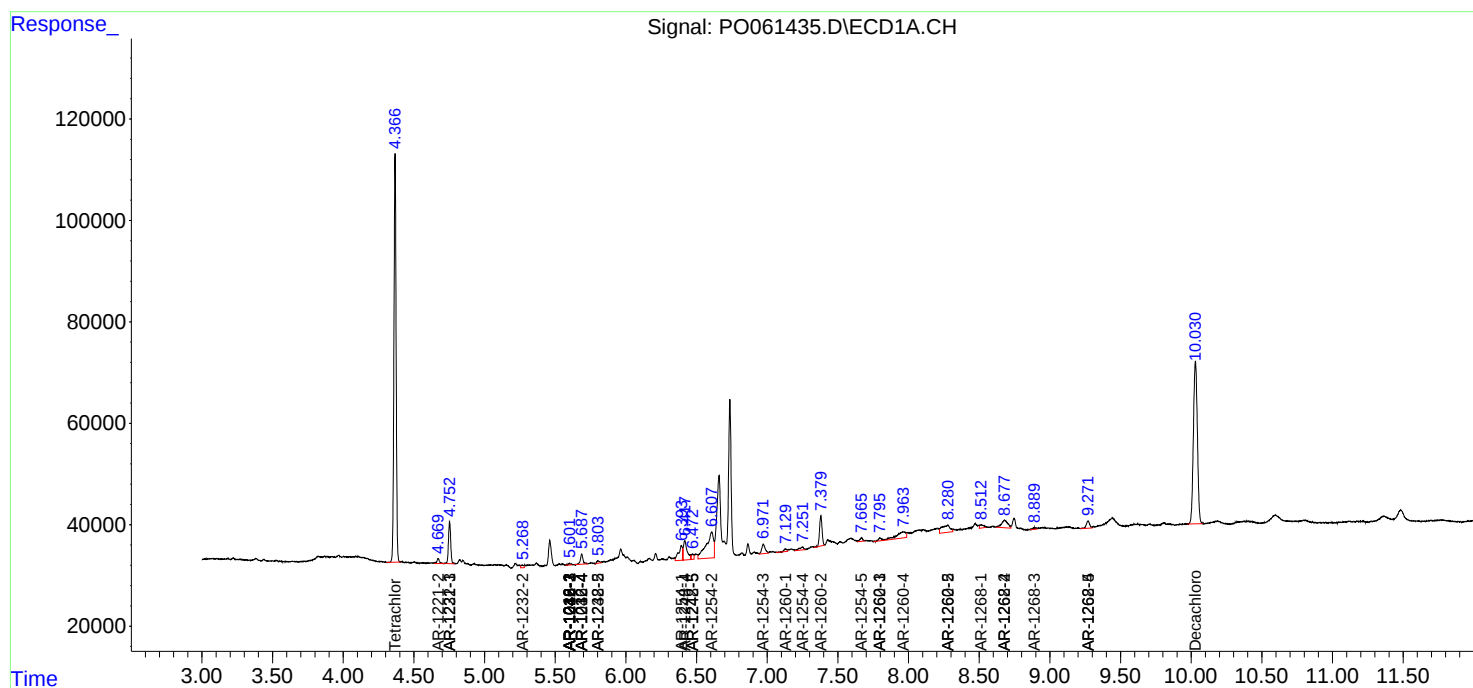


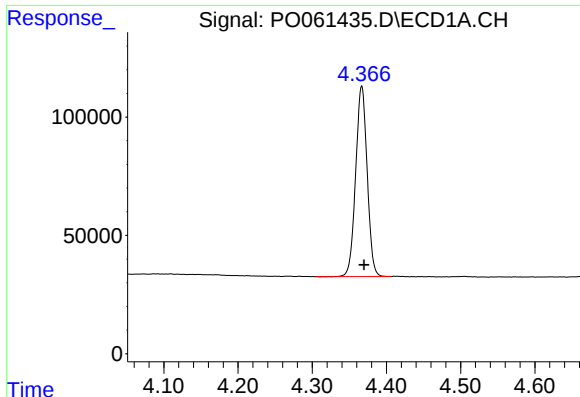

#1 Tetrachloro-m-xylene


R.T.: 4.367 min
Delta R.T.: -0.003 min
Response: 866836
Conc: 23.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

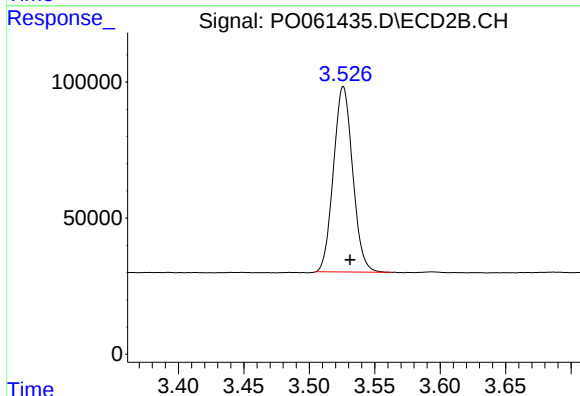


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.005 min
Response: 696541
Conc: 24.95 ng/ml

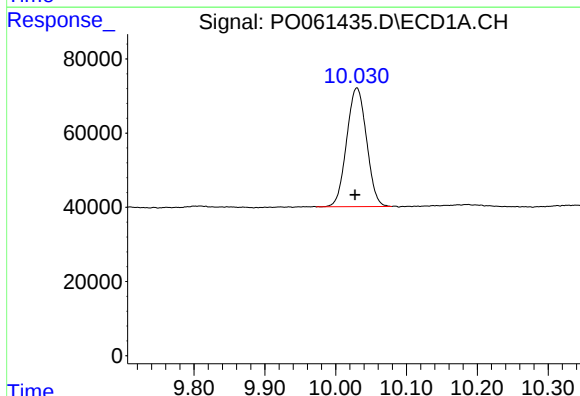


#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.002 min
Response: 623712
Conc: 13.57 ng/ml

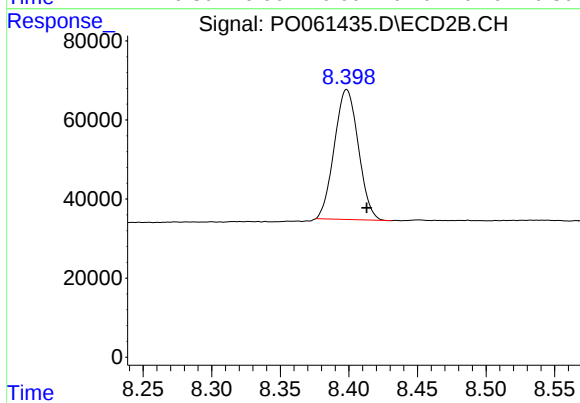

#2 Decachlorobiphenyl


R.T.: 8.398 min
Delta R.T.: -0.015 min
Response: 400657
Conc: 11.43 ng/ml

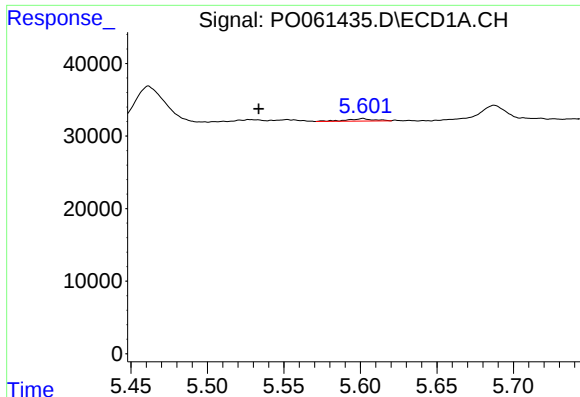

#3 AR-1016-1


R.T.: 5.602 min
Delta R.T.: 0.068 min
Response: 4176
Conc: 2.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

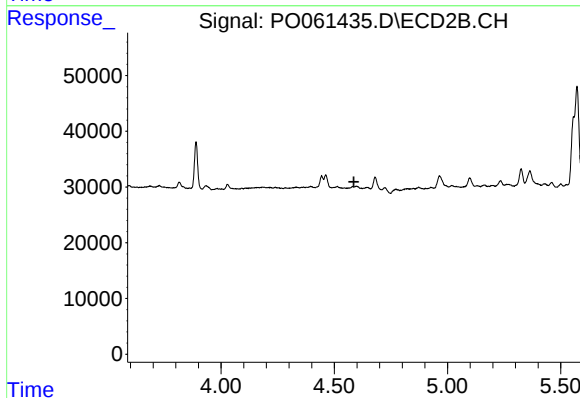


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.586 min
Response: 0
Conc: N.D.

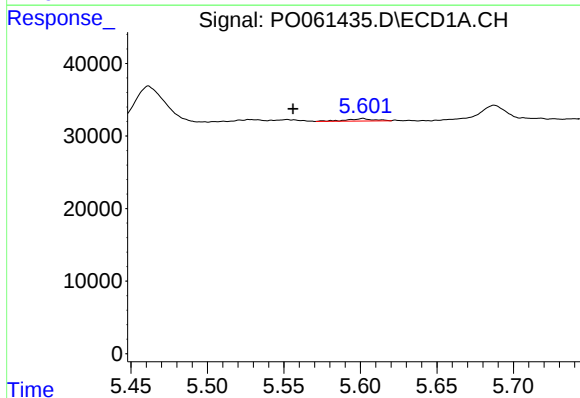


#4 AR-1016-2

R.T.: 5.602 min
Delta R.T.: 0.046 min
Response: 4176
Conc: 1.82 ng/ml

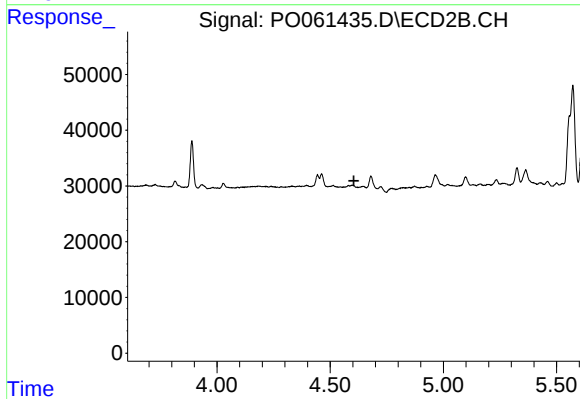

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.605 min
Response: 0
Conc: N.D.

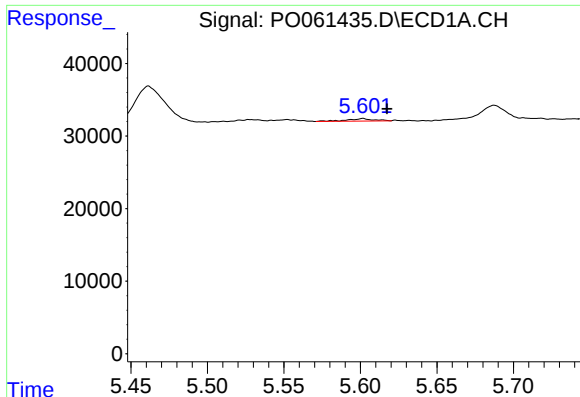

#5 AR-1016-3


R.T.: 5.602 min
Delta R.T.: -0.016 min
Response: 4176
Conc: 2.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

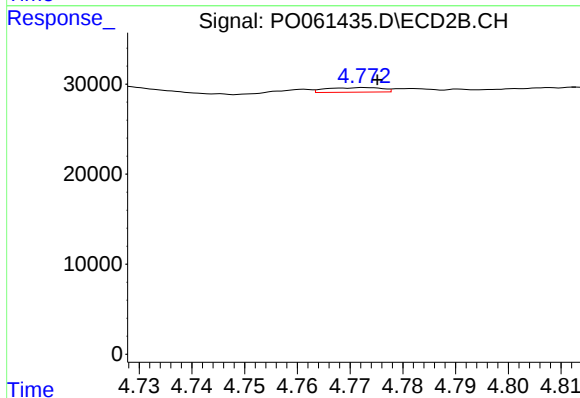


#5 AR-1016-3

R.T.: 4.773 min
Delta R.T.: -0.002 min
Response: 3775
Conc: 3.89 ng/ml

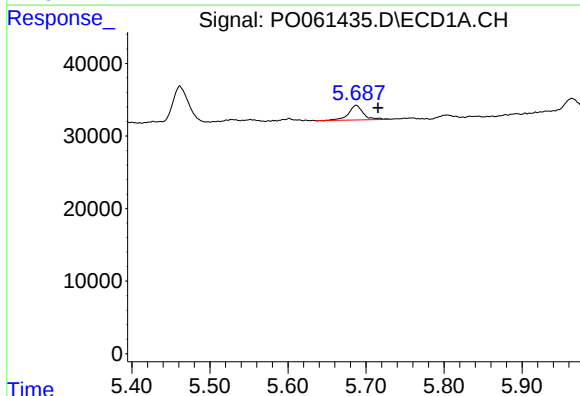


#6 AR-1016-4

R.T.: 5.688 min
Delta R.T.: -0.028 min
Response: 26379
Conc: 22.36 ng/ml

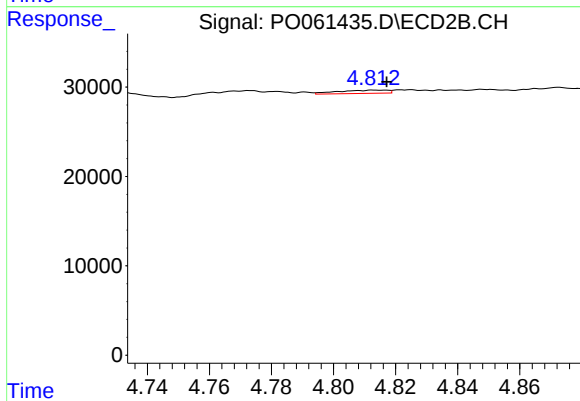

#6 AR-1016-4


R.T.: 4.813 min
Delta R.T.: -0.004 min
Response: 4002
Conc: 4.89 ng/ml

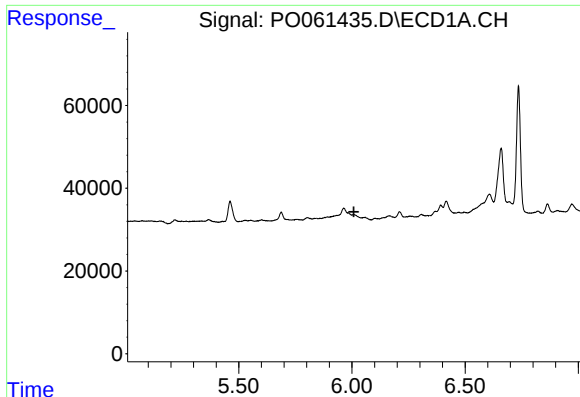

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

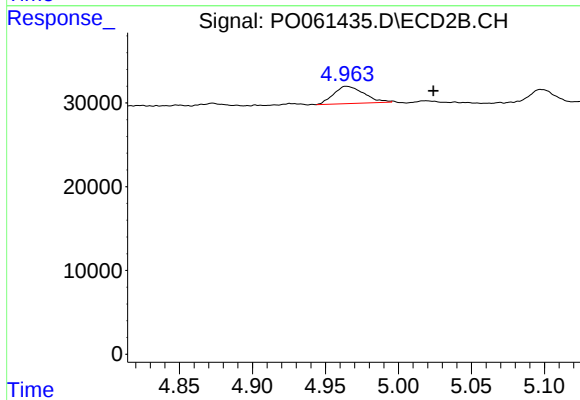


#7 AR-1016-5

R.T.: 4.964 min
Delta R.T.: -0.060 min
Response: 29900
Conc: 28.55 ng/ml

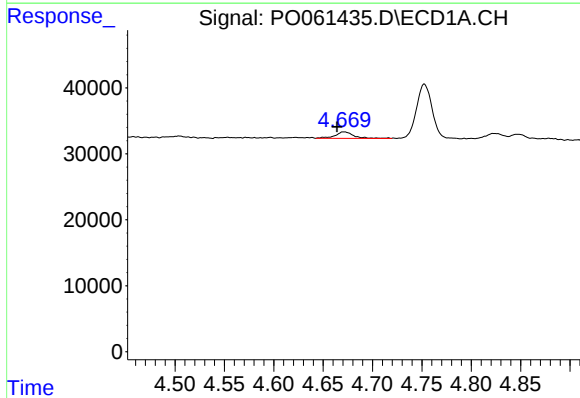


#9 AR-1221-2

R.T.: 4.671 min
Delta R.T.: 0.007 min
Response: 12775
Conc: 37.40 ng/ml

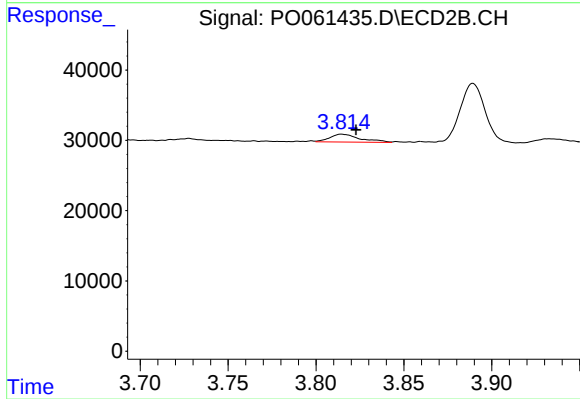

#9 AR-1221-2


R.T.: 3.815 min
Delta R.T.: -0.008 min
Response: 13221
Conc: 47.04 ng/ml

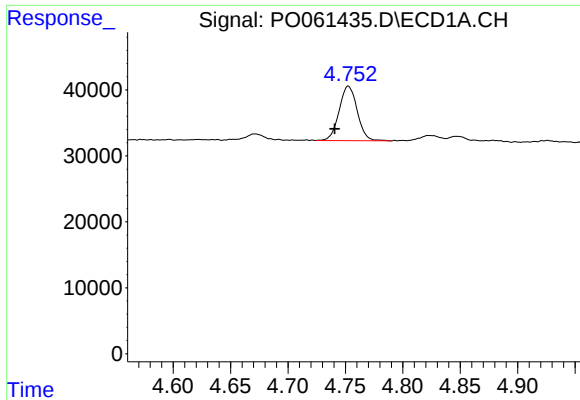

#10 AR-1221-3


R.T.: 4.753 min
Delta R.T.: 0.012 min
Response: 90987
Conc: 85.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

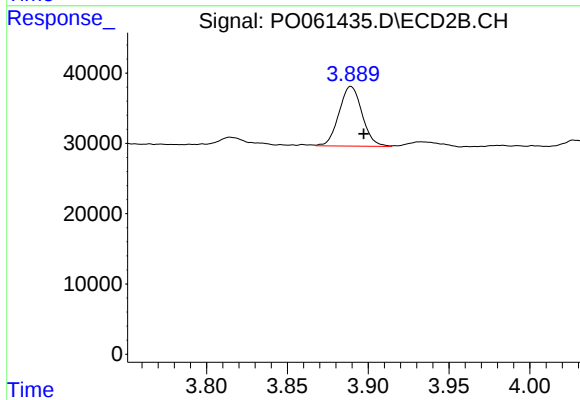


#10 AR-1221-3

R.T.: 3.889 min
Delta R.T.: -0.008 min
Response: 84022
Conc: 101.22 ng/ml

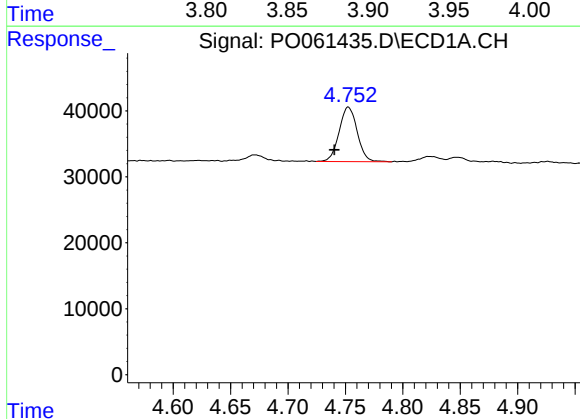


#11 AR-1232-1

R.T.: 4.753 min
Delta R.T.: 0.012 min
Response: 90987
Conc: 77.98 ng/ml

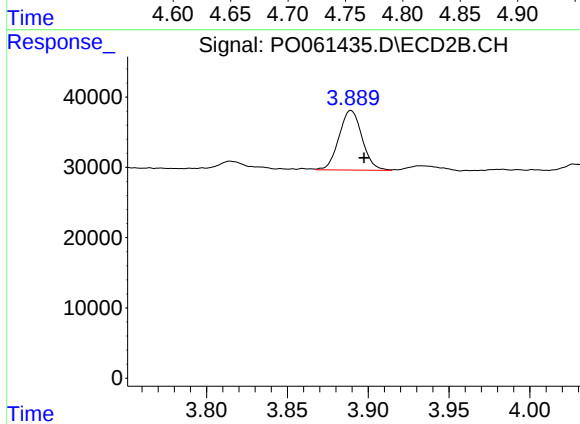

#11 AR-1232-1


R.T.: 3.889 min
Delta R.T.: -0.008 min
Response: 84022
Conc: 92.20 ng/ml

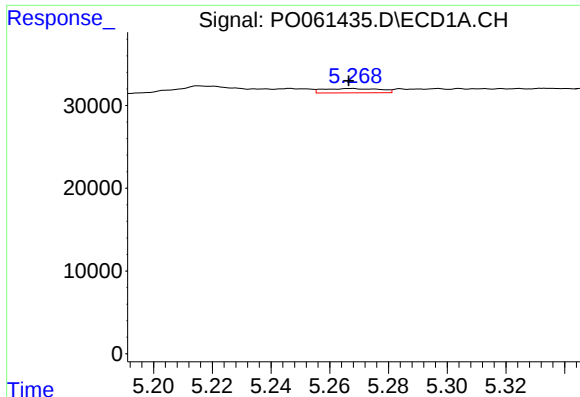

#12 AR-1232-2


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 6975
Conc: 10.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

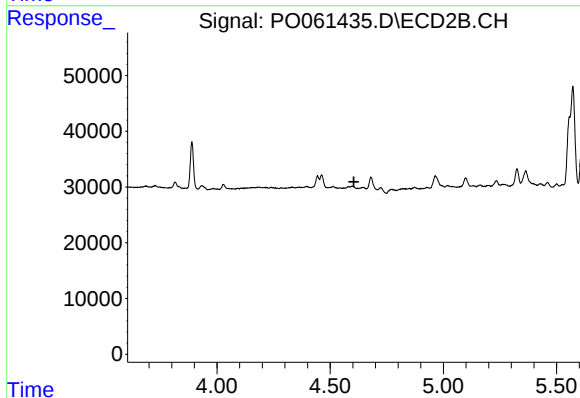


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.605 min
Response: 0
Conc: N.D.

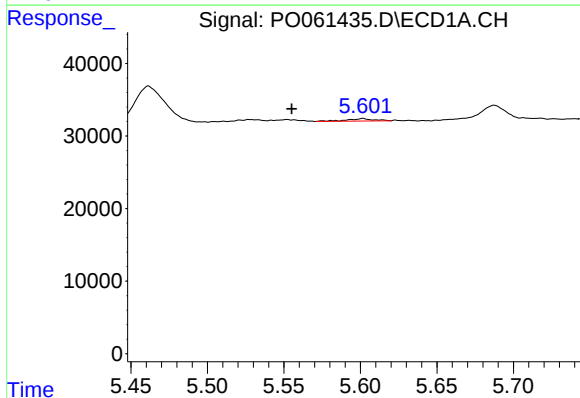


#13 AR-1232-3

R.T.: 5.602 min
Delta R.T.: 0.047 min
Response: 4176
Conc: 3.12 ng/ml

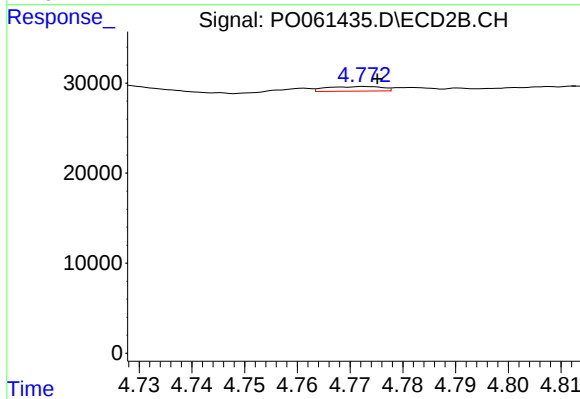

#13 AR-1232-3


R.T.: 4.773 min
Delta R.T.: -0.002 min
Response: 3775
Conc: 6.73 ng/ml

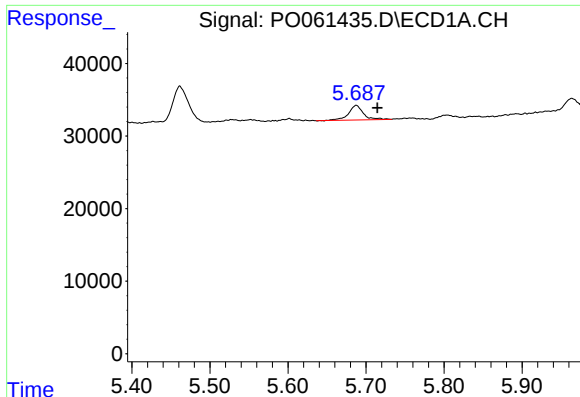

#14 AR-1232-4


R.T.: 5.688 min
Delta R.T.: -0.027 min
Response: 26379
Conc: 38.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

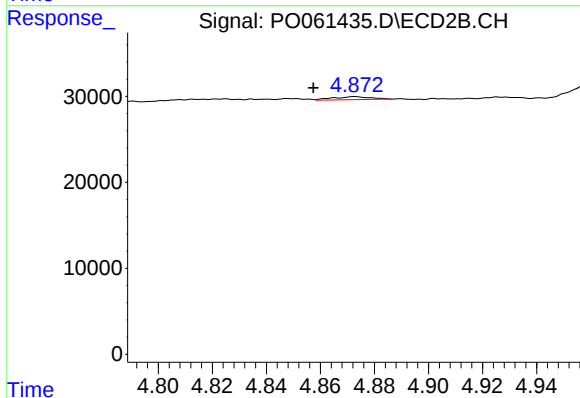


#14 AR-1232-4

R.T.: 4.873 min
Delta R.T.: 0.015 min
Response: 3392
Conc: 6.50 ng/ml

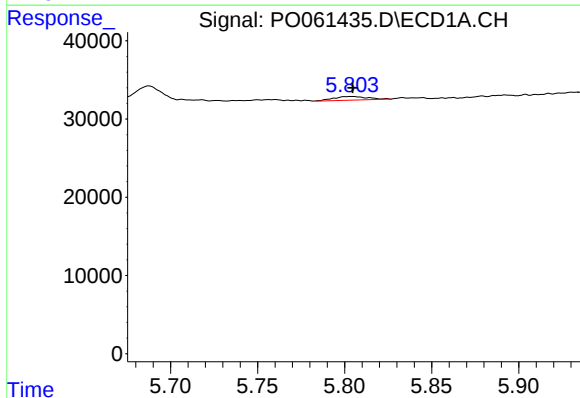


#15 AR-1232-5

R.T.: 5.804 min
Delta R.T.: -0.001 min
Response: 6347
Conc: 11.59 ng/ml

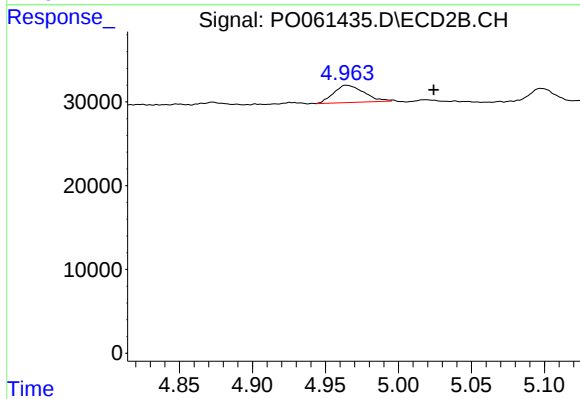

#15 AR-1232-5


R.T.: 4.964 min
Delta R.T.: -0.060 min
Response: 29900
Conc: 52.83 ng/ml

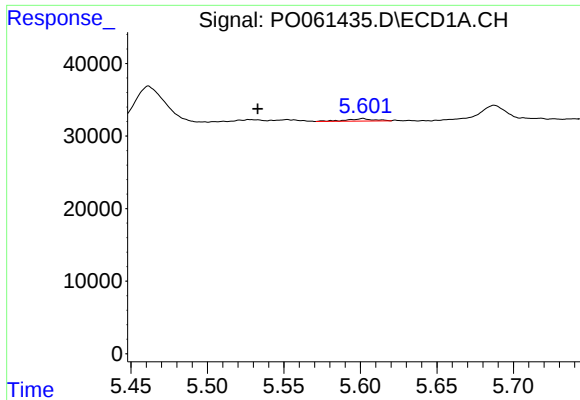

#16 AR-1242-1


R.T.: 5.602 min
Delta R.T.: 0.069 min
Response: 4176
Conc: 3.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

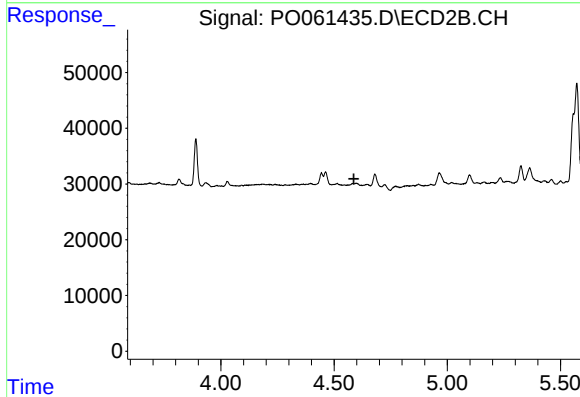


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.587 min
Response: 0
Conc: N.D.

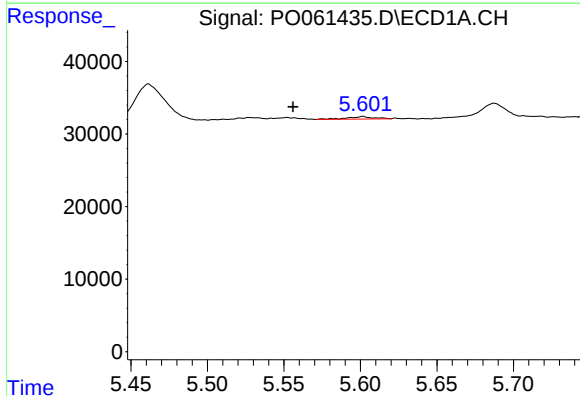


#17 AR-1242-2

R.T.: 5.602 min
Delta R.T.: 0.046 min
Response: 4176
Conc: 2.44 ng/ml

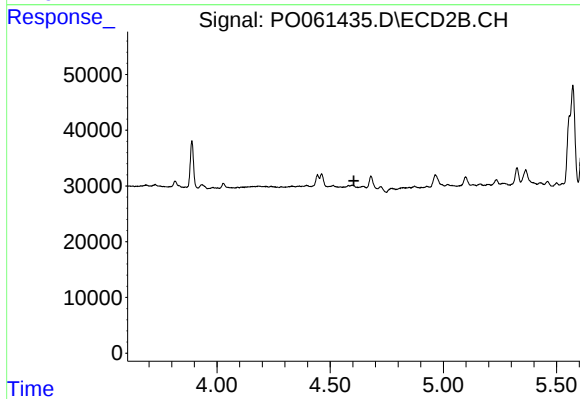

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T. : 4.605 min
Response: 0
Conc: N.D.

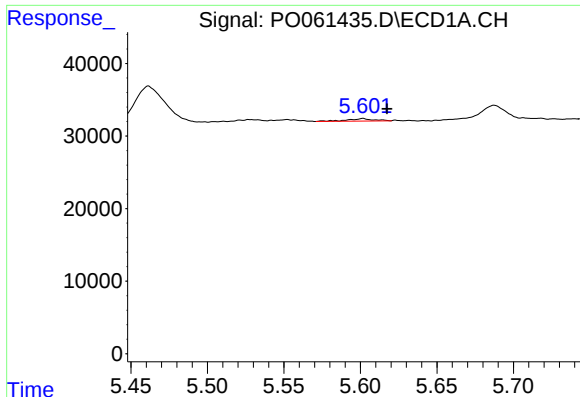

#18 AR-1242-3


R.T.: 5.602 min
Delta R.T.: -0.016 min
Response: 4176
Conc: 3.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

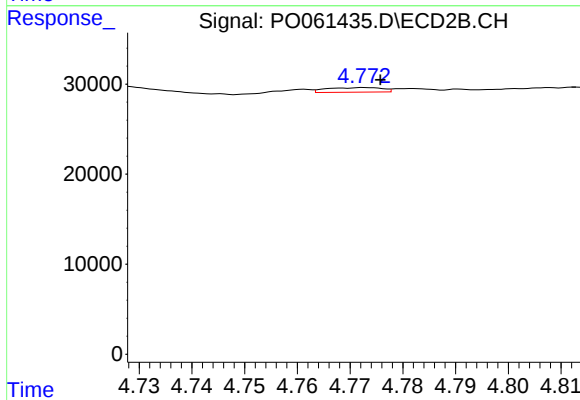


#18 AR-1242-3

R.T.: 4.773 min
Delta R.T.: -0.003 min
Response: 3775
Conc: 5.28 ng/ml

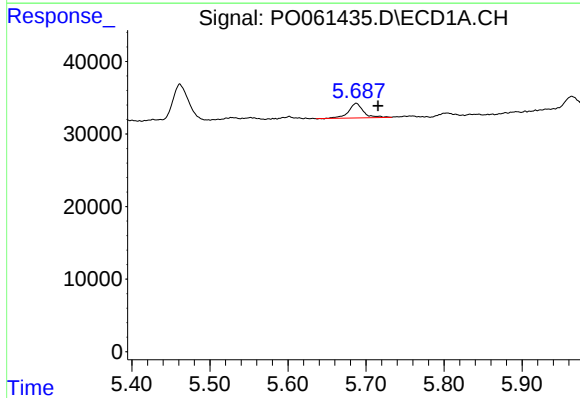


#19 AR-1242-4

R.T.: 5.688 min
Delta R.T.: -0.028 min
Response: 26379
Conc: 29.88 ng/ml

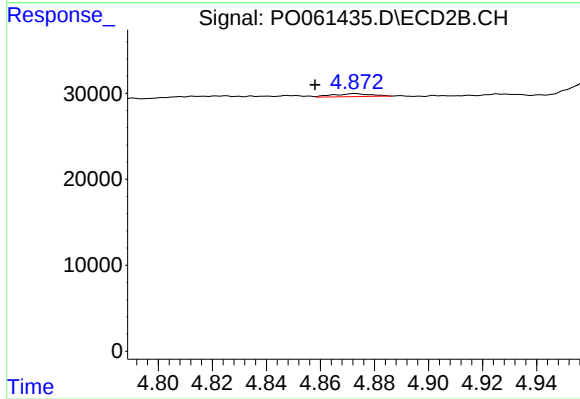

#19 AR-1242-4


R.T.: 4.873 min
Delta R.T.: 0.015 min
Response: 3392
Conc: 4.66 ng/ml

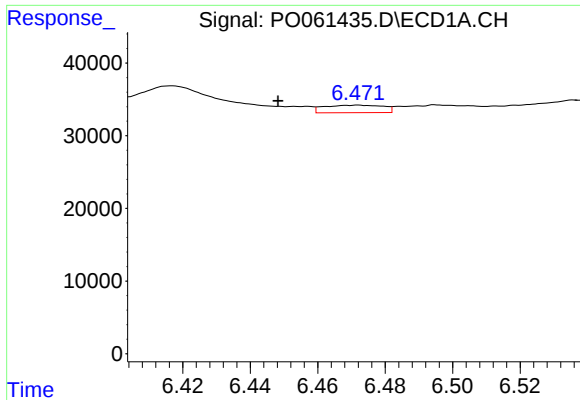

#20 AR-1242-5


R.T.: 6.472 min
Delta R.T.: 0.024 min
Response: 12640
Conc: 11.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

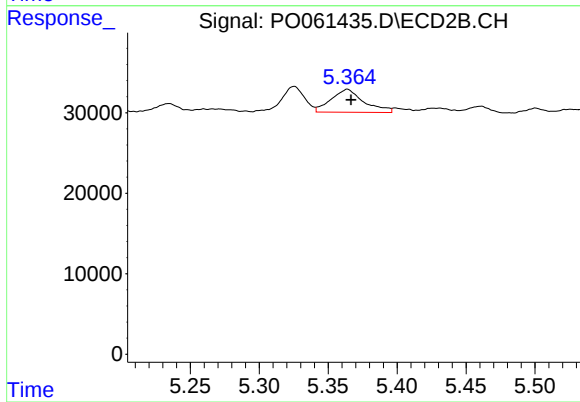


#20 AR-1242-5

R.T.: 5.364 min
Delta R.T.: -0.003 min
Response: 47209
Conc: 47.69 ng/ml

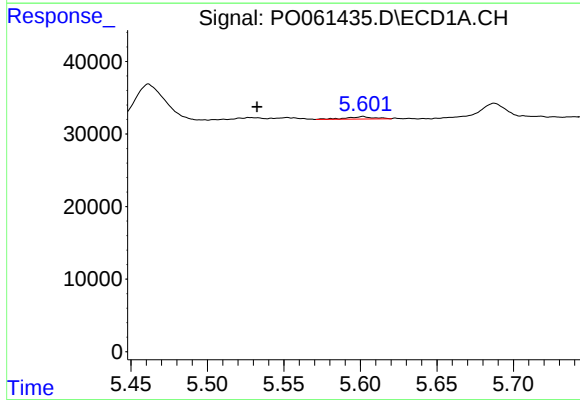


#21 AR-1248-1

R.T.: 5.602 min
Delta R.T.: 0.069 min
Response: 4176
Conc: 4.54 ng/ml

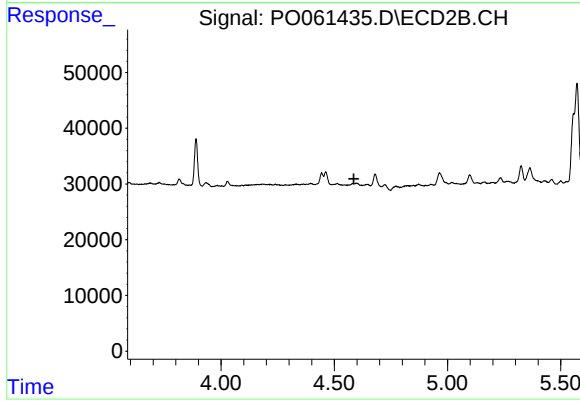

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 4.586 min
Response: 0
Conc: N.D.

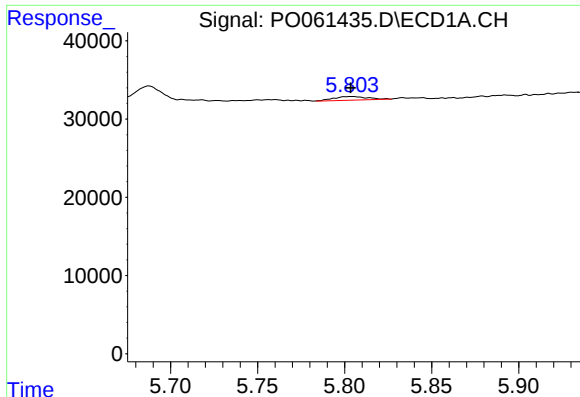

#22 AR-1248-2


R.T.: 5.804 min
Delta R.T.: 0.000 min
Response: 6347
Conc: 4.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

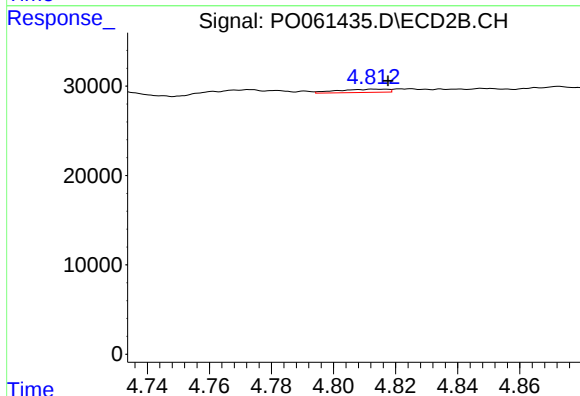


#22 AR-1248-2

R.T.: 4.813 min
Delta R.T.: -0.005 min
Response: 4002
Conc: 4.14 ng/ml

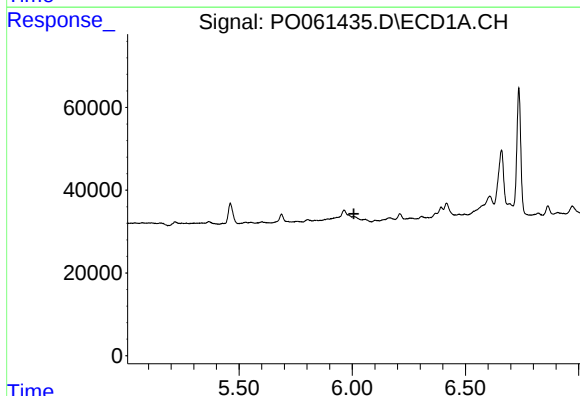


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 6.007 min
Response: 0
Conc: N.D.

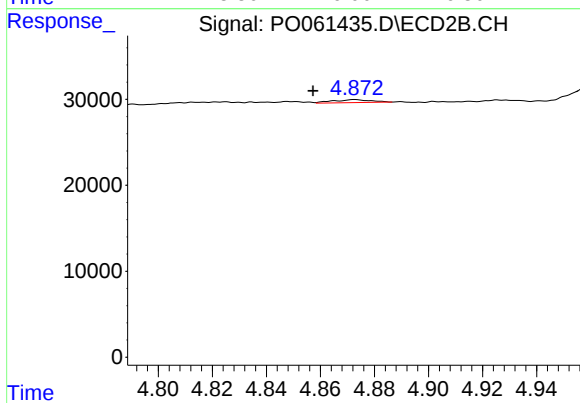

#23 AR-1248-3


R.T.: 4.873 min
Delta R.T.: 0.016 min
Response: 3392
Conc: 3.37 ng/ml

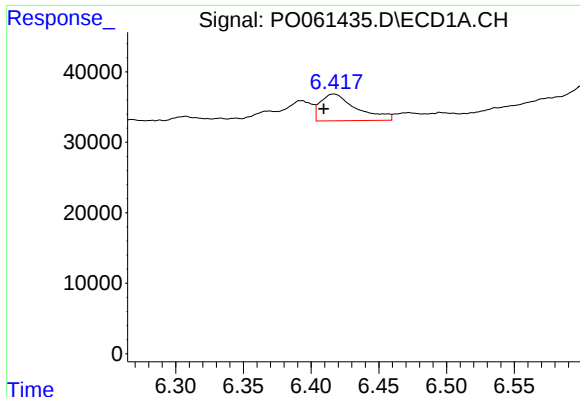

#24 AR-1248-4


R.T.: 6.417 min
Delta R.T.: 0.007 min
Response: 70323
Conc: 38.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

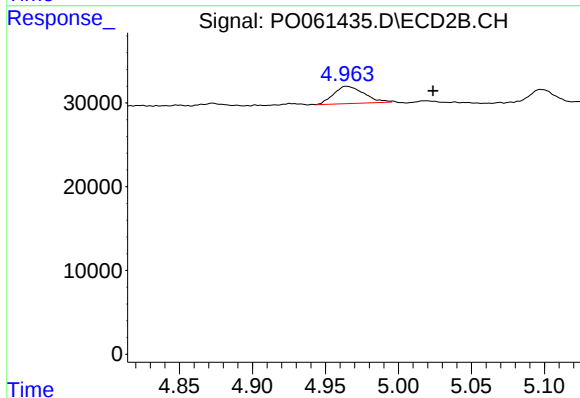


#24 AR-1248-4

R.T.: 4.964 min
Delta R.T.: -0.060 min
Response: 29900
Conc: 24.90 ng/ml

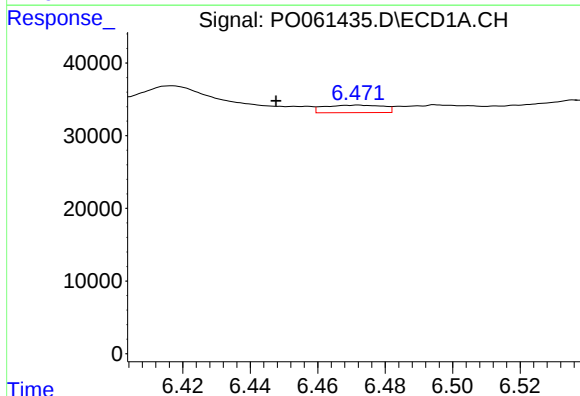


#25 AR-1248-5

R.T.: 6.472 min
Delta R.T.: 0.024 min
Response: 12640
Conc: 7.22 ng/ml

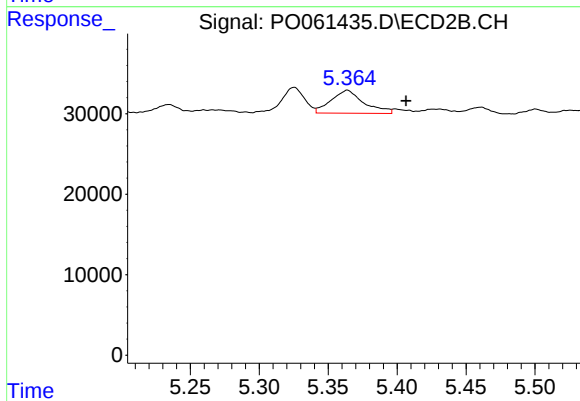

#25 AR-1248-5


R.T.: 5.364 min
Delta R.T.: -0.043 min
Response: 47209
Conc: 37.34 ng/ml

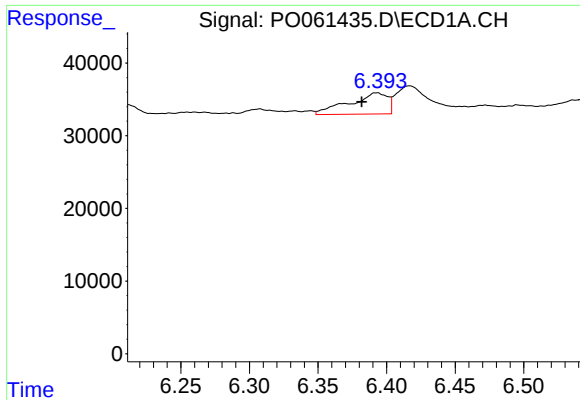

#26 AR-1254-1


R.T.: 6.393 min
Delta R.T.: 0.011 min
Response: 56745
Conc: 29.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

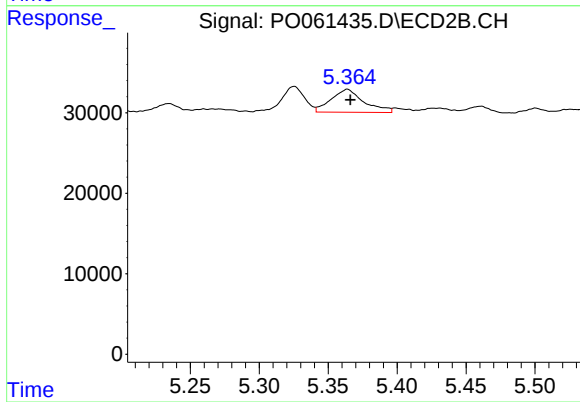


#26 AR-1254-1

R.T.: 5.364 min
Delta R.T.: -0.002 min
Response: 47209
Conc: 22.91 ng/ml

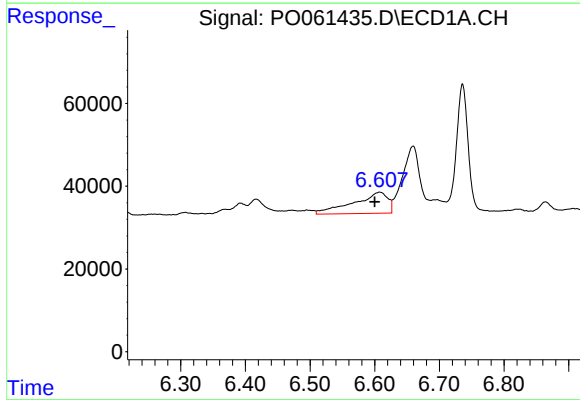


#27 AR-1254-2

R.T.: 6.608 min
Delta R.T.: 0.008 min
Response: 188741
Conc: 59.98 ng/ml

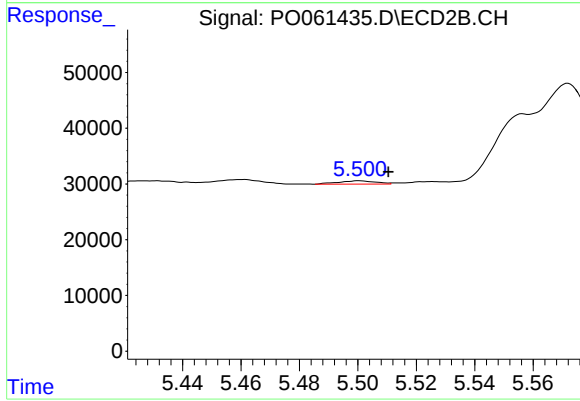

#27 AR-1254-2


R.T.: 5.500 min
Delta R.T.: -0.010 min
Response: 5213
Conc: 2.76 ng/ml

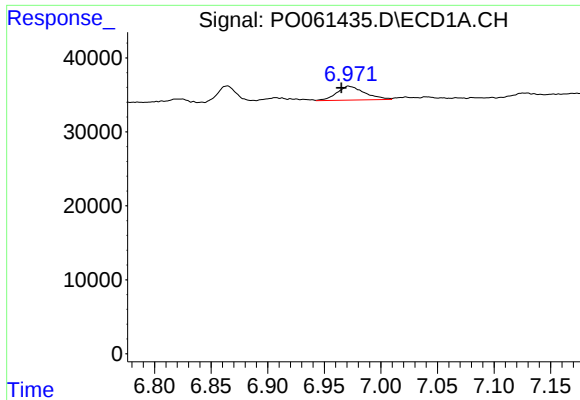

#28 AR-1254-3


R.T.: 6.972 min
Delta R.T.: 0.006 min
Response: 31982
Conc: 9.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

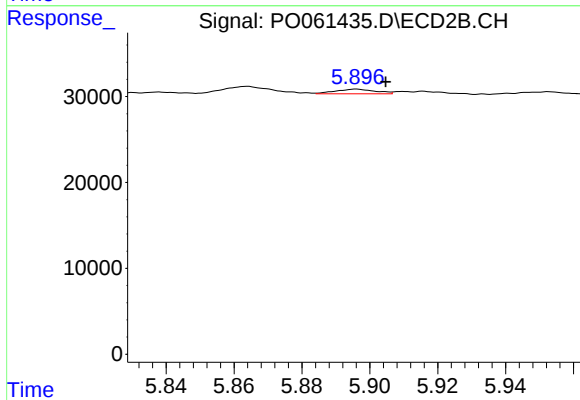


#28 AR-1254-3

R.T.: 5.896 min
Delta R.T.: -0.009 min
Response: 4477
Conc: 1.41 ng/ml

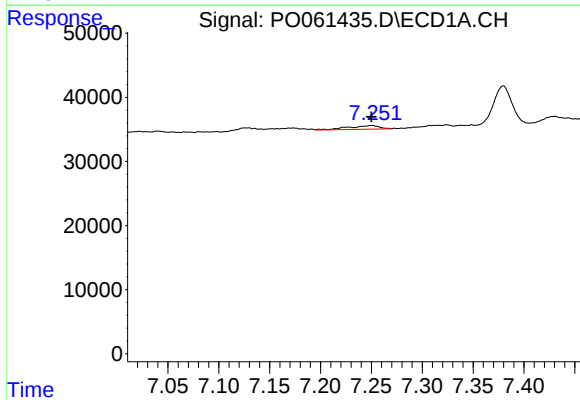


#29 AR-1254-4

R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 12184
Conc: 4.50 ng/ml

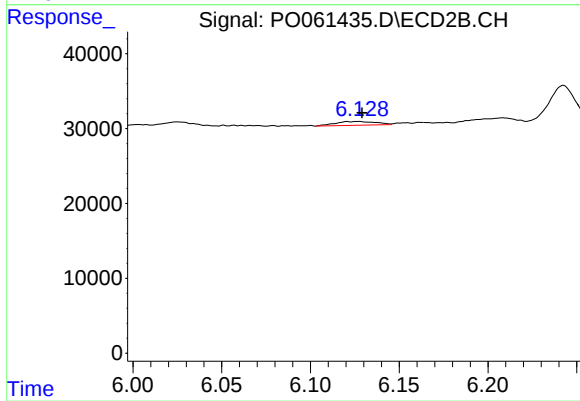

#29 AR-1254-4


R.T.: 6.128 min
Delta R.T.: -0.001 min
Response: 7959
Conc: 3.82 ng/ml

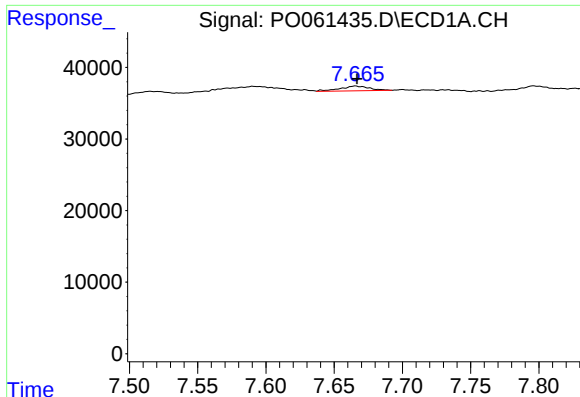

#30 AR-1254-5


R.T.: 7.666 min
Delta R.T.: -0.001 min
Response: 9961
Conc: 3.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

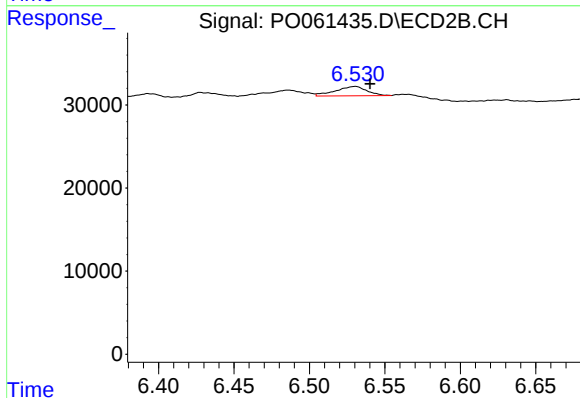


#30 AR-1254-5

R.T.: 6.531 min
Delta R.T.: -0.010 min
Response: 16402
Conc: 5.18 ng/ml

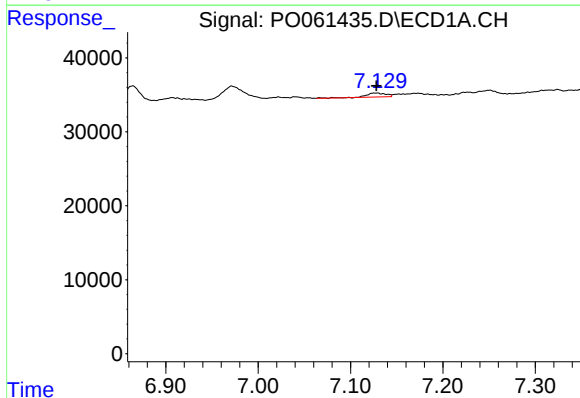


#31 AR-1260-1

R.T.: 7.128 min
Delta R.T.: 0.000 min
Response: 7942
Conc: 3.26 ng/ml

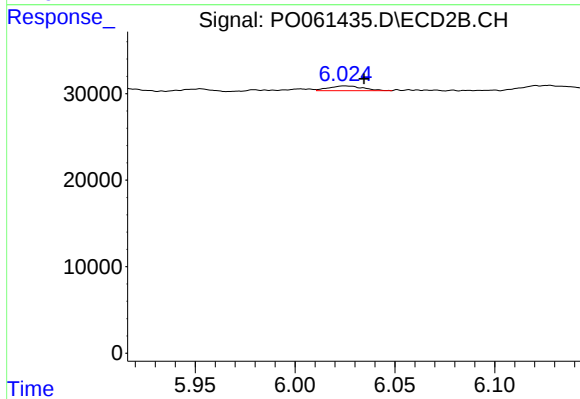

#31 AR-1260-1


R.T.: 6.025 min
Delta R.T.: -0.010 min
Response: 6598
Conc: 3.14 ng/ml

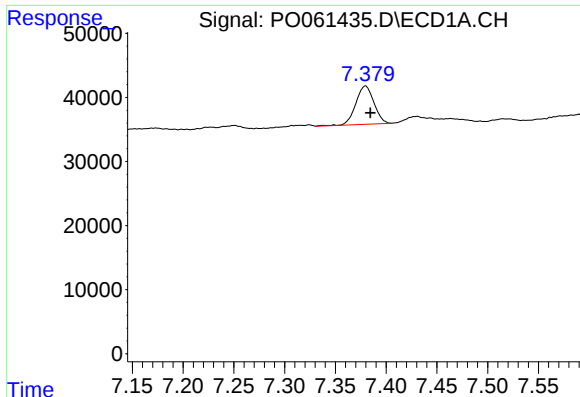

#32 AR-1260-2


R.T.: 7.380 min
Delta R.T.: -0.005 min
Response: 74388
Conc: 24.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

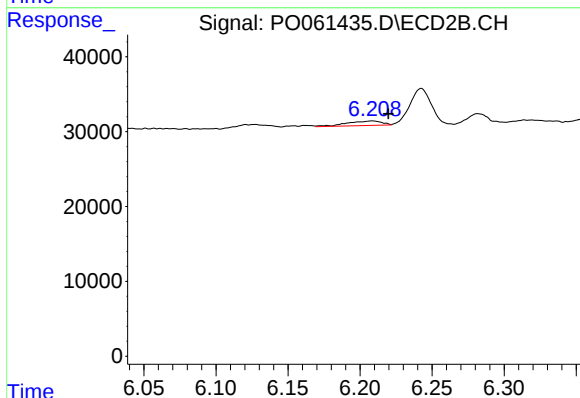


#32 AR-1260-2

R.T.: 6.208 min
Delta R.T.: -0.011 min
Response: 10151
Conc: 3.94 ng/ml

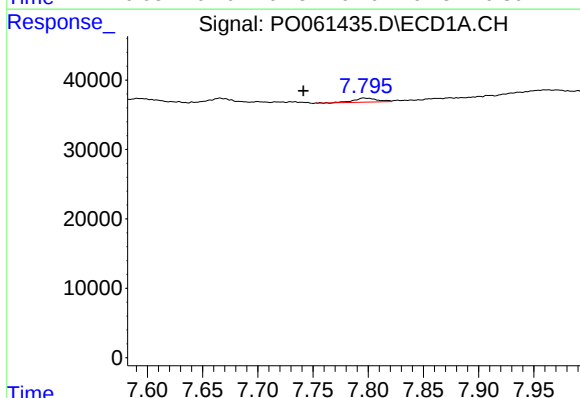


#33 AR-1260-3

R.T.: 7.796 min
Delta R.T.: 0.055 min
Response: 8687
Conc: 3.64 ng/ml

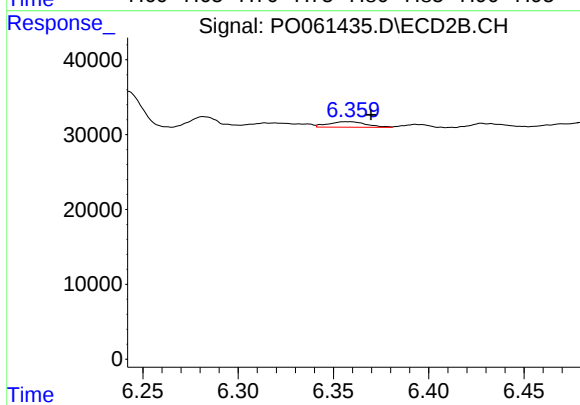

#33 AR-1260-3


R.T.: 6.359 min
Delta R.T.: -0.010 min
Response: 10321
Conc: 4.29 ng/ml

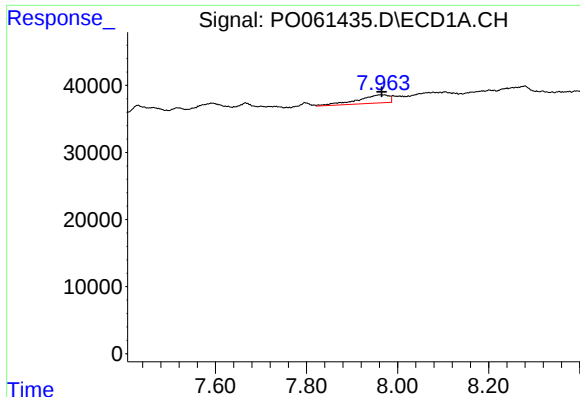

#34 AR-1260-4


R.T.: 7.963 min
Delta R.T.: -0.003 min
Response: 58722
Conc: 20.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

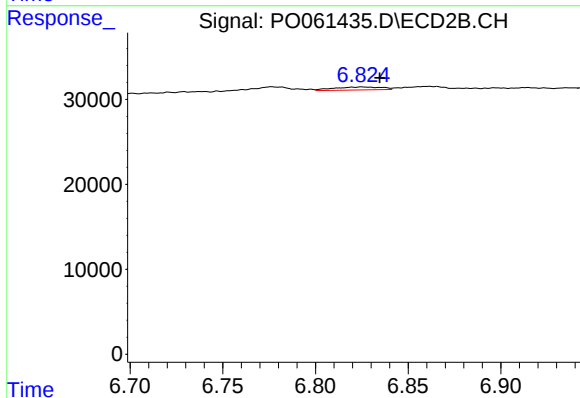


#34 AR-1260-4

R.T.: 6.825 min
Delta R.T.: -0.010 min
Response: 6296
Conc: 2.94 ng/ml

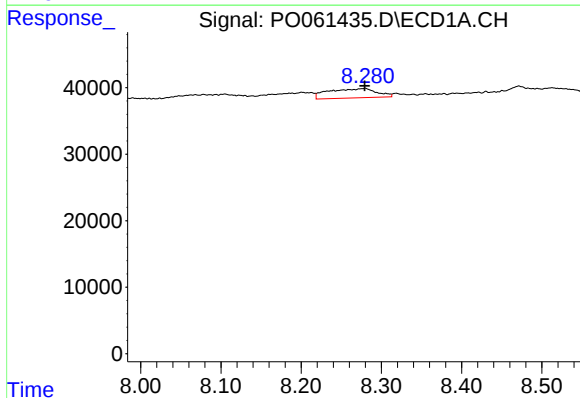


#35 AR-1260-5

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 58320
Conc: 10.71 ng/ml

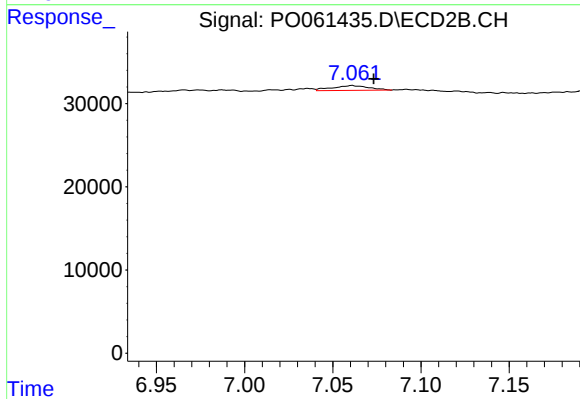

#35 AR-1260-5


R.T.: 7.061 min
Delta R.T.: -0.012 min
Response: 8428
Conc: 1.74 ng/ml

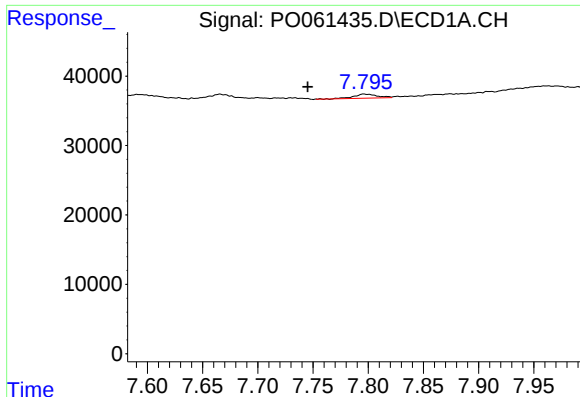

#36 AR-1262-1


R.T.: 7.796 min
Delta R.T.: 0.051 min
Response: 8687
Conc: 2.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

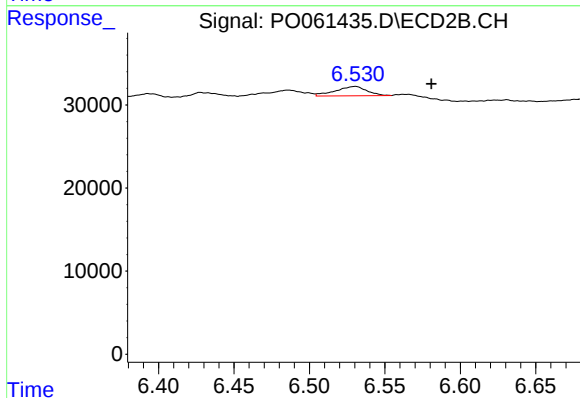


#36 AR-1262-1

R.T.: 6.531 min
Delta R.T.: -0.050 min
Response: 16402
Conc: 5.49 ng/ml

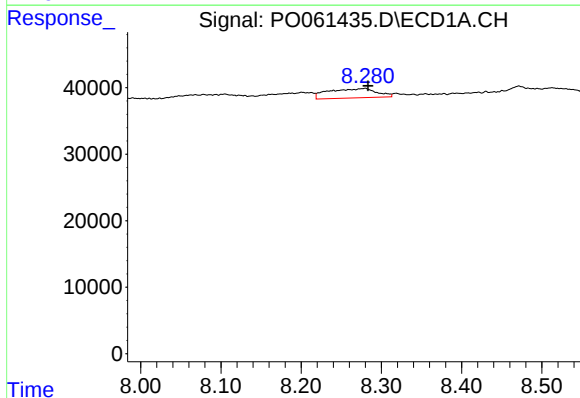


#37 AR-1262-2

R.T.: 8.280 min
Delta R.T.: -0.004 min
Response: 58320
Conc: 9.35 ng/ml

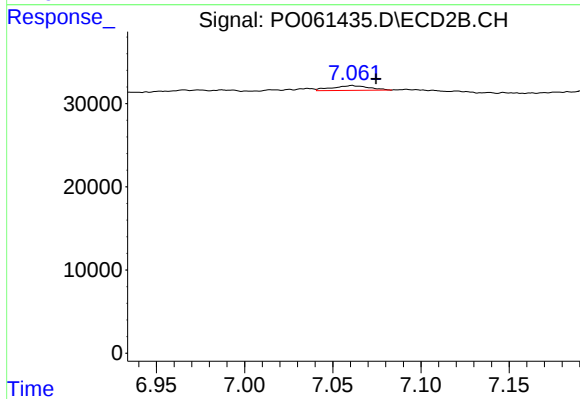

#37 AR-1262-2


R.T.: 7.061 min
Delta R.T.: -0.014 min
Response: 8428
Conc: 1.62 ng/ml

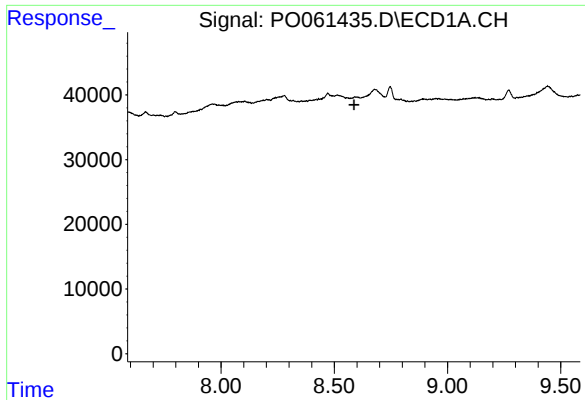

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

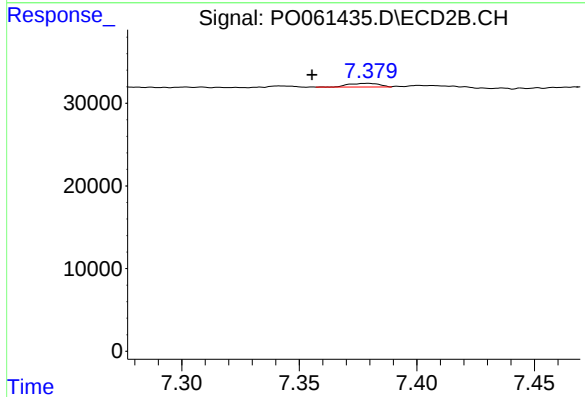


#38 AR-1262-3

R.T.: 7.379 min
Delta R.T.: 0.024 min
Response: 4052
Conc: 1.91 ng/ml

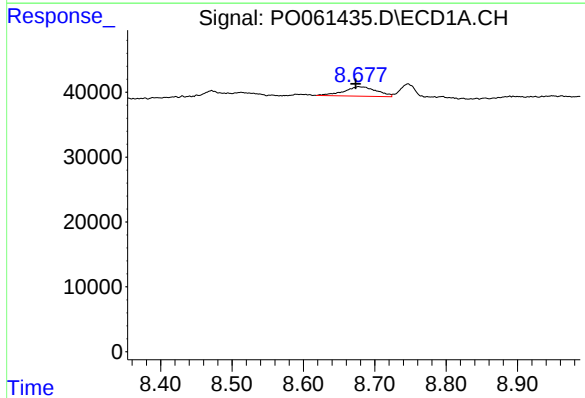


#39 AR-1262-4

R.T.: 8.677 min
Delta R.T.: 0.004 min
Response: 46383
Conc: 14.23 ng/ml

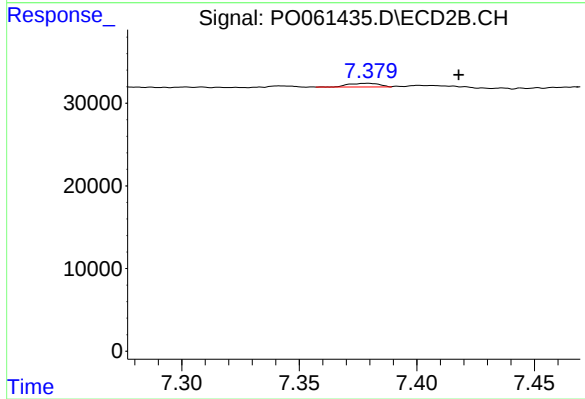

#39 AR-1262-4


R.T.: 7.379 min
Delta R.T.: -0.038 min
Response: 4052
Conc: 1.06 ng/ml

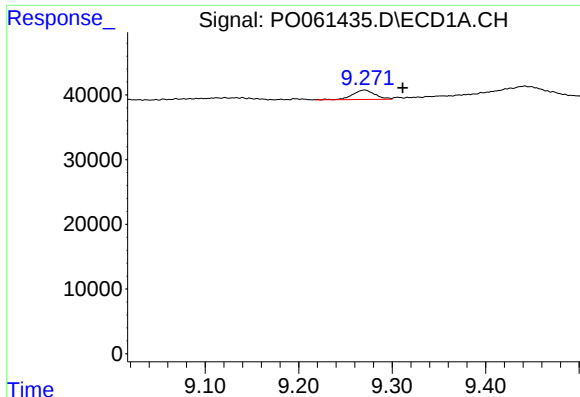

#40 AR-1262-5


R.T.: 9.271 min
Delta R.T.: -0.041 min
Response: 23899
Conc: 11.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

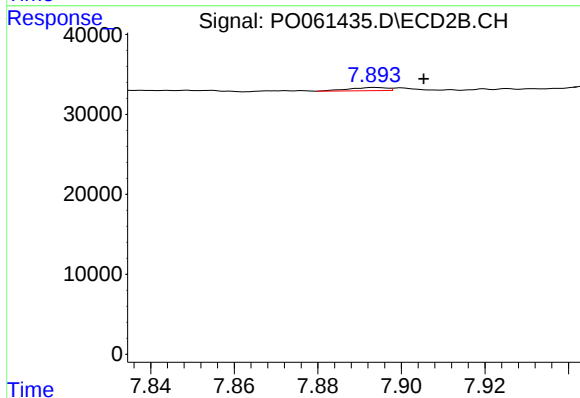


#40 AR-1262-5

R.T.: 7.894 min
Delta R.T.: -0.012 min
Response: 2484
Conc: 1.48 ng/ml

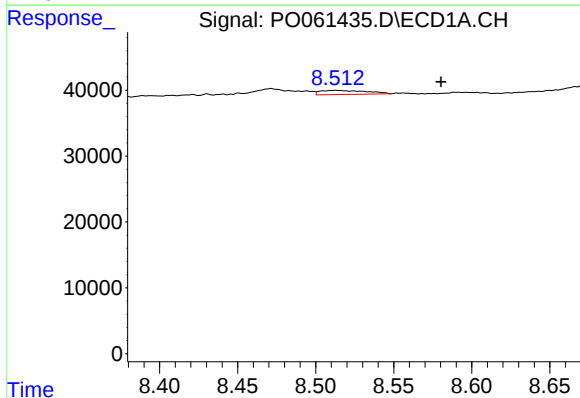


#41 AR-1268-1

R.T.: 8.513 min
Delta R.T.: -0.067 min
Response: 12649
Conc: 1.71 ng/ml

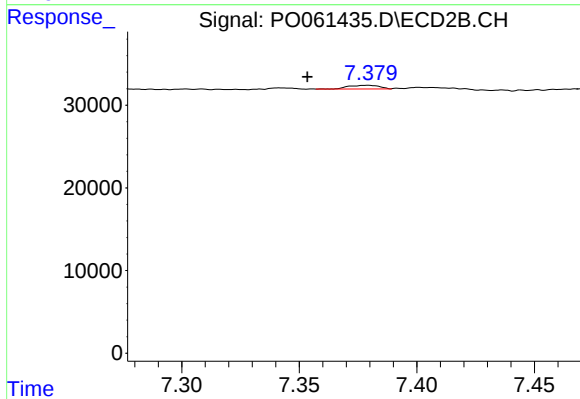

#41 AR-1268-1


R.T.: 7.379 min
Delta R.T.: 0.026 min
Response: 4052
Conc: 0.69 ng/ml

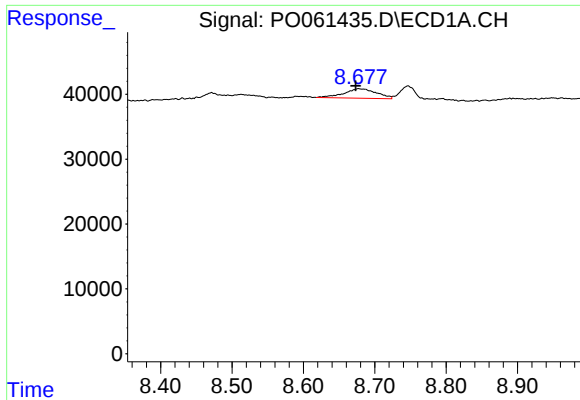

#42 AR-1268-2


R.T.: 8.677 min
Delta R.T.: 0.004 min
Response: 46383
Conc: 6.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

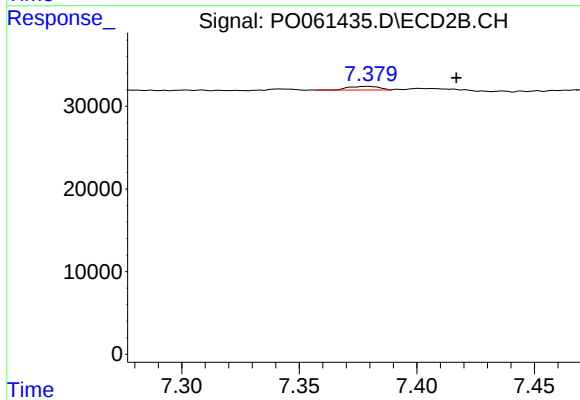


#42 AR-1268-2

R.T.: 7.379 min
Delta R.T.: -0.037 min
Response: 4052
Conc: 0.76 ng/ml

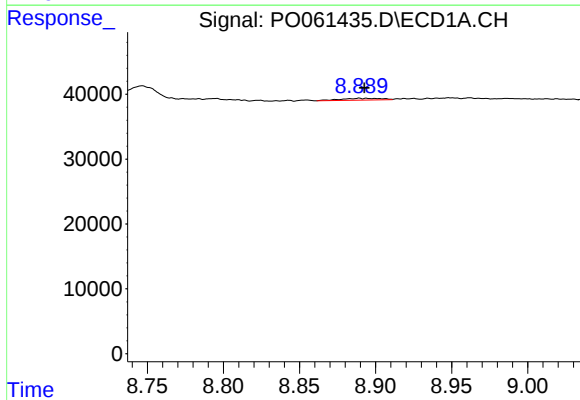


#43 AR-1268-3

R.T.: 8.889 min
Delta R.T.: -0.003 min
Response: 5236
Conc: 0.93 ng/ml

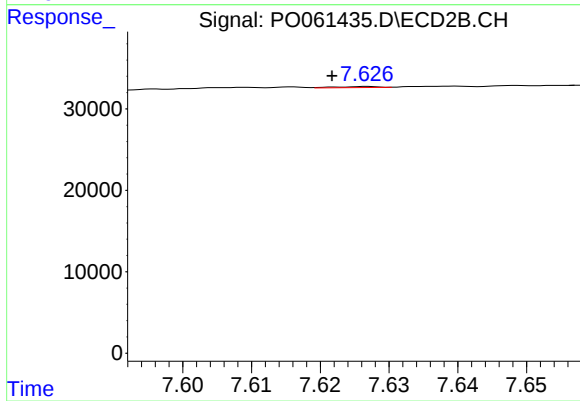

#43 AR-1268-3


R.T.: 7.627 min
Delta R.T.: 0.005 min
Response: 567
Conc: 0.13 ng/ml

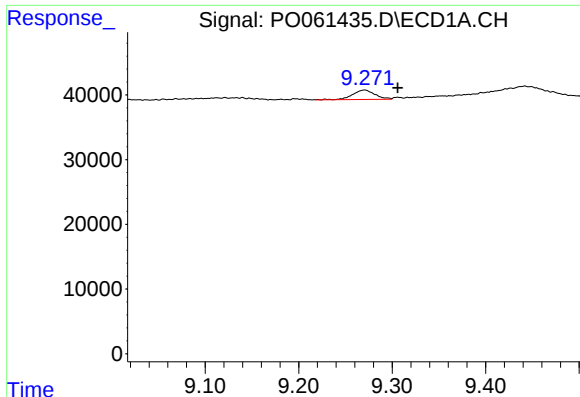

#44 AR-1268-4


R.T.: 9.271 min
Delta R.T.: -0.036 min
Response: 23899
Conc: 10.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-060

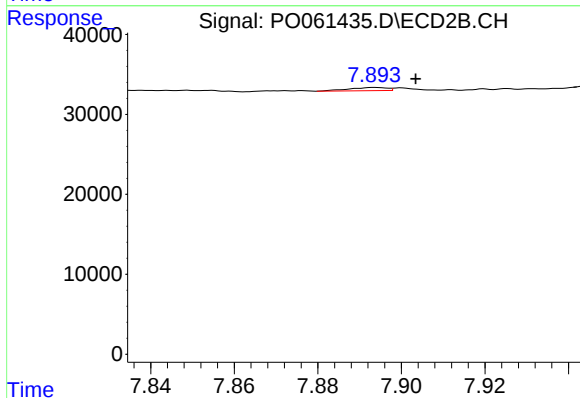


#44 AR-1268-4

R.T.: 7.894 min
Delta R.T.: -0.010 min
Response: 2484
Conc: 1.30 ng/ml

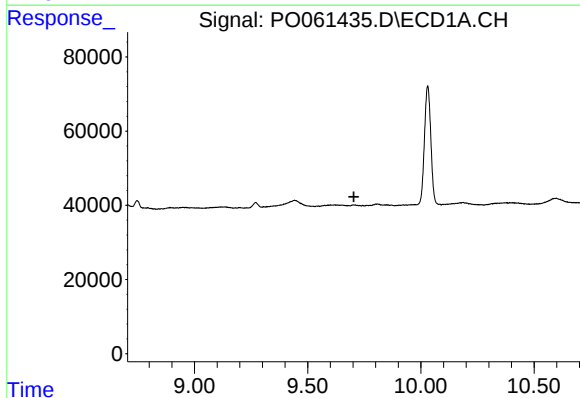

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.704 min
Response: 0
Conc: N.D.

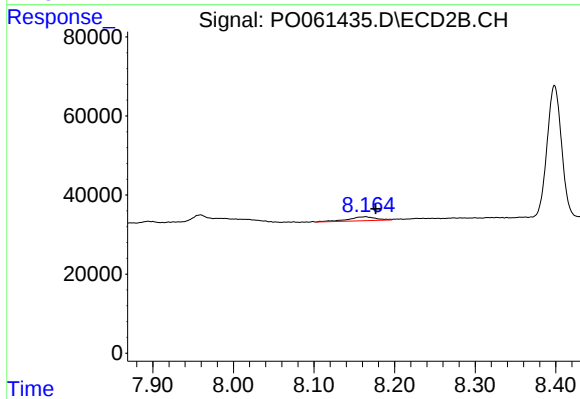

#45 AR-1268-5

R.T.: 8.164 min
Delta R.T.: -0.012 min
Response: 24054
Conc: 2.00 ng/ml