

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 14:42
 Operator : SM/AJ
 Sample : K5039-19 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30430

Manual Integrations
 APPROVED

Ankita
 10/1/2019 8:44:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 17:28:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.532	211323	172479	5.744m	6.177
2) SA Decachlor...	10.036	8.401	297720	197156	6.480m	5.625m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 14:42
Operator : SM/AJ
Sample : K5039-19 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30430


Manual Integrations
APPROVED

Ankita
10/1/2019 8:44:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 17:28:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

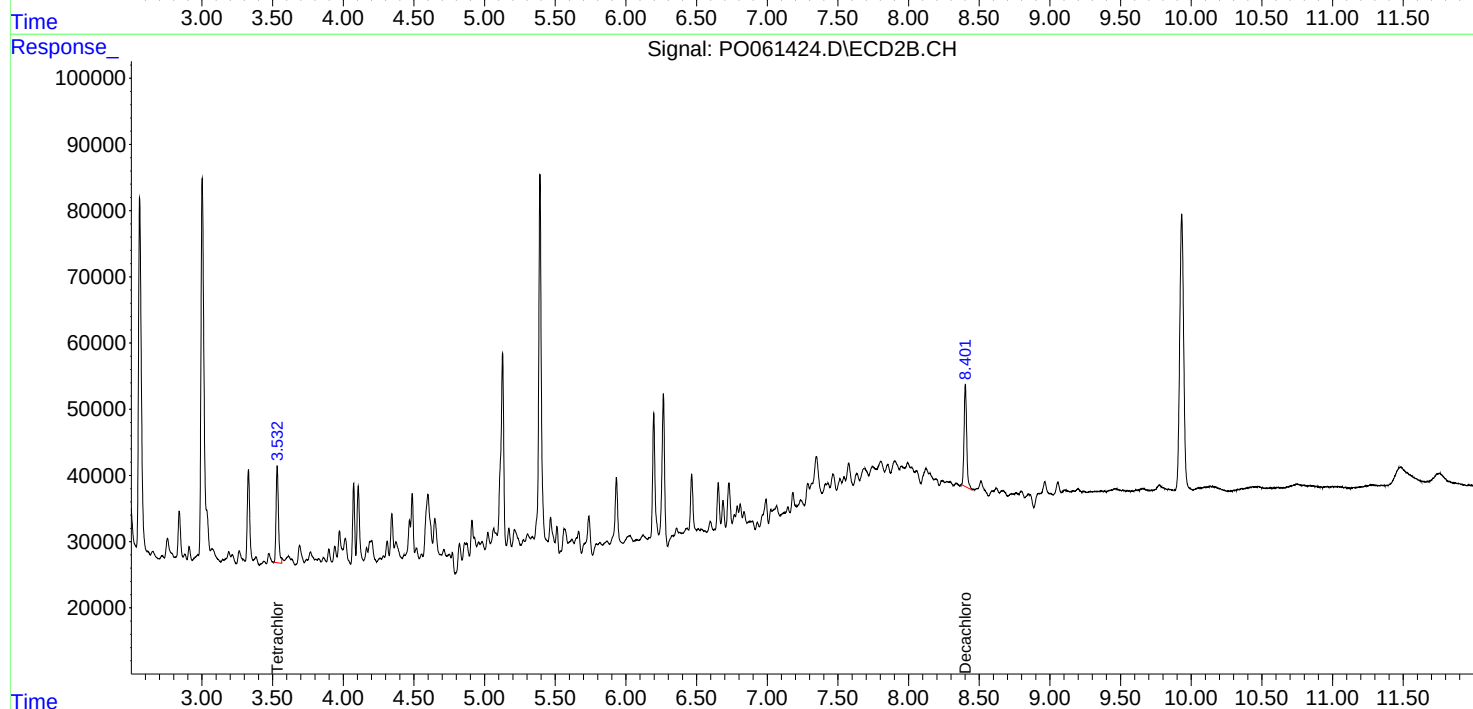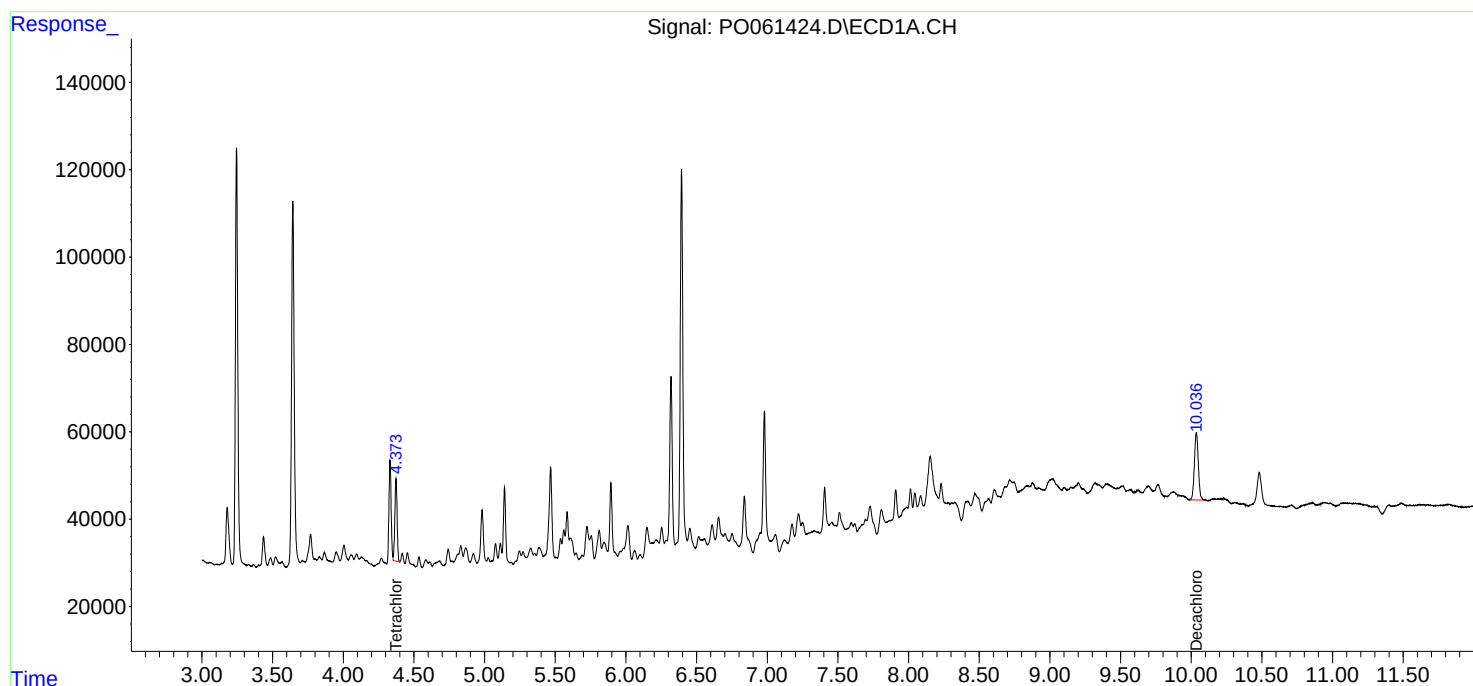

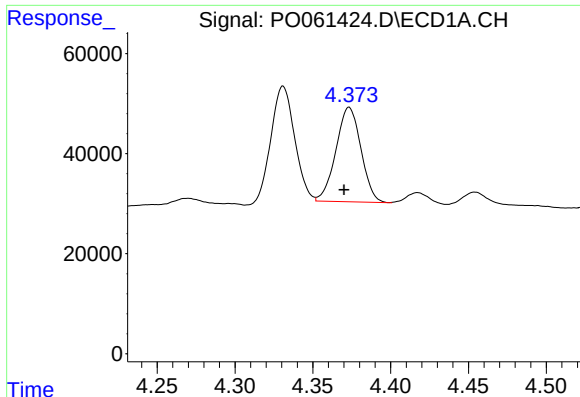


#1 Tetrachloro-m-xylene

R.T.: 4.373 min
Delta R.T.: 0.003 min
Response: 211323
Conc: 5.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
30430


Manual Integrations
APPROVED

Ankita
10/1/2019 8:44:10 AM

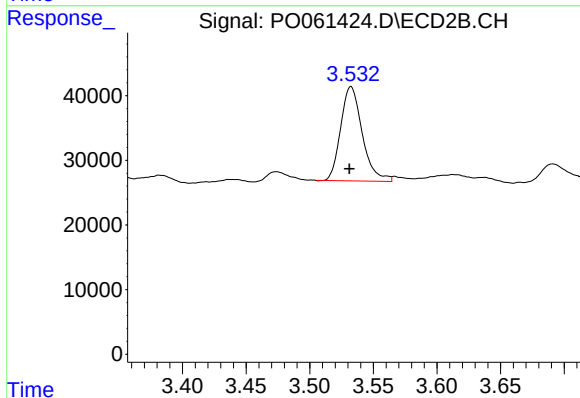


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.001 min
Response: 172479
Conc: 6.18 ng/ml

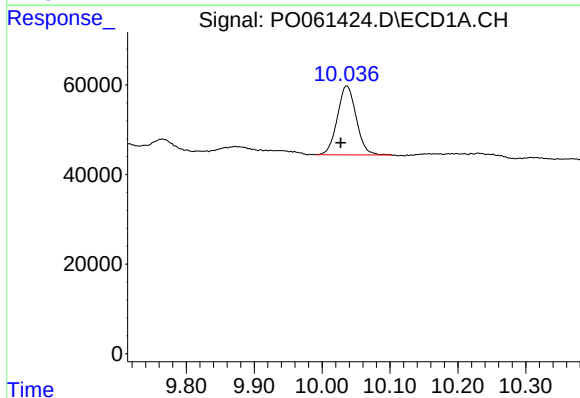

#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: 0.009 min
Response: 297720
Conc: 6.48 ng/ml m

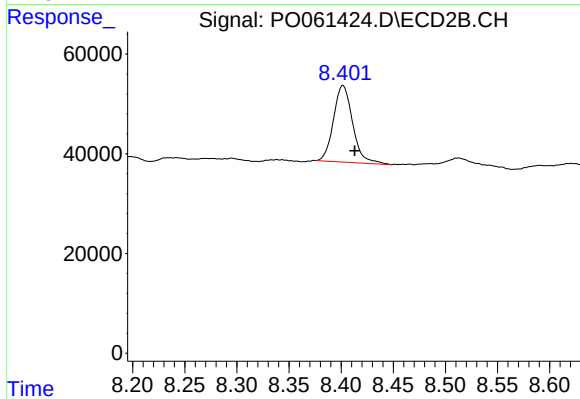

#2 Decachlorobiphenyl

R.T.: 8.401 min
Delta R.T.: -0.012 min
Response: 197156
Conc: 5.62 ng/ml m