

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061430.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 17:30
Operator : HP/AJ
Sample : PB123427BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB123427BL

Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:54:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.526	912877	696021	24.813	24.927
2) SA Decachlor...	10.030	8.399	1141729	794198	24.849	22.658m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061430.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 17:30
Operator : HP/AJ
Sample : PB123427BL
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB123427BL


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:54:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

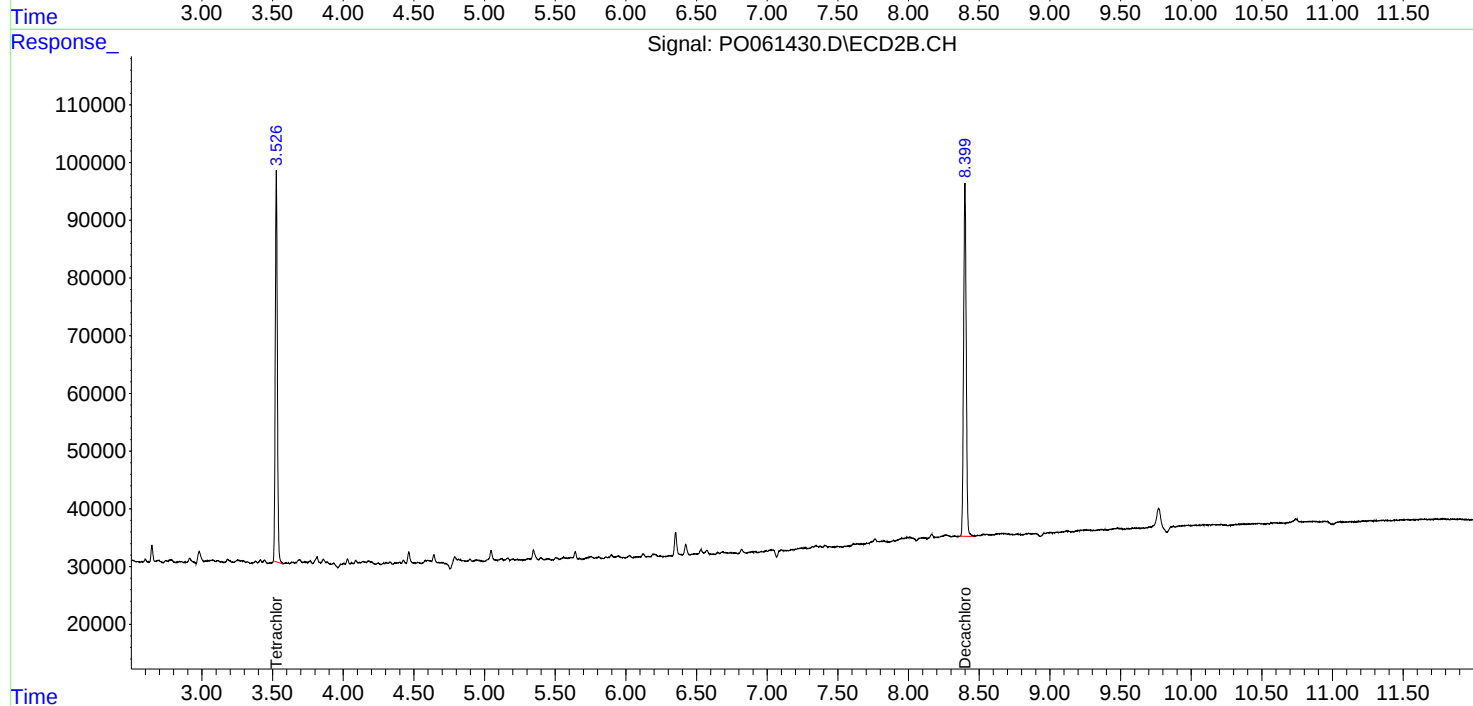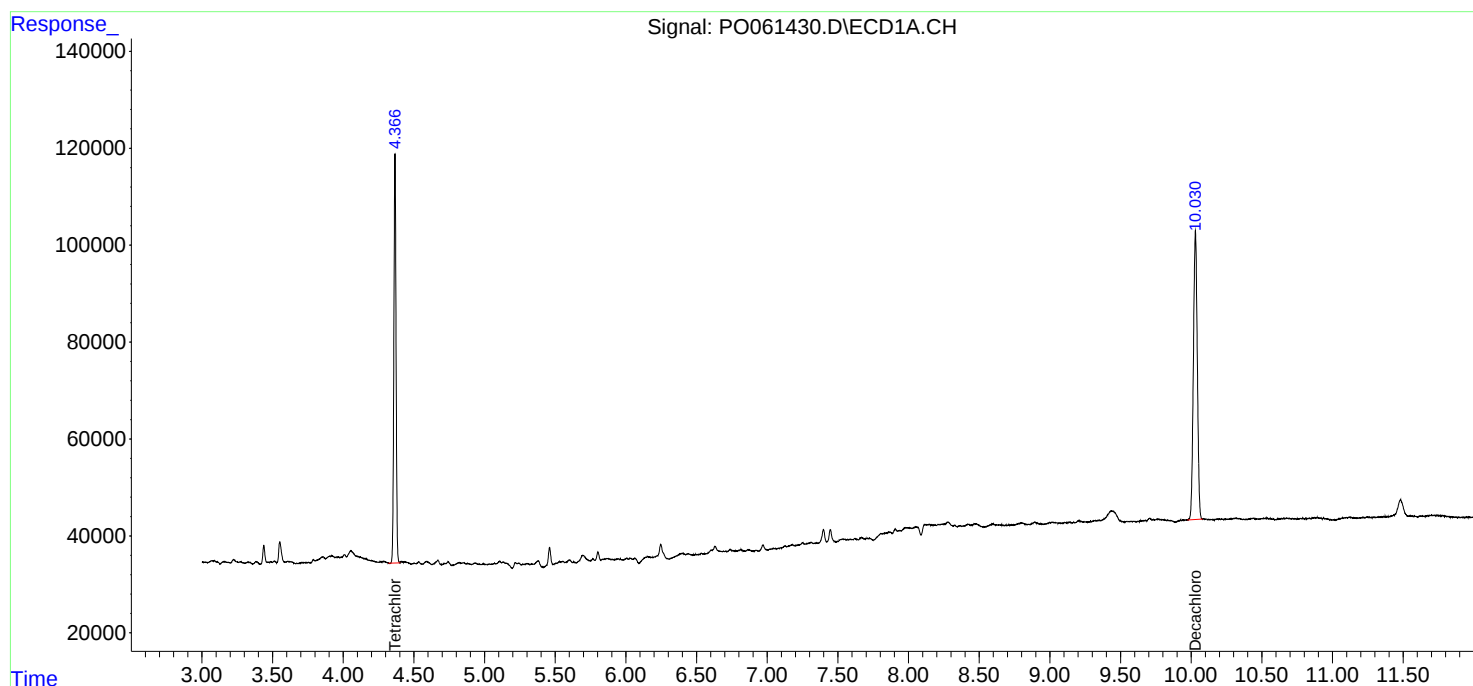

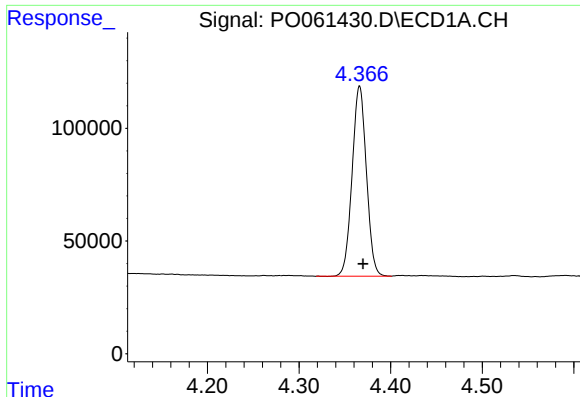


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.004 min
Response: 912877
Conc: 24.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB123427BL


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:04 PM

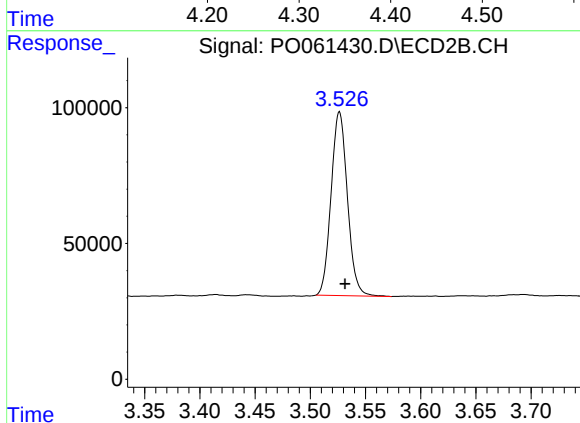


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.005 min
Response: 696021
Conc: 24.93 ng/ml

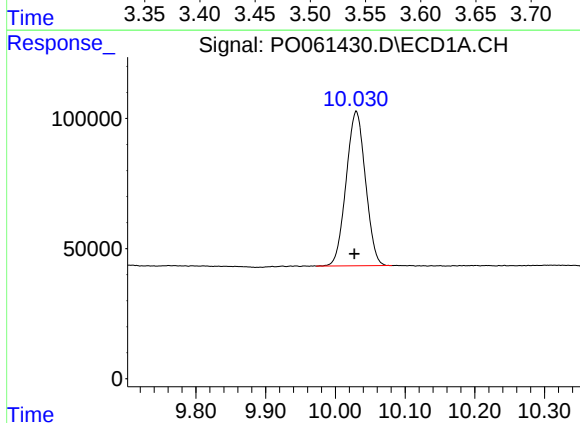

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.002 min
Response: 1141729
Conc: 24.85 ng/ml

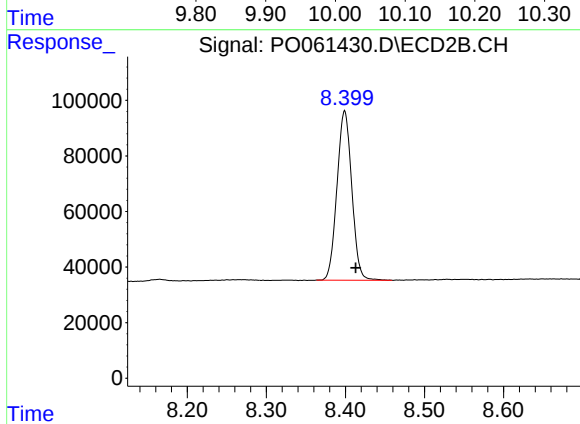

#2 Decachlorobiphenyl

R.T.: 8.399 min
Delta R.T.: -0.014 min
Response: 794198
Conc: 22.66 ng/ml m