

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
 Data File : P0061436.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2019 19:07
 Operator : HP/AJ
 Sample : K5064-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUM-COMP

Manual Integrations
 APPROVED

Ankita
 9/30/2019 1:53:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 23:56:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 14 00:06:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.367	3.526	1040376	856362	28.278	30.670m
2) SA Decachlor...	10.032	8.401	877810	564449	19.105	16.103

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0092719\
Data File : P0061436.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2019 19:07
Operator : HP/AJ
Sample : K5064-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUM-COMP


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 23:56:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0091319.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 14 00:06:36 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

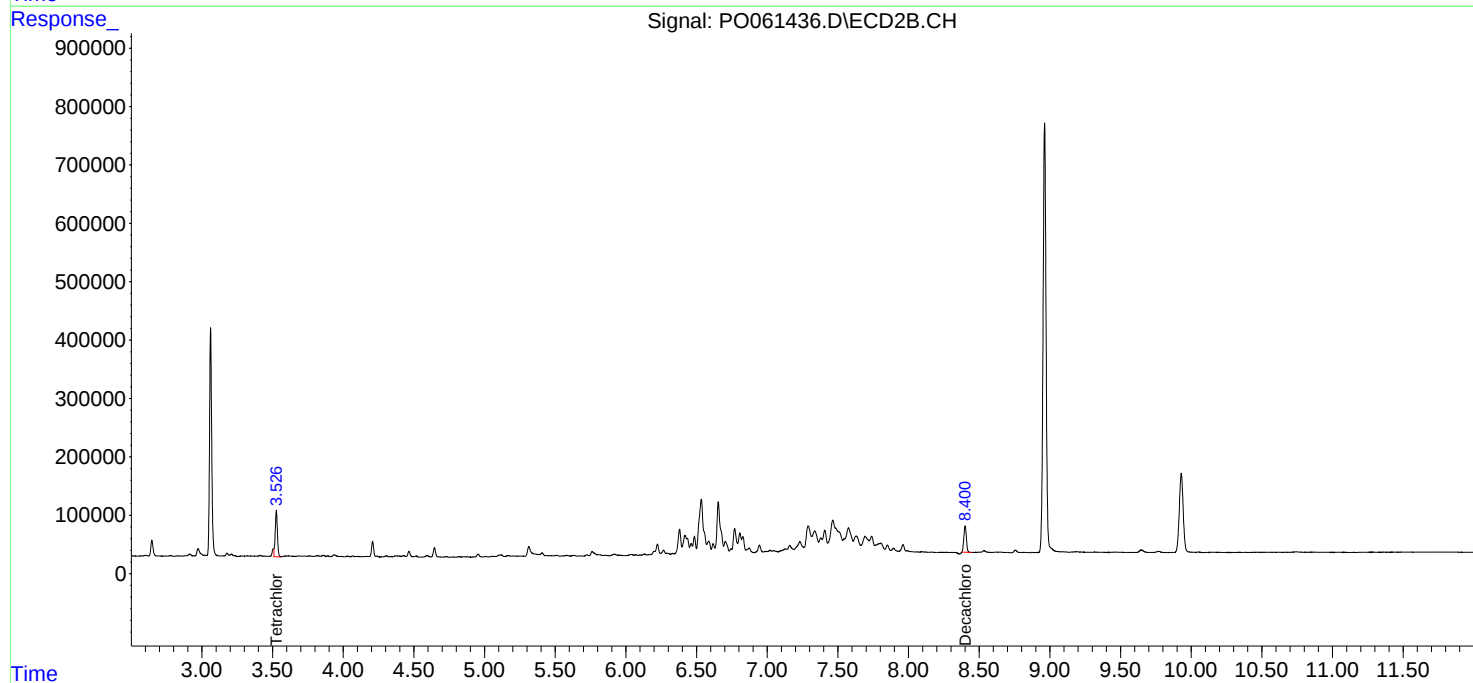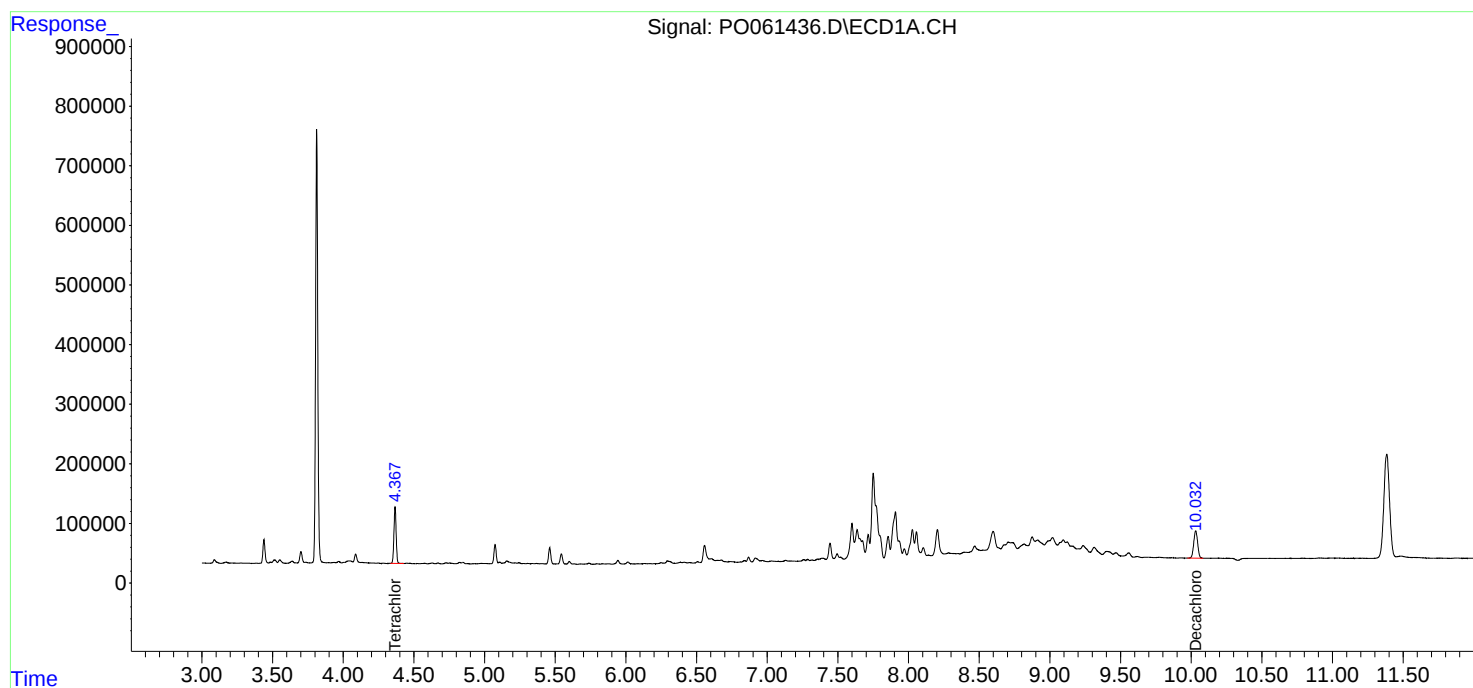

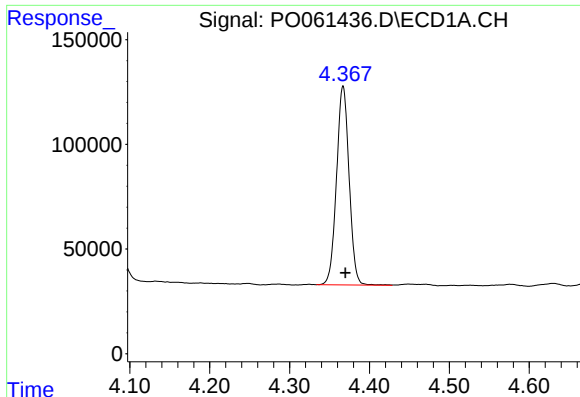


#1 Tetrachloro-m-xylene

R.T.: 4.367 min
Delta R.T.: -0.003 min
Response: 1040376
Conc: 28.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRUM-COMP


Manual Integrations
APPROVED

Ankita
9/30/2019 1:53:25 PM

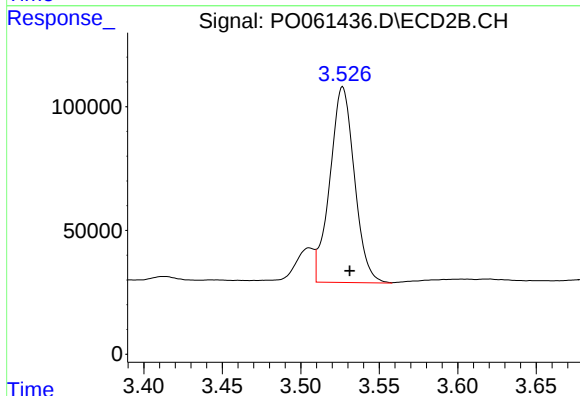


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.005 min
Response: 856362
Conc: 30.67 ng/ml m

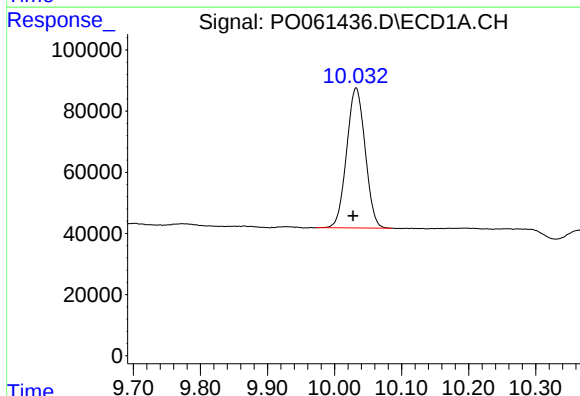

#2 Decachlorobiphenyl

R.T.: 10.032 min
Delta R.T.: 0.005 min
Response: 877810
Conc: 19.11 ng/ml

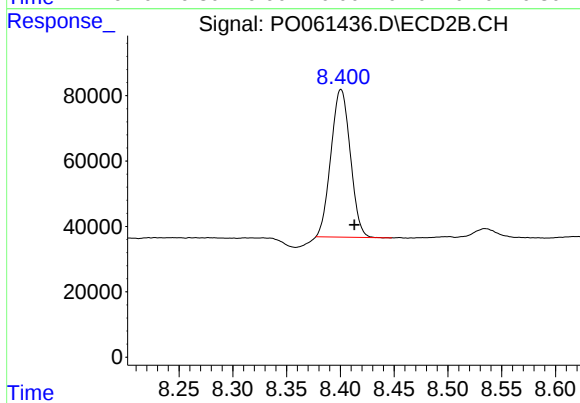

#2 Decachlorobiphenyl

R.T.: 8.401 min
Delta R.T.: -0.013 min
Response: 564449
Conc: 16.10 ng/ml